

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
 Data File : PL057132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 18:12
 Operator : AJ\MA
 Sample : L1753-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 03:00:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.461	3.959	172.0E6	43738908	20.178	20.501
28) SA Decachlor...	8.211	8.986	169.7E6	38286316	17.554	18.019
Target Compounds						
4) MA Heptachlor	0.000	5.144	0	32026072	N.D.	10.290 #
8) B Heptachlo...	0.000	5.803	0	7438084	N.D.	2.684 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
Data File : PL057132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 18:12
Operator : AJ\MA
Sample : L1753-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 03:00:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

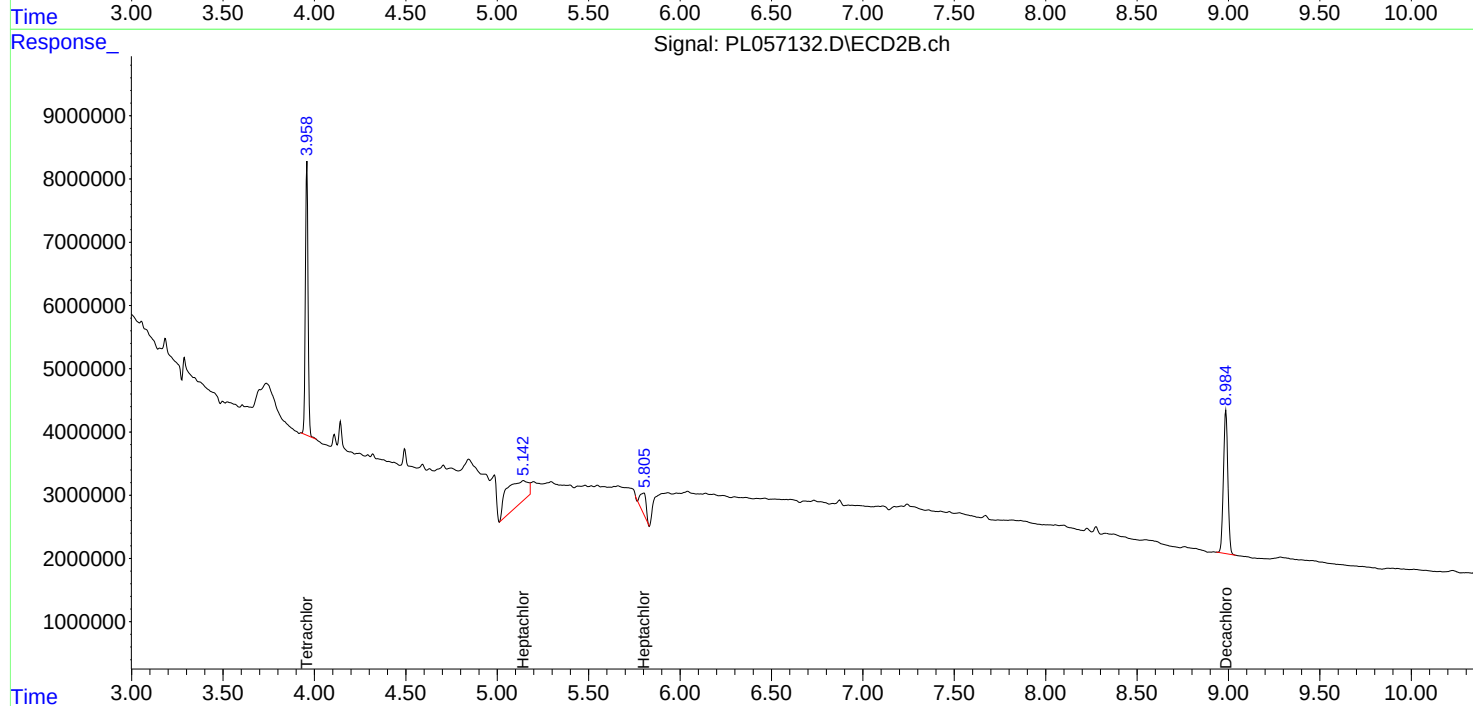


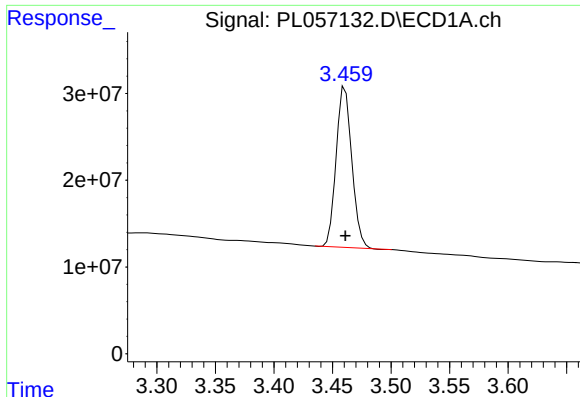

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 171958949
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

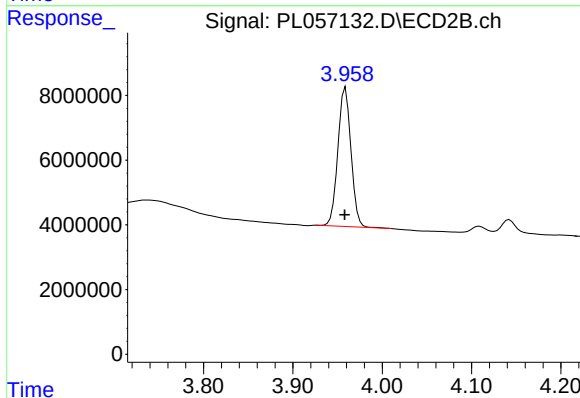


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 43738908
Conc: 20.50 ng/ml

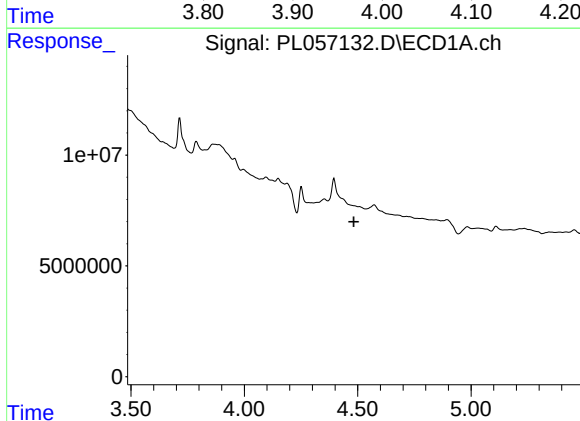


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

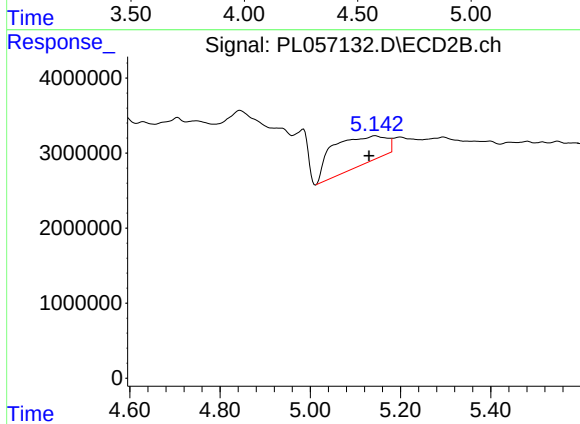

#4 Heptachlor


R.T.: 5.144 min
Delta R.T.: 0.013 min
Response: 32026072
Conc: 10.29 ng/ml

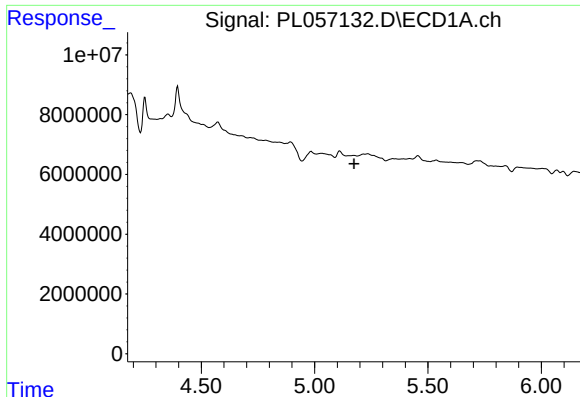

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

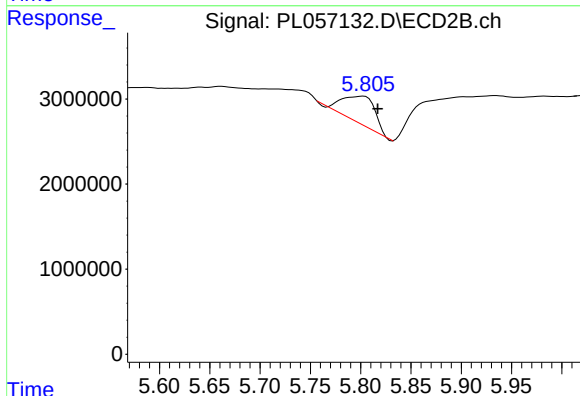


#8 Heptachlor epoxide

R.T.: 5.803 min
Delta R.T.: -0.014 min
Response: 7438084
Conc: 2.68 ng/ml

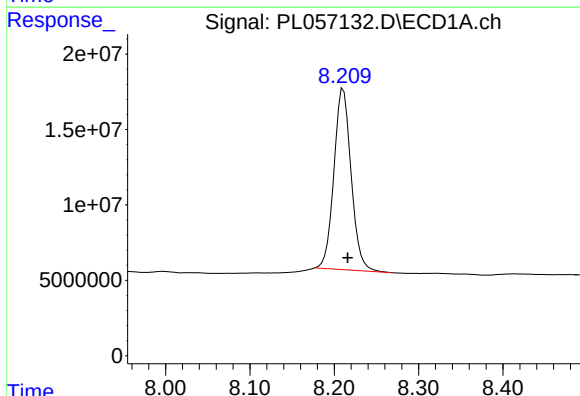

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: -0.005 min
Response: 169664630
Conc: 17.55 ng/ml

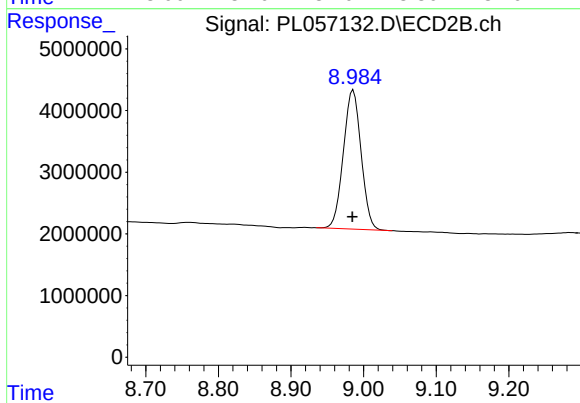

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: 0.001 min
Response: 38286316
Conc: 18.02 ng/ml