

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 11:40
 Operator : AR\AJ
 Sample : PB134955BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:09:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	4.099	58163317	46125441	19.781	18.575
28)	SA Decachlor...	8.149	9.261	54484775	40600302	19.633	18.484
Target Compounds							
6)	B beta-BHC	4.358f	0.000	743545	0	0.398	N.D. #
14)	MA Endrin	5.963	0.000	2881537	0	0.839	N.D. #
18)	B Endrin al...	6.406f	0.000	2771562	0	1.081	N.D. #
23)	Chlordane-1	4.276	0.000	2199074	0	17.253	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 11:40
Operator : AR\AJ
Sample : PB134955BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:09:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

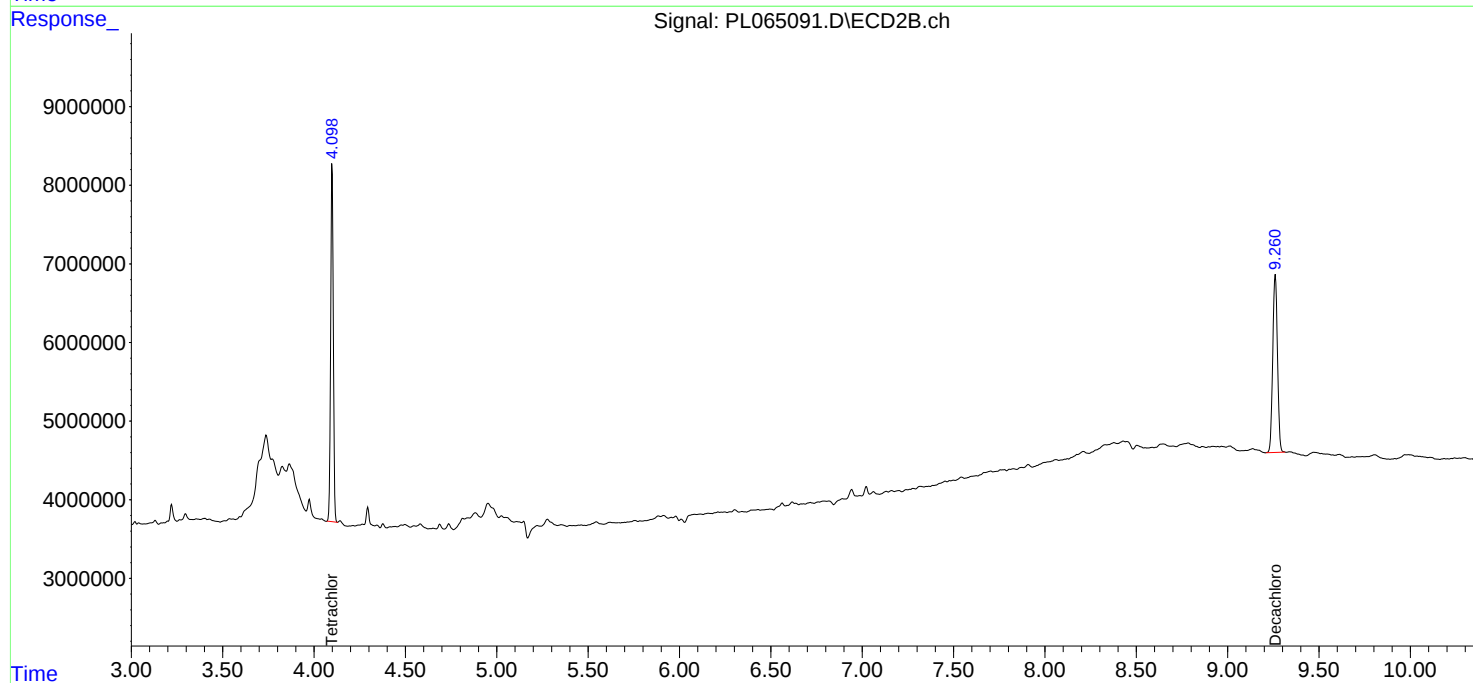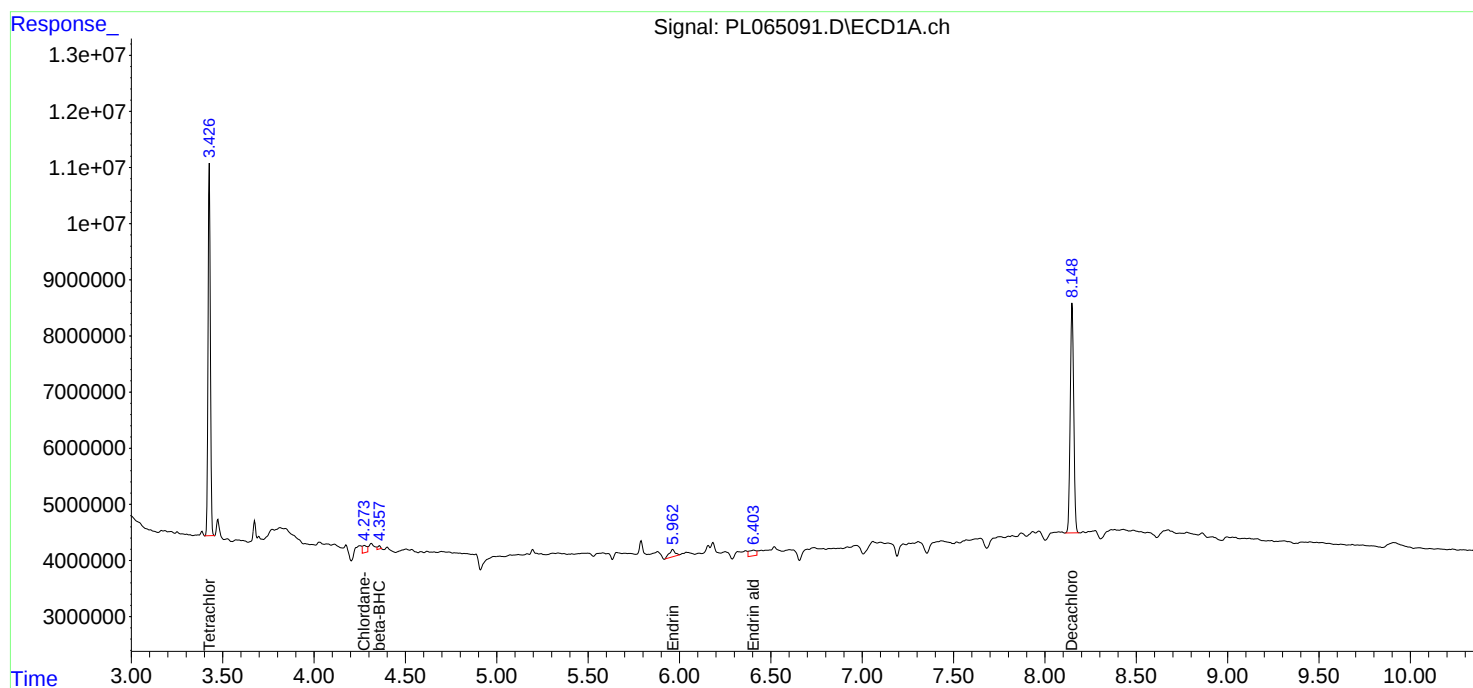


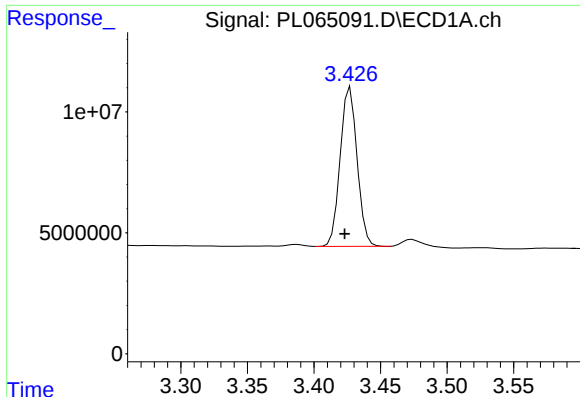

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: 0.004 min
Response: 58163317
Conc: 19.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

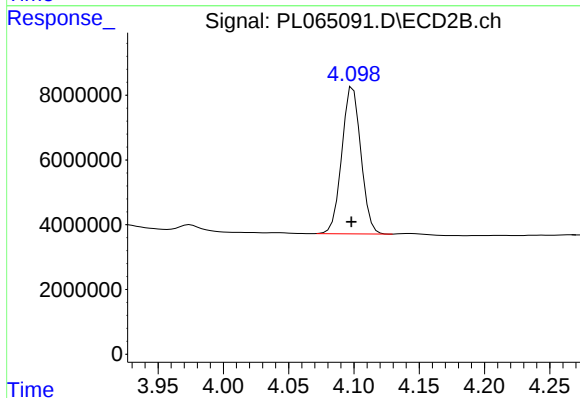


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.001 min
Response: 46125441
Conc: 18.57 ng/ml

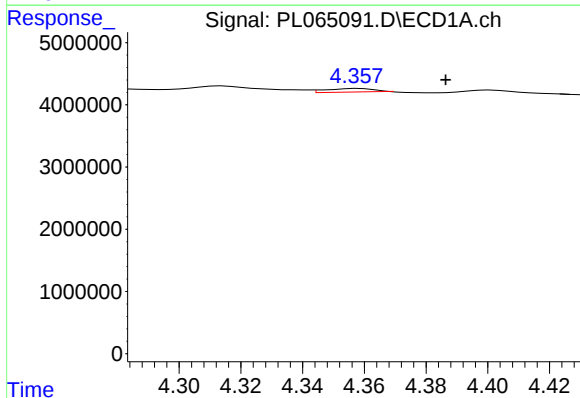


#6 beta-BHC

R.T.: 4.358 min
Delta R.T.: -0.028 min
Response: 743545
Conc: 0.40 ng/ml

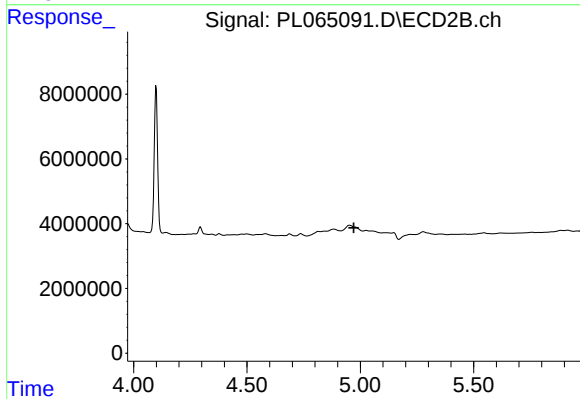

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.972 min
Response: 0
Conc: N.D.

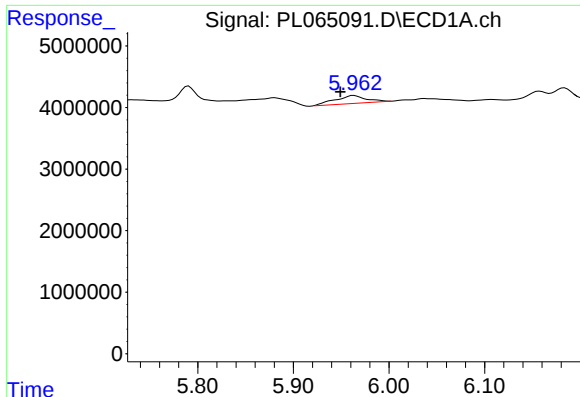

#14 Endrin


R.T.: 5.963 min
Delta R.T.: 0.014 min
Response: 2881537
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

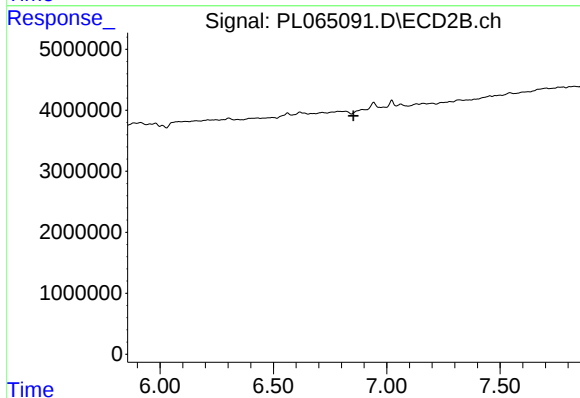


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

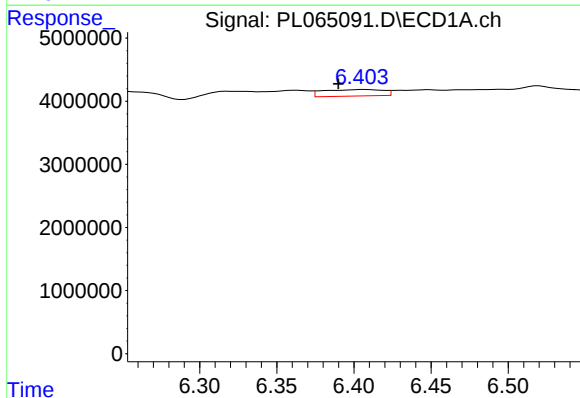


#18 Endrin aldehyde

R.T.: 6.406 min
Delta R.T.: 0.016 min
Response: 2771562
Conc: 1.08 ng/ml

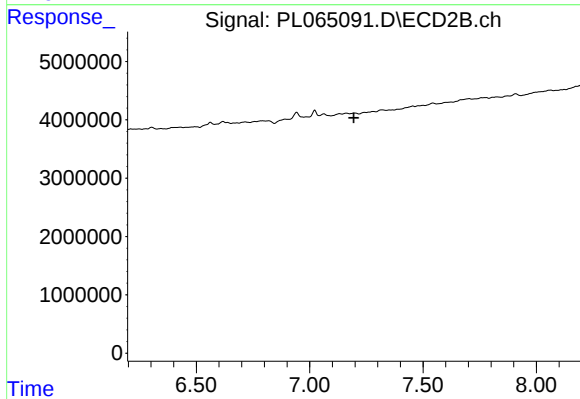

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.194 min
Response: 0
Conc: N.D.

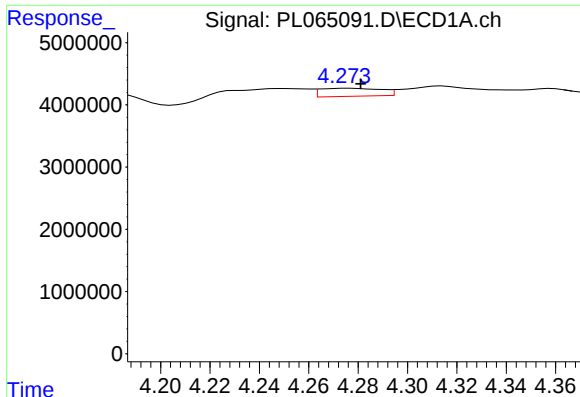

#23 Chlordane-1


R.T.: 4.276 min
Delta R.T.: -0.006 min
Response: 2199074
Conc: 17.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

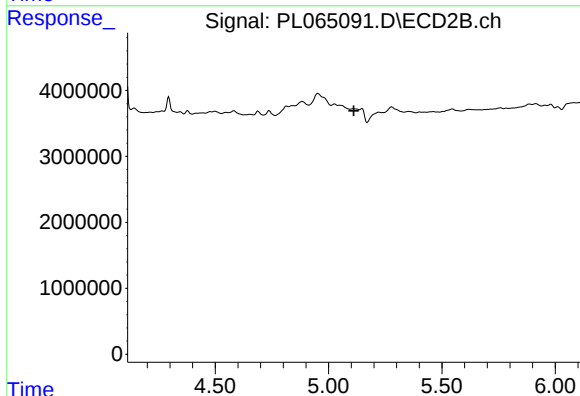


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

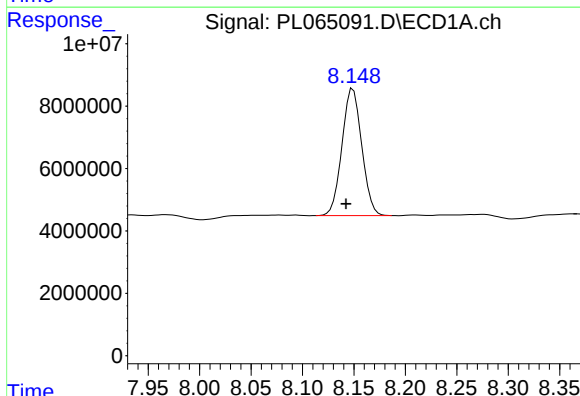

#28 Decachlorobiphenyl

R.T.: 8.149 min
Delta R.T.: 0.007 min
Response: 54484775
Conc: 19.63 ng/ml

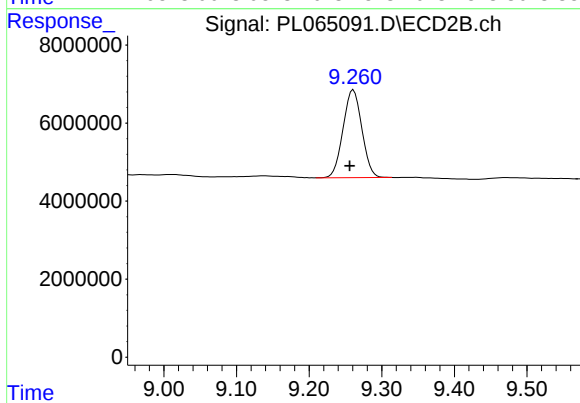

#28 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.005 min
Response: 40600302
Conc: 18.48 ng/ml