

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 14:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:12:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	66747316	52982344	22.700	21.336
28)	SA Decachlor...	8.143	9.257	57827464	46818200	20.838	21.315
Target Compounds							
6)	B beta-BHC	0.000	4.972	0	5155011	N.D.	3.371 #
14)	MA Endrin	5.956	0.000	3100004	0	0.903	N.D. #
23)	Chlordane-1	4.309f	0.000	6814742	0	53.466	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 14:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:12:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

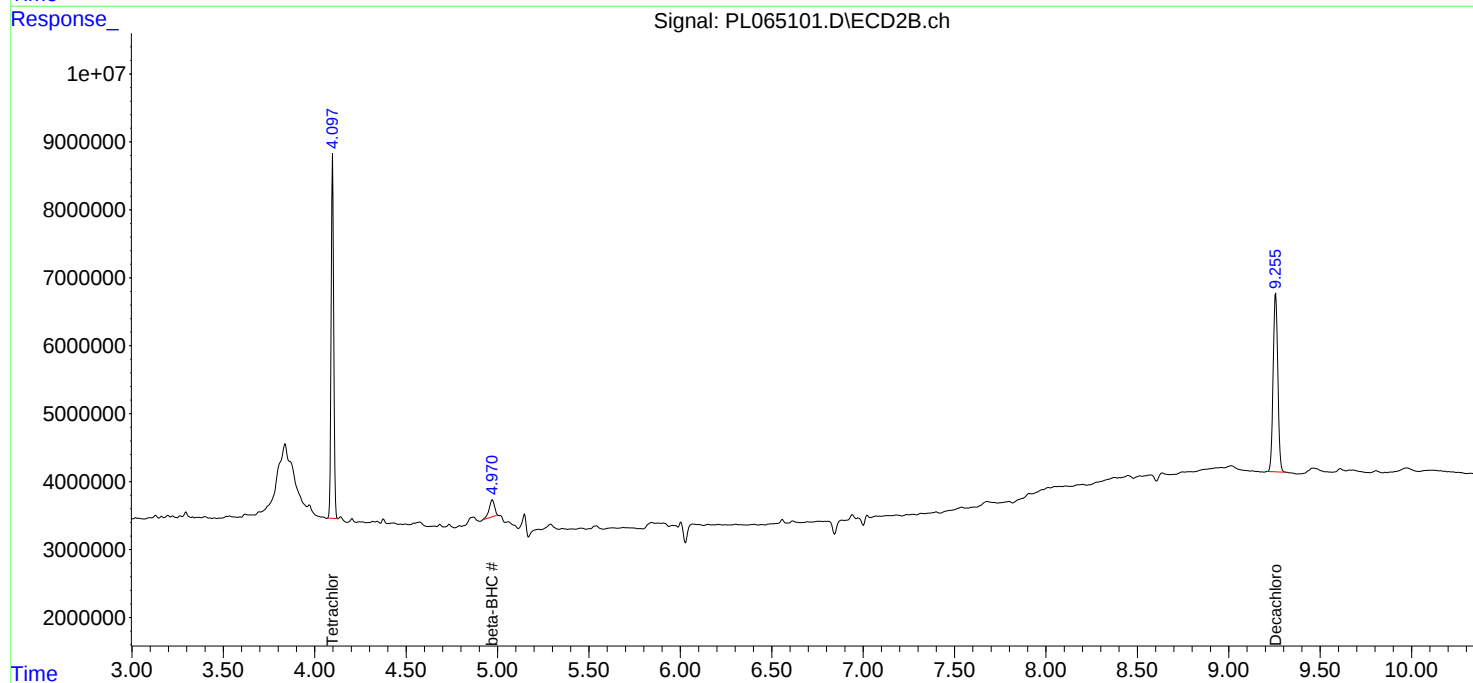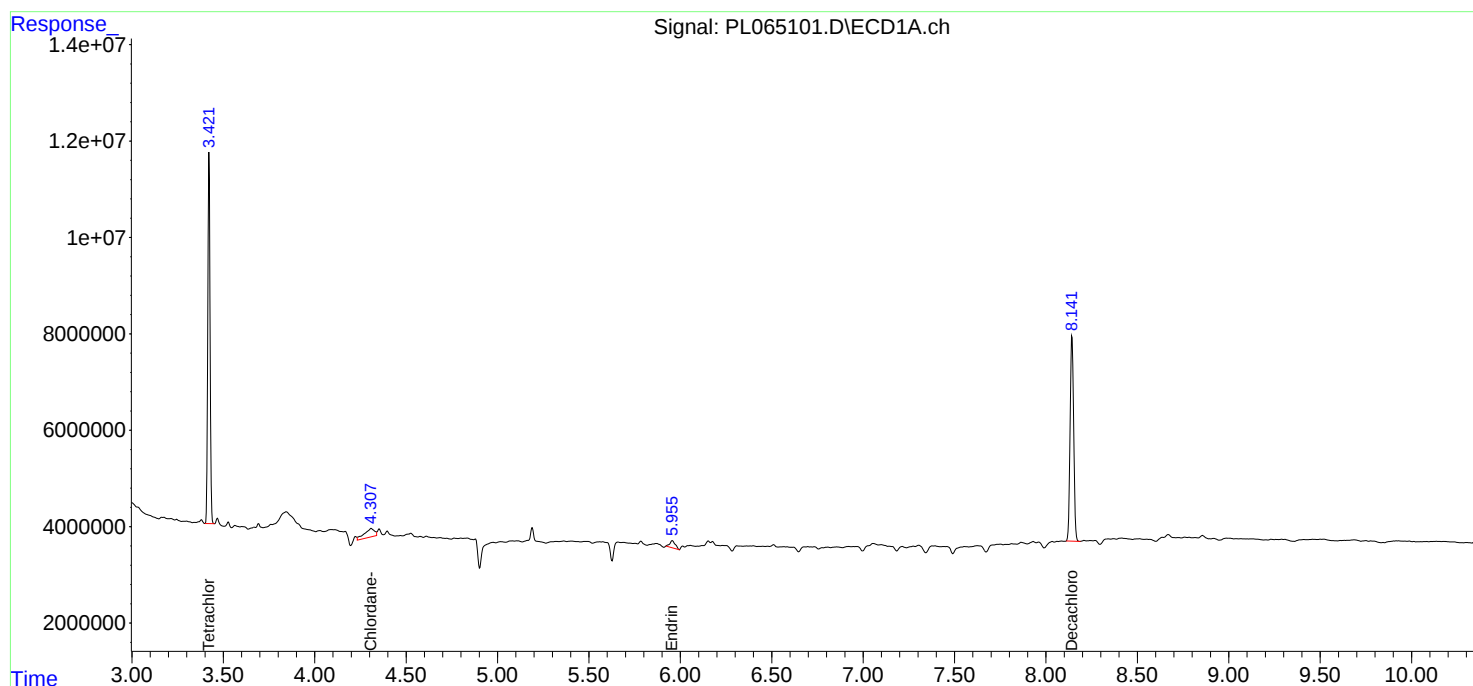


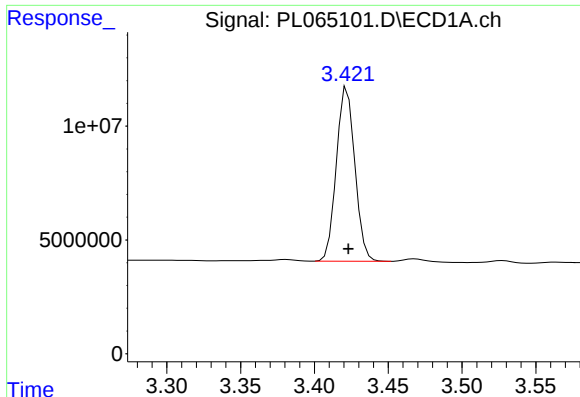

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 66747316
Conc: 22.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

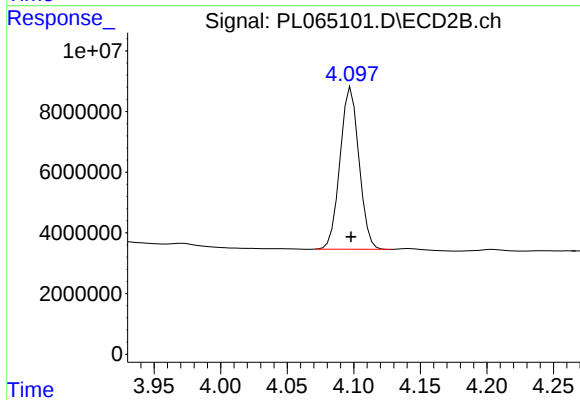


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 52982344
Conc: 21.34 ng/ml

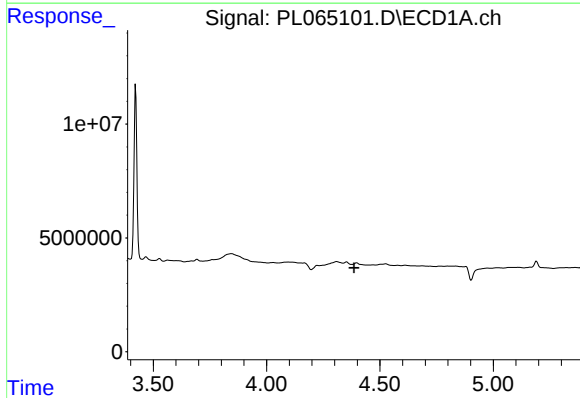


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.386 min
Response: 0
Conc: N.D.

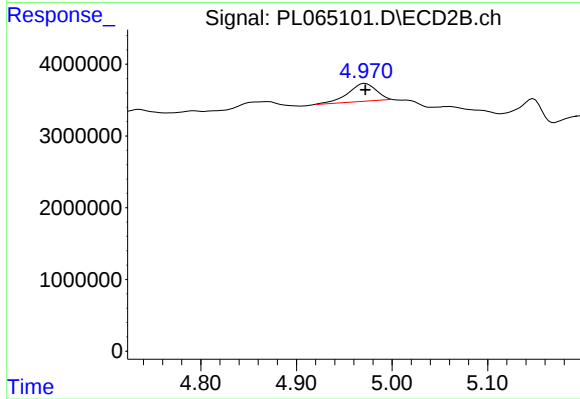

#6 beta-BHC


R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 5155011
Conc: 3.37 ng/ml

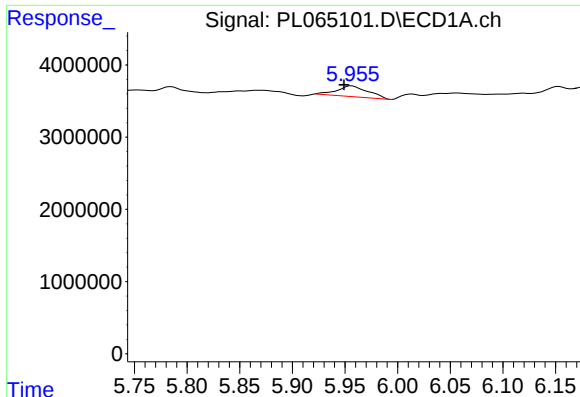

#14 Endrin


R.T.: 5.956 min
Delta R.T.: 0.007 min
Response: 3100004
Conc: 0.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

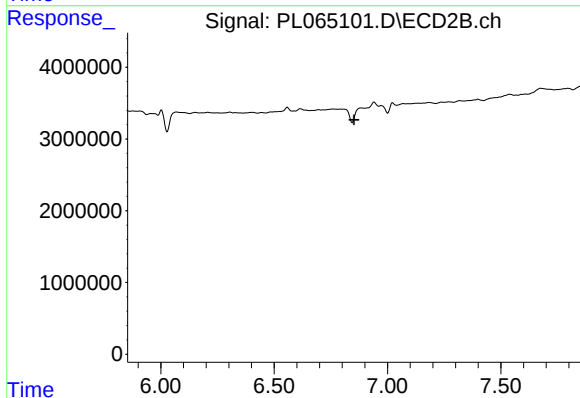


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

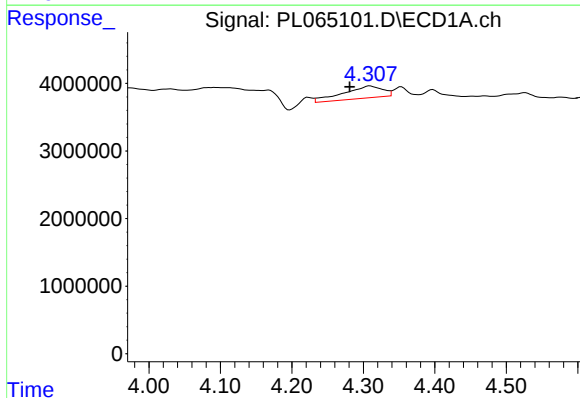


#23 Chlordane-1

R.T.: 4.309 min
Delta R.T.: 0.028 min
Response: 6814742
Conc: 53.47 ng/ml

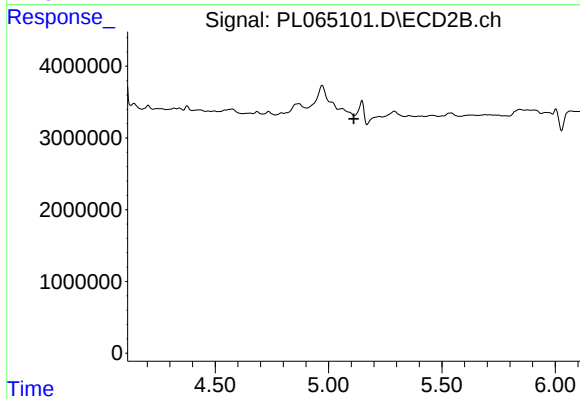

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

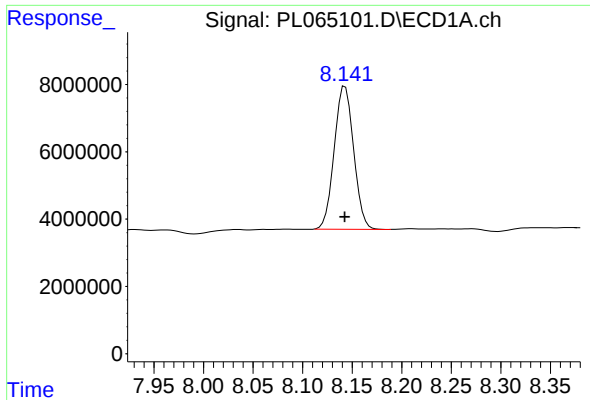

#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 57827464
Conc: 20.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

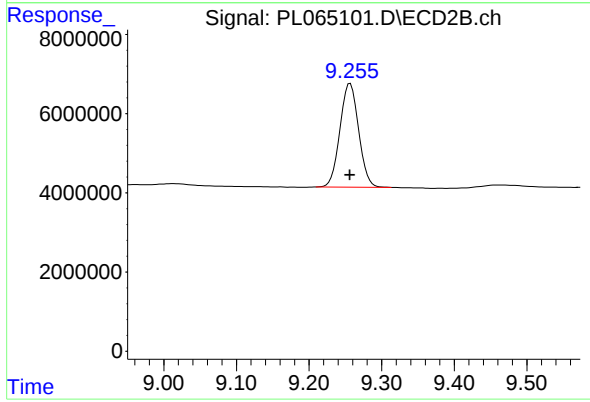

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: 0.000 min
Response: 46818200
Conc: 21.31 ng/ml