

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030621\  
 Data File : PL065107.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 05 Mar 2021 16:16  
 Operator : AR\AJ  
 Sample : M1565-06  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 05 22:14:12 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL030521.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Mar 05 02:26:14 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|---------|
| -----                       |                 |        |       |          |          |        |         |
| System Monitoring Compounds |                 |        |       |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.422  | 4.098 | 33890863 | 26746083 | 11.526 | 10.771  |
| 28)                         | SA Decachlor... | 8.143  | 9.257 | 30016524 | 23232073 | 10.816 | 10.577  |
| Target Compounds            |                 |        |       |          |          |        |         |
| 10)                         | B gamma-Chl...  | 5.344  | 0.000 | 8475179  | 0        | 2.164  | N.D. #  |
| 11)                         | B alpha-Chl...  | 5.400  | 0.000 | 24483735 | 0        | 6.389  | N.D. #  |
| 12)                         | B 4,4'-DDE      | 5.566  | 6.473 | 28818560 | 5004067  | 8.018  | 2.002 # |
| 17)                         | MA 4,4'-DDT     | 6.314  | 0.000 | 5429007  | 0        | 1.947  | N.D. #  |
| 18)                         | B Endrin al...  | 6.404  | 0.000 | 1465199  | 0        | 0.572  | N.D. #  |
| 23)                         | Chlordane-1     | 4.306f | 0.000 | 7592470  | 0        | 59.568 | N.D. #  |
| 25)                         | Chlordane-3     | 5.344  | 0.000 | 8475179  | 0        | 21.245 | N.D. #  |
| 26)                         | Chlordane-4     | 5.400  | 0.000 | 24483735 | 0        | 72.985 | N.D. #  |
| -----                       |                 |        |       |          |          |        |         |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030621\  
Data File : PL065107.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 05 Mar 2021 16:16  
Operator : AR\AJ  
Sample : M1565-06  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampled :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 05 22:14:12 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL030521.M  
Quant Title : GC Extractables  
QLast Update : Fri Mar 05 02:26:14 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

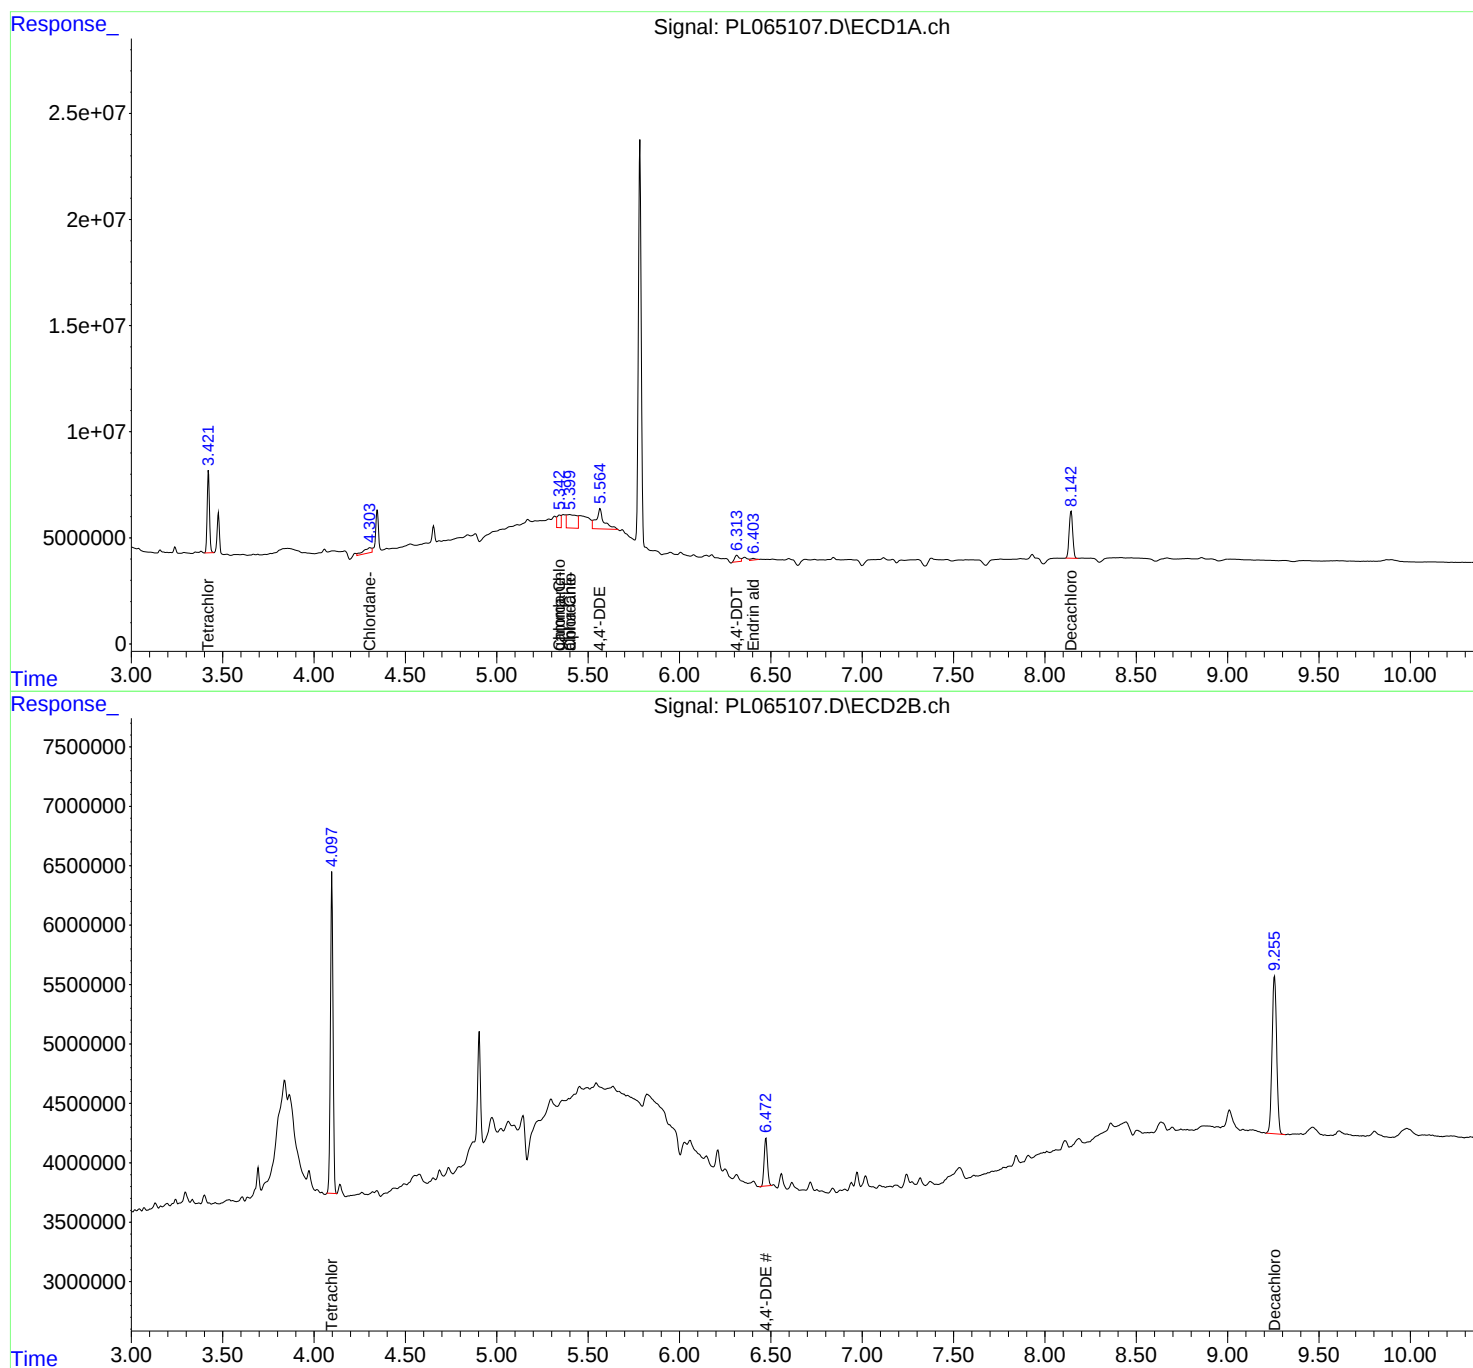


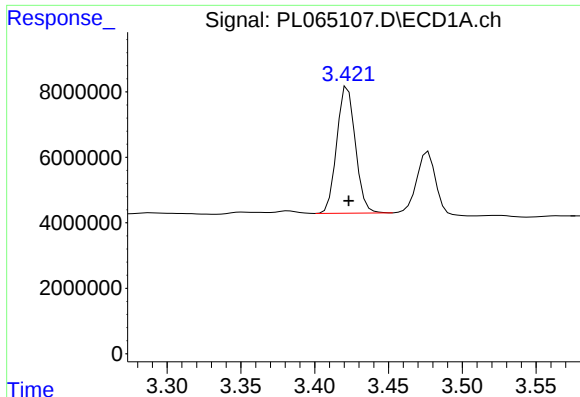

#1 Tetrachloro-m-xylene


R.T.: 3.422 min  
Delta R.T.: 0.000 min  
Response: 33890863  
Conc: 11.53 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

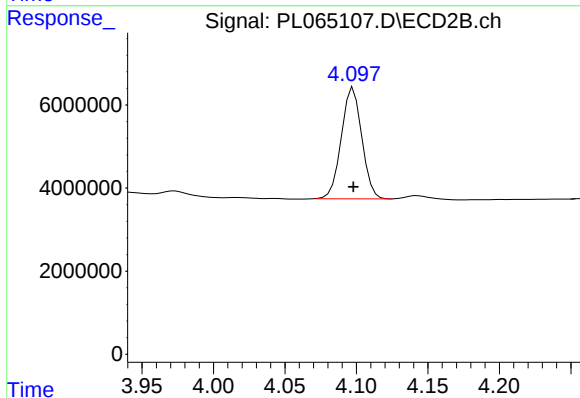


#1 Tetrachloro-m-xylene

R.T.: 4.098 min  
Delta R.T.: 0.000 min  
Response: 26746083  
Conc: 10.77 ng/ml

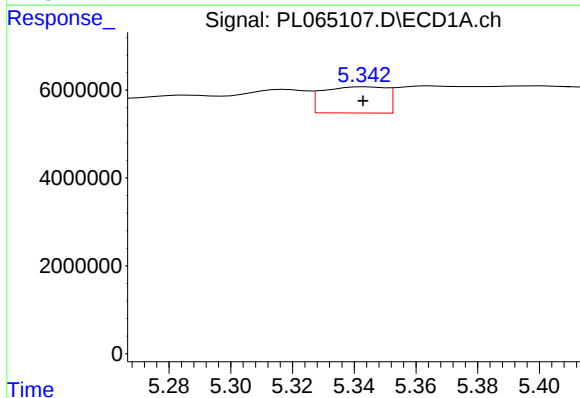


#10 gamma-Chlordane

R.T.: 5.344 min  
Delta R.T.: 0.000 min  
Response: 8475179  
Conc: 2.16 ng/ml

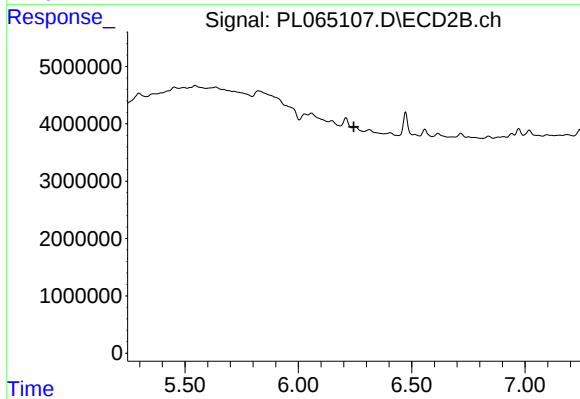

#10 gamma-Chlordane


R.T.: 0.000 min  
Exp R.T.: 6.245 min  
Response: 0  
Conc: N.D.

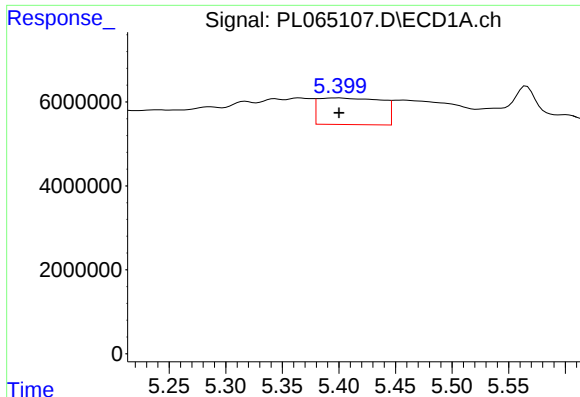

#11 alpha-Chlordane


R.T.: 5.400 min  
Delta R.T.: 0.000 min  
Response: 24483735  
Conc: 6.39 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

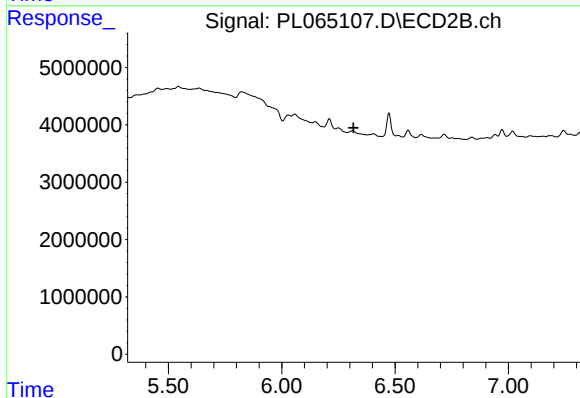


#11 alpha-Chlordane

R.T.: 0.000 min  
Exp R.T. : 6.317 min  
Response: 0  
Conc: N.D.

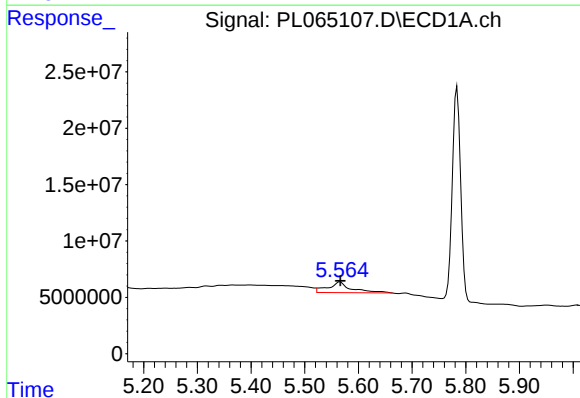


#12 4,4'-DDE

R.T.: 5.566 min  
Delta R.T.: 0.000 min  
Response: 28818560  
Conc: 8.02 ng/ml

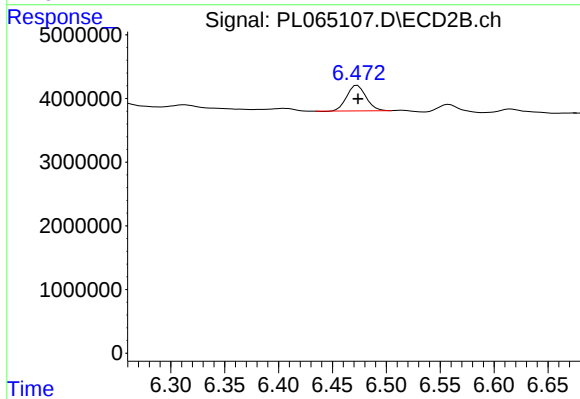

#12 4,4'-DDE


R.T.: 6.473 min  
Delta R.T.: 0.000 min  
Response: 5004067  
Conc: 2.00 ng/ml

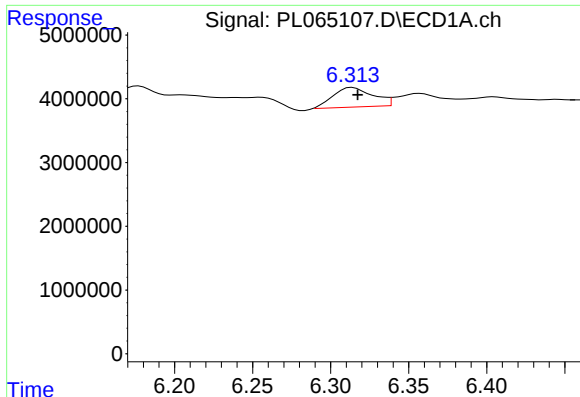

#17 4,4'-DDT


R.T.: 6.314 min  
Delta R.T.: -0.003 min  
Response: 5429007  
Conc: 1.95 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

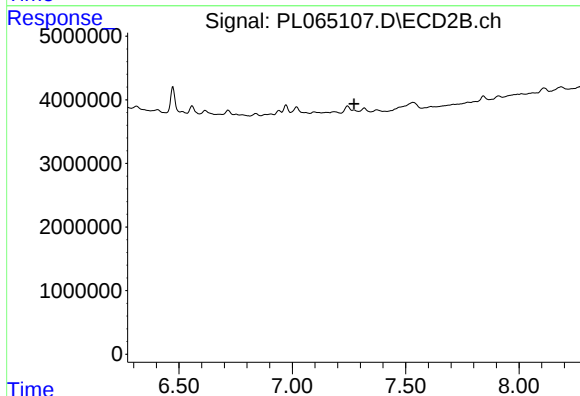


#17 4,4'-DDT

R.T.: 0.000 min  
Exp R.T. : 7.273 min  
Response: 0  
Conc: N.D.

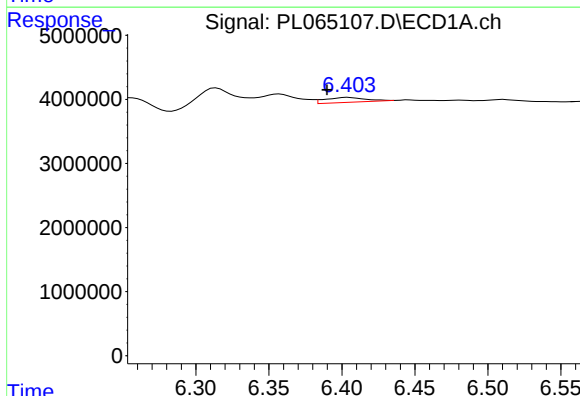


#18 Endrin aldehyde

R.T.: 6.404 min  
Delta R.T.: 0.014 min  
Response: 1465199  
Conc: 0.57 ng/ml

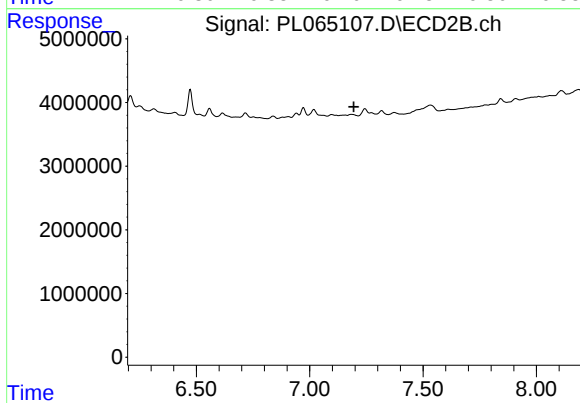

#18 Endrin aldehyde


R.T.: 0.000 min  
Exp R.T. : 7.194 min  
Response: 0  
Conc: N.D.

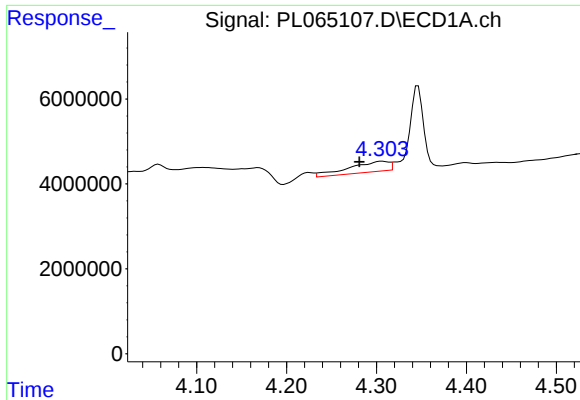

#23 Chlordane-1


R.T.: 4.306 min  
Delta R.T.: 0.025 min  
Response: 7592470  
Conc: 59.57 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

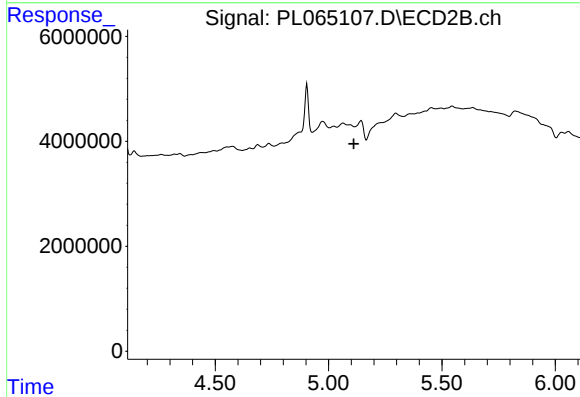


#23 Chlordane-1

R.T.: 0.000 min  
Exp R.T. : 5.112 min  
Response: 0  
Conc: N.D.

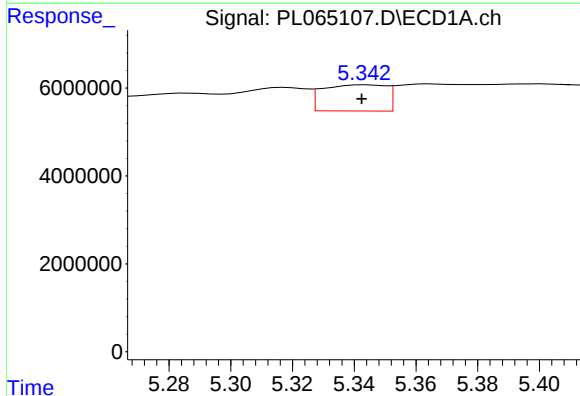


#25 Chlordane-3

R.T.: 5.344 min  
Delta R.T.: 0.001 min  
Response: 8475179  
Conc: 21.24 ng/ml

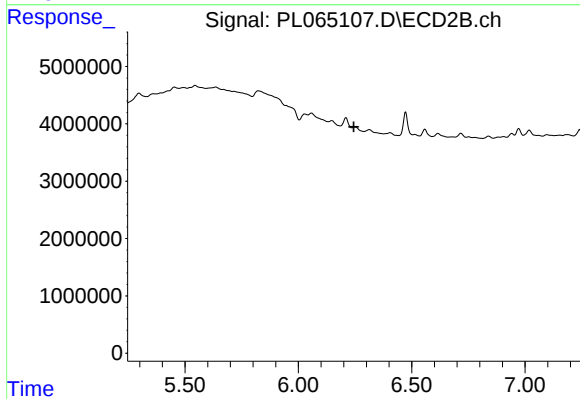

#25 Chlordane-3


R.T.: 0.000 min  
Exp R.T. : 6.244 min  
Response: 0  
Conc: N.D.

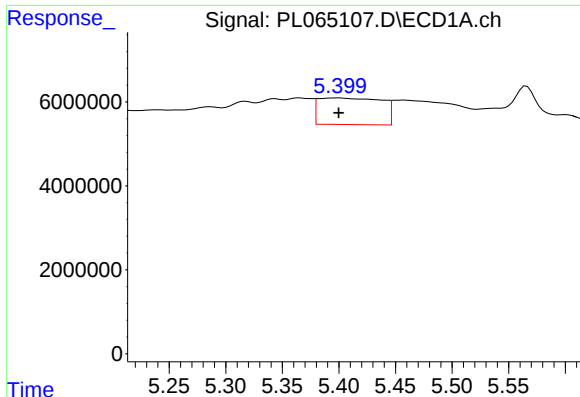

#26 Chlordane-4


R.T.: 5.400 min  
Delta R.T.: 0.000 min  
Response: 24483735  
Conc: 72.98 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

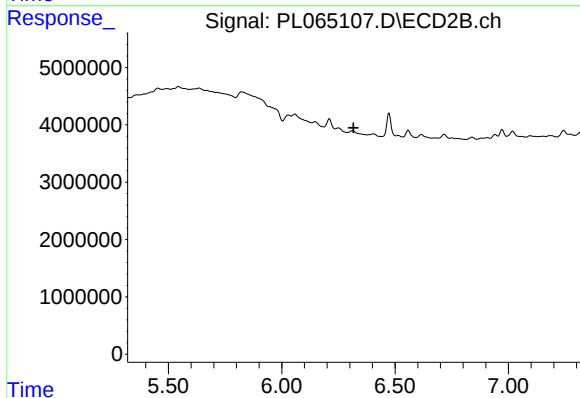


#26 Chlordane-4

R.T.: 0.000 min  
Exp R.T. : 6.317 min  
Response: 0  
Conc: N.D.

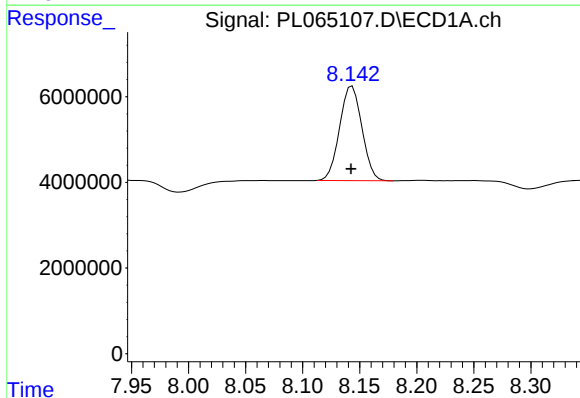

#28 Decachlorobiphenyl

R.T.: 8.143 min  
Delta R.T.: 0.001 min  
Response: 30016524  
Conc: 10.82 ng/ml

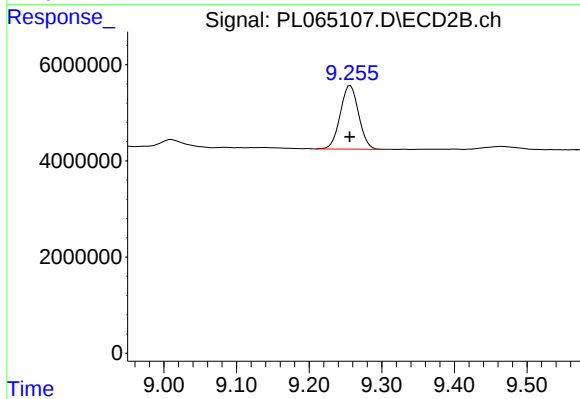

#28 Decachlorobiphenyl

R.T.: 9.257 min  
Delta R.T.: 0.000 min  
Response: 23232073  
Conc: 10.58 ng/ml