

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 17:57
 Operator : AR\AJ
 Sample : M1568-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:16:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	61018488	49591795	20.752	19.971
28)	SA Decachlor...	8.142	9.258	50962052	43350005	18.364	19.736
Target Compounds							
4)	MA Heptachlor	4.418	0.000	1763800	0	0.401	N.D. #
6)	B beta-BHC	4.393	4.974	4592160	4048528	2.459	2.648
7)	B delta-BHC	0.000	5.194	0	3668259	N.D.	1.211 #
12)	B 4,4'-DDE	5.588f	0.000	2149725	0	0.598	N.D. #
16)	A 4,4'-DDD	6.098f	0.000	414691	0	0.139	N.D. #
23)	Chlordane-1	4.310f	0.000	5713749	0	44.828	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 17:57
Operator : AR\AJ
Sample : M1568-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:16:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

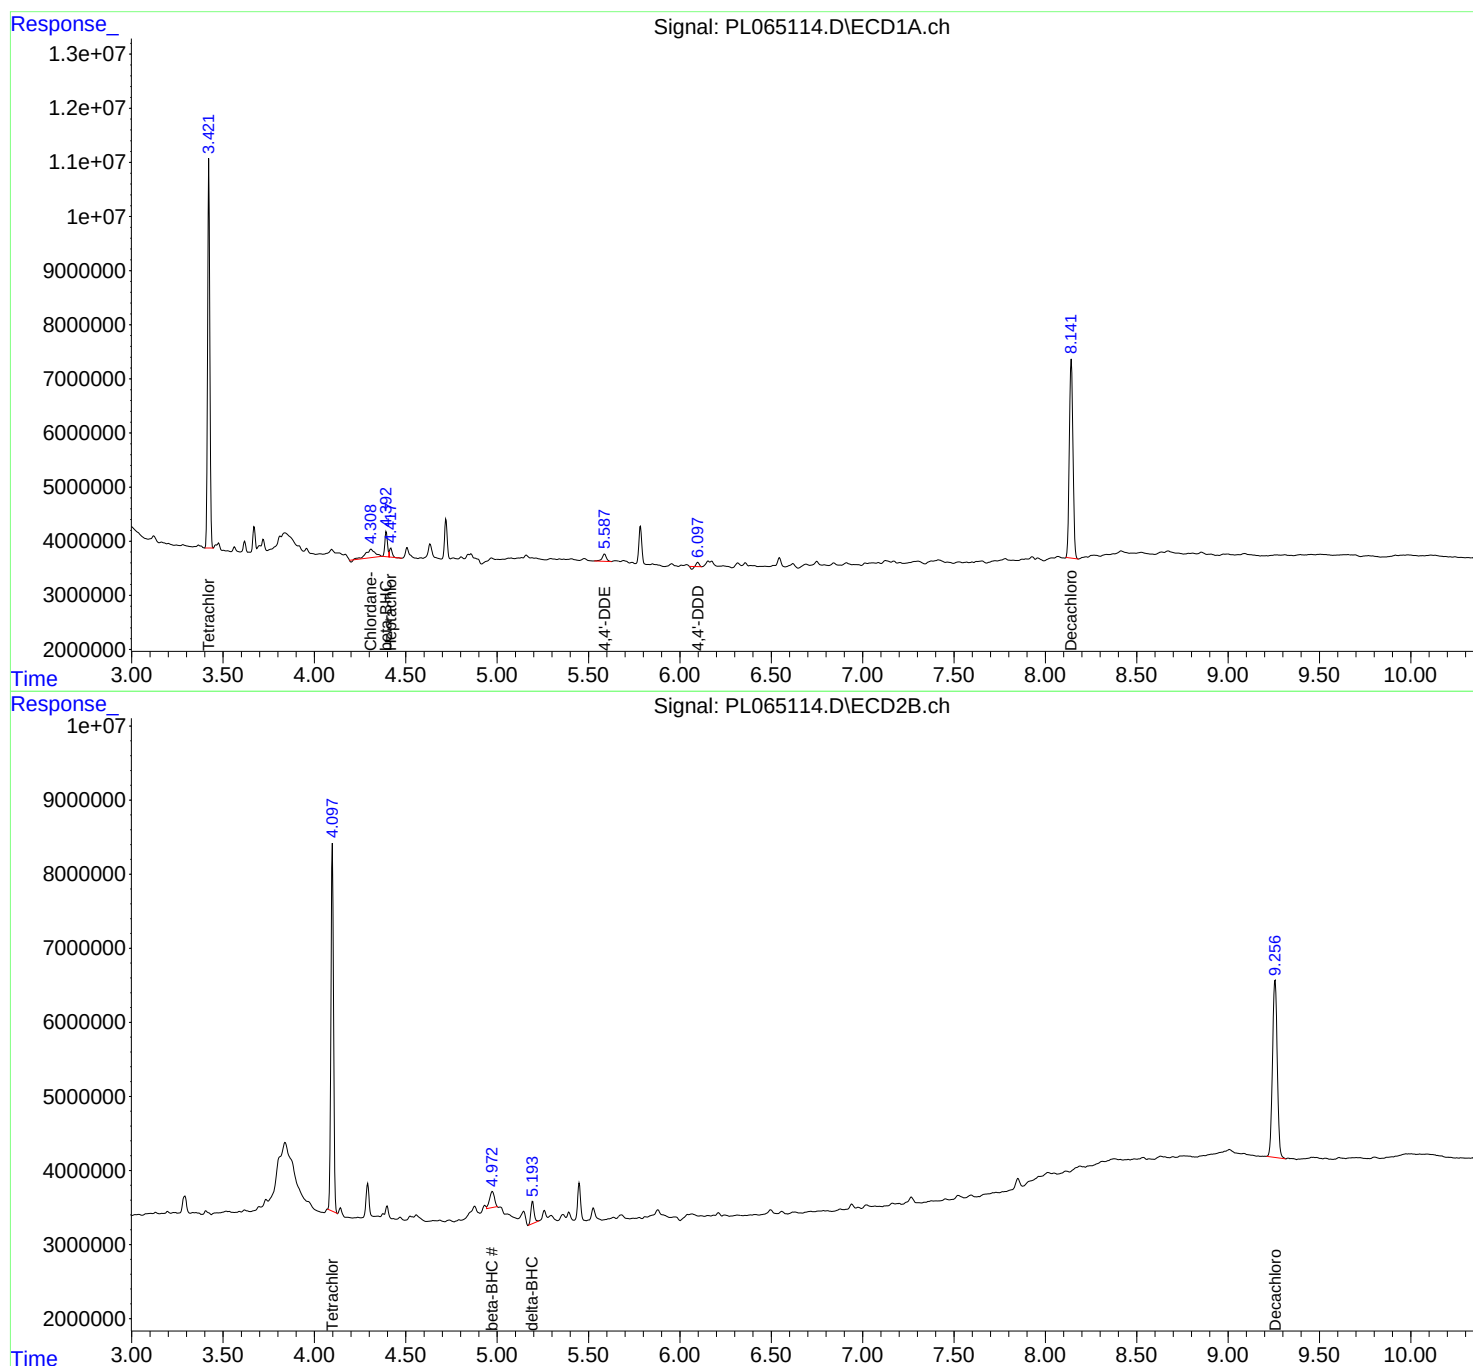


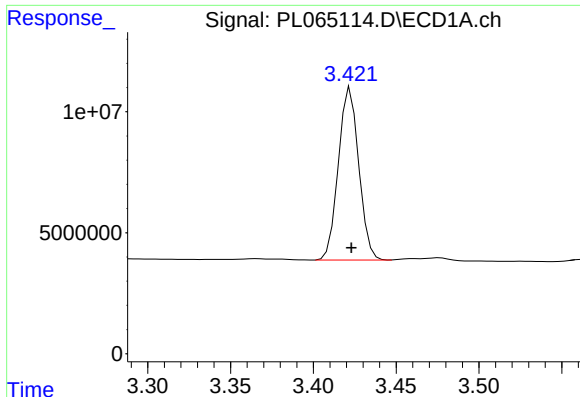

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.000 min
Response: 61018488
Conc: 20.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

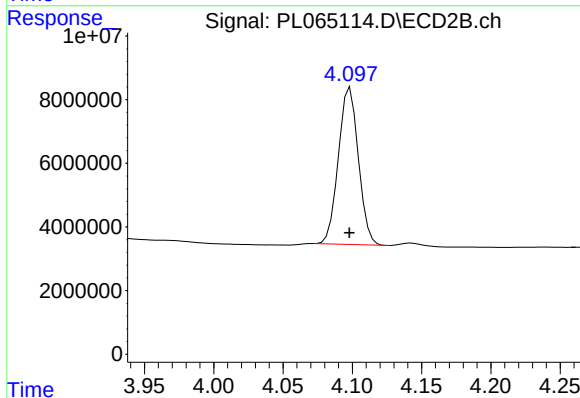


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 49591795
Conc: 19.97 ng/ml

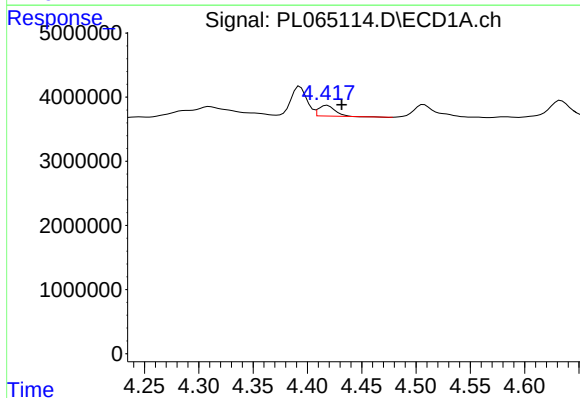


#4 Heptachlor

R.T.: 4.418 min
Delta R.T.: -0.013 min
Response: 1763800
Conc: 0.40 ng/ml

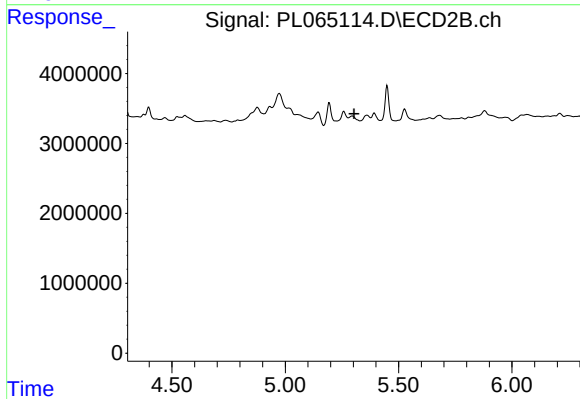

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.304 min
Response: 0
Conc: N.D.

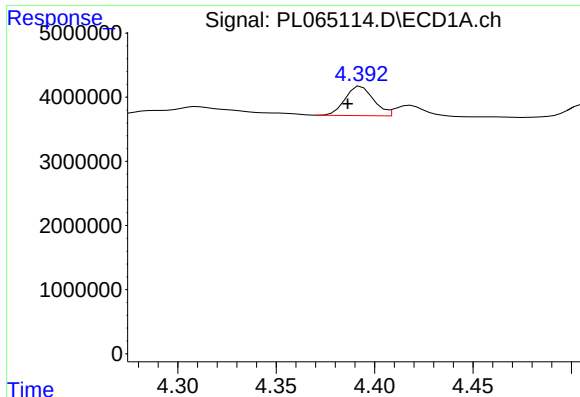

#6 beta-BHC


R.T.: 4.393 min
Delta R.T.: 0.007 min
Response: 4592160
Conc: 2.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

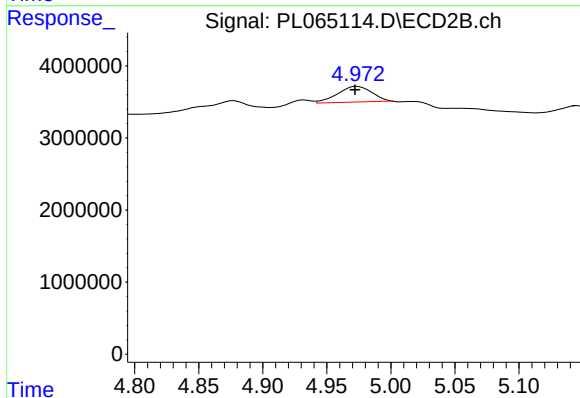


#6 beta-BHC

R.T.: 4.974 min
Delta R.T.: 0.002 min
Response: 4048528
Conc: 2.65 ng/ml

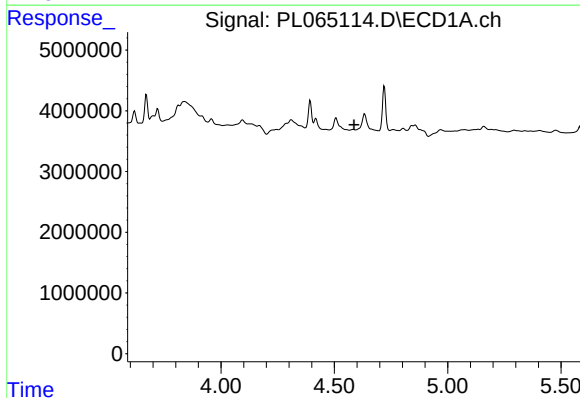


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.587 min
Response: 0
Conc: N.D.

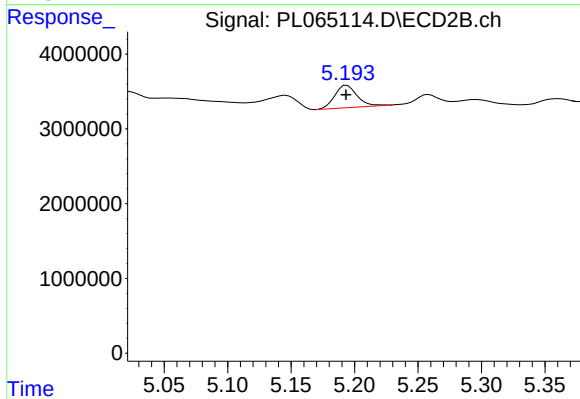

#7 delta-BHC


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 3668259
Conc: 1.21 ng/ml

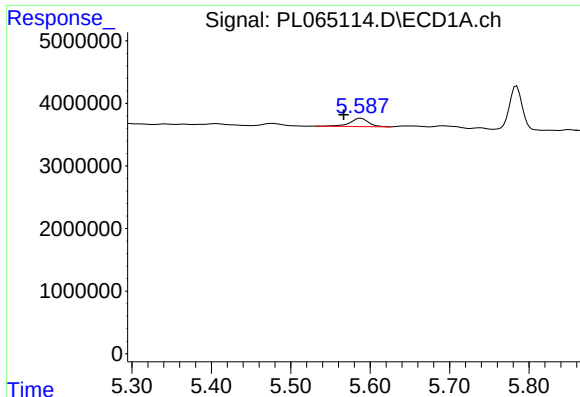

#12 4,4'-DDE


R.T.: 5.588 min
Delta R.T.: 0.022 min
Response: 2149725
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

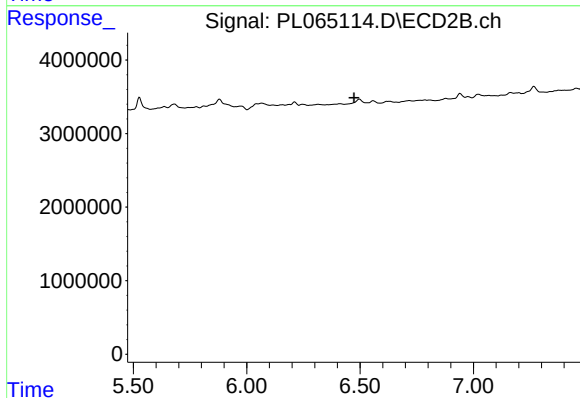


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

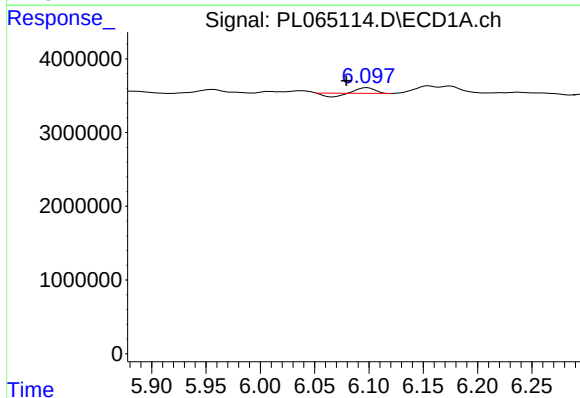


#16 4,4'-DDD

R.T.: 6.098 min
Delta R.T.: 0.019 min
Response: 414691
Conc: 0.14 ng/ml

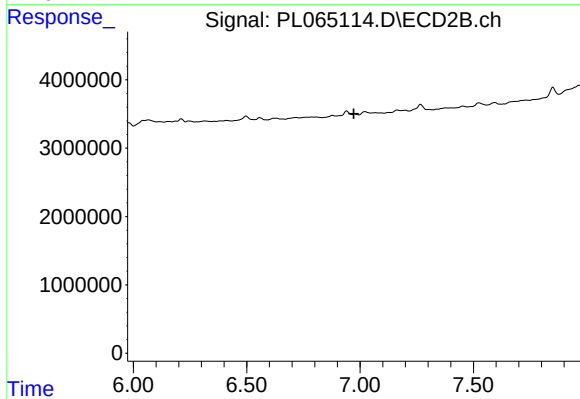

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.973 min
Response: 0
Conc: N.D.

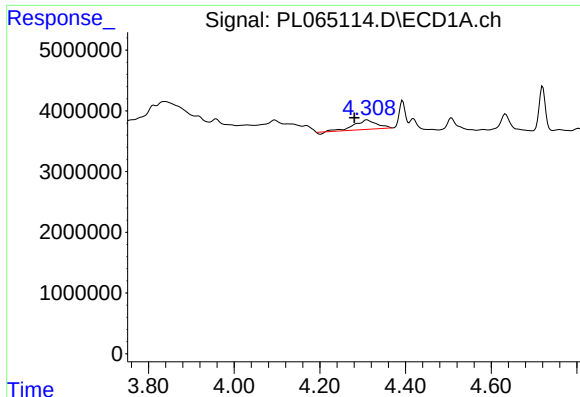

#23 Chlordane-1


R.T.: 4.310 min
Delta R.T.: 0.029 min
Response: 5713749
Conc: 44.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

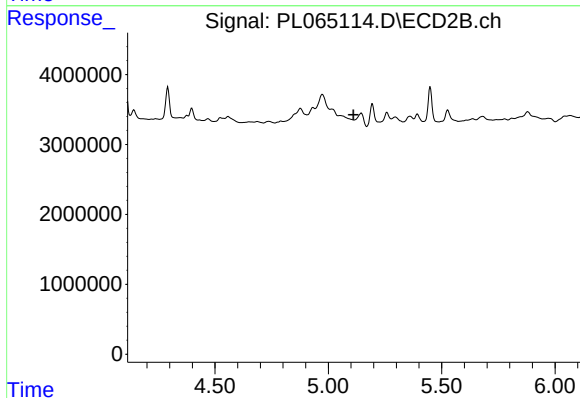


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

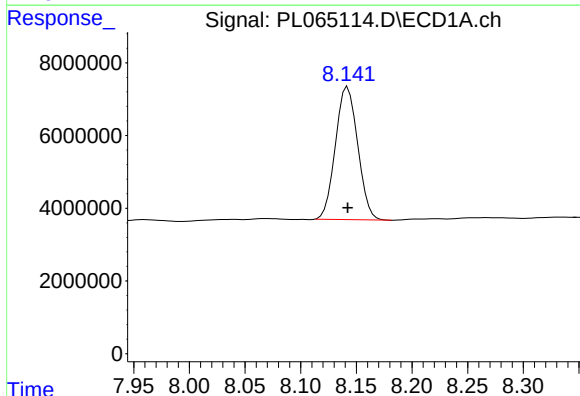

#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 50962052
Conc: 18.36 ng/ml

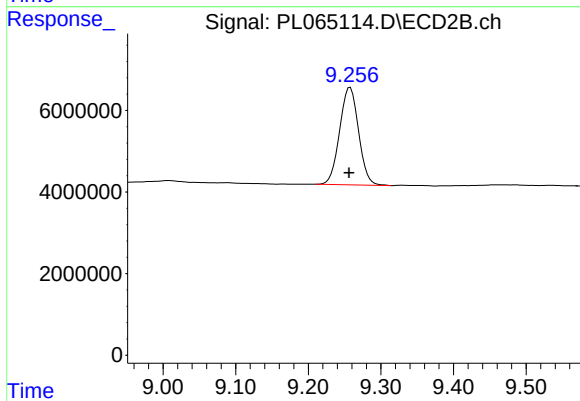

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: 0.002 min
Response: 43350005
Conc: 19.74 ng/ml