

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 18:11
 Operator : AR\AJ
 Sample : M1568-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:16:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	66474402	53796943	22.607	21.664
28)	SA Decachlor...	8.143	9.256	54623265	45106141	19.683	20.535
Target Compounds							
6)	B beta-BHC	4.393	4.974	5735133	3631550	3.071	2.375
7)	B delta-BHC	4.606f	5.194	-139269	5672287	N.D.	1.873
9)	A Endosulfan I	5.475f	0.000	3564712	0	0.997	N.D. #
12)	B 4,4'-DDE	5.588f	0.000	3972057	0	1.105	N.D. #
14)	MA Endrin	5.955	0.000	1238568	0	0.361	N.D. #
16)	A 4,4'-DDD	6.098f	0.000	72429	0	0.024	N.D. #
17)	MA 4,4'-DDT	6.317	0.000	2504881	0	0.898	N.D. #
23)	Chlordane-1	4.290	0.000	3416046	0	26.801	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 18:11
Operator : AR\AJ
Sample : M1568-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:16:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

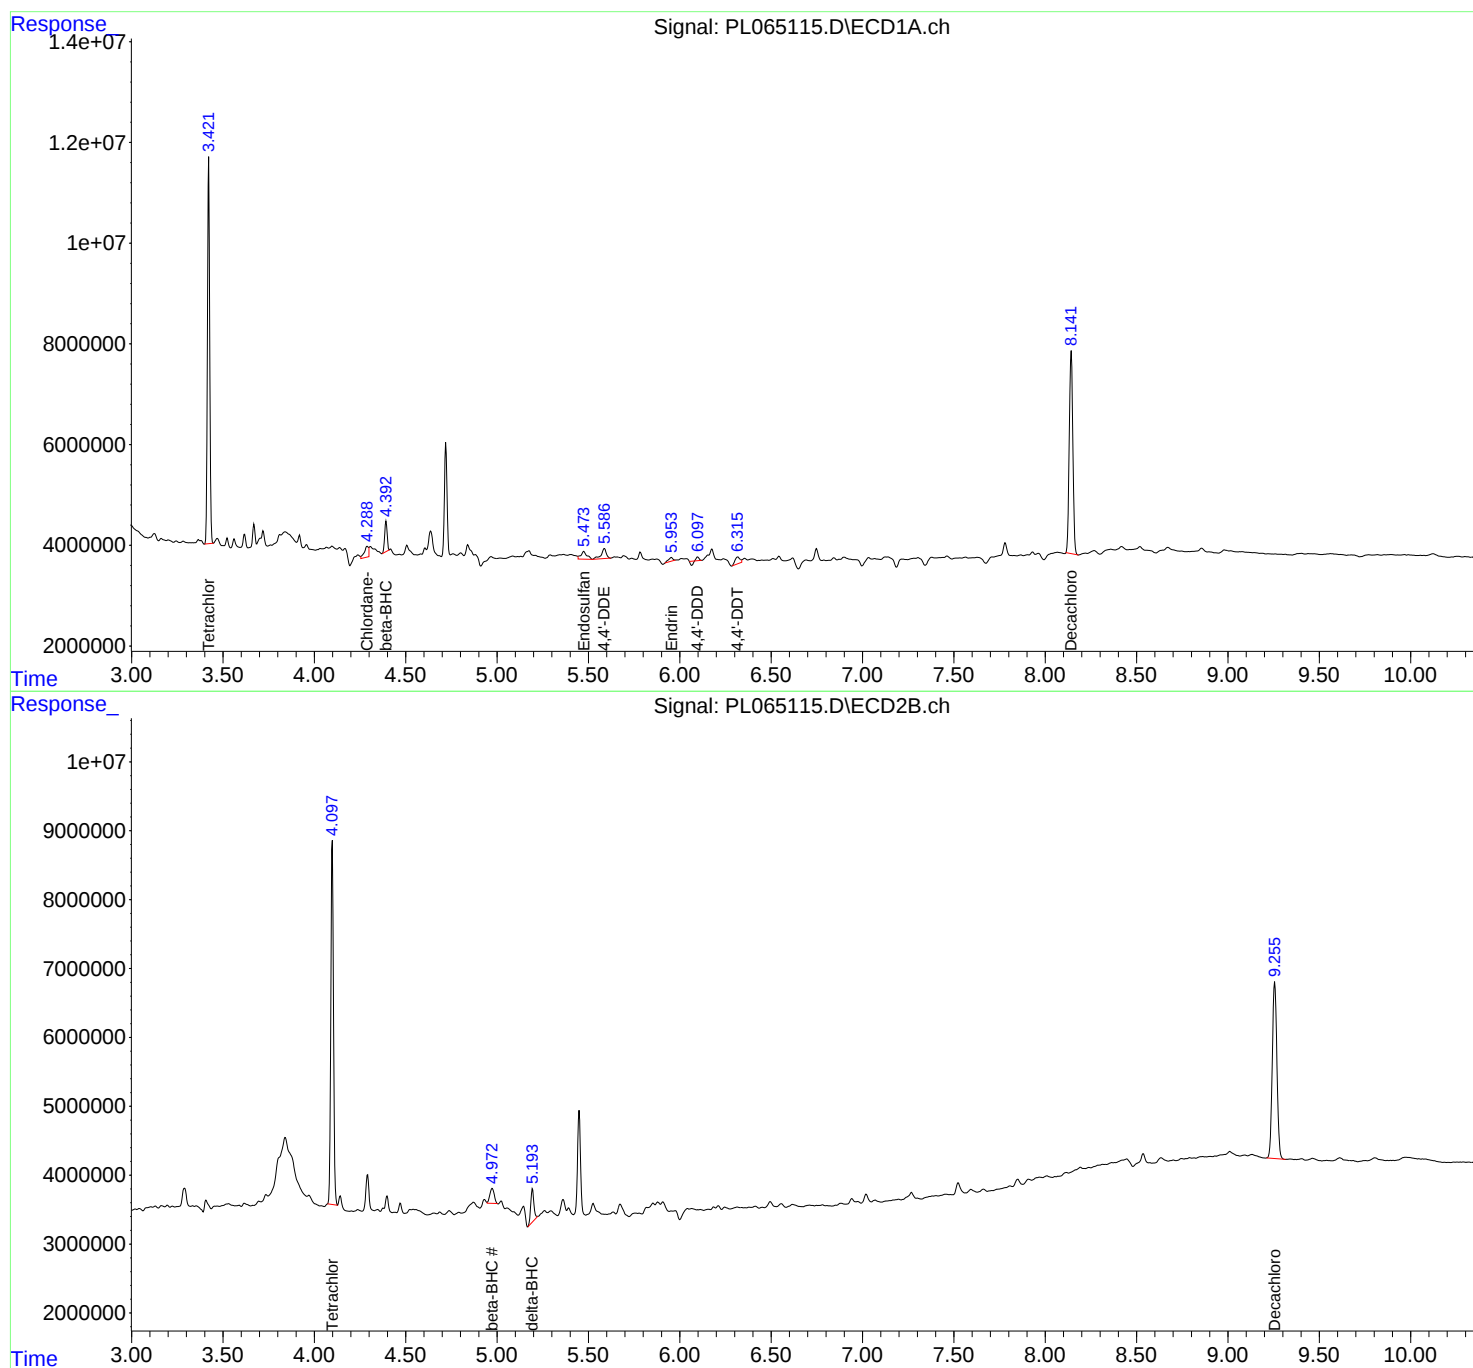


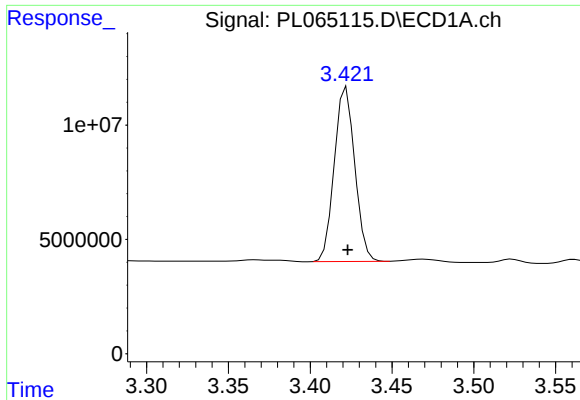

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 66474402
Conc: 22.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

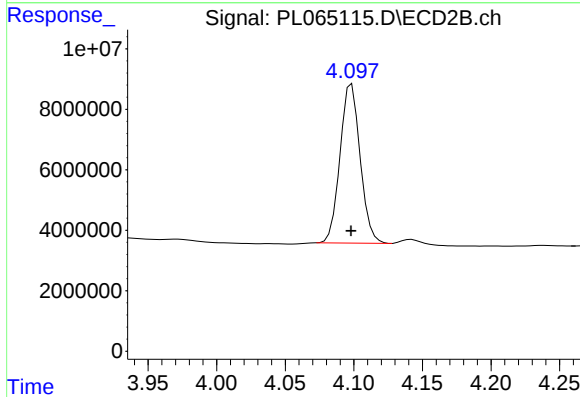


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 53796943
Conc: 21.66 ng/ml

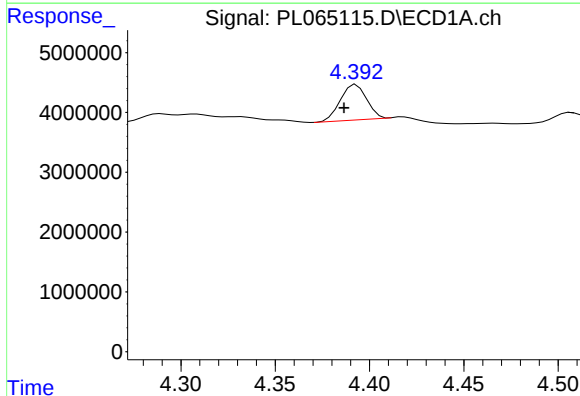


#6 beta-BHC

R.T.: 4.393 min
Delta R.T.: 0.007 min
Response: 5735133
Conc: 3.07 ng/ml

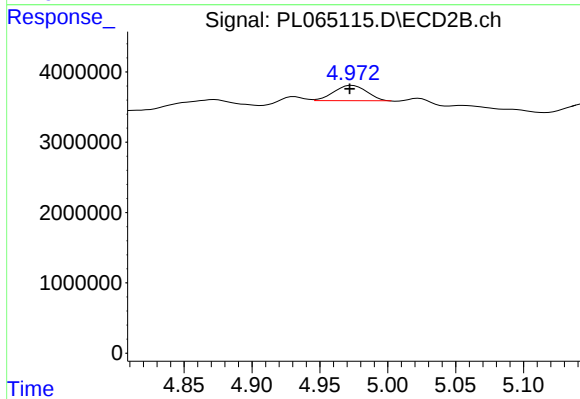

#6 beta-BHC


R.T.: 4.974 min
Delta R.T.: 0.002 min
Response: 3631550
Conc: 2.38 ng/ml

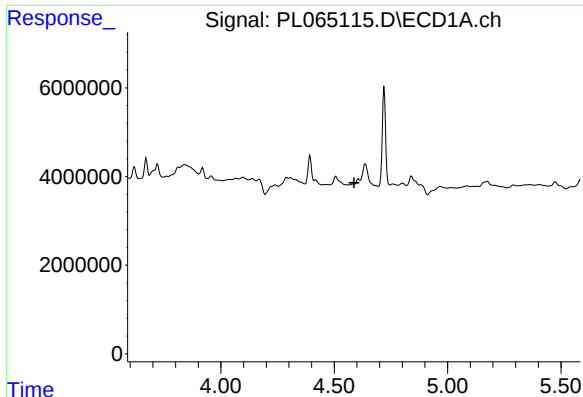

#7 delta-BHC


R.T.: 4.606 min
Delta R.T.: 0.019 min
Response: -139269
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

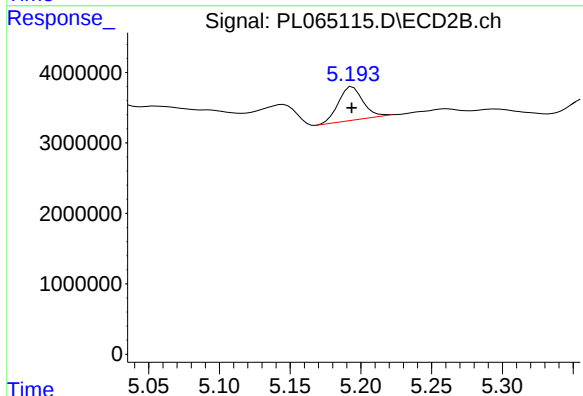


#7 delta-BHC

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 5672287
Conc: 1.87 ng/ml

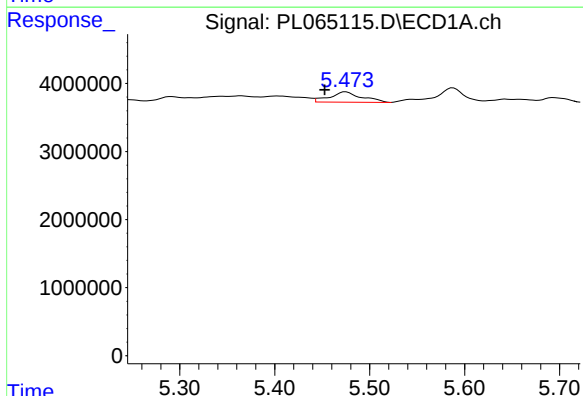


#9 Endosulfan I

R.T.: 5.475 min
Delta R.T.: 0.022 min
Response: 3564712
Conc: 1.00 ng/ml

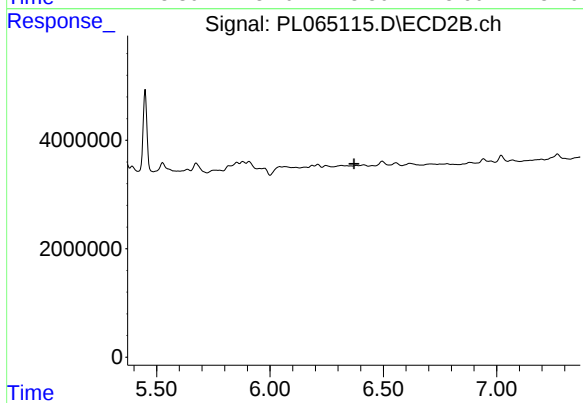

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

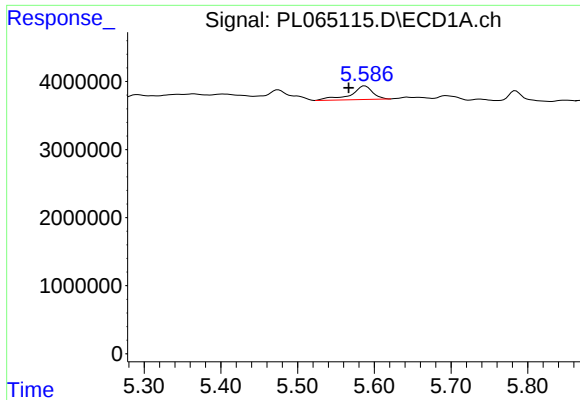

#12 4,4'-DDE


R.T.: 5.588 min
Delta R.T.: 0.021 min
Response: 3972057
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

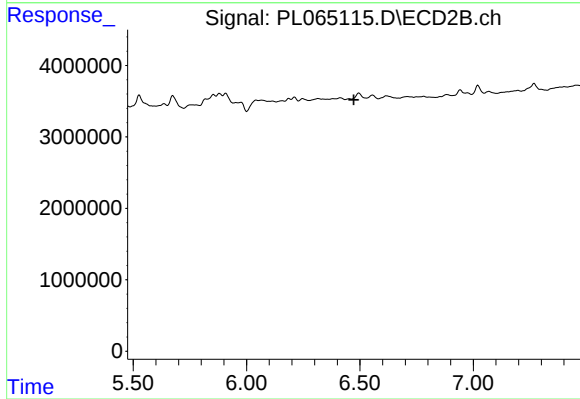


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

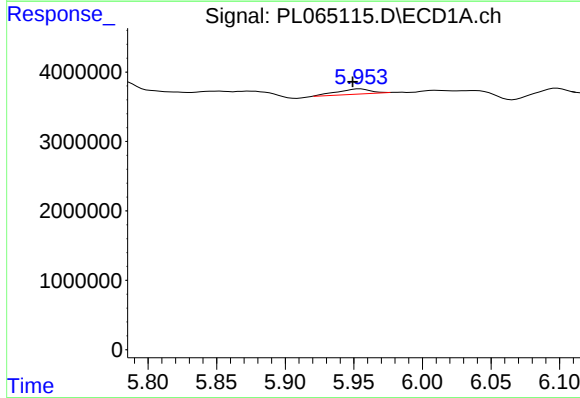


#14 Endrin

R.T.: 5.955 min
Delta R.T.: 0.006 min
Response: 1238568
Conc: 0.36 ng/ml

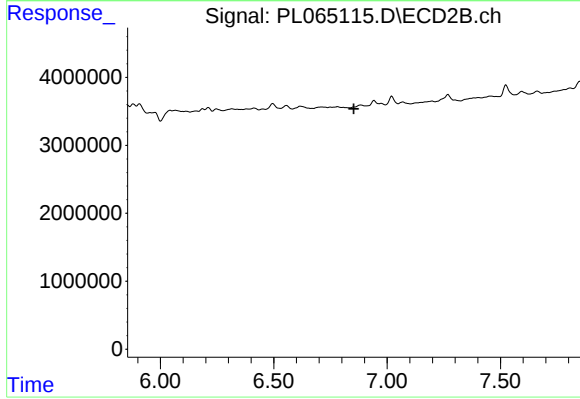

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

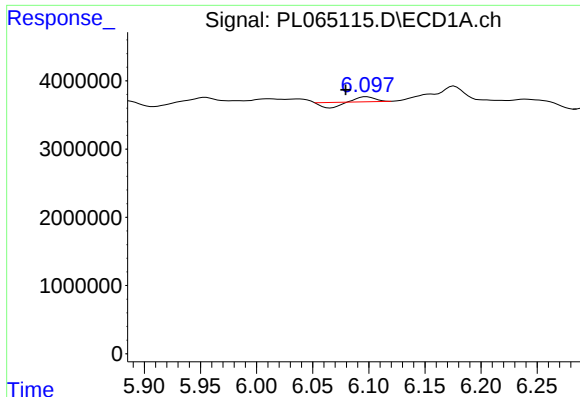

#16 4,4'-DDD


R.T.: 6.098 min
Delta R.T.: 0.019 min
Response: 72429
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

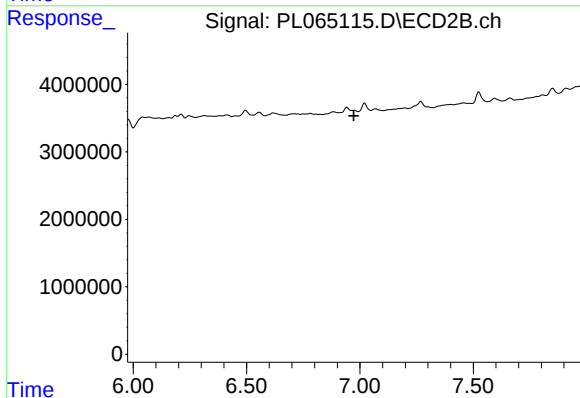


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.973 min
Response: 0
Conc: N.D.

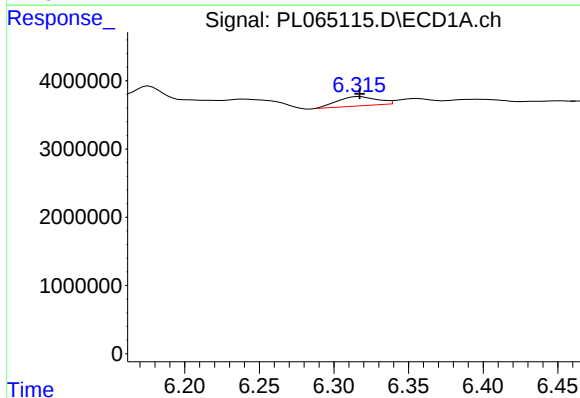


#17 4,4'-DDT

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 2504881
Conc: 0.90 ng/ml

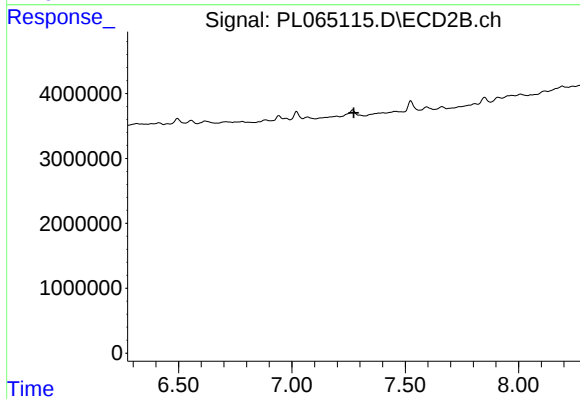

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

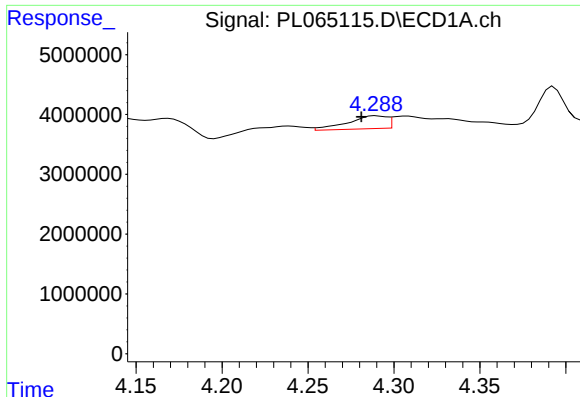

#23 Chlordane-1


R.T.: 4.290 min
Delta R.T.: 0.008 min
Response: 3416046
Conc: 26.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

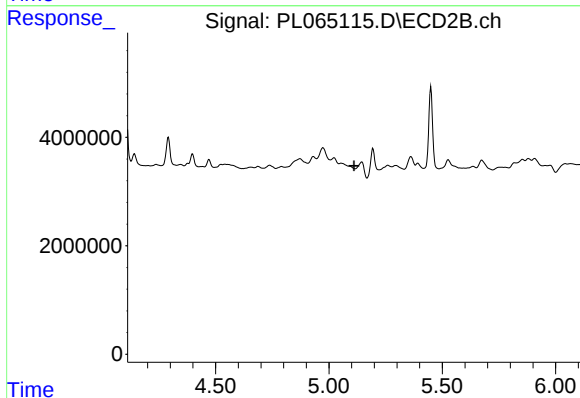


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

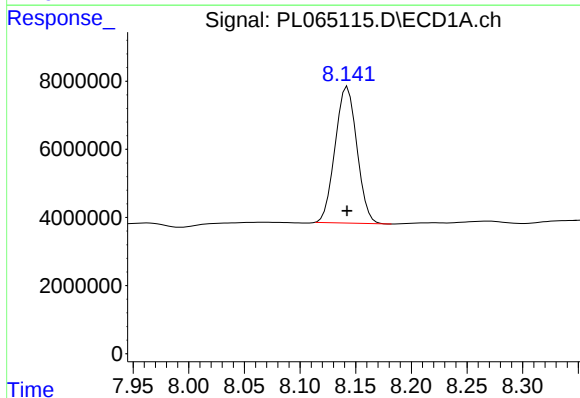

#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 54623265
Conc: 19.68 ng/ml

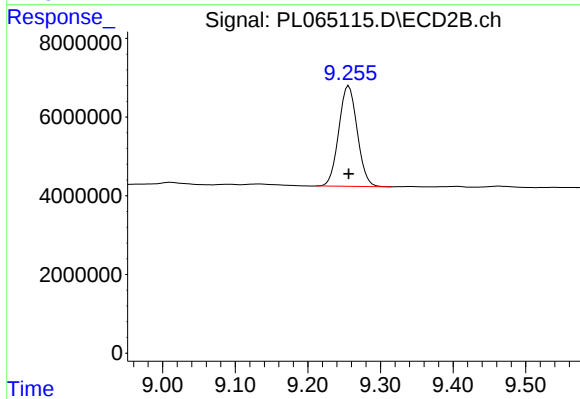

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: 0.000 min
Response: 45106141
Conc: 20.54 ng/ml