

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 18:25
 Operator : AR\AJ
 Sample : M1568-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:16:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	62498761	50940174	21.255	20.514
28)	SA Decachlor...	8.142	9.258	52640770	43082479	18.969	19.614
Target Compounds							
6)	B beta-BHC	4.393	4.974	5903669	3750781	3.161	2.453
7)	B delta-BHC	4.605f	5.194	632308	6721720	0.145	2.219 #
9)	A Endosulfan I	5.475f	0.000	2734902	0	0.765	N.D. #
12)	B 4,4'-DDE	5.588f	0.000	3583524	0	0.997	N.D. #
16)	A 4,4'-DDD	6.098f	0.000	509611	0	0.171	N.D. #
23)	Chlordane-1	4.288	0.000	3538699	0	27.763	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 18:25
Operator : AR\AJ
Sample : M1568-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:16:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

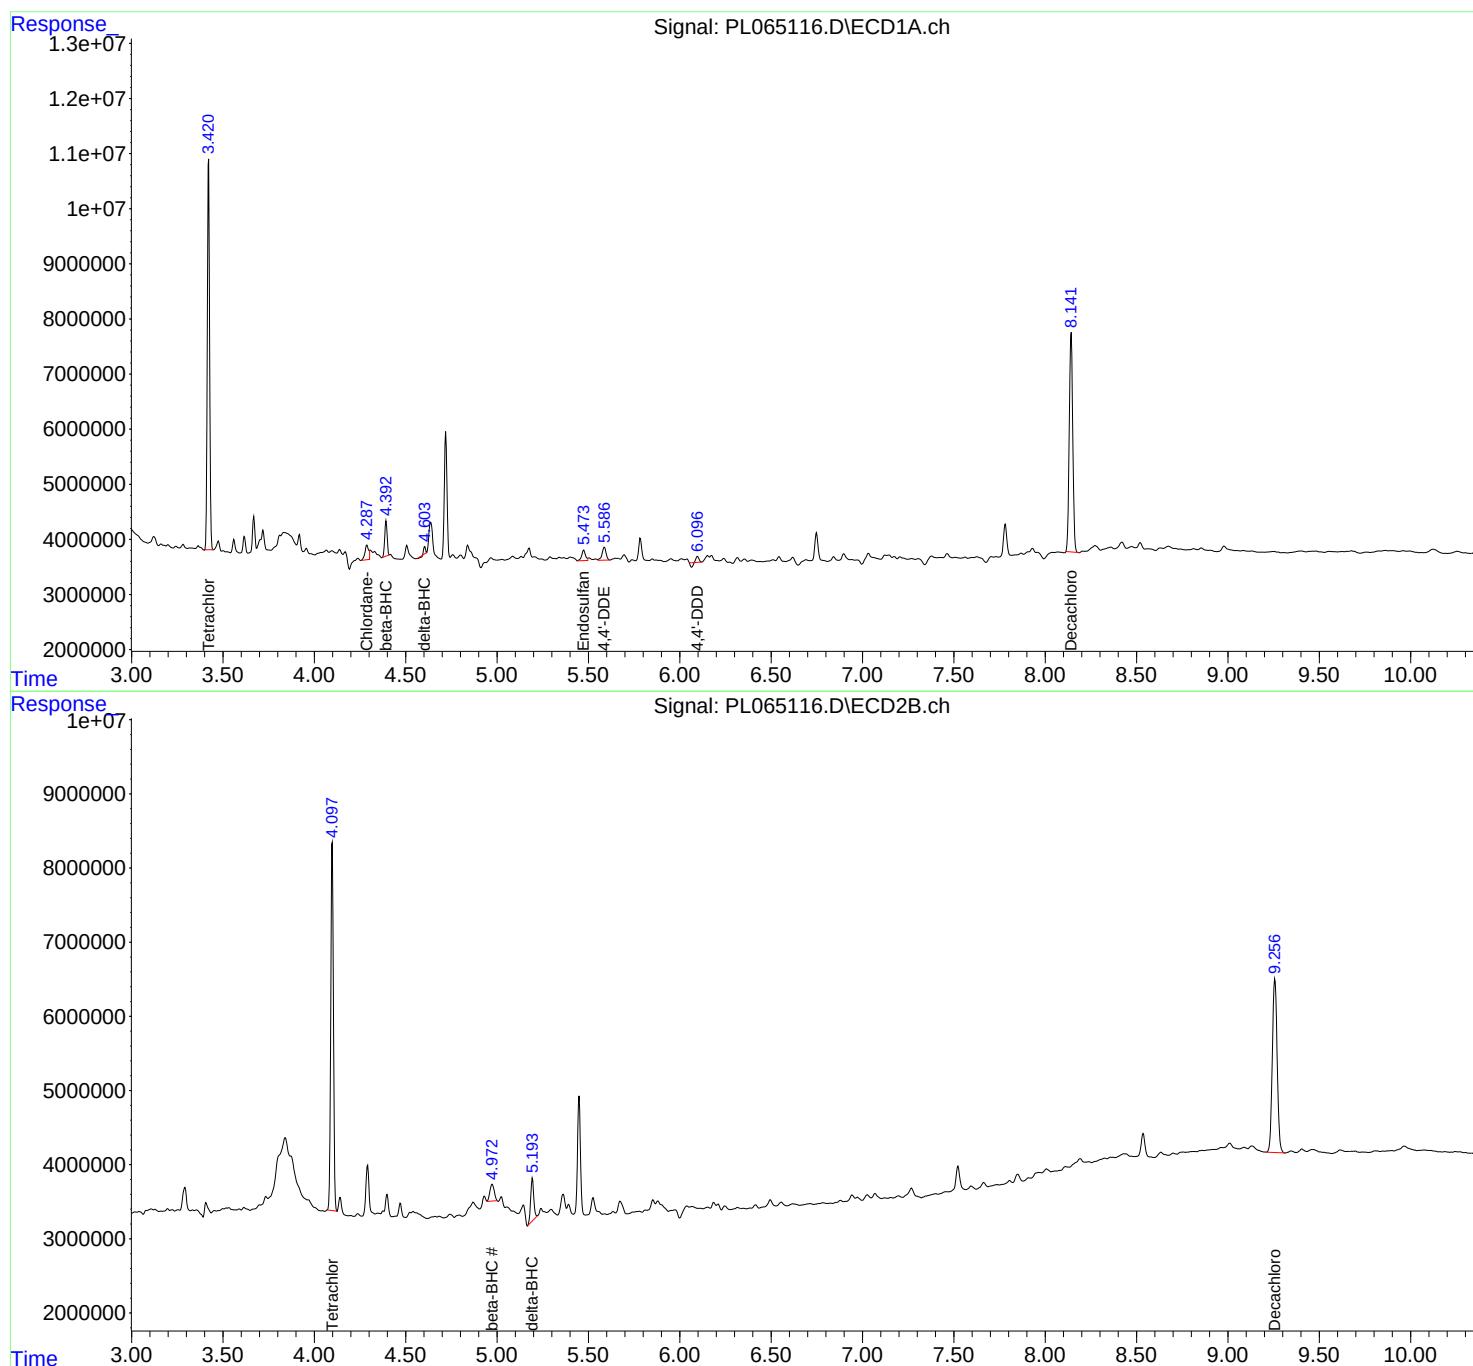


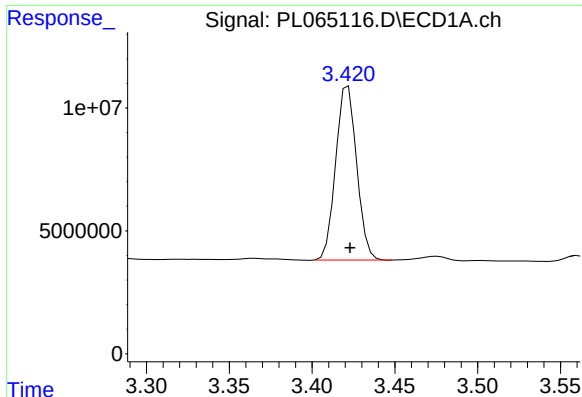

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 62498761
Conc: 21.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

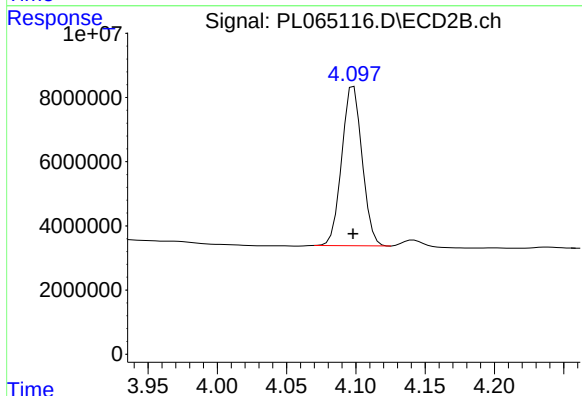


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 50940174
Conc: 20.51 ng/ml

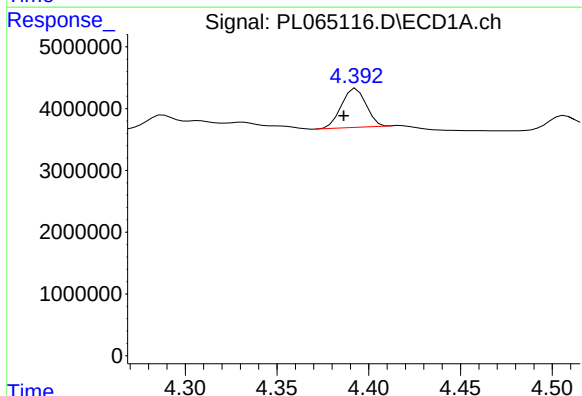


#6 beta-BHC

R.T.: 4.393 min
Delta R.T.: 0.007 min
Response: 5903669
Conc: 3.16 ng/ml

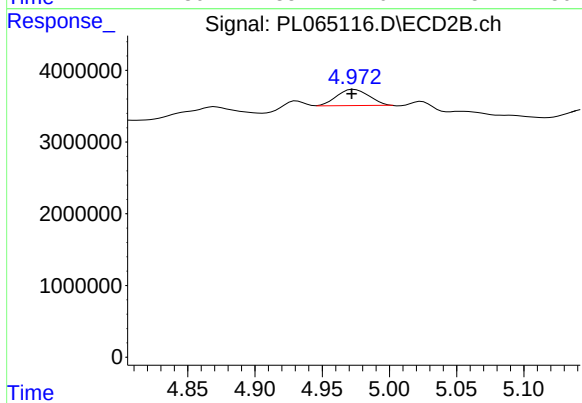

#6 beta-BHC


R.T.: 4.974 min
Delta R.T.: 0.002 min
Response: 3750781
Conc: 2.45 ng/ml

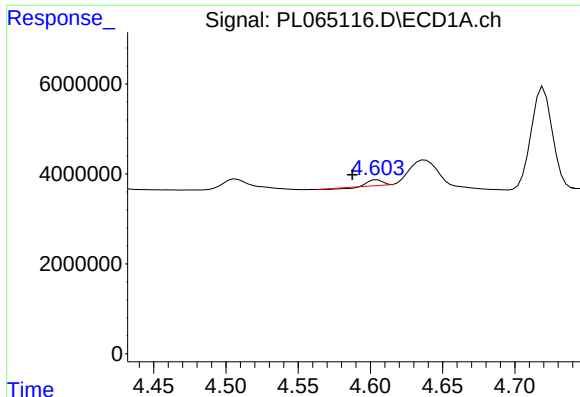

#7 delta-BHC


R.T.: 4.605 min
Delta R.T.: 0.017 min
Response: 632308
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

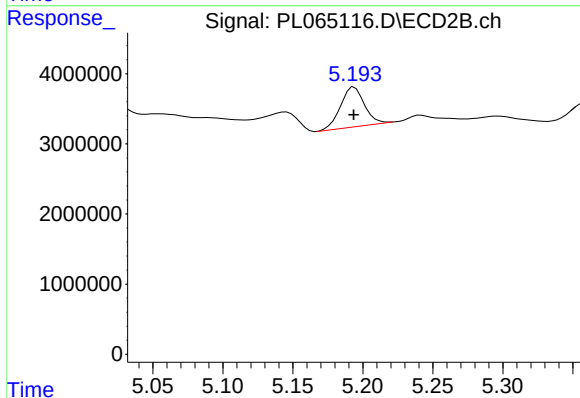


#7 delta-BHC

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 6721720
Conc: 2.22 ng/ml

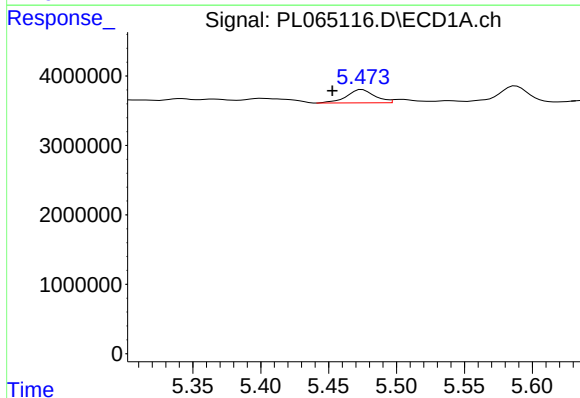


#9 Endosulfan I

R.T.: 5.475 min
Delta R.T.: 0.022 min
Response: 2734902
Conc: 0.76 ng/ml

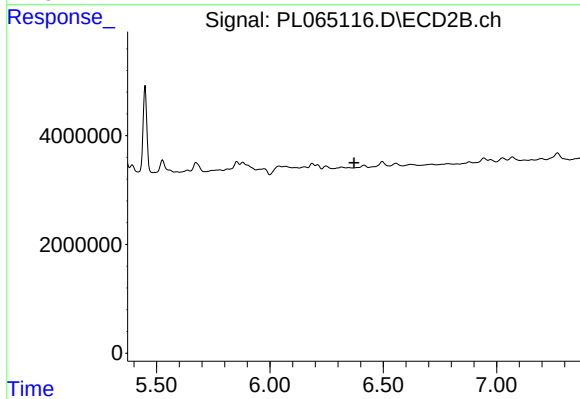

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.371 min
Response: 0
Conc: N.D.

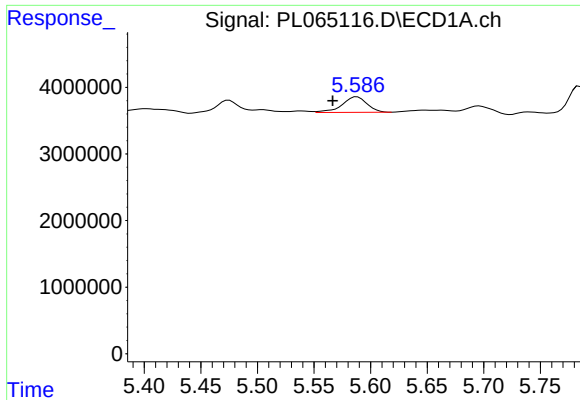

#12 4,4'-DDE


R.T.: 5.588 min
Delta R.T.: 0.021 min
Response: 3583524
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

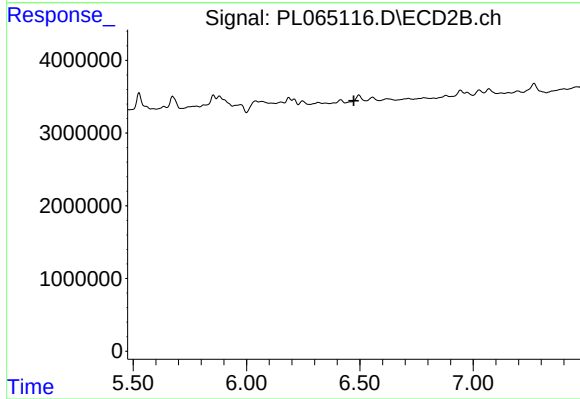


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

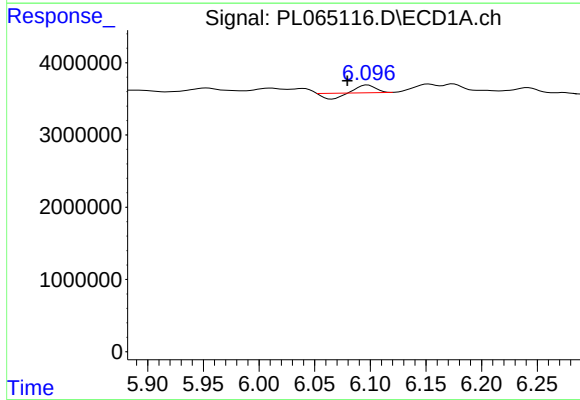


#16 4,4'-DDD

R.T.: 6.098 min
Delta R.T.: 0.018 min
Response: 509611
Conc: 0.17 ng/ml

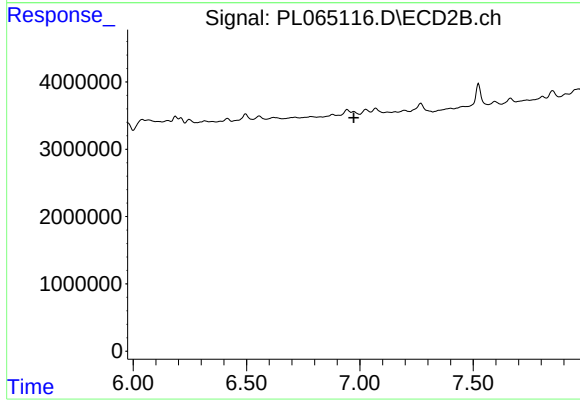

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.973 min
Response: 0
Conc: N.D.

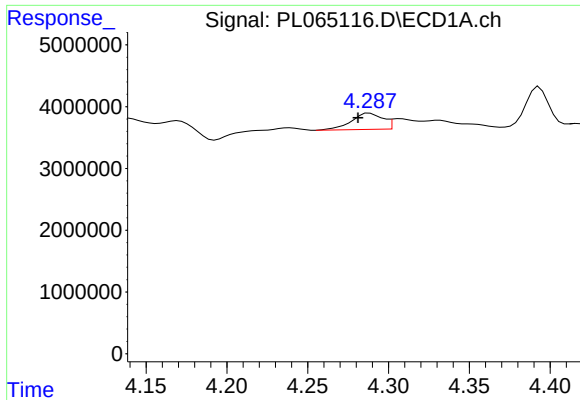

#23 Chlordane-1


R.T.: 4.288 min
Delta R.T.: 0.007 min
Response: 3538699
Conc: 27.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

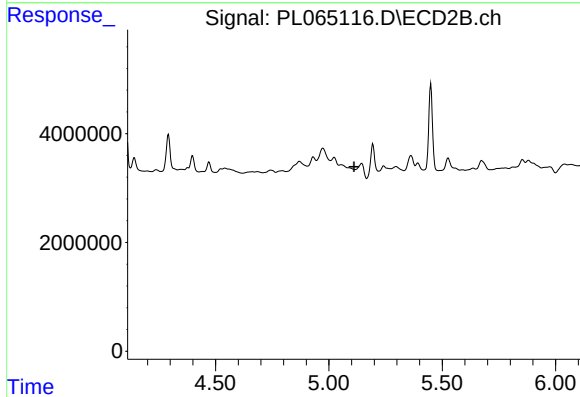


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

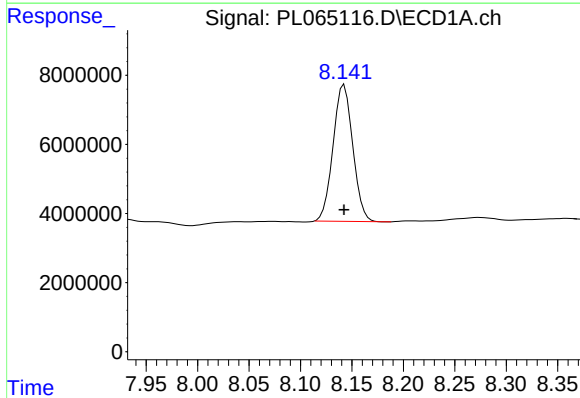

#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 52640770
Conc: 18.97 ng/ml

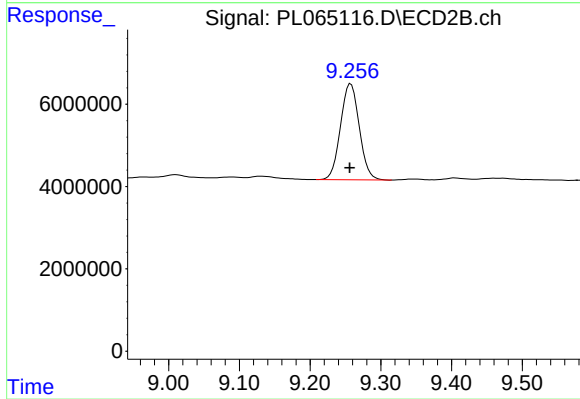

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: 0.001 min
Response: 43082479
Conc: 19.61 ng/ml