

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 20:20
 Operator : AR\AJ
 Sample : M1525-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:19:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	66688635	54854946	22.680	22.090
28)	SA Decachlor...	8.142	9.257	48697559	39450243	17.548	17.960
Target Compounds							
7)	B delta-BHC	0.000	5.205	0	4868835	N.D.	1.608 #
10)	B gamma-Chl...	5.354	0.000	1692838	0	0.432	N.D. #
16)	A 4,4'-DDD	6.097f	0.000	5391054	0	1.811	N.D. #
17)	MA 4,4'-DDT	0.000	7.267	0	7646955	N.D.	3.902 #
23)	Chlordane-1	4.286	0.000	2881114	0	22.604	N.D. #
25)	Chlordane-3	5.354	0.000	1692838	0	4.243	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 20:20
Operator : AR\AJ
Sample : M1525-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:19:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

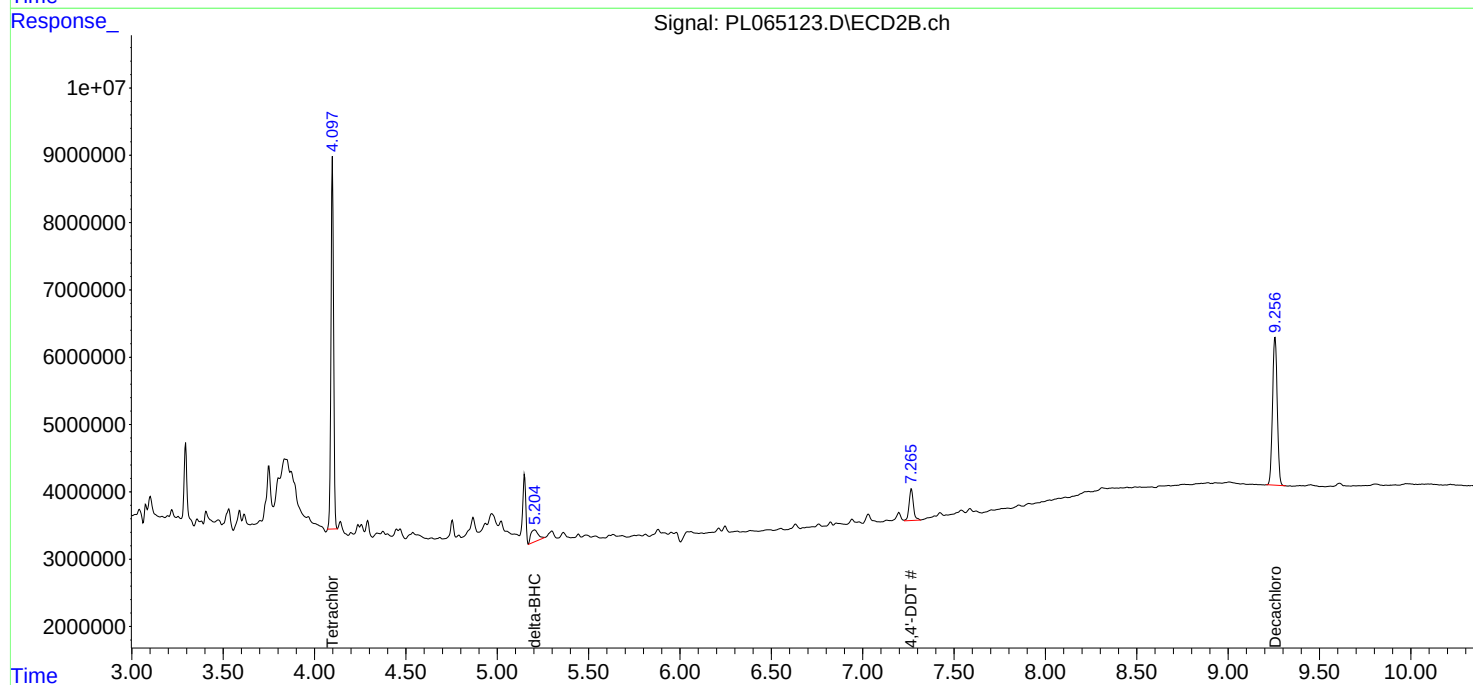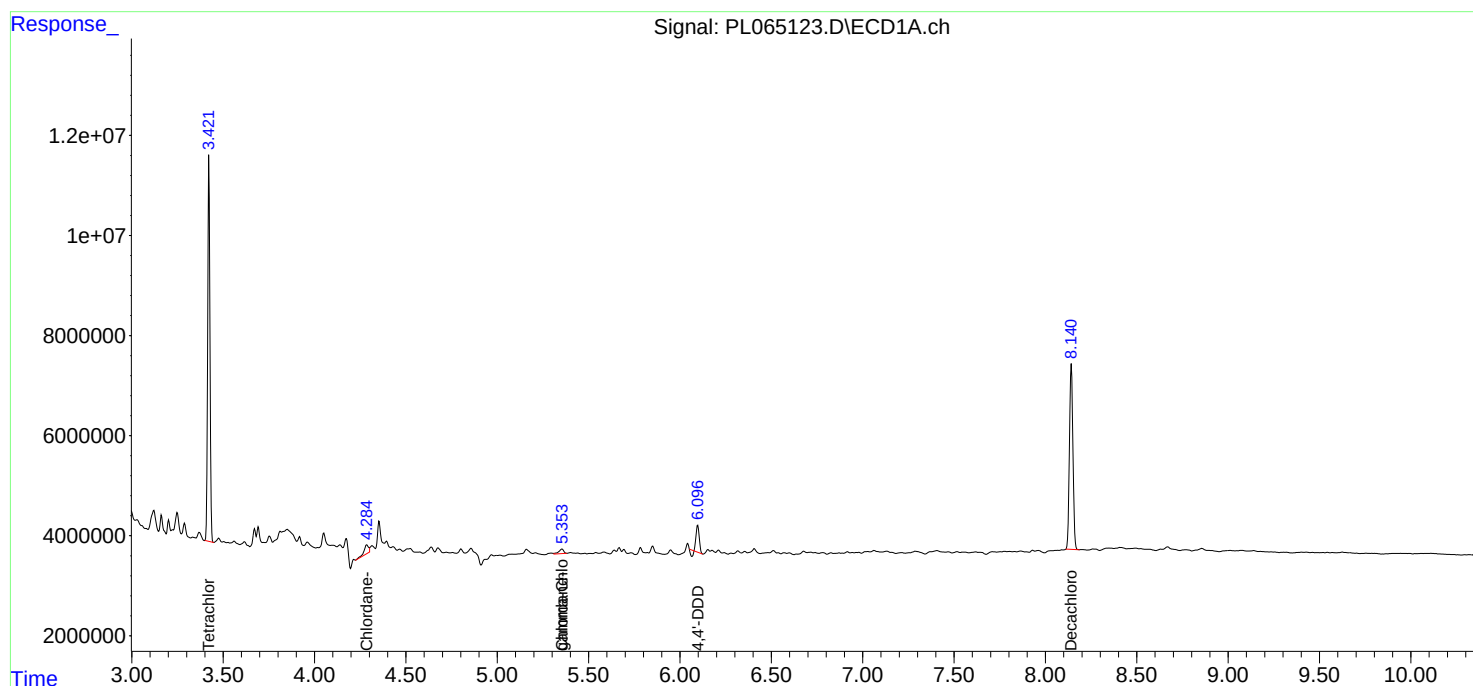


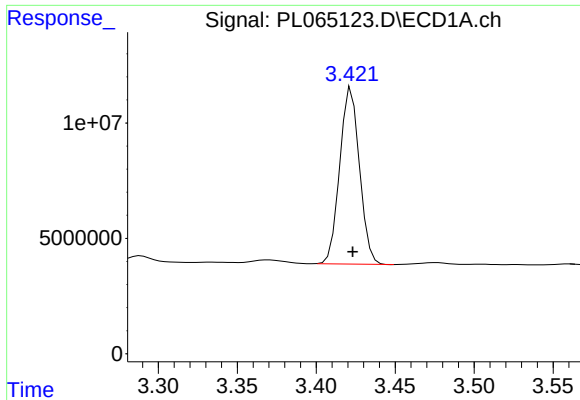

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 66688635
Conc: 22.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

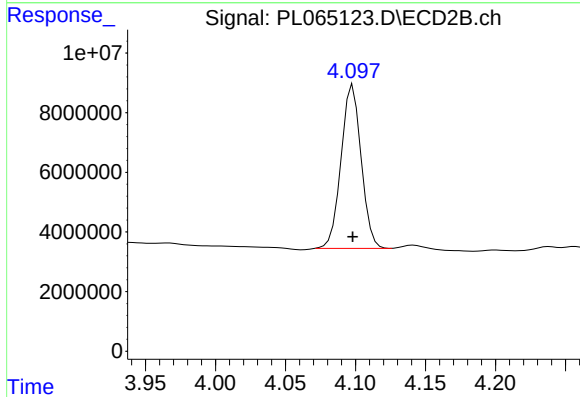


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 54854946
Conc: 22.09 ng/ml

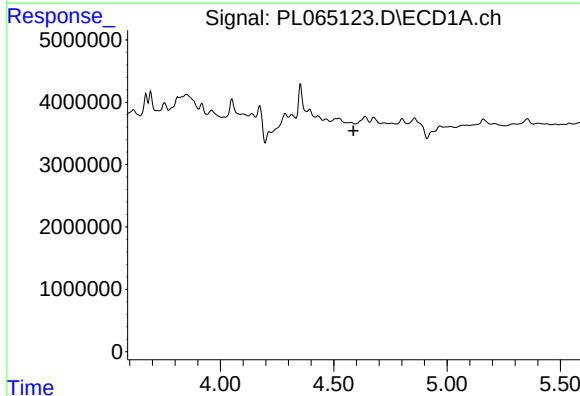


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.587 min
Response: 0
Conc: N.D.

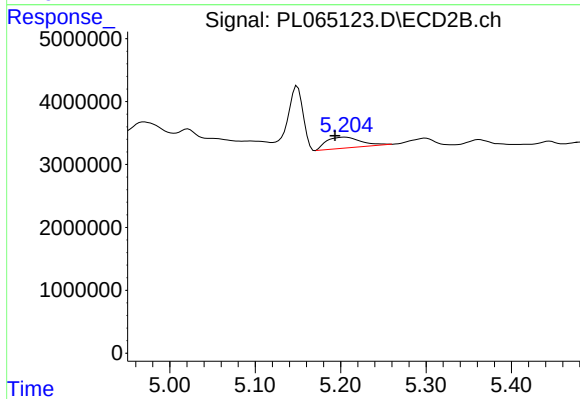

#7 delta-BHC


R.T.: 5.205 min
Delta R.T.: 0.012 min
Response: 4868835
Conc: 1.61 ng/ml

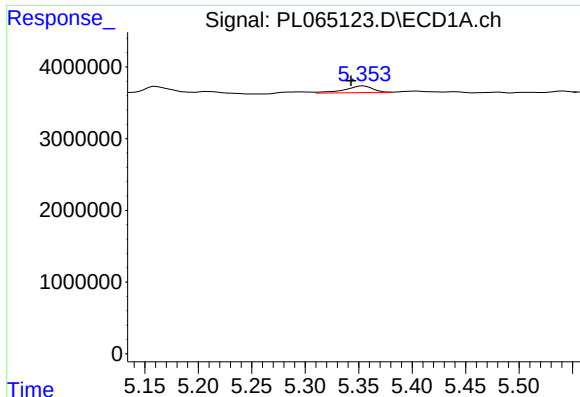

#10 gamma-Chlordane


R.T.: 5.354 min
Delta R.T.: 0.011 min
Response: 1692838
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

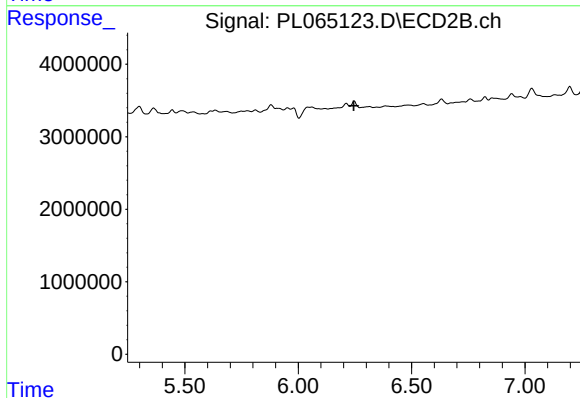


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

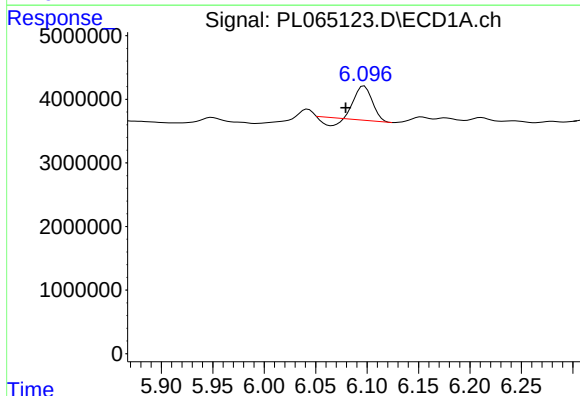


#16 4,4'-DDD

R.T.: 6.097 min
Delta R.T.: 0.018 min
Response: 5391054
Conc: 1.81 ng/ml

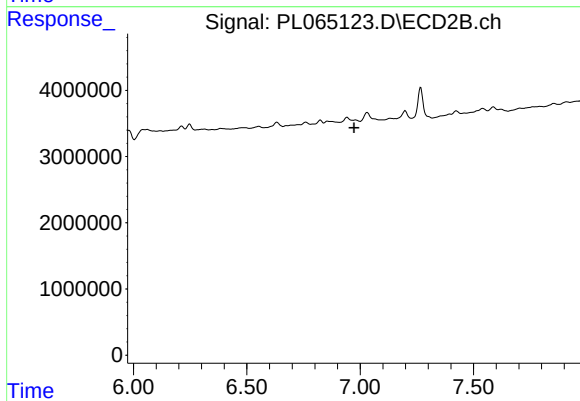

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.973 min
Response: 0
Conc: N.D.

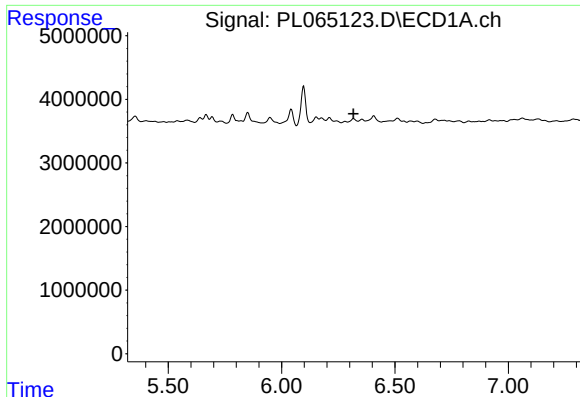

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

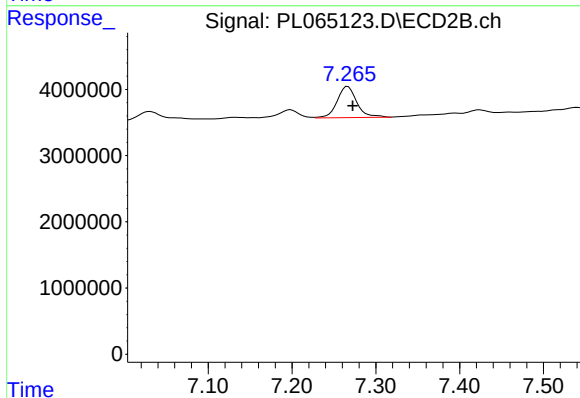


#17 4,4'-DDT

R.T.: 7.267 min
Delta R.T.: -0.006 min
Response: 7646955
Conc: 3.90 ng/ml

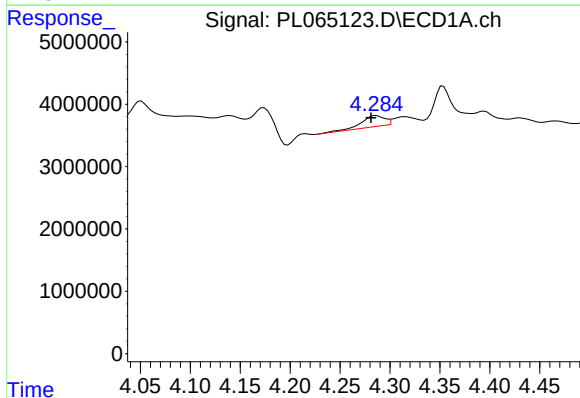


#23 Chlordane-1

R.T.: 4.286 min
Delta R.T.: 0.005 min
Response: 2881114
Conc: 22.60 ng/ml

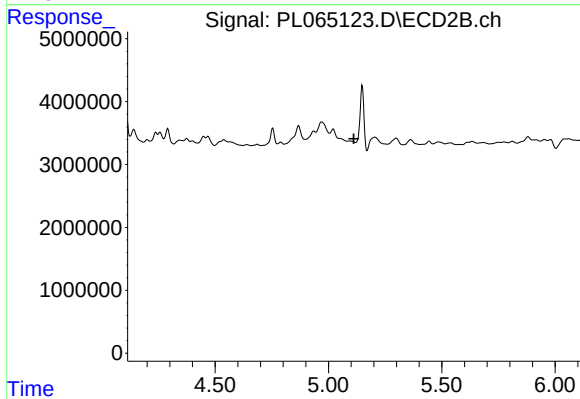

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.112 min
Response: 0
Conc: N.D.

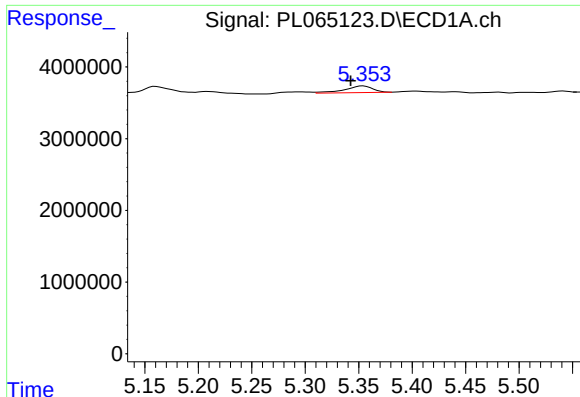

#25 Chlordane-3


R.T.: 5.354 min
Delta R.T.: 0.012 min
Response: 1692838
Conc: 4.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

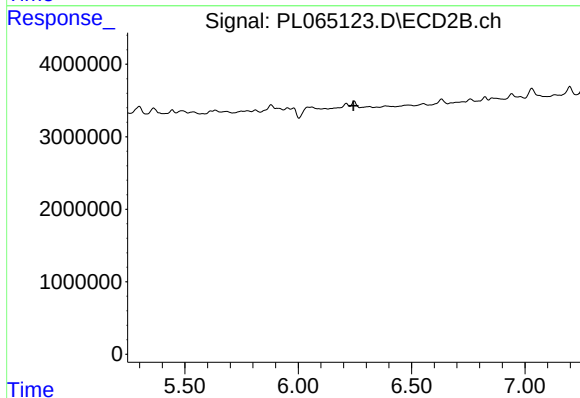


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

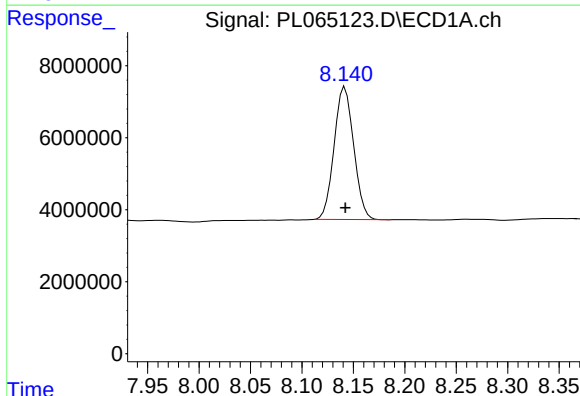

#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 48697559
Conc: 17.55 ng/ml

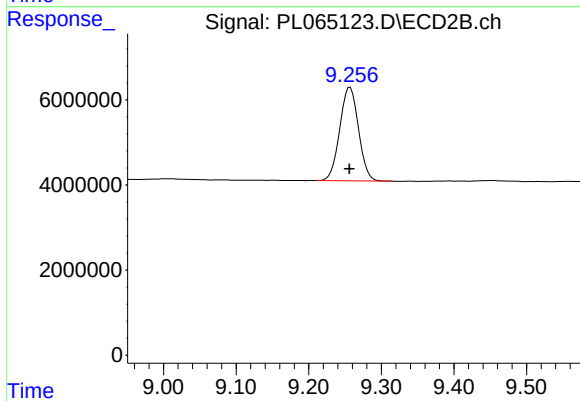

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: 0.000 min
Response: 39450243
Conc: 17.96 ng/ml