

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 11:22
 Operator : AR\AJ
 Sample : M1507-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-41114-15

Manual Integrations
 APPROVED

Ankita
 3/8/2021 11:18:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 13:36:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.427	4.100	63322460	43343307	21.535m	17.454
28) SA Decachlor...	8.150	9.261	25540395	20221843	9.203	9.206

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 11:22
Operator : AR\AJ
Sample : M1507-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
COMP-41114-15


Manual Integrations
APPROVED

Ankita
3/8/2021 11:18:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 13:36:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

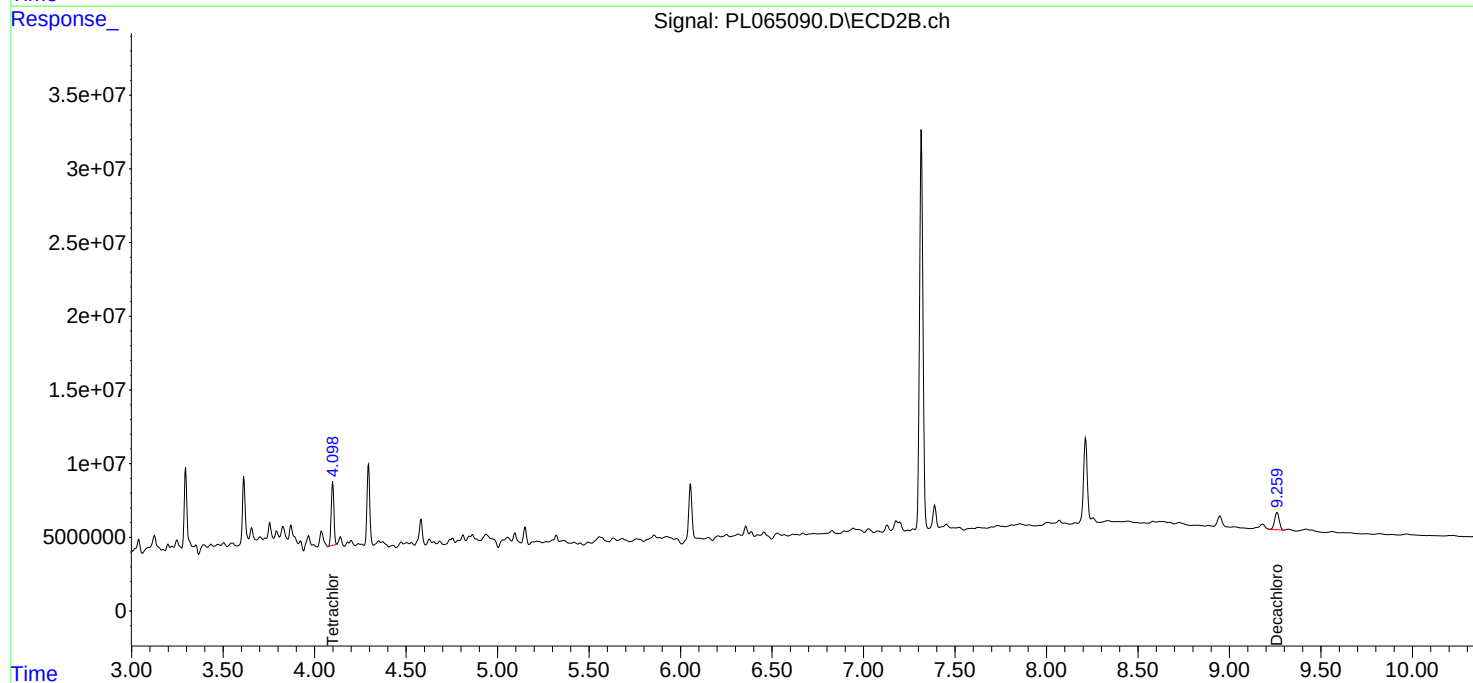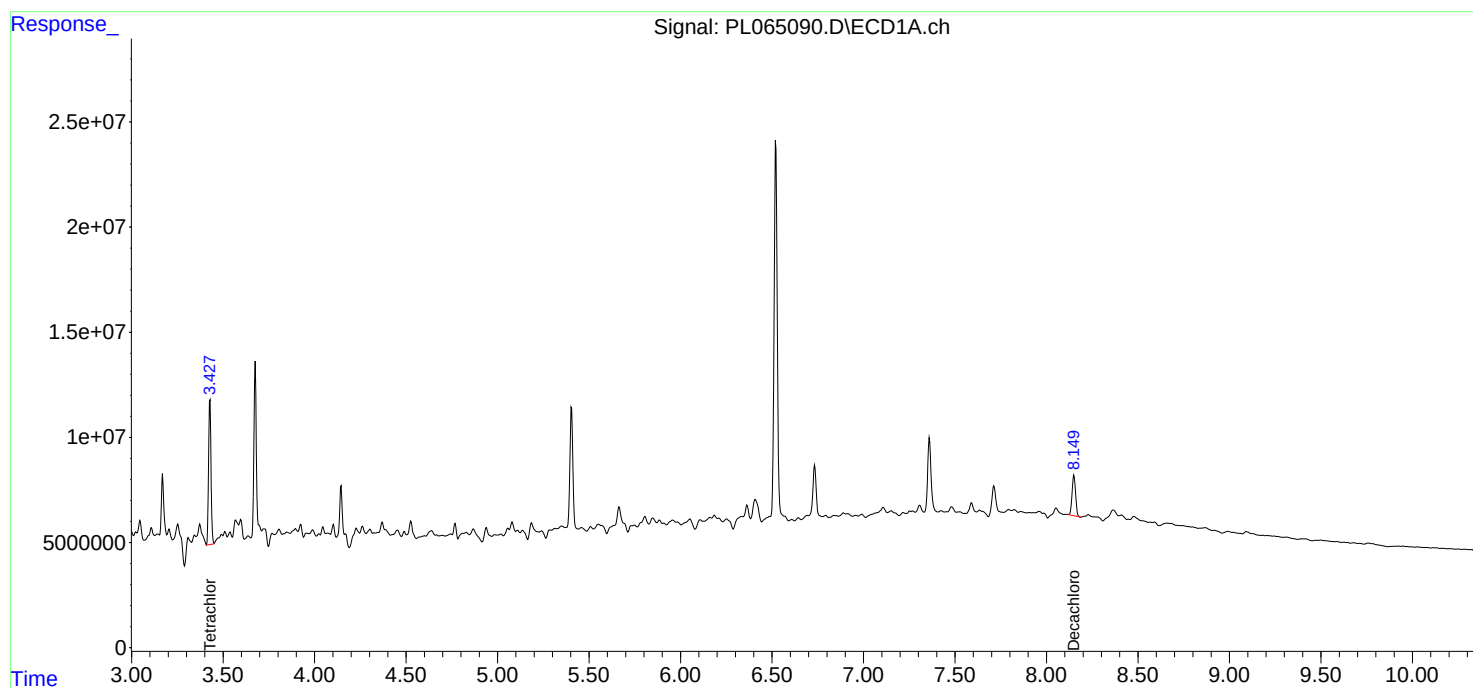

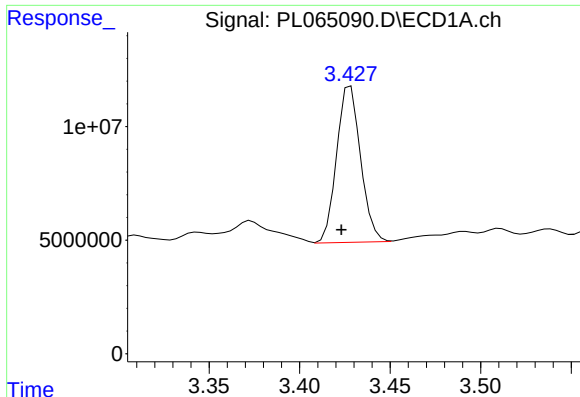

#1 Tetrachloro-m-xylene

R.T.: 3.427 min

Delta R.T.: 0.004 min


Response: 63322460

Conc: 21.54 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMP-41114-15

Manual Integrations
APPROVED

Ankita
3/8/2021 11:18:24 AM

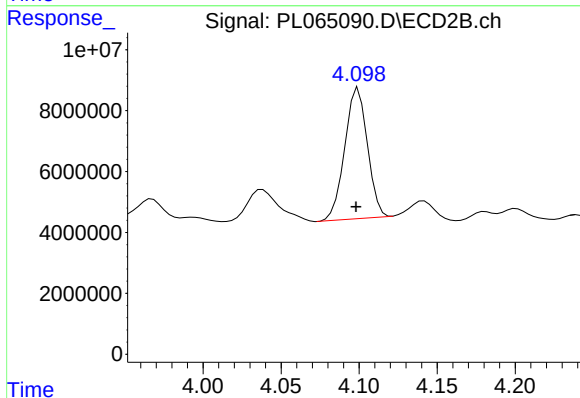


#1 Tetrachloro-m-xylene

R.T.: 4.100 min

Delta R.T.: 0.002 min

Response: 43343307

Conc: 17.45 ng/ml

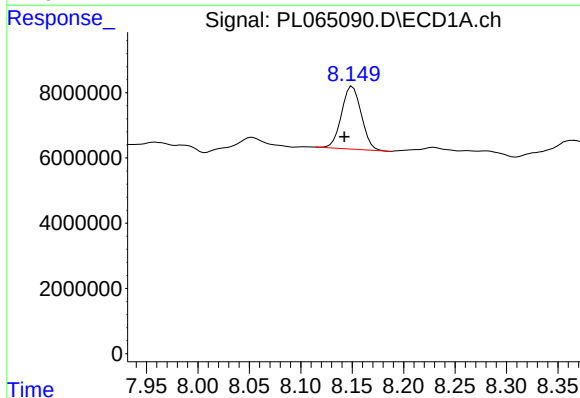


#28 Decachlorobiphenyl

R.T.: 8.150 min

Delta R.T.: 0.008 min

Response: 25540395

Conc: 9.20 ng/ml

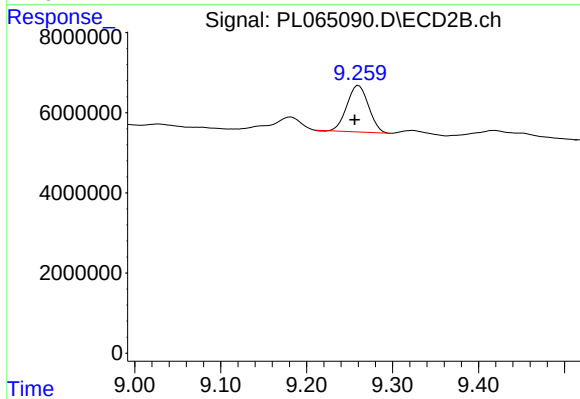

#28 Decachlorobiphenyl

R.T.: 9.261 min

Delta R.T.: 0.005 min

Response: 20221843

Conc: 9.21 ng/ml