

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 13:54
 Operator : AR\AJ
 Sample : M1556-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-030321

Manual Integrations
 APPROVED

Ankita
 3/8/2021 11:19:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:12:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	44351210	36117992	15.083	14.545
28)	SA Decachlor...	8.143	9.257	41957484	34147617	15.119	15.546
Target Compounds							
12)	B 4,4'-DDE	5.564	6.472	34241431	23901835	9.527m	9.561m
17)	MA 4,4'-DDT	6.317	7.270	22111218	14842691	7.931	7.573m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 13:54
Operator : AR\AJ
Sample : M1556-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-04-030321


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:12:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

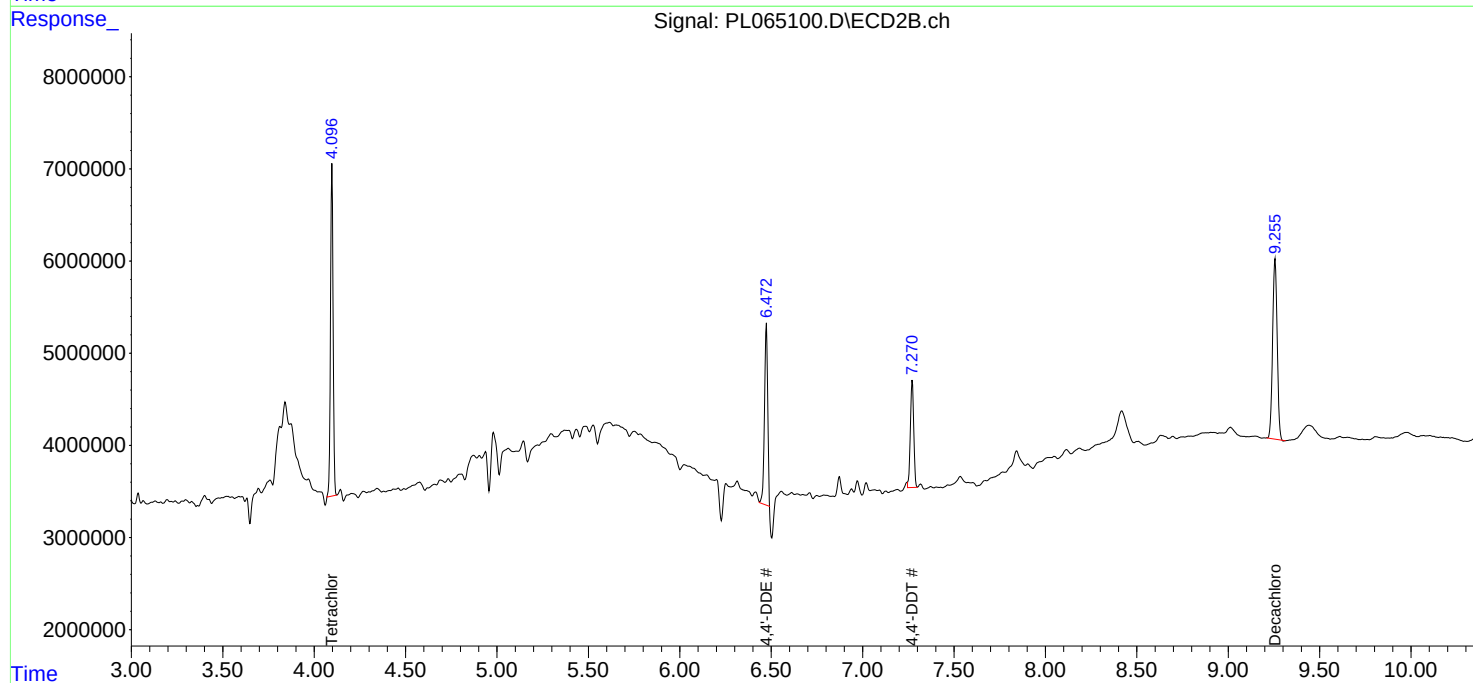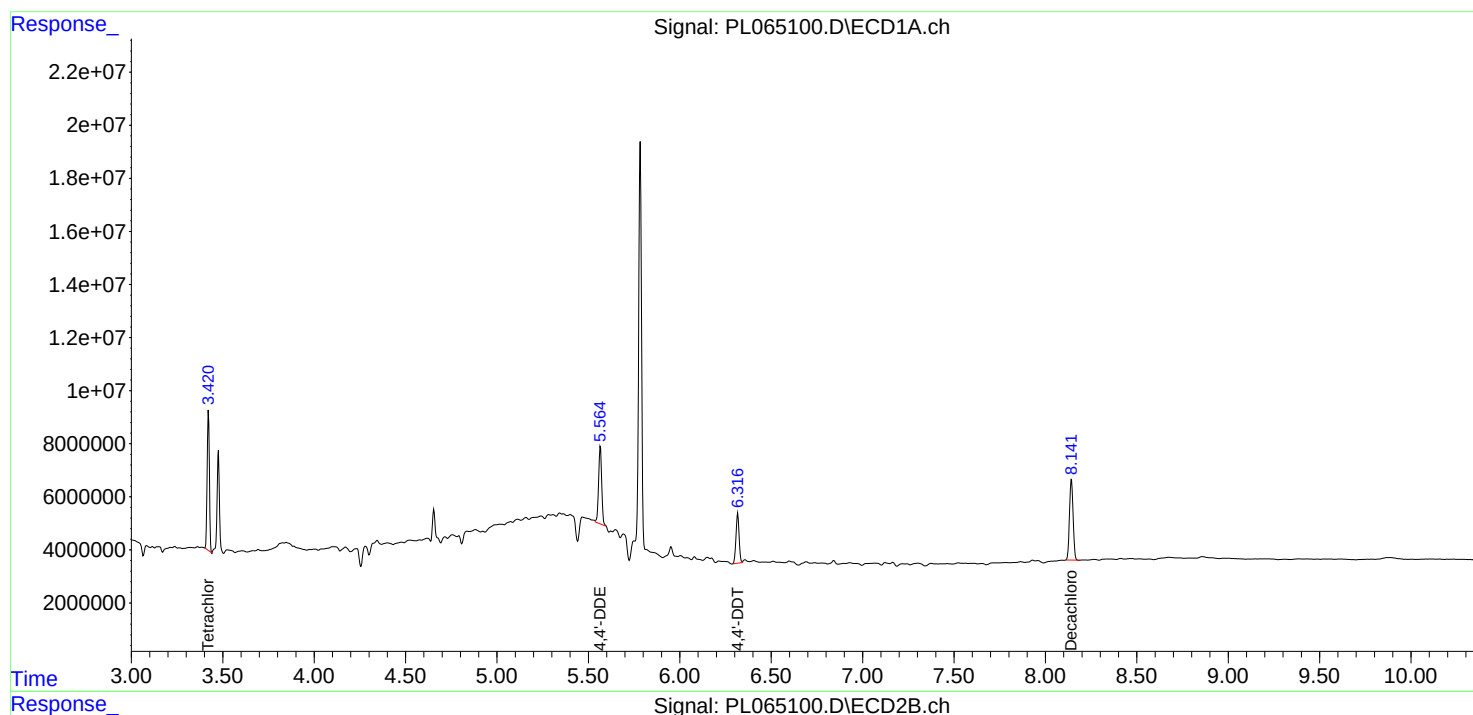

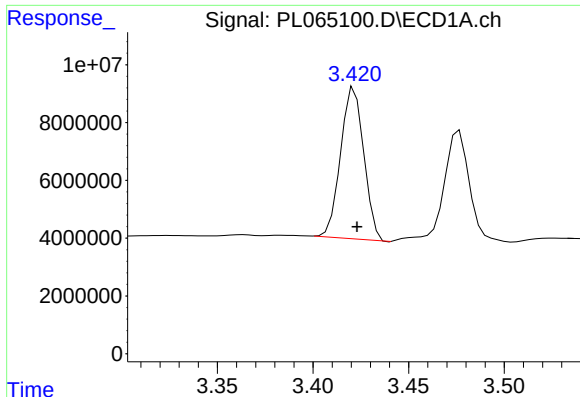


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 44351210
Conc: 15.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-030321


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:00 AM

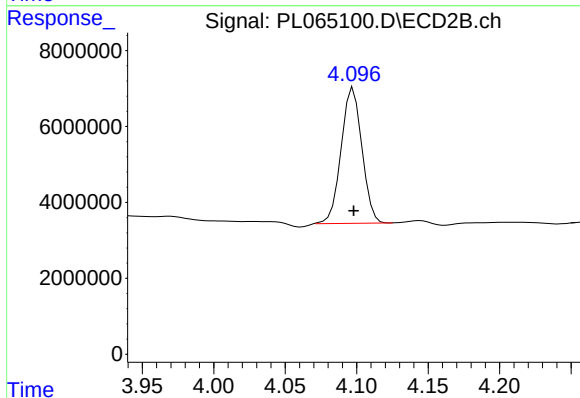


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 36117992
Conc: 14.54 ng/ml

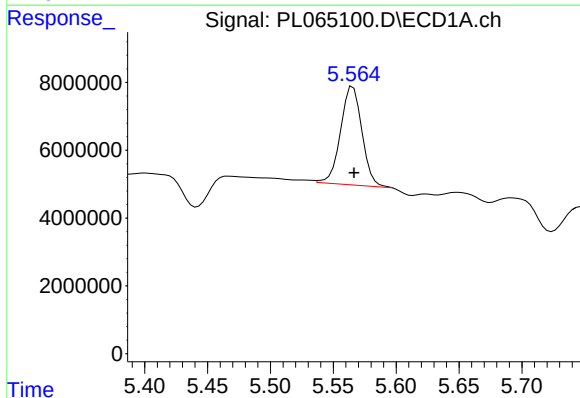


#12 4,4'-DDE

R.T.: 5.564 min
Delta R.T.: -0.002 min
Response: 34241431
Conc: 9.53 ng/ml m

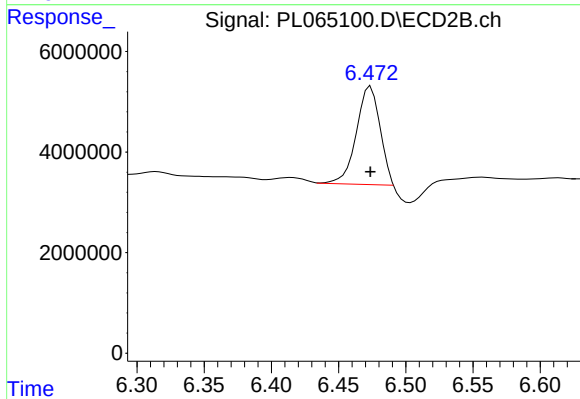

#12 4,4'-DDE

R.T.: 6.472 min
Delta R.T.: -0.001 min
Response: 23901835
Conc: 9.56 ng/ml m

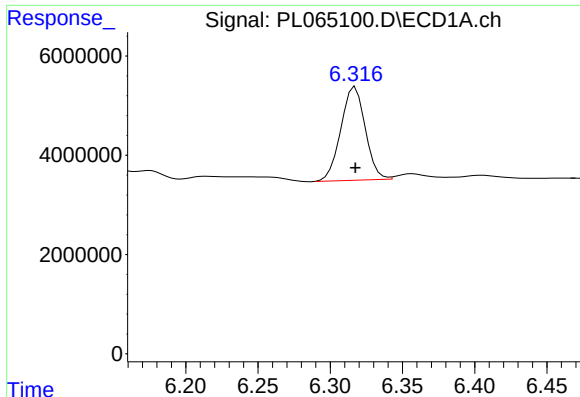


#17 4,4'-DDT

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 22111218
Conc: 7.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-030321


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:00 AM

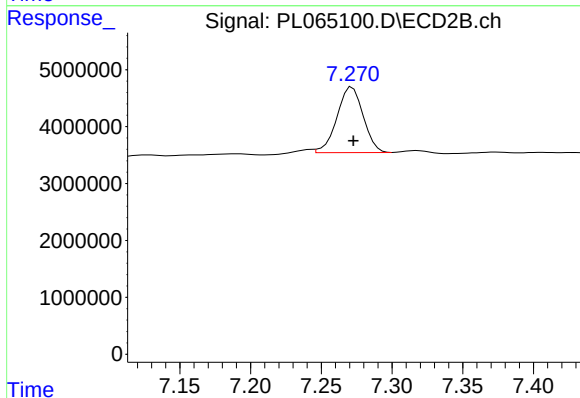


#17 4,4'-DDT

R.T.: 7.270 min
Delta R.T.: -0.002 min
Response: 14842691
Conc: 7.57 ng/ml m

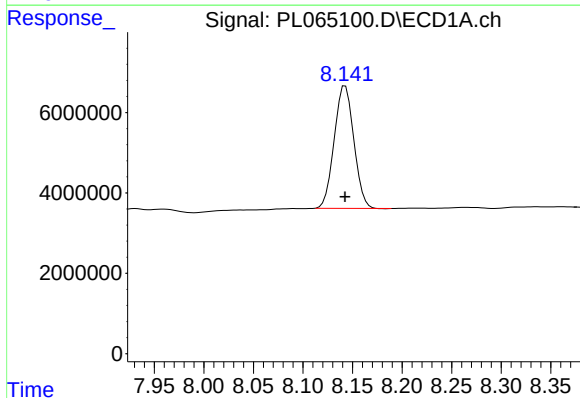

#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 41957484
Conc: 15.12 ng/ml

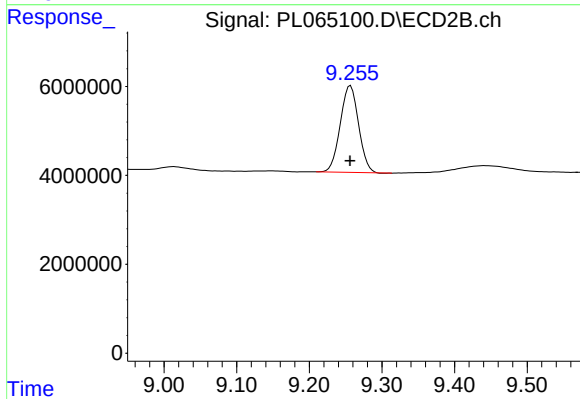

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: 0.000 min
Response: 34147617
Conc: 15.55 ng/ml