

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 16:16
 Operator : AR\AJ
 Sample : M1565-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 3/8/2021 1:08:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 22:14:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	33890863	26746083	11.526	10.771
28)	SA Decachlor...	8.143	9.257	30016524	23232073	10.816	10.577
Target Compounds							
12)	B 4,4'-DDE	5.564	6.473	7080577	5004067	1.970m	2.002

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 16:16
Operator : AR\AJ
Sample : M1565-05
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
3/8/2021 1:08:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 22:14:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

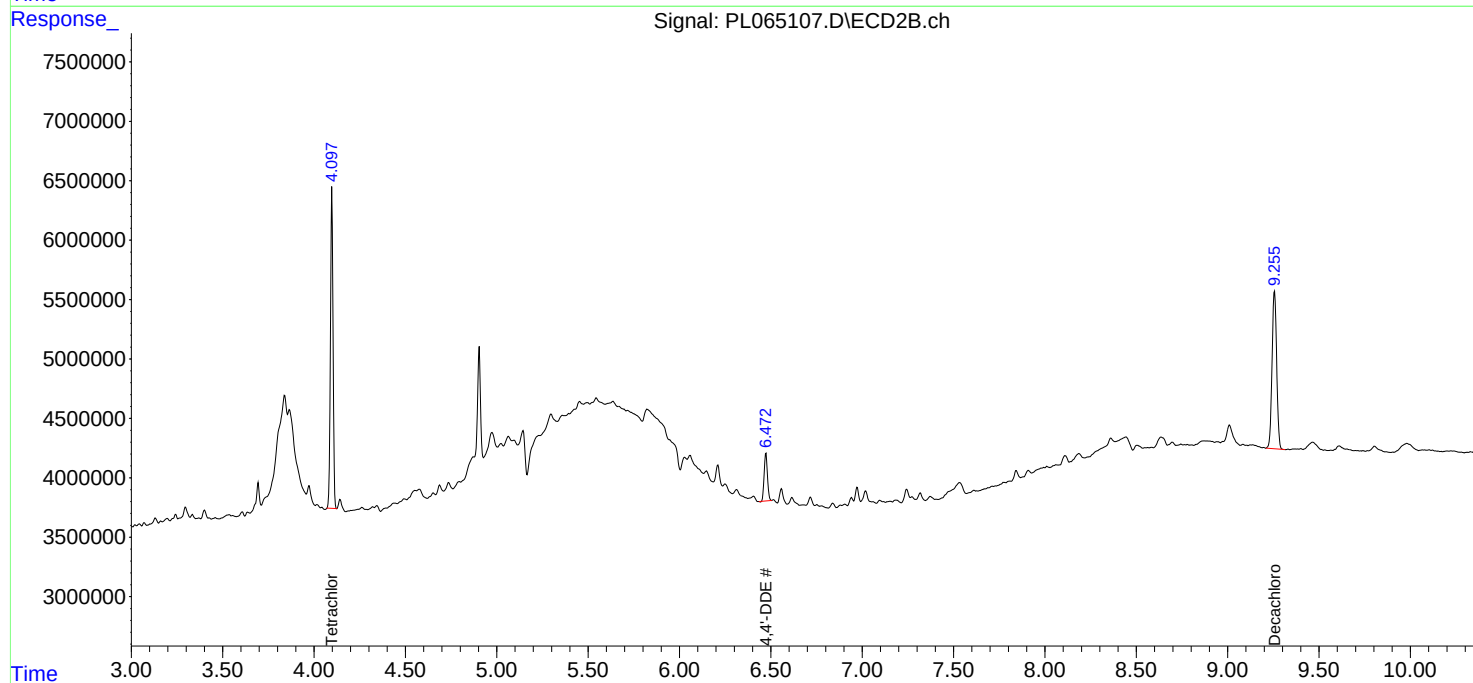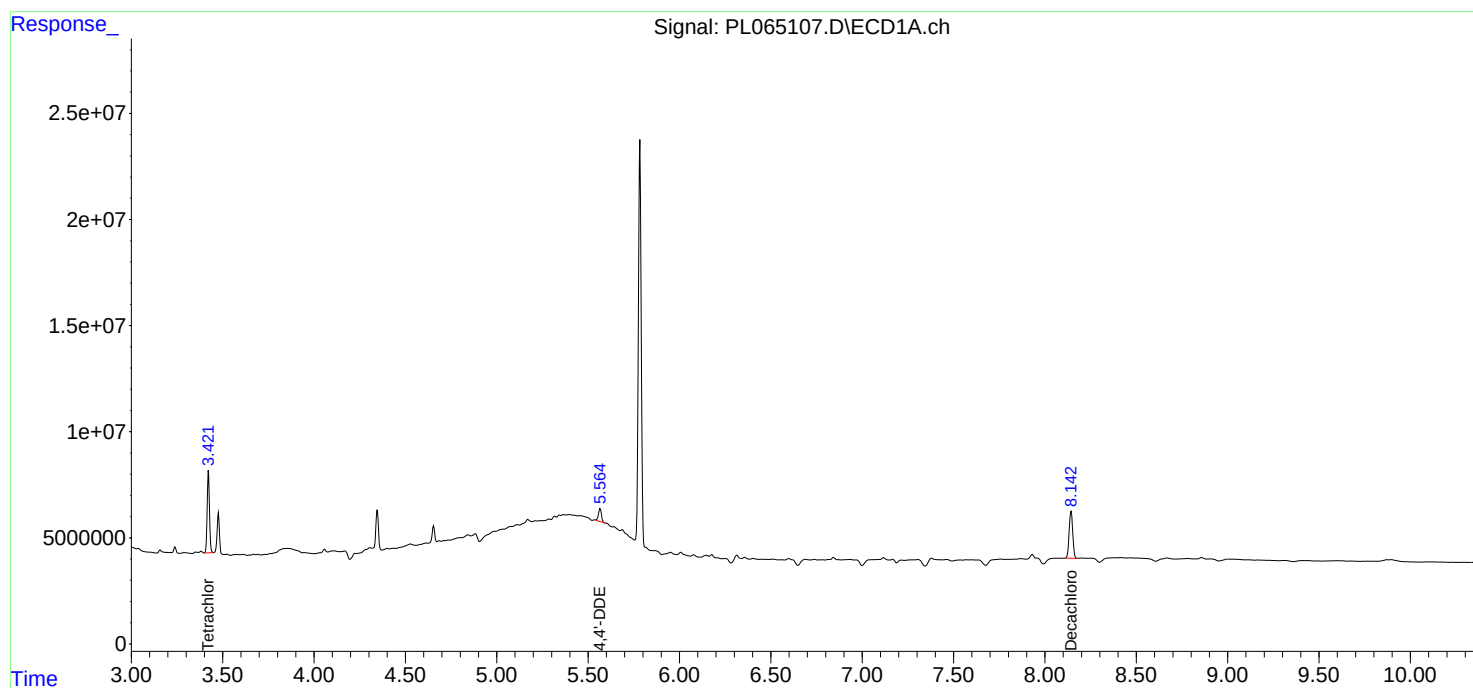

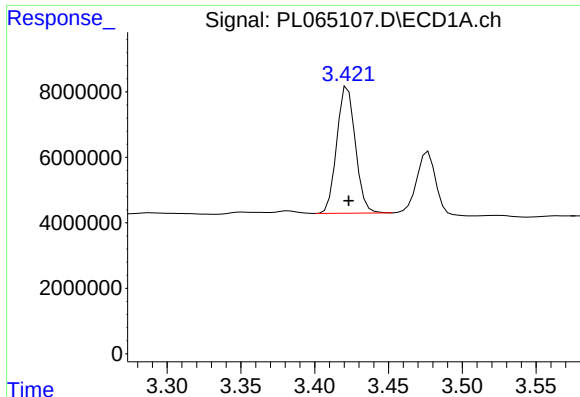


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 33890863
Conc: 11.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
3/8/2021 1:08:34 PM

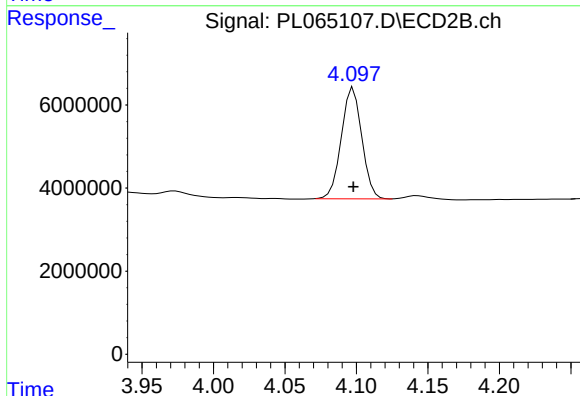


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 26746083
Conc: 10.77 ng/ml

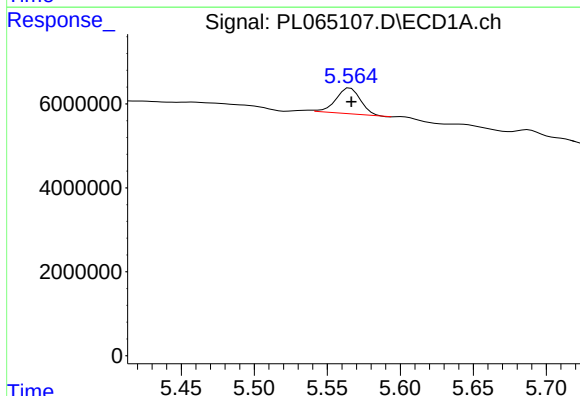


#12 4,4'-DDE

R.T.: 5.564 min
Delta R.T.: -0.002 min
Response: 7080577
Conc: 1.97 ng/ml m

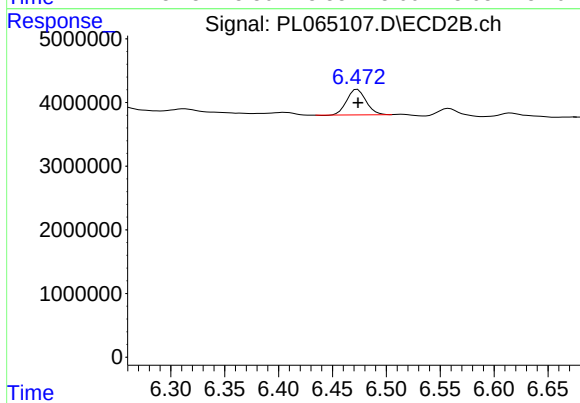

#12 4,4'-DDE

R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 5004067
Conc: 2.00 ng/ml

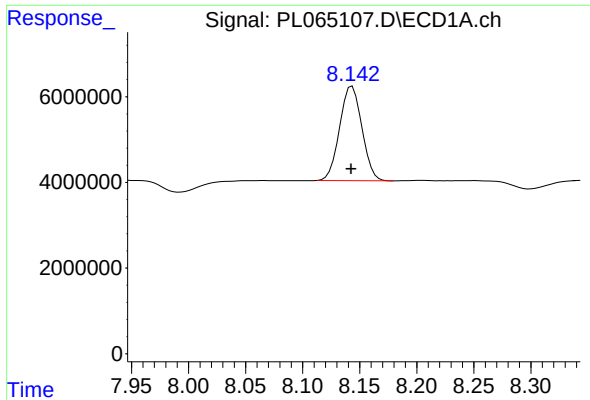


#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.001 min
Response: 30016524
Conc: 10.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Ankita
3/8/2021 1:08:34 PM

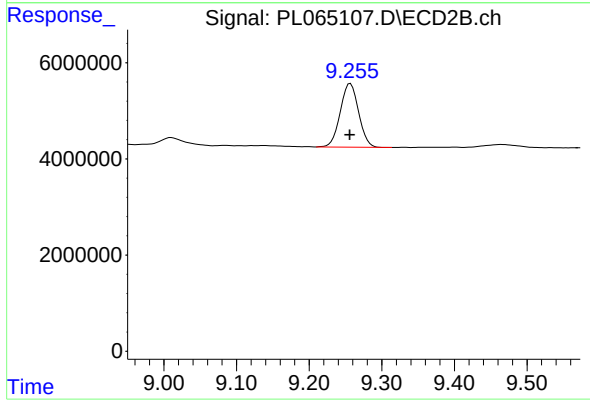

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: 0.000 min
Response: 23232073
Conc: 10.58 ng/ml