

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 17:28
 Operator : AR\AJ
 Sample : M1566-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VEOLIA-72-11977

Manual Integrations
 APPROVED

Ankita
 3/8/2021 11:19:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 04:30:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.422	4.097	38568494	31791923	13.117	12.803m
28) SA Decachlor...	8.142	9.256	42569087	29555238	15.340m	13.455m
Target Compounds						
12) B 4,4'-DDE	5.564	6.474	6978845	5975246	1.942m	2.390
17) MA 4,4'-DDT	6.316	7.271	8409641	2438992	3.016	1.244m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065112.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 17:28
Operator : AR\AJ
Sample : M1566-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VEOLIA-72-11977


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 04:30:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

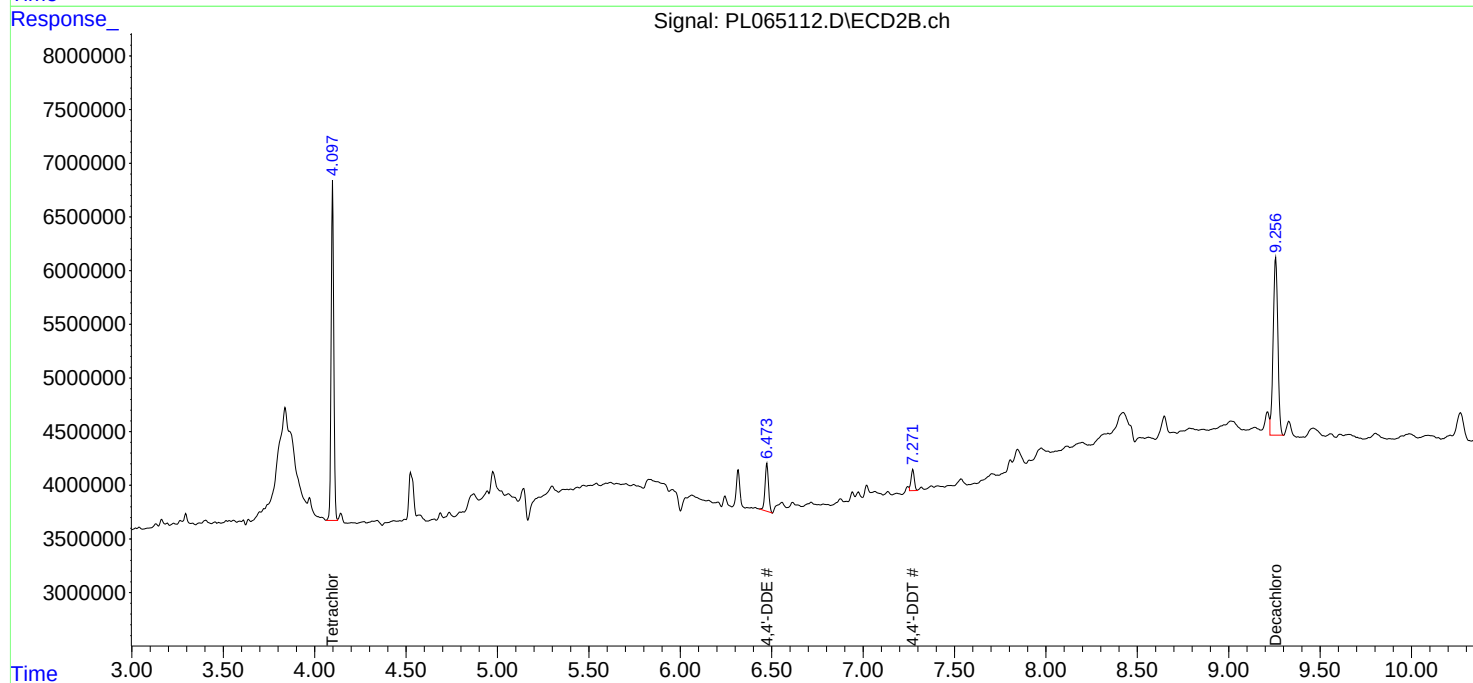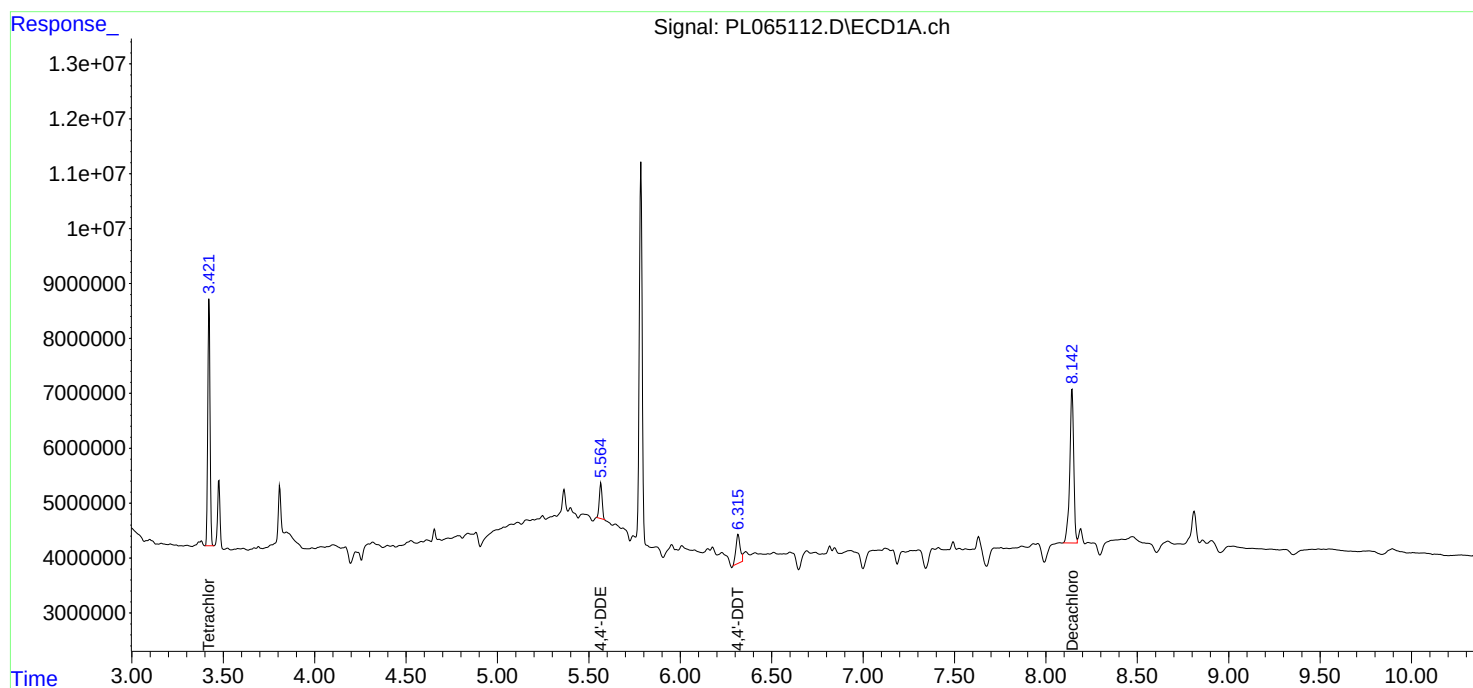

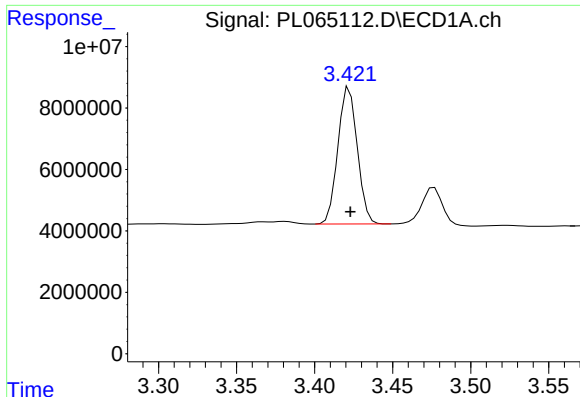


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 38568494
Conc: 13.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-72-11977


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:18 AM

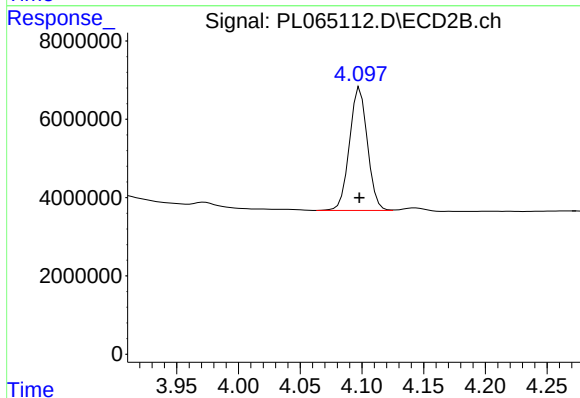


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 31791923
Conc: 12.80 ng/ml m

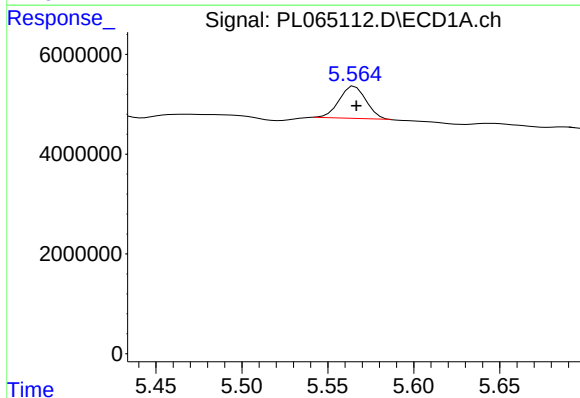


#12 4,4'-DDE

R.T.: 5.564 min
Delta R.T.: -0.002 min
Response: 6978845
Conc: 1.94 ng/ml m

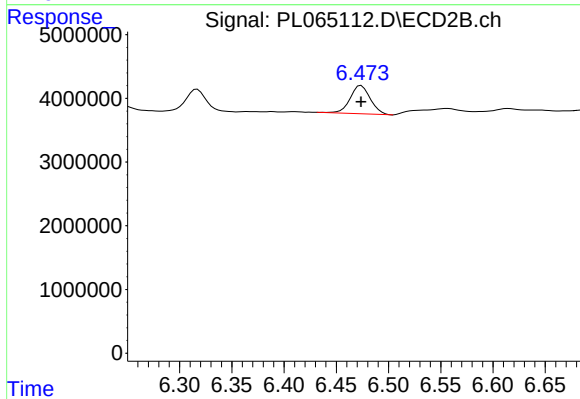

#12 4,4'-DDE

R.T.: 6.474 min
Delta R.T.: 0.000 min
Response: 5975246
Conc: 2.39 ng/ml

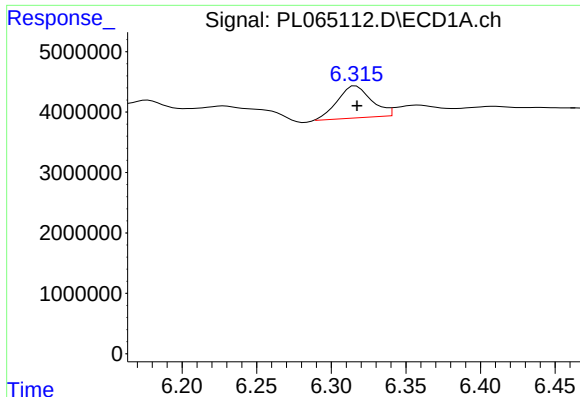


#17 4,4'-DDT

R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 8409641
Conc: 3.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-72-11977


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:18 AM

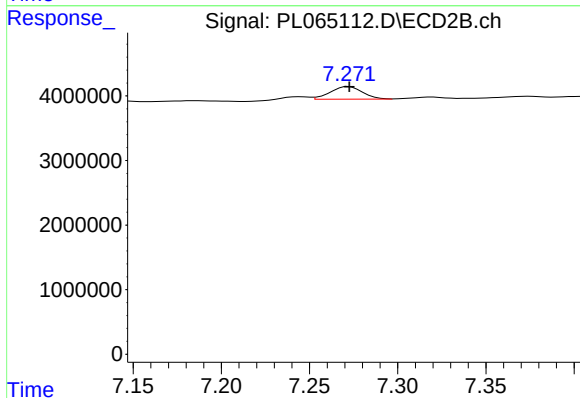


#17 4,4'-DDT

R.T.: 7.271 min
Delta R.T.: -0.002 min
Response: 2438992
Conc: 1.24 ng/ml m

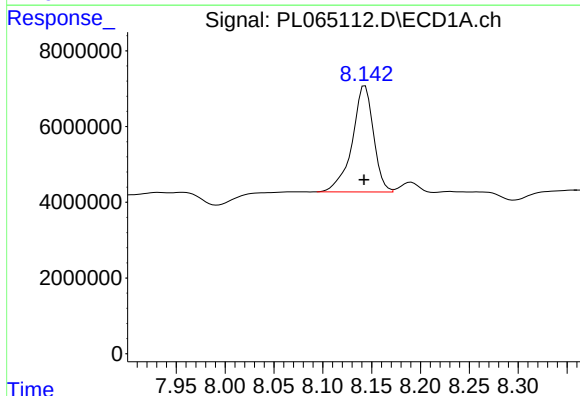

#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 42569087
Conc: 15.34 ng/ml m

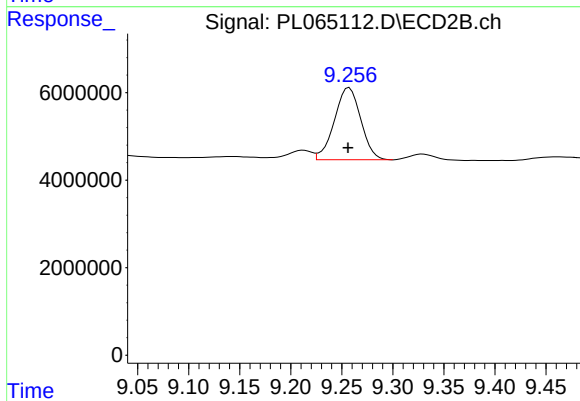

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: 0.000 min
Response: 29555238
Conc: 13.46 ng/ml m