

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
 Data File : PL065116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 18:25
 Operator : AR\AJ
 Sample : M1568-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NORTHSIDE

Manual Integrations
 APPROVED

Ankita
 3/8/2021 11:19:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 05:12:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.422	4.098	62498761	50940174	21.255	20.514
28) SA Decachlor...	8.142	9.258	53265977	43082479	19.194	19.614
Target Compounds						
6) B beta-BHC	4.392	4.974	6021525	3750781	3.224m	2.453

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030621\
Data File : PL065116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 18:25
Operator : AR\AJ
Sample : M1568-05
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NORTHSIDE


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 05:12:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

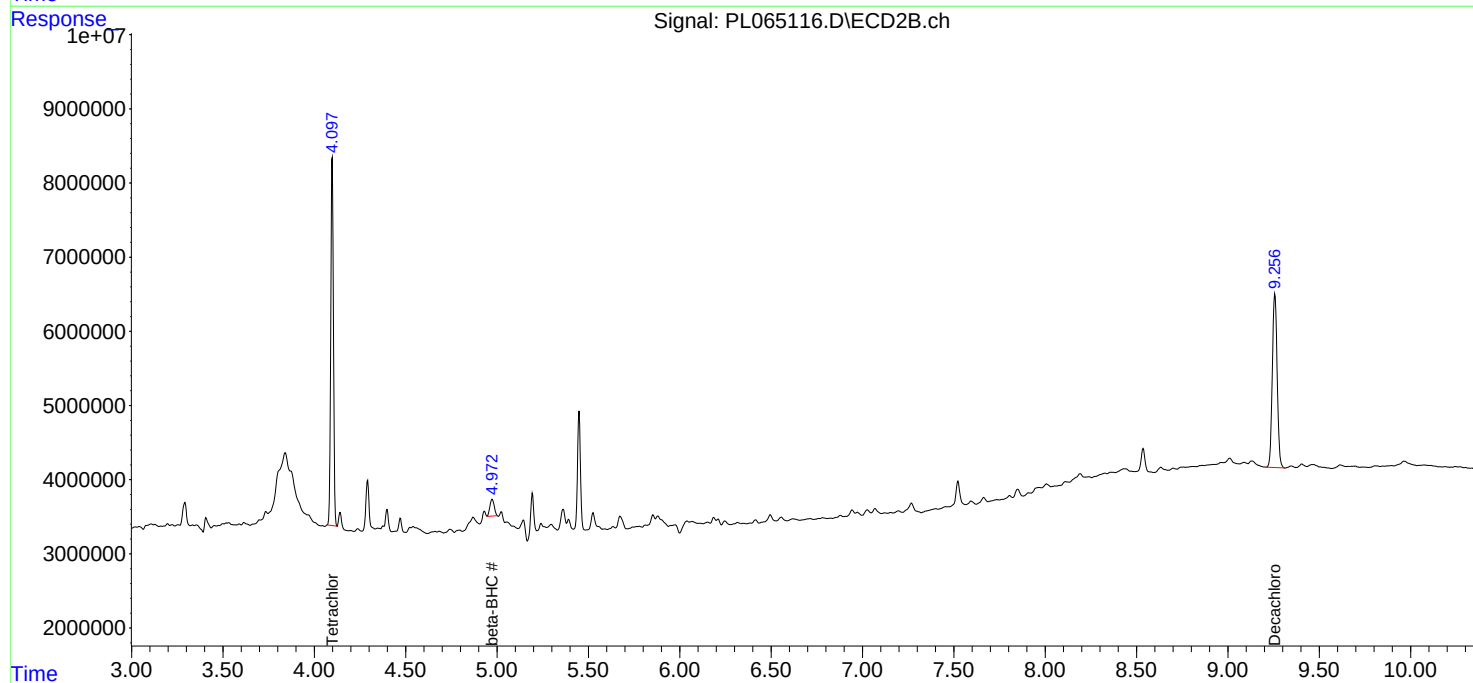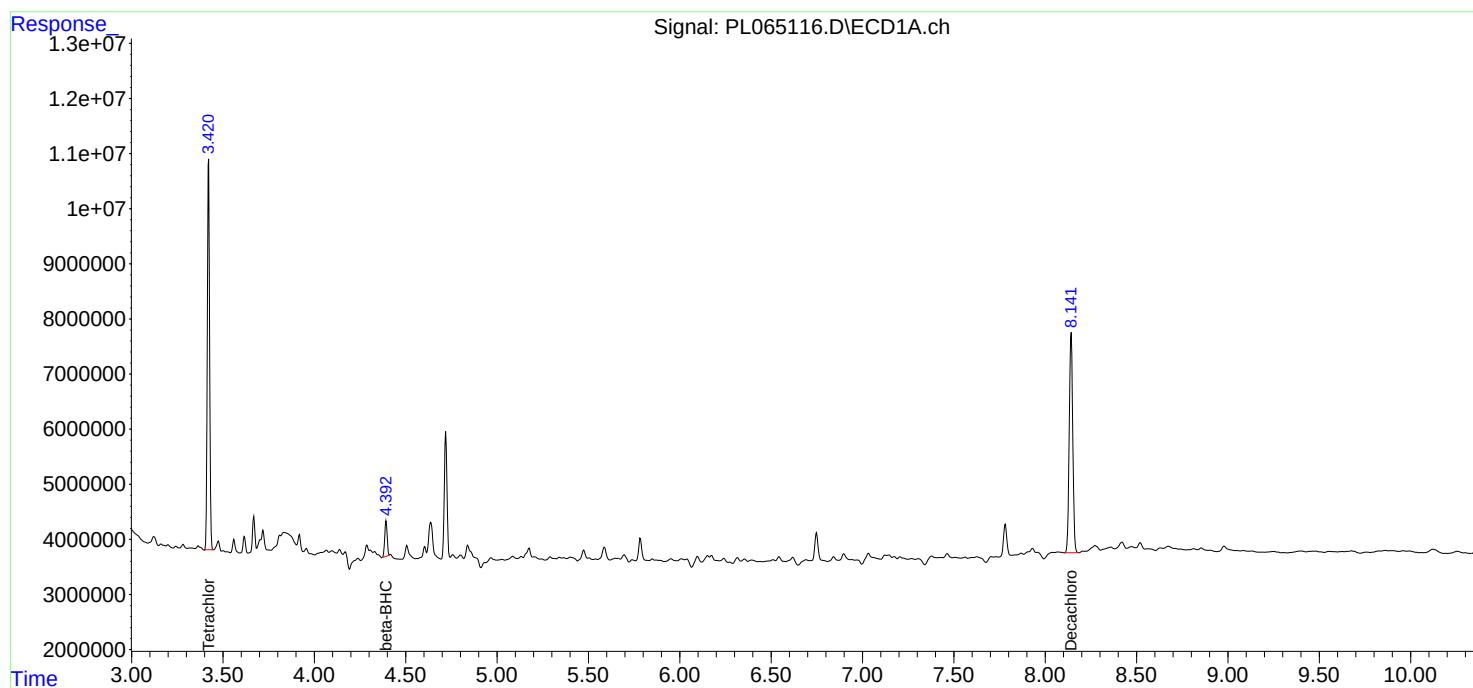

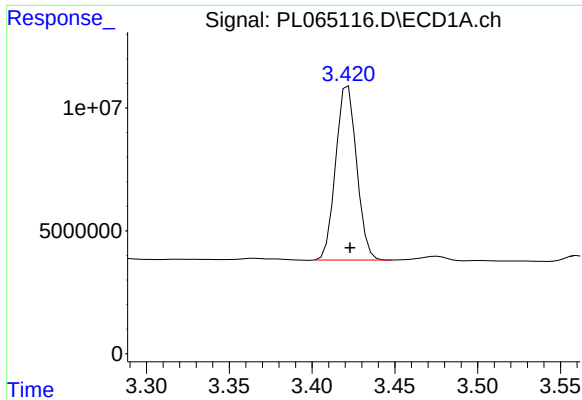


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 62498761
Conc: 21.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
NORTHSIDE


Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:29 AM

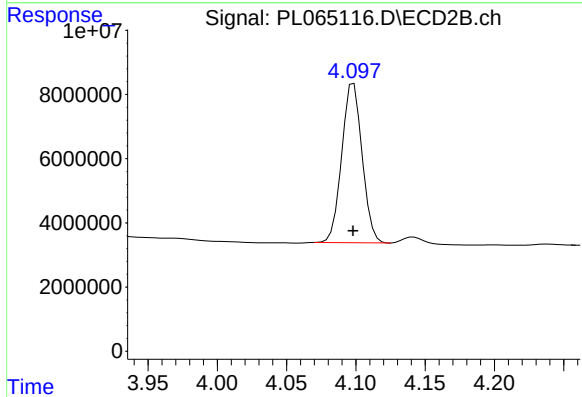


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 50940174
Conc: 20.51 ng/ml

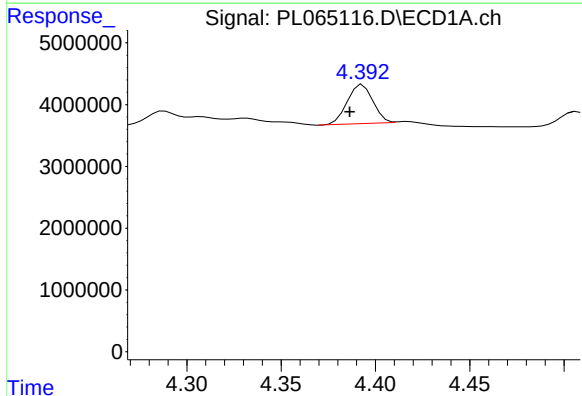


#6 beta-BHC

R.T.: 4.392 min
Delta R.T.: 0.005 min
Response: 6021525
Conc: 3.22 ng/ml m

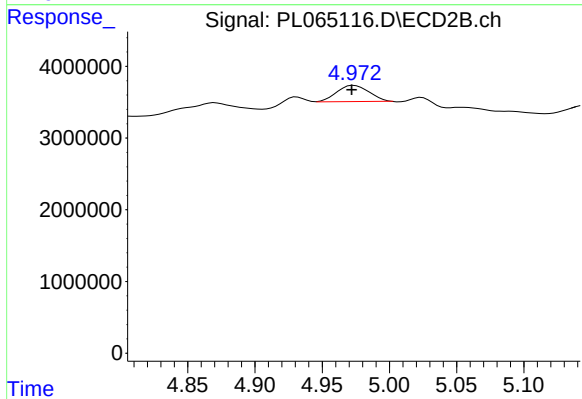

#6 beta-BHC

R.T.: 4.974 min
Delta R.T.: 0.002 min
Response: 3750781
Conc: 2.45 ng/ml

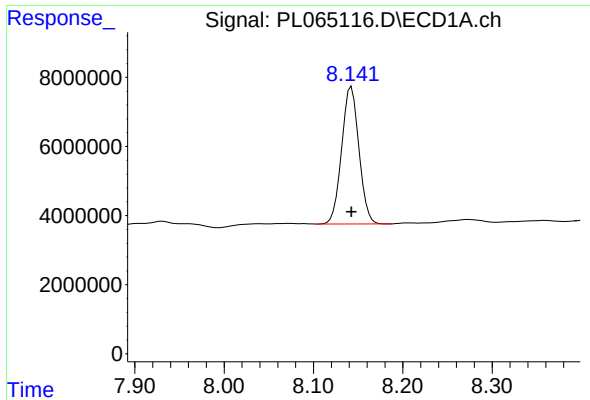


#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 53265977
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
NORTHSIDE

Manual Integrations
APPROVED

Ankita
3/8/2021 11:19:29 AM

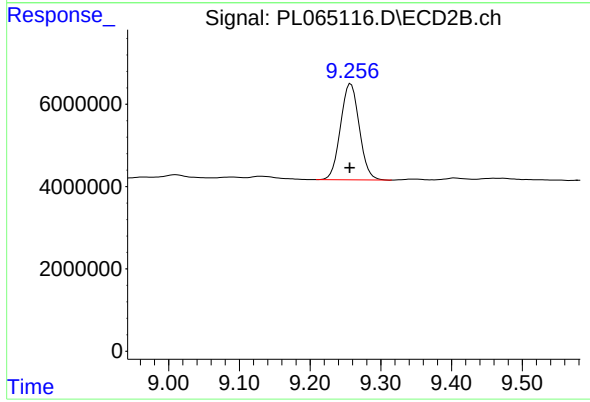

#28 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: 0.001 min
Response: 43082479
Conc: 19.61 ng/ml