

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030623\
 Data File : PL081258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2023 10:16
 Operator : AR\AJ
 Sample : 01751-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MONTHLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/07/2023
 Supervised By :Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 20:39:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.334	2.666	27875936	29958115	12.902	14.803
28) SA Decachlor...	8.757	7.788	19999163	27698081	13.118m	14.460

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030623\
Data File : PL081258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2023 10:16
Operator : AR\AJ
Sample : 01751-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/07/2023
Supervised By : Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 20:39:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

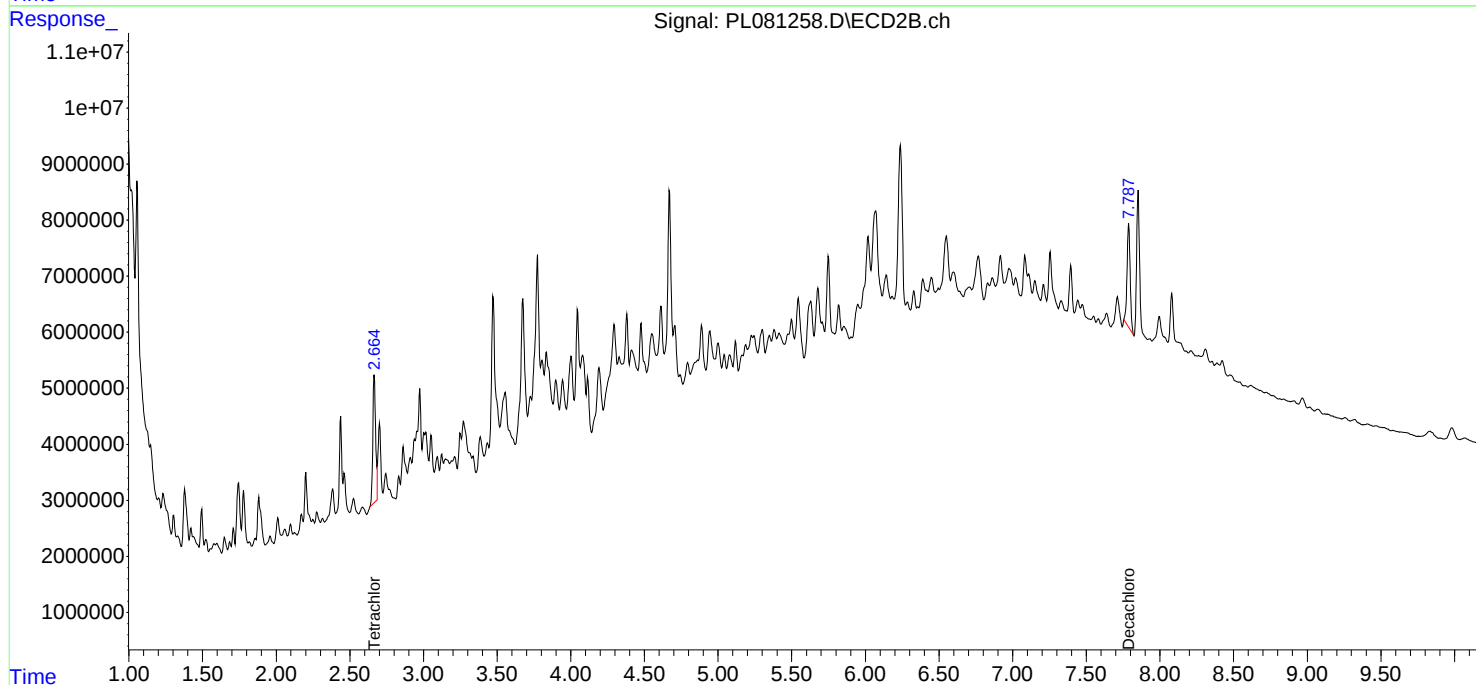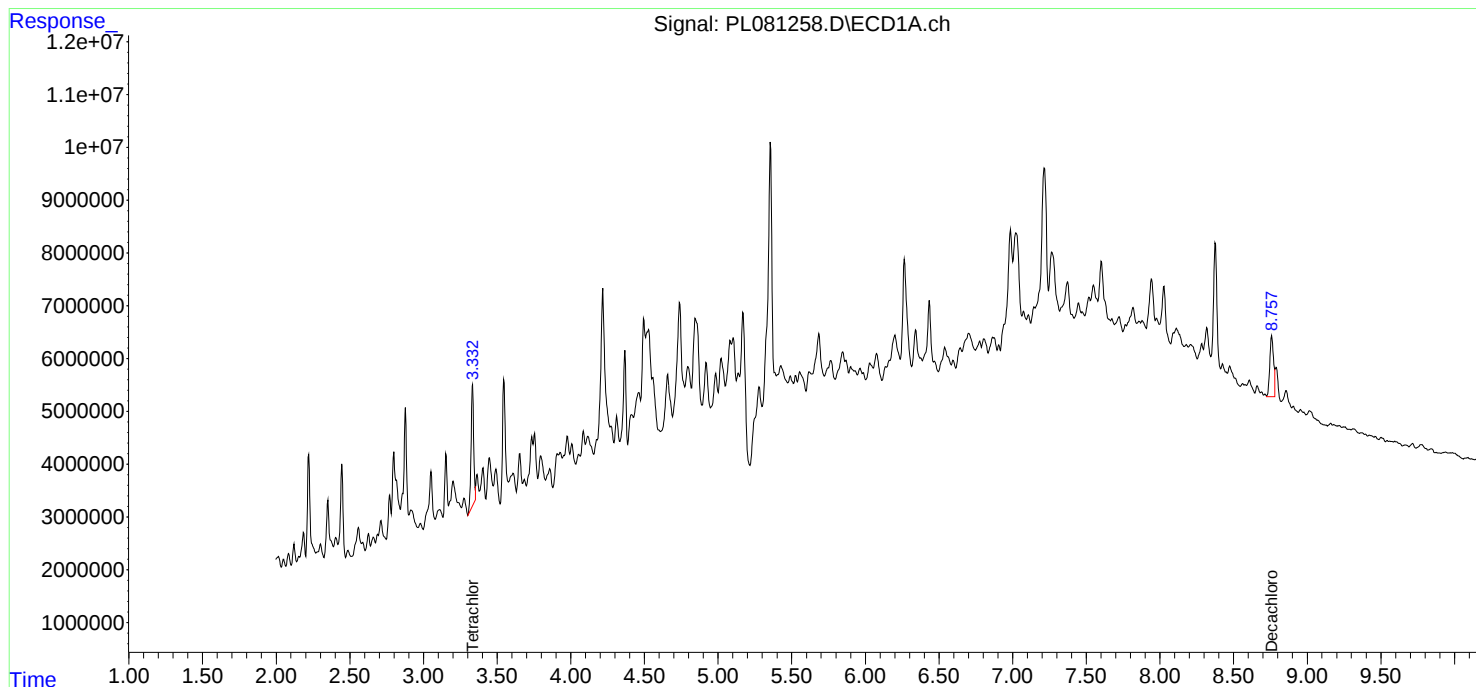

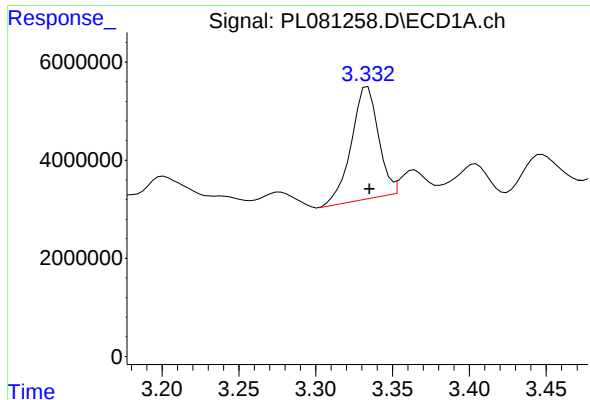


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: -0.001 min
Response: 27875936
Conc: 12.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/07/2023
Supervised By :Ankita Jodhani 03/07/2023

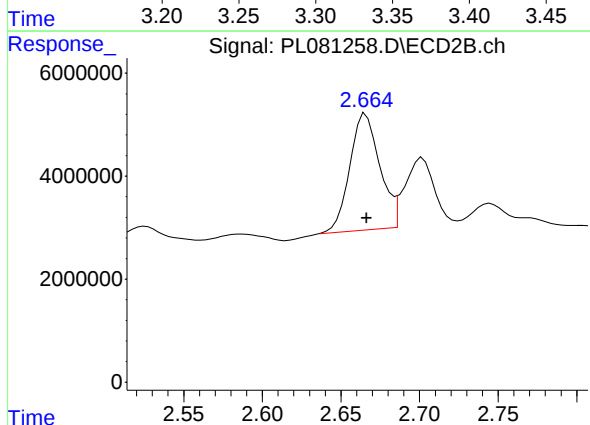


#1 Tetrachloro-m-xylene

R.T.: 2.666 min
Delta R.T.: 0.000 min
Response: 29958115
Conc: 14.80 ng/ml

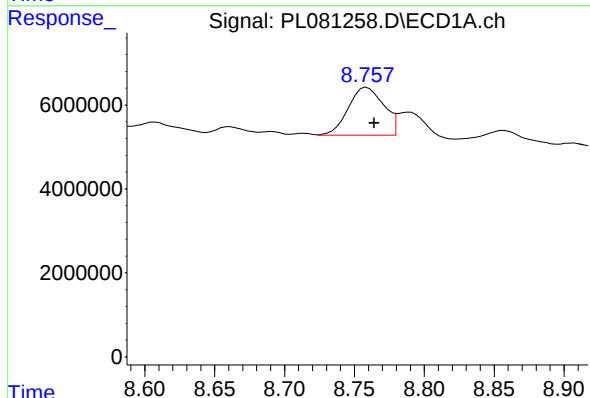

#28 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: -0.007 min
Response: 19999163
Conc: 13.12 ng/ml m

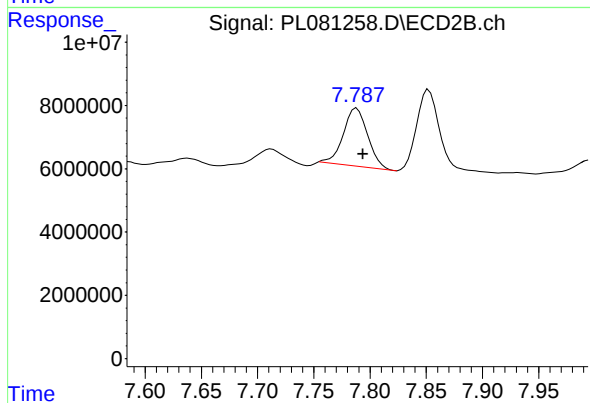

#28 Decachlorobiphenyl

R.T.: 7.788 min
Delta R.T.: -0.006 min
Response: 27698081
Conc: 14.46 ng/ml