

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030624\
 Data File : PL088425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2024 14:33
 Operator : AR\AJ
 Sample : P1682-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-04-03052024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/07/2024
 Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 00:23:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.643	2.853	30614956	16480835	11.146m	11.751m
28) SA Decachlor...	9.315	8.088	29040522	16482976	15.079m	12.945

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030624\
Data File : PL088425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2024 14:33
Operator : AR\AJ
Sample : P1682-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HR-04-03052024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/07/2024
Supervised By : Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:23:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

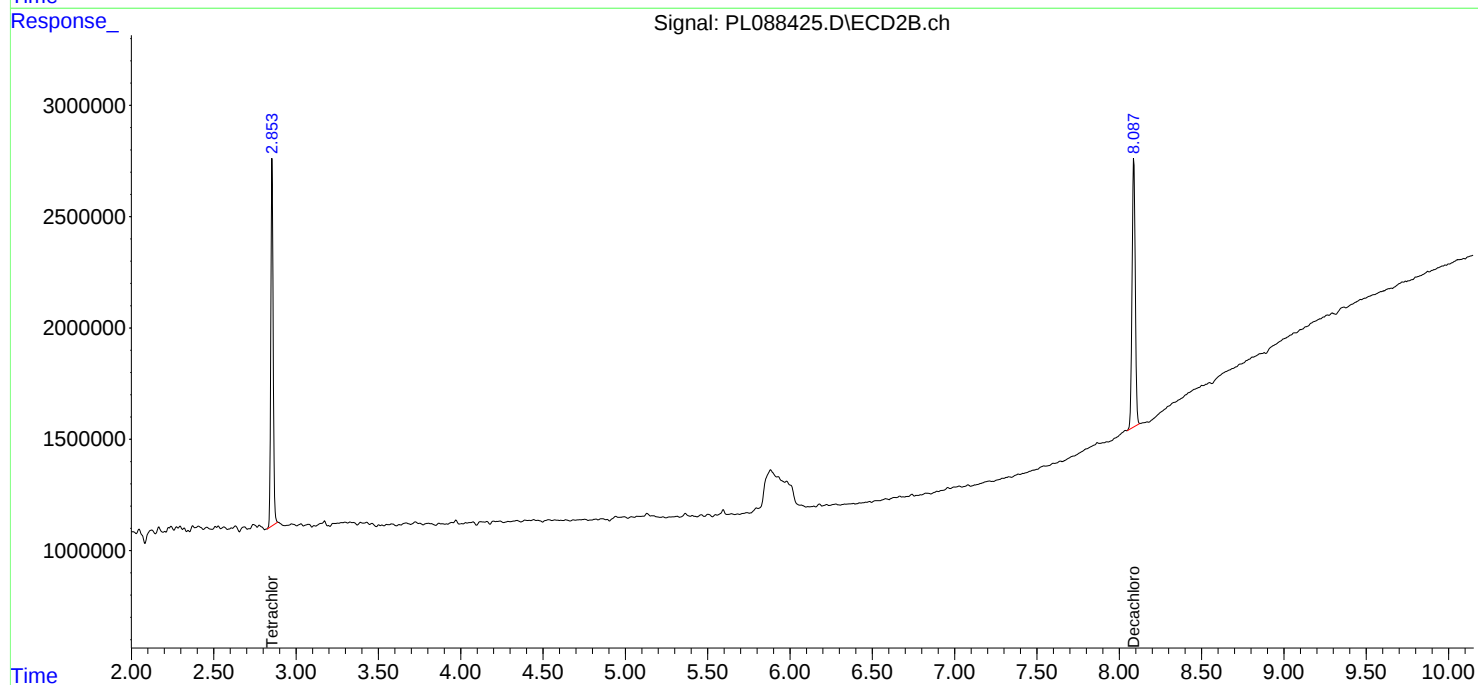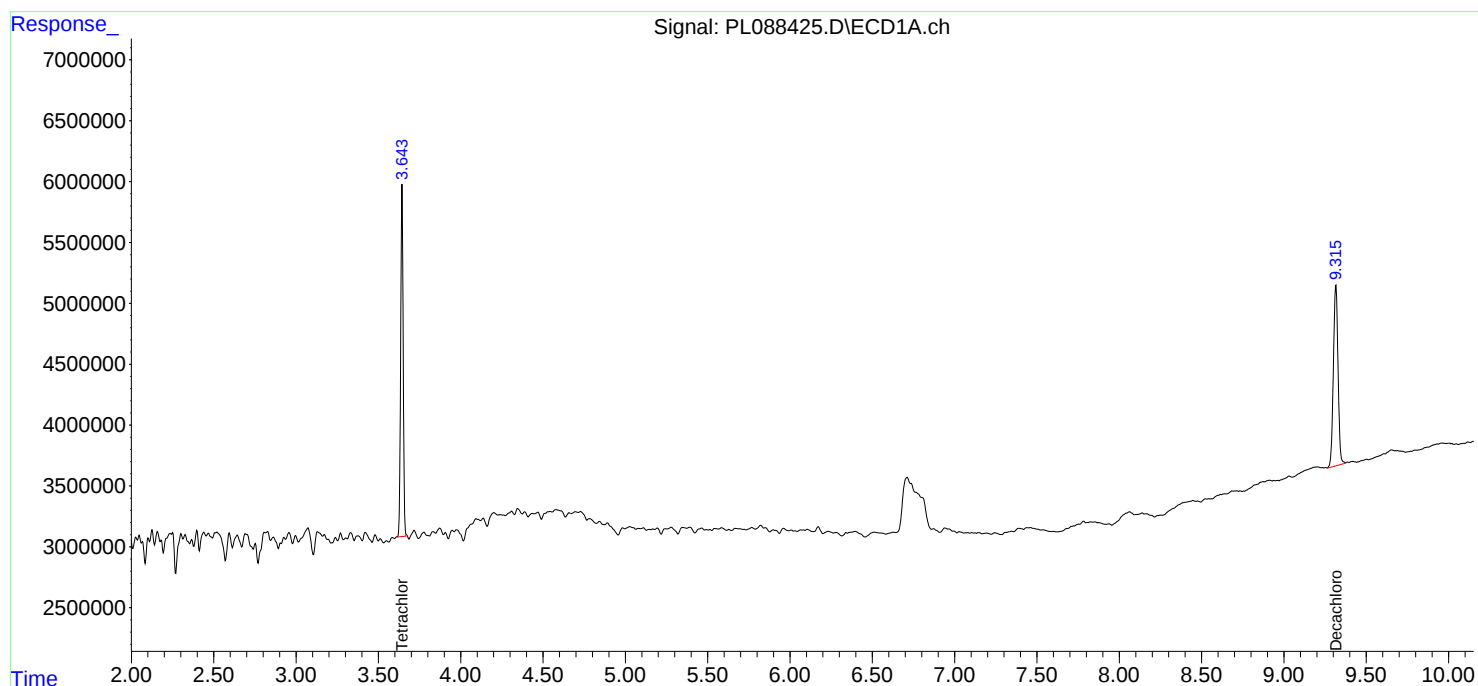

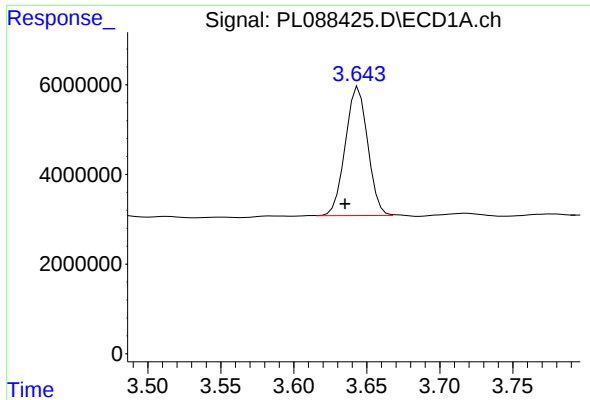


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: 0.008 min
Response: 30614956
Conc: 11.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-04-03052024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/07/2024
Supervised By :Ankita Jodhani 03/08/2024

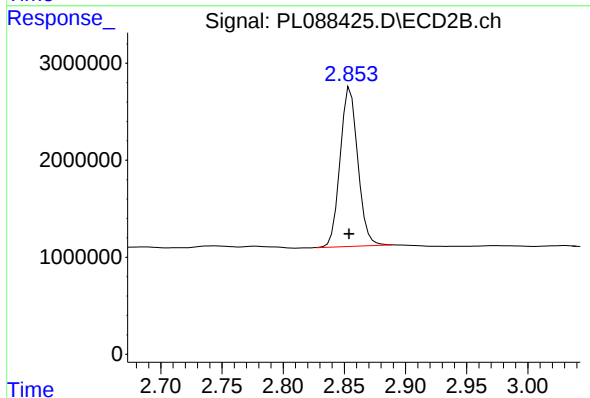


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: 0.000 min
Response: 16480835
Conc: 11.75 ng/ml m

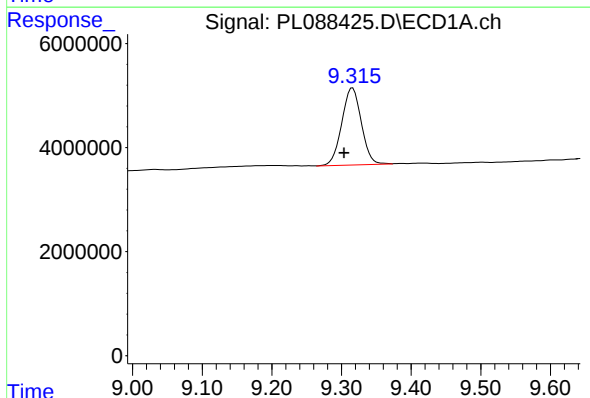

#28 Decachlorobiphenyl

R.T.: 9.315 min
Delta R.T.: 0.011 min
Response: 29040522
Conc: 15.08 ng/ml m

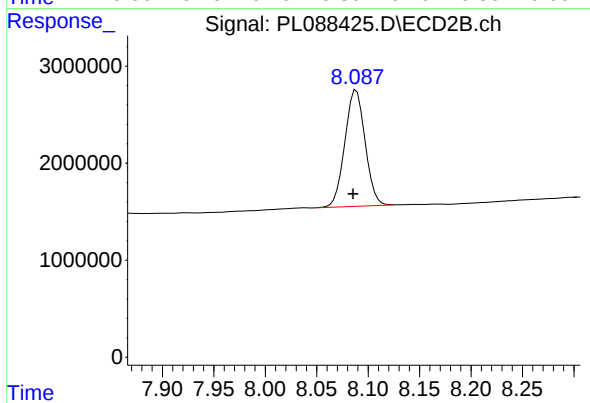

#28 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: 0.003 min
Response: 16482976
Conc: 12.95 ng/ml