

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030719\
 Data File : PL045570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 15:33
 Operator : AJ\SJ
 Sample : K1757-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6AB-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 03:40:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.363	3.981	54625386	18183602	7.941	8.491
28) SA Decachlor...	8.045	9.038	75648047	21856381	9.041	9.565
Target Compounds						
12) B 4,4'-DDE	5.483	6.317	10664862	3544836	1.215	1.518



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030719\
Data File : PL045570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 15:33
Operator : AJ\SJ
Sample : K1757-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6AB-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 03:40:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

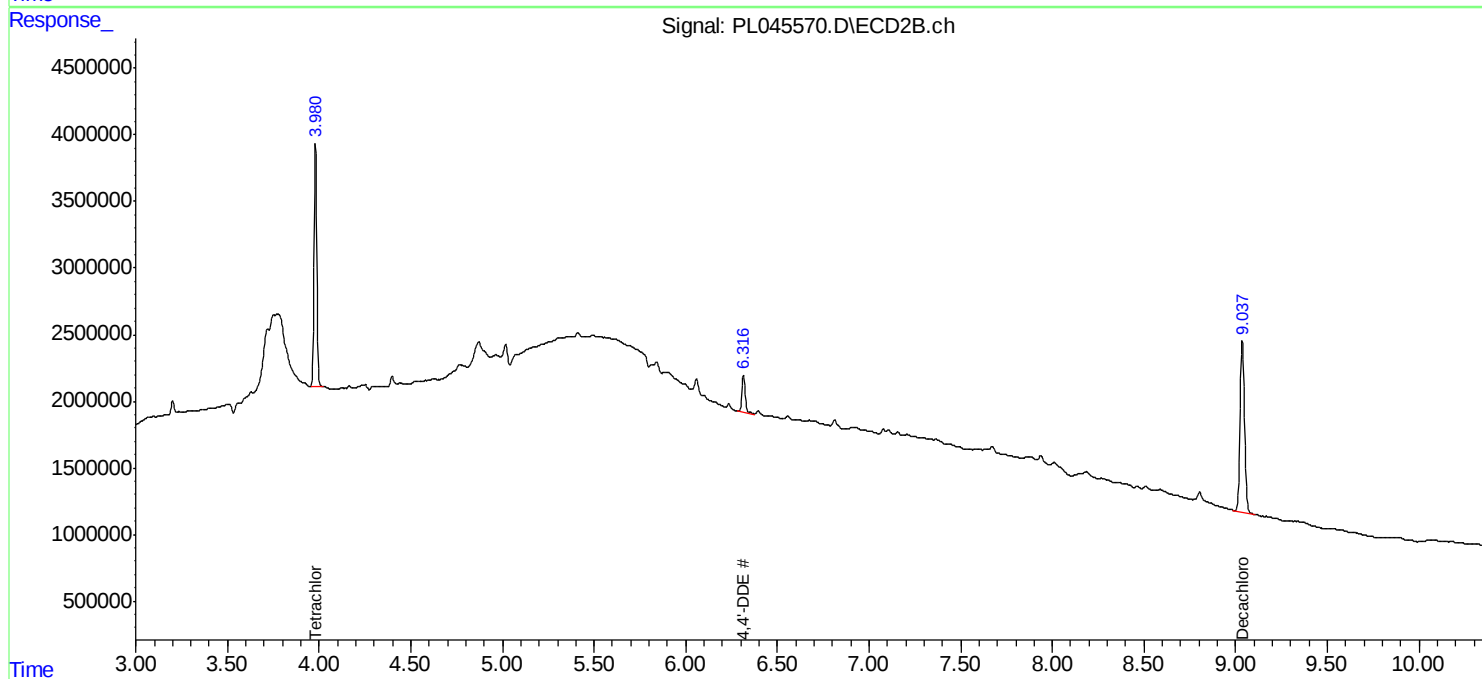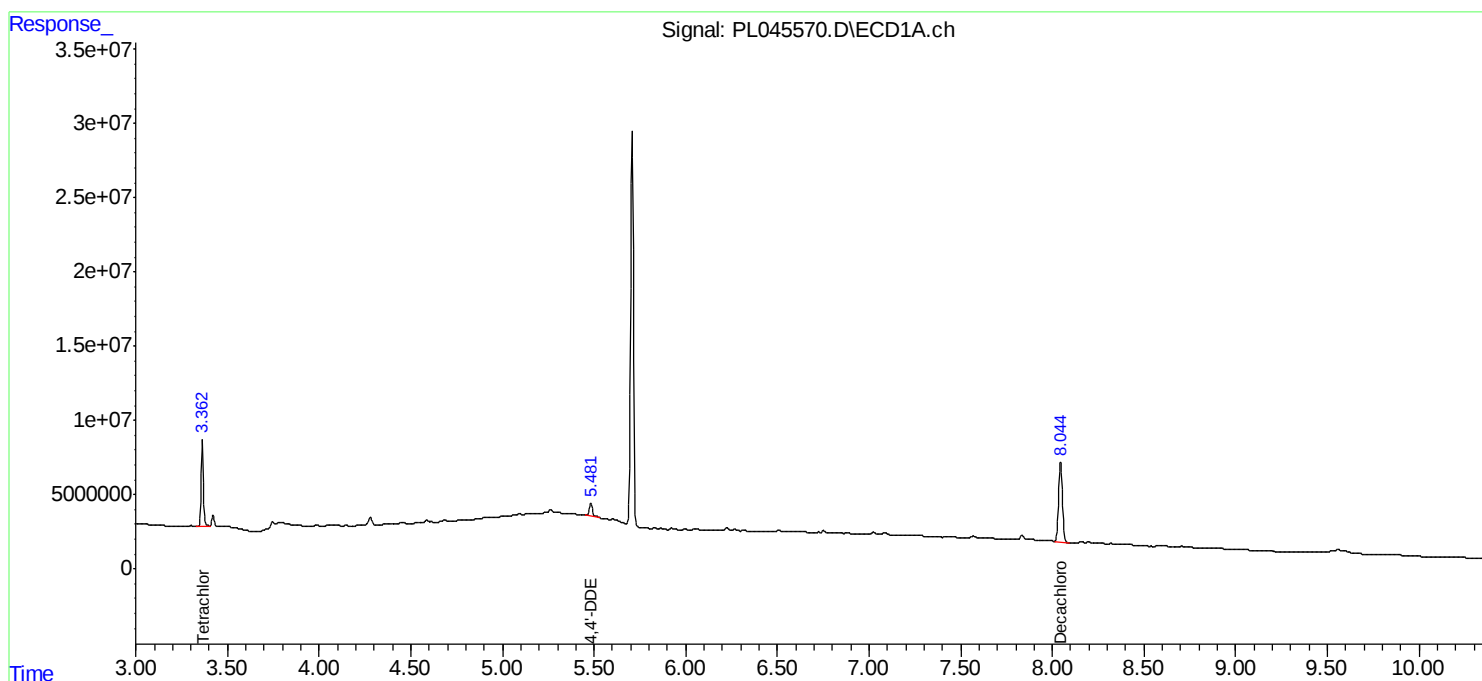


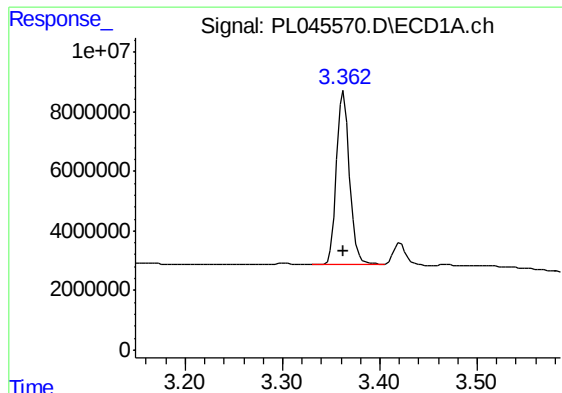

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 54625386
Conc: 7.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6AB-S

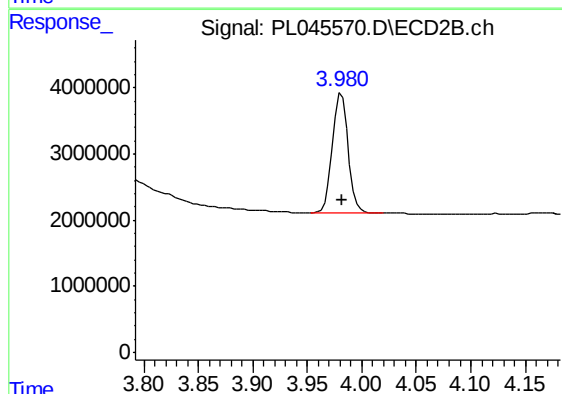


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 18183602
Conc: 8.49 ng/ml

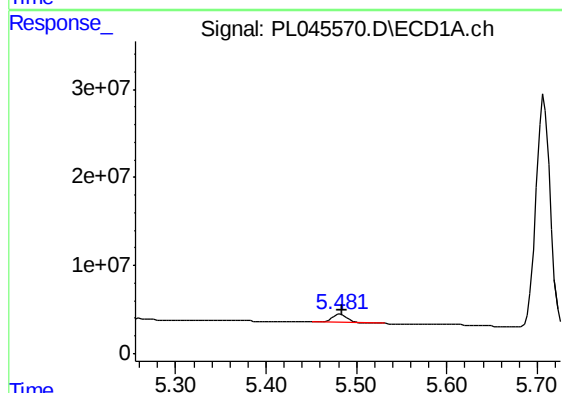


#12 4,4'-DDE

R.T.: 5.483 min
Delta R.T.: -0.002 min
Response: 10664862
Conc: 1.21 ng/ml

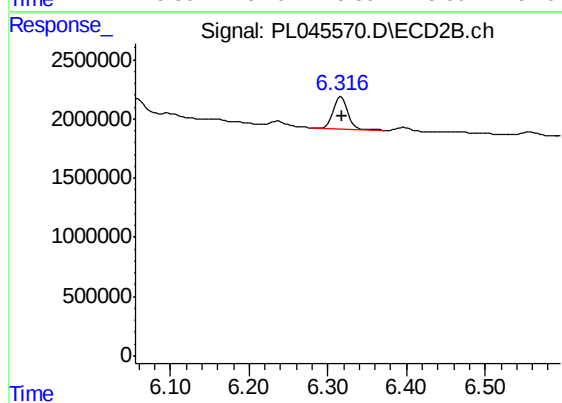

#12 4,4'-DDE


R.T.: 6.317 min
Delta R.T.: -0.001 min
Response: 3544836
Conc: 1.52 ng/ml

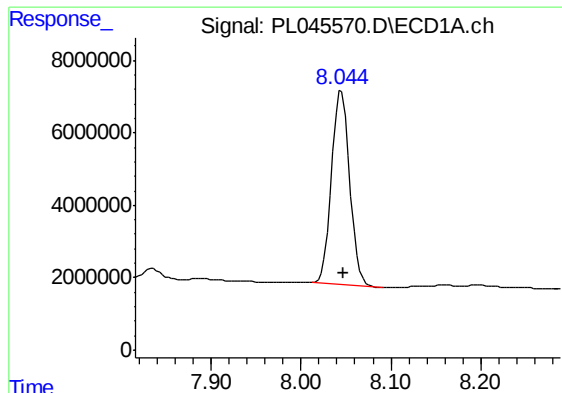

#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: -0.002 min
Response: 75648047
Conc: 9.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6AB-S

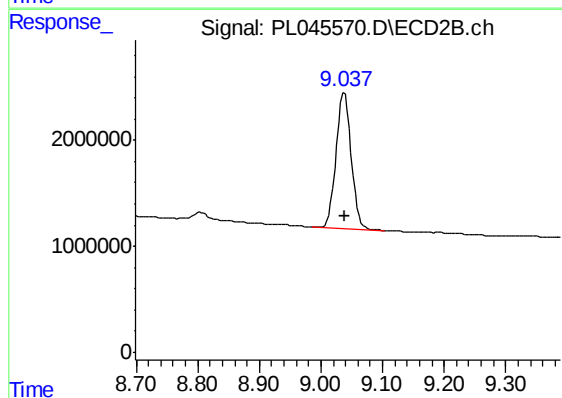

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: 0.000 min
Response: 21856381
Conc: 9.57 ng/ml