

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030719\
 Data File : PL045573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2019 16:22
 Operator : AJ\SJ
 Sample : K1757-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6AB-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 03:41:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.367	3.981	49841933	16344404	7.245	7.632
28) SA Decachlor...	8.049	9.041	48008229	13266638	5.737	5.806
Target Compounds						
6) B beta-BHC	0.000	4.853f	0	1528379	N.D.	1.203 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030719\
Data File : PL045573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2019 16:22
Operator : AJ\SJ
Sample : K1757-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6AB-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 03:41:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

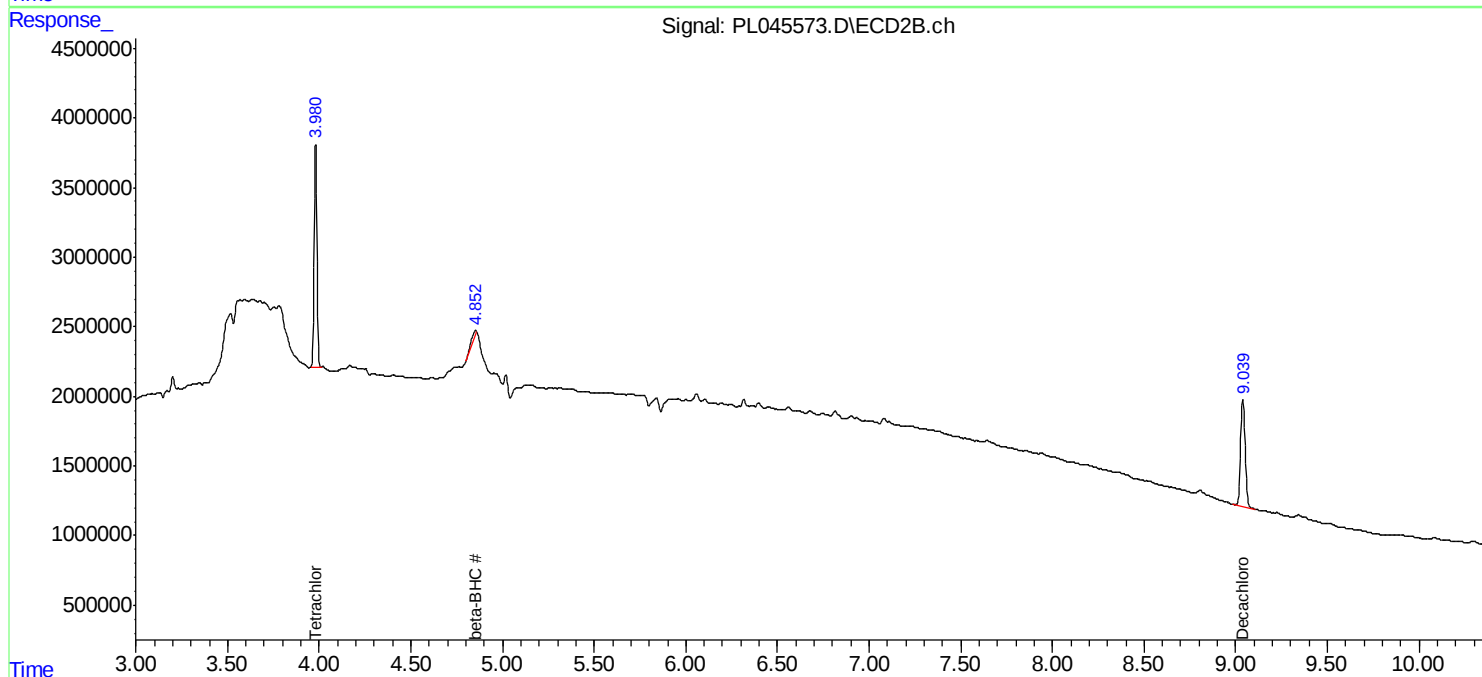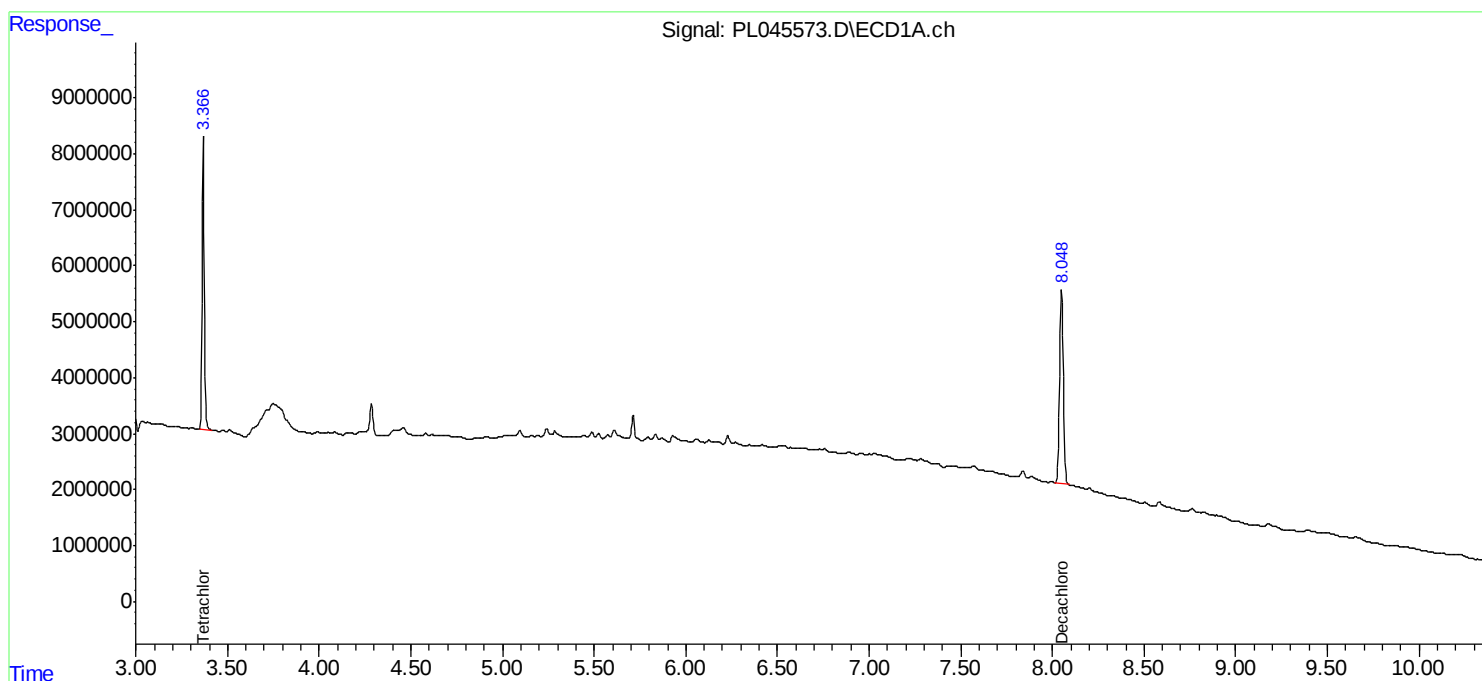


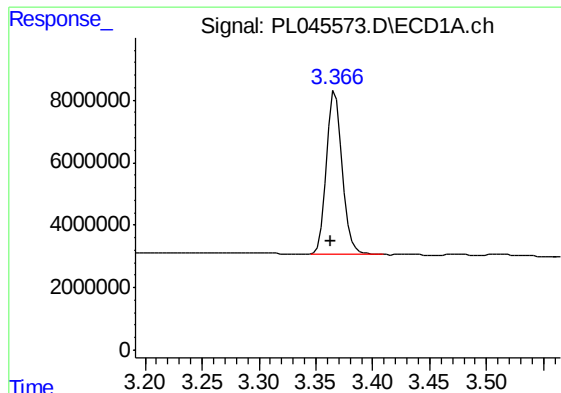

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.004 min
Response: 49841933
Conc: 7.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6AB-D

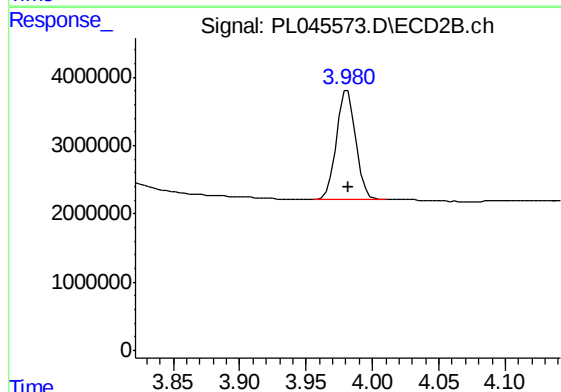


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 16344404
Conc: 7.63 ng/ml

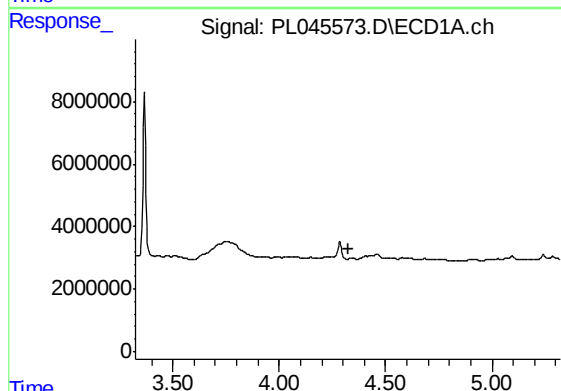


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.324 min
Response: 0
Conc: N.D.

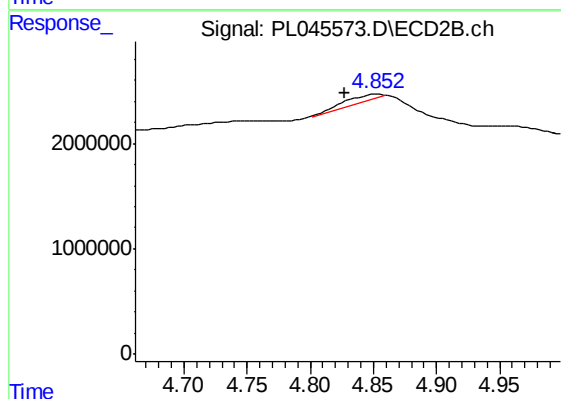

#6 beta-BHC


R.T.: 4.853 min
Delta R.T.: 0.025 min
Response: 1528379
Conc: 1.20 ng/ml

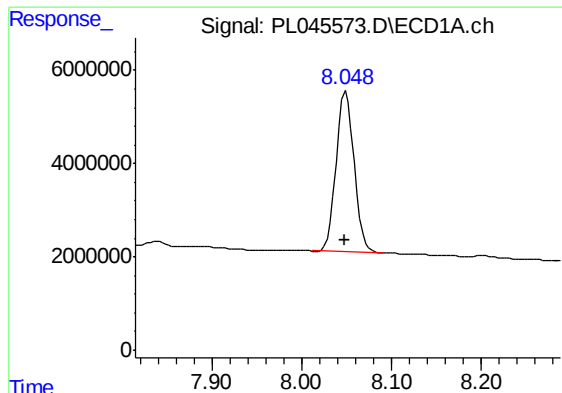

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.002 min
Response: 48008229
Conc: 5.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6AB-D

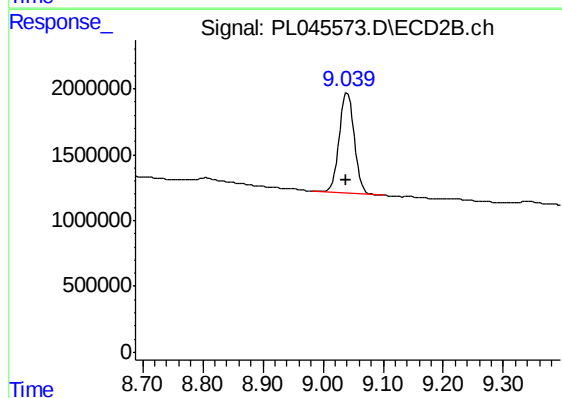

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.002 min
Response: 13266638
Conc: 5.81 ng/ml