

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030722\
 Data File : PL073181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2022 15:43
 Operator : AR\AJ
 Sample : N1733-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 04:51:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.492	5073966	24383405	14.754	15.619
27)	SA Decachlor...	10.425	11.331	14801901	48775795	30.785	30.177
Target Compounds							
2)	A alpha-BHC	0.000	6.028	0	428441	N.D.	0.222
4)	MA Heptachlor	0.000	7.104	0	179277	N.D.	<MDL
6)	B beta-BHC	0.000	6.668	0	1361563	N.D.	1.392
7)	B delta-BHC	0.000	6.944	0	3683781	N.D.	1.905
8)	B Heptachlo...	0.000	7.966f	0	82129	N.D.	<MDL
10)	B trans-Chl...	0.000	8.195	0	866016	N.D.	0.496
15)	B Endosulfa...	8.323f	0.000	1342346	0	2.865	N.D. #
16)	A 4,4'-DDD	0.000	8.940f	0	5406015	N.D.	4.116
20)	A Methoxychlor	0.000	9.782	0	2236084	N.D.	2.920
26)	Toxaphene-5	0.000	9.782f	0	2236084	N.D.	131.740


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030722\
Data File : PL073181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2022 15:43
Operator : AR\AJ
Sample : N1733-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 04:51:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

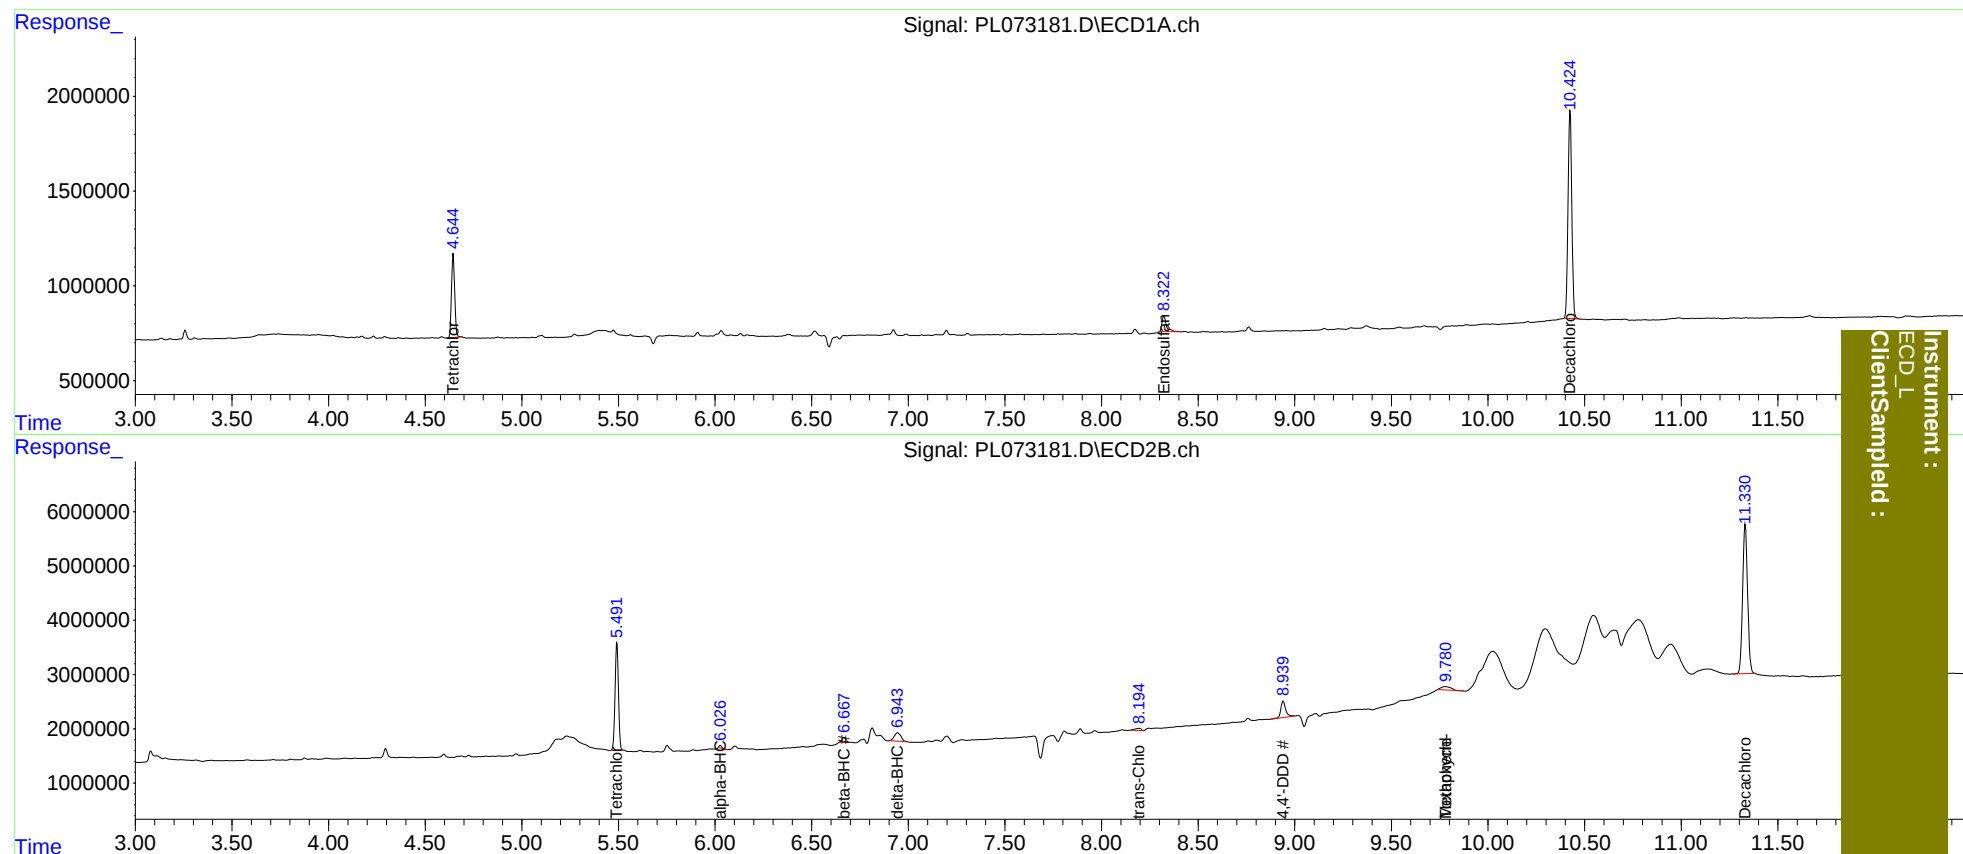


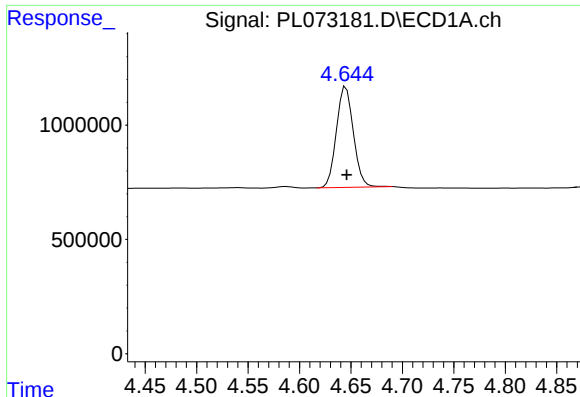

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 5073966
Conc: 14.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

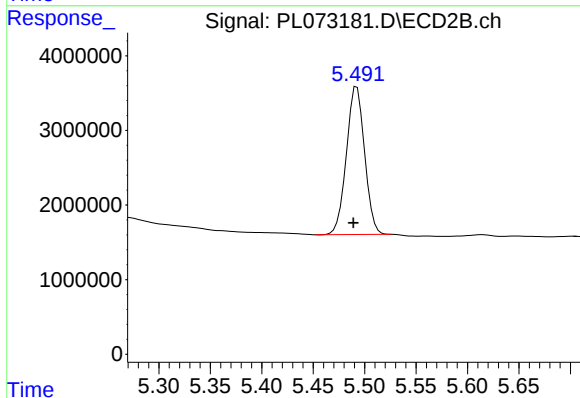


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.003 min
Response: 24383405
Conc: 15.62 ng/ml

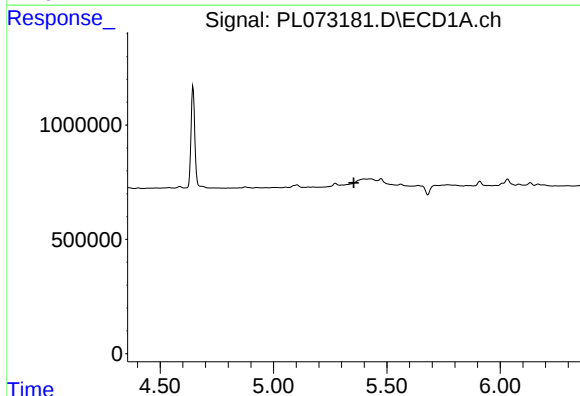


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

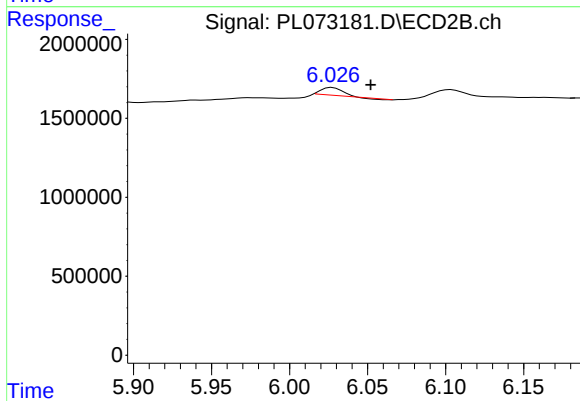

#2 alpha-BHC


R.T.: 6.028 min
Delta R.T.: -0.024 min
Response: 428441
Conc: 0.22 ng/ml

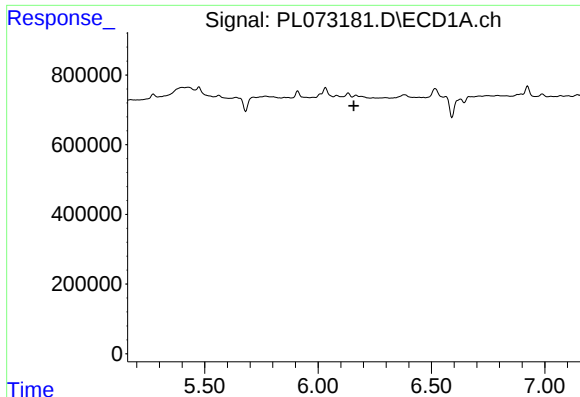

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

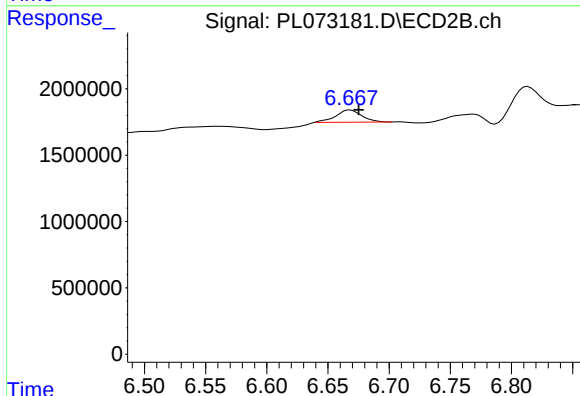


#6 beta-BHC

R.T.: 6.668 min
Delta R.T.: -0.007 min
Response: 1361563
Conc: 1.39 ng/ml

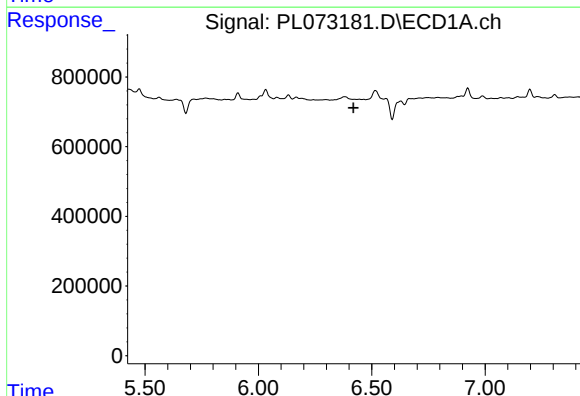


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

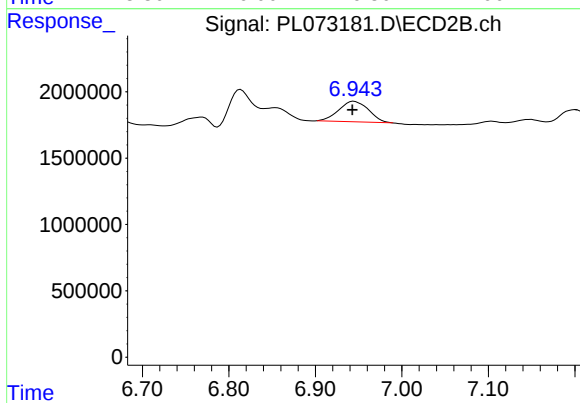

#7 delta-BHC


R.T.: 6.944 min
Delta R.T.: 0.002 min
Response: 3683781
Conc: 1.91 ng/ml

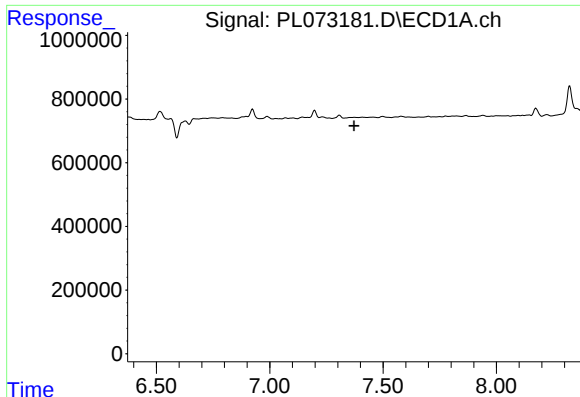

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

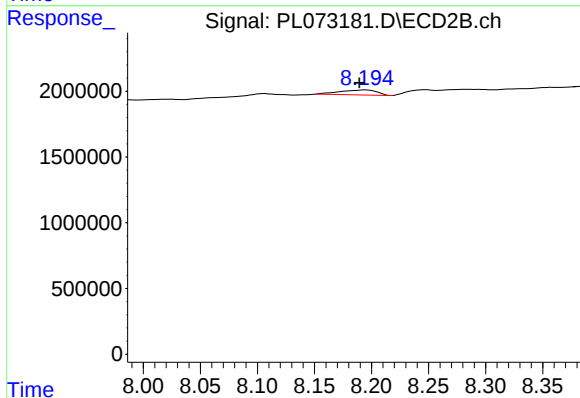


#10 trans-Chlordane

R.T.: 8.195 min
Delta R.T.: 0.005 min
Response: 866016
Conc: 0.50 ng/ml

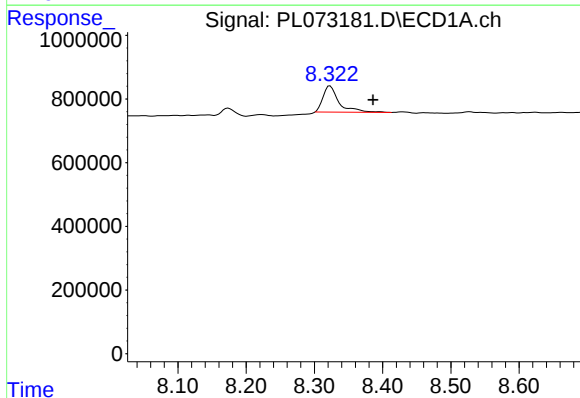


#15 Endosulfan II

R.T.: 8.323 min
Delta R.T.: -0.063 min
Response: 1342346
Conc: 2.86 ng/ml

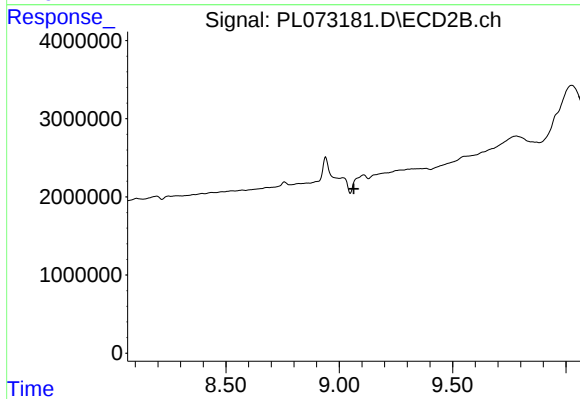

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 9.064 min
Response: 0
Conc: N.D.

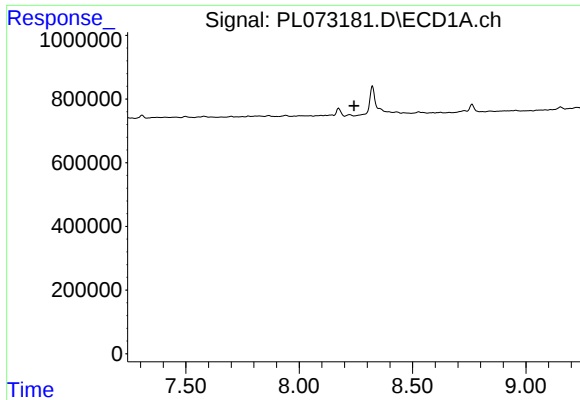

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

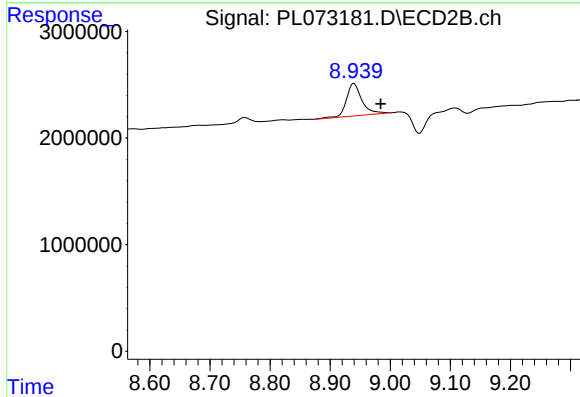


#16 4,4'-DDD

R.T.: 8.940 min
Delta R.T.: -0.044 min
Response: 5406015
Conc: 4.12 ng/ml

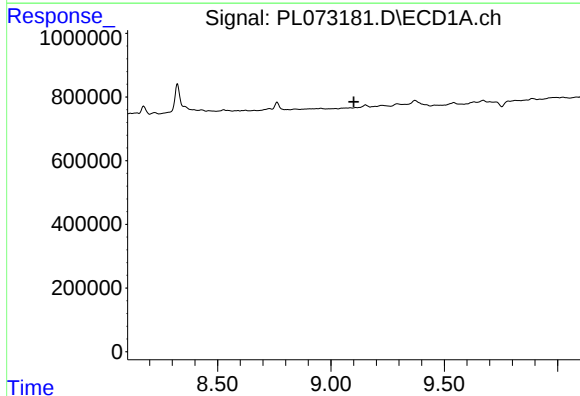


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

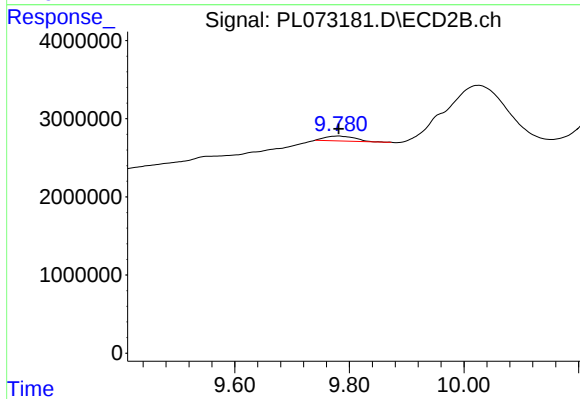

#20 Methoxychlor


R.T.: 9.782 min
Delta R.T.: 0.000 min
Response: 2236084
Conc: 2.92 ng/ml

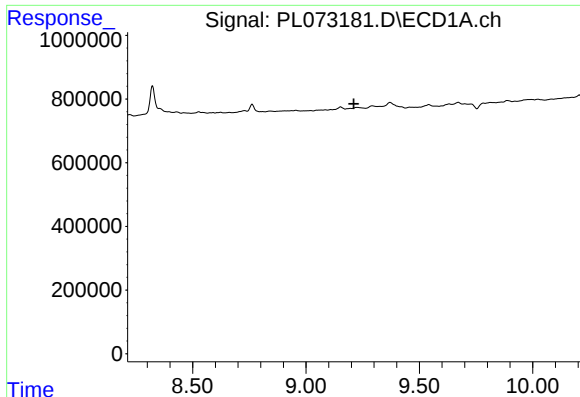

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 9.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

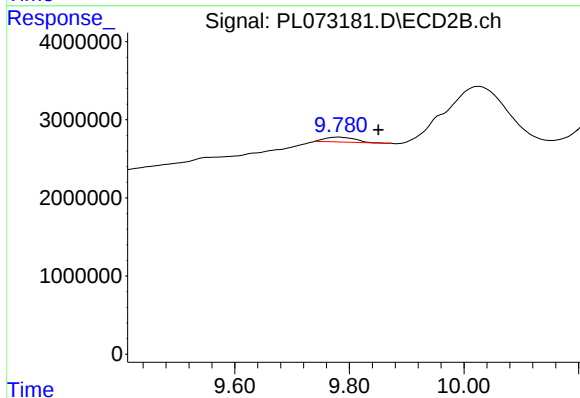


#26 Toxaphene-5

R.T.: 9.782 min
Delta R.T.: -0.069 min
Response: 2236084
Conc: 131.74 ng/ml

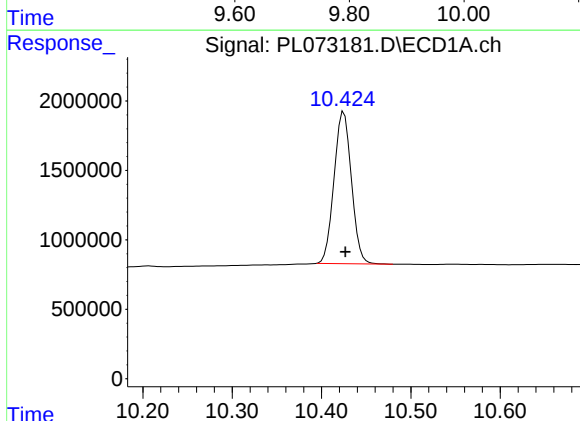

#27 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: -0.002 min
Response: 14801901
Conc: 30.78 ng/ml

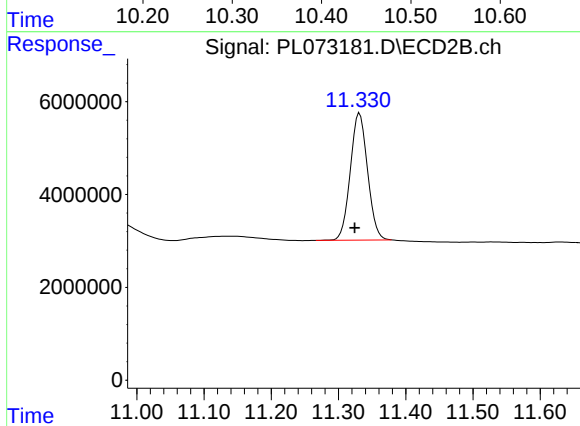

#27 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.007 min
Response: 48775795
Conc: 30.18 ng/ml