

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030722\
 Data File : PL073191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2022 18:41
 Operator : AR\AJ
 Sample : N1733-27
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 04:53:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.492	6197235	31108338	18.021	19.927
27)	SA Decachlor...	10.425	11.333	15145848	50759474	31.500	31.404
Target Compounds							
2)	A alpha-BHC	0.000	6.027f	0	584056	N.D.	0.302
4)	MA Heptachlor	0.000	7.104	0	259376	N.D.	0.128
5)	MB Aldrin	6.517	0.000	484298	0	1.071	N.D. #
6)	B beta-BHC	0.000	6.668	0	1551594	N.D.	1.586
7)	B delta-BHC	0.000	6.944	0	4238223	N.D.	2.192
8)	B Heptachlo...	0.000	7.926	0	132015	N.D.	<MDL
15)	B Endosulfa...	8.323f	9.107f	1019650	-2216973	2.176	N.D. #
16)	A 4,4'-DDD	0.000	8.940f	0	6130652	N.D.	4.668
20)	A Methoxychlor	0.000	9.791	0	438444	N.D.	0.572
26)	Toxaphene-5	0.000	9.868	0	81321	N.D.	4.791


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030722\
Data File : PL073191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2022 18:41
Operator : AR\AJ
Sample : N1733-27
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 04:53:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

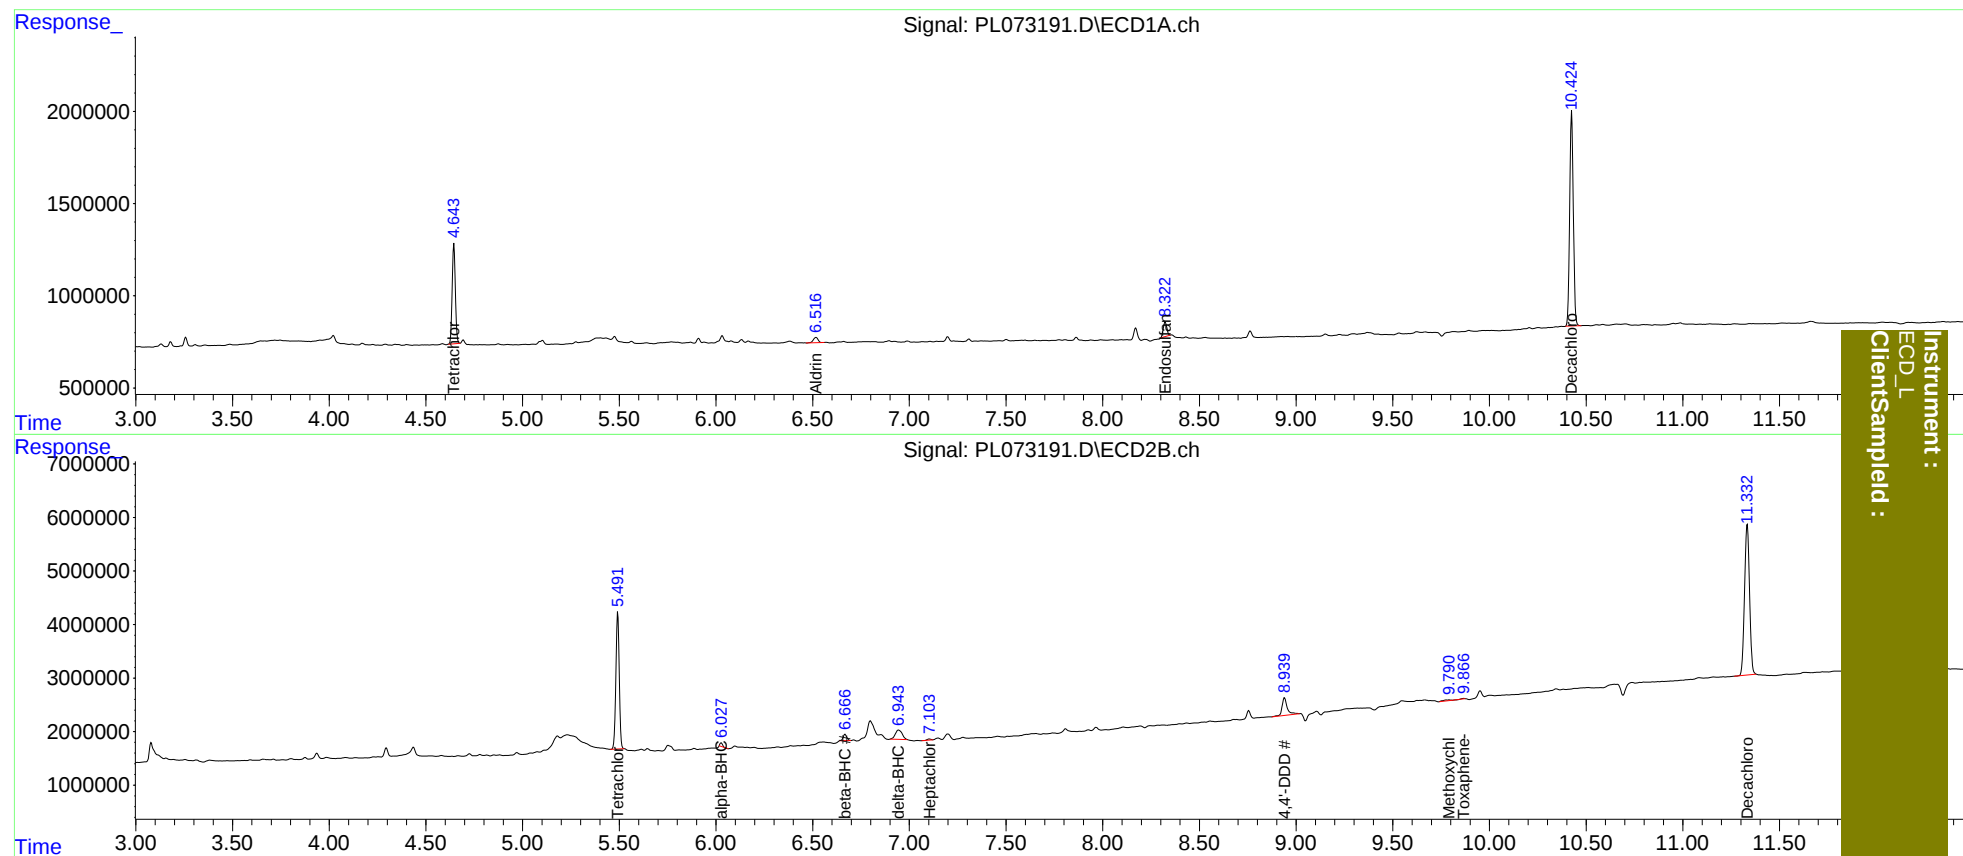


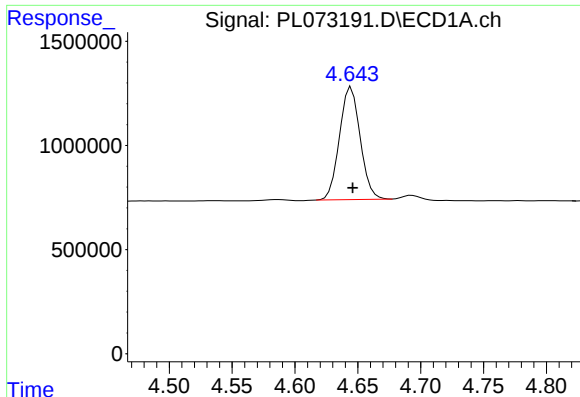

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: -0.001 min
Response: 6197235
Conc: 18.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

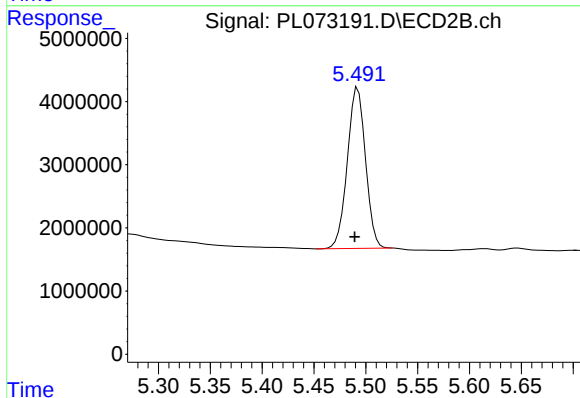


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.003 min
Response: 31108338
Conc: 19.93 ng/ml

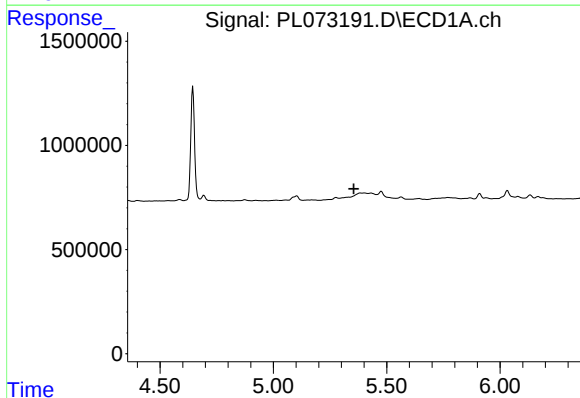


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

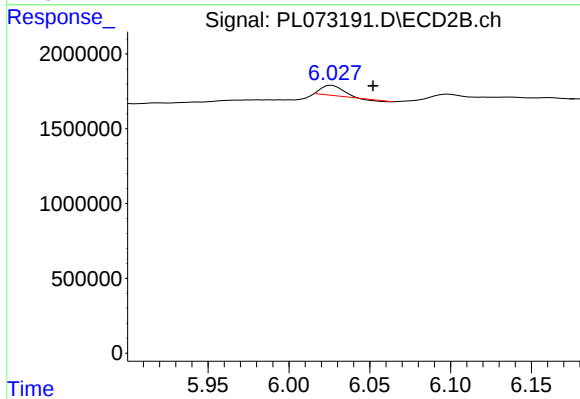

#2 alpha-BHC


R.T.: 6.027 min
Delta R.T.: -0.025 min
Response: 584056
Conc: 0.30 ng/ml

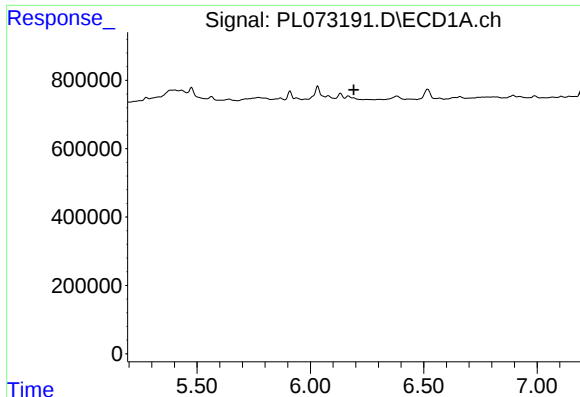

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

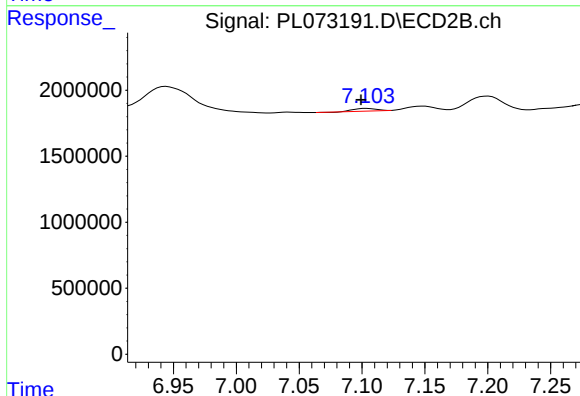


#4 Heptachlor

R.T.: 7.104 min
Delta R.T.: 0.005 min
Response: 259376
Conc: 0.13 ng/ml

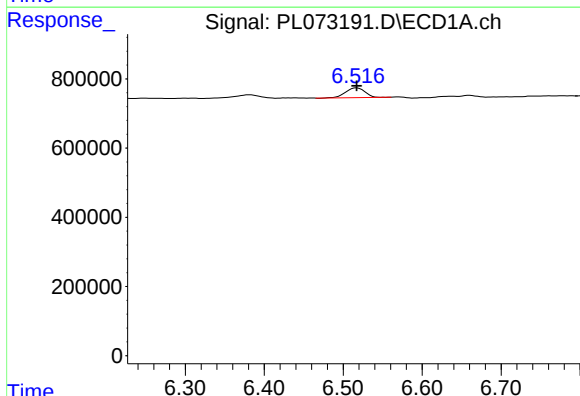


#5 Aldrin

R.T.: 6.517 min
Delta R.T.: 0.000 min
Response: 484298
Conc: 1.07 ng/ml

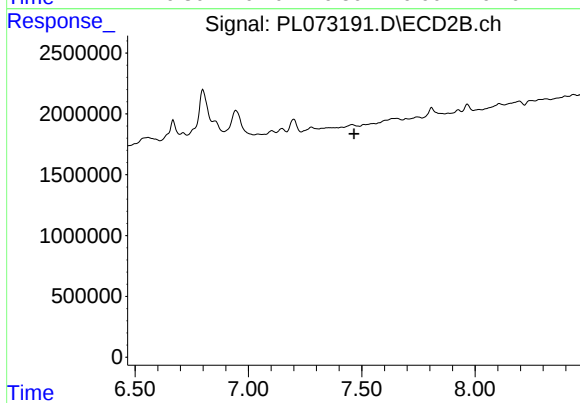

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 7.466 min
Response: 0
Conc: N.D.

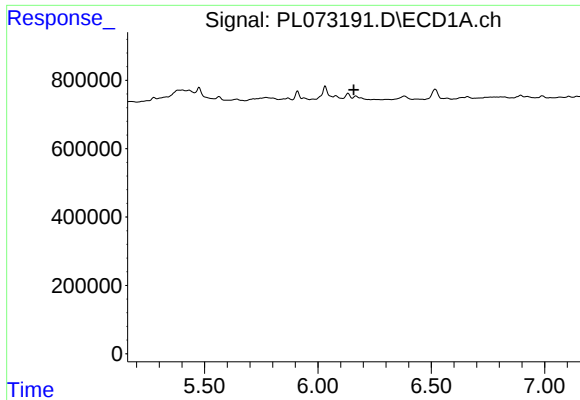

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

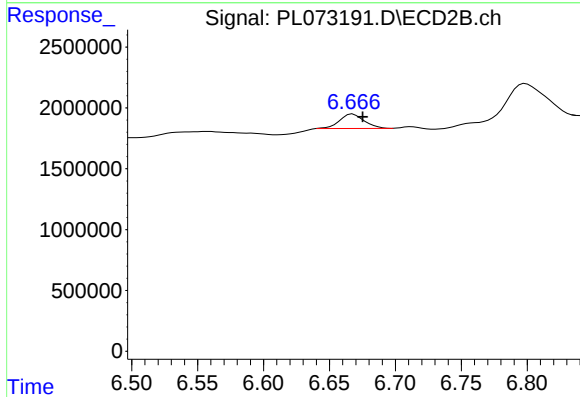


#6 beta-BHC

R.T.: 6.668 min
Delta R.T.: -0.008 min
Response: 1551594
Conc: 1.59 ng/ml

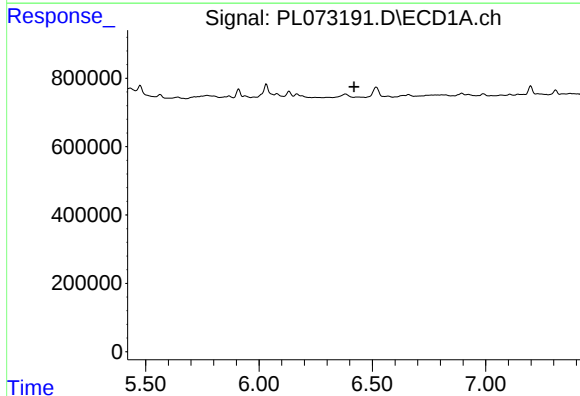


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

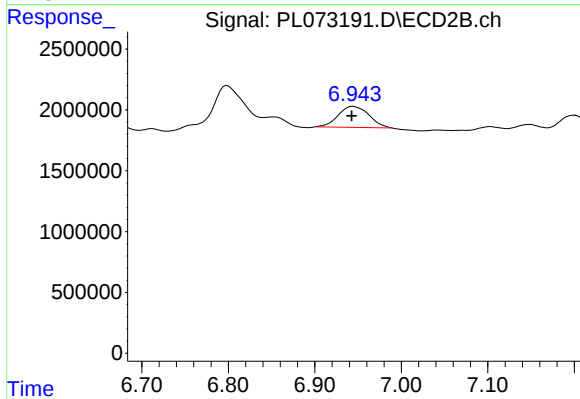

#7 delta-BHC


R.T.: 6.944 min
Delta R.T.: 0.002 min
Response: 4238223
Conc: 2.19 ng/ml

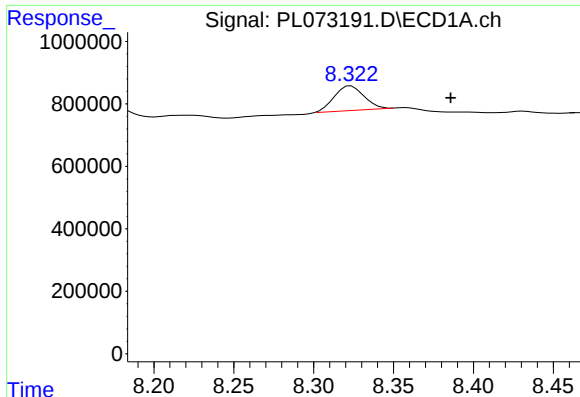

#15 Endosulfan II


R.T.: 8.323 min
Delta R.T.: -0.062 min
Response: 1019650
Conc: 2.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

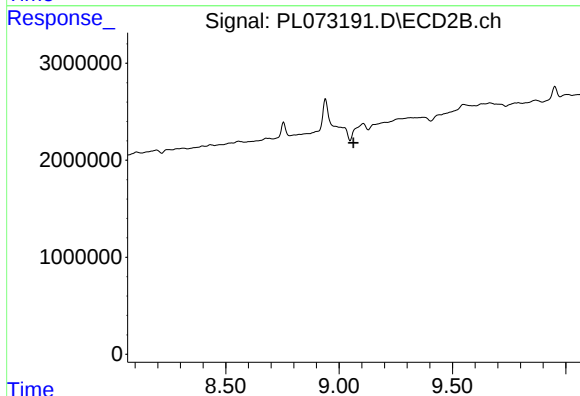


#15 Endosulfan II

R.T.: 9.107 min
Delta R.T.: 0.043 min
Response: -2216973
Conc: N.D.

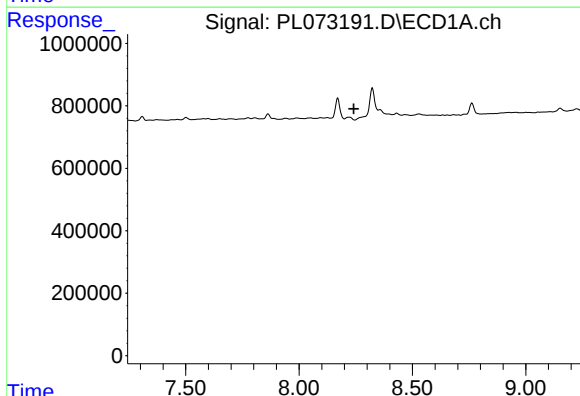


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

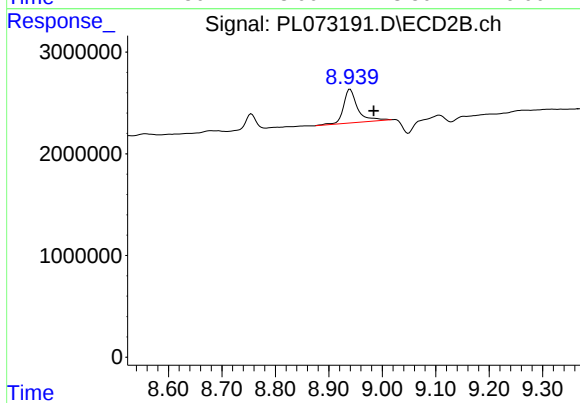

#16 4,4'-DDD


R.T.: 8.940 min
Delta R.T.: -0.044 min
Response: 6130652
Conc: 4.67 ng/ml

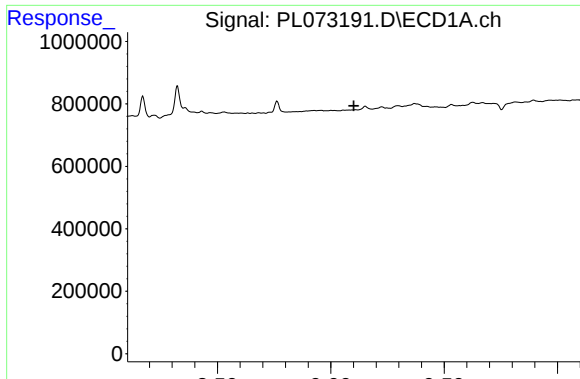

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

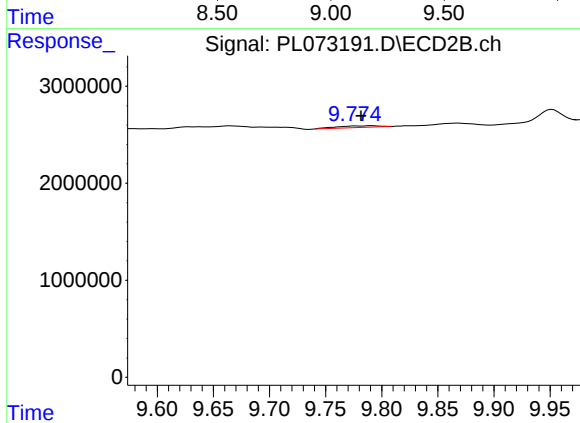


#20 Methoxychlor

R.T.: 9.791 min
Delta R.T.: 0.010 min
Response: 438444
Conc: 0.57 ng/ml

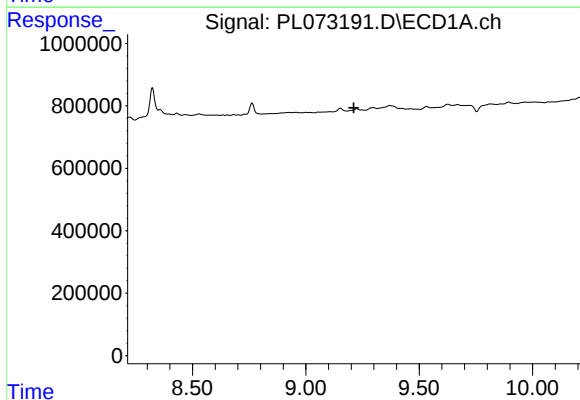


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 9.212 min
Response: 0
Conc: N.D.

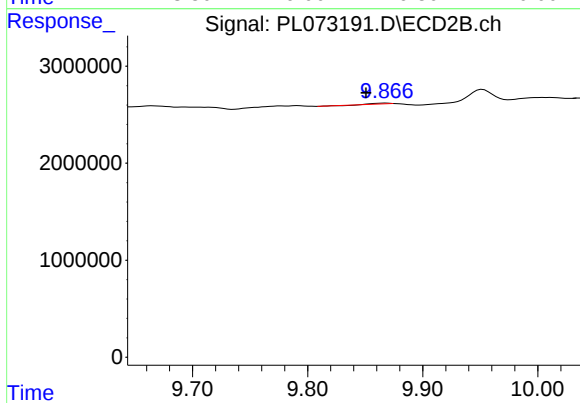

#26 Toxaphene-5


R.T.: 9.868 min
Delta R.T.: 0.017 min
Response: 81321
Conc: 4.79 ng/ml

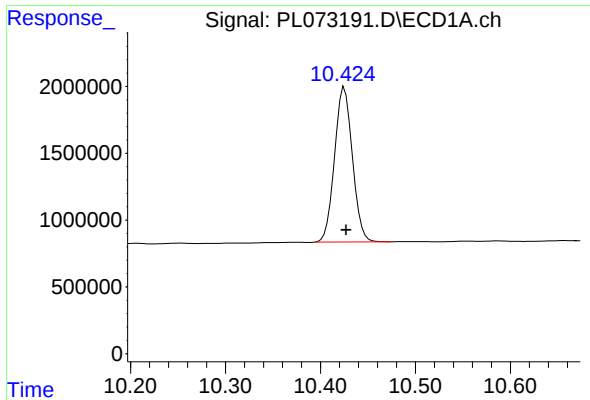

#27 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: -0.002 min
Response: 15145848
Conc: 31.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

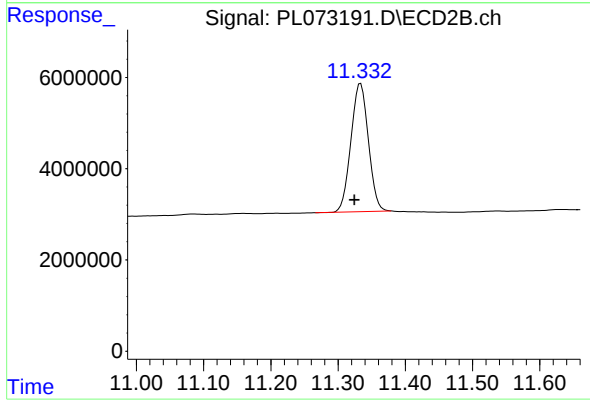

#27 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.009 min
Response: 50759474
Conc: 31.40 ng/ml