

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030722\
 Data File : PL073196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2022 20:04
 Operator : AR\AJ
 Sample : PIBLK242
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 04:55:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.645	5.492	7320050	36066778	21.286	23.103
27)	SA Decachlor...	10.426	11.334	22790207	77518775	47.399	47.960
Target Compounds							
6)	B beta-BHC	0.000	6.678	0	1174817	N.D.	1.201
7)	B delta-BHC	0.000	6.958	0	2663664	N.D.	1.378
8)	B Heptachlo...	0.000	7.928	0	251703	N.D.	0.148
10)	B trans-Chl...	0.000	8.199	0	183271	N.D.	0.105
12)	B 4,4'-DDE	0.000	8.519f	0	335420	N.D.	0.222
15)	B Endosulfa...	8.323f	0.000	1386684	0	2.959	N.D. #
16)	A 4,4'-DDD	0.000	8.942f	0	6797648	N.D.	5.176
20)	A Methoxychlor	0.000	9.715f	0	399884	N.D.	0.522
22)	Toxaphene-1	0.000	8.519	0	335420	N.D.	34.865

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073196\
Data File : PL073196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2022 20:04
Operator : AR\AJ
Sample : PIBLK242
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 04:55:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

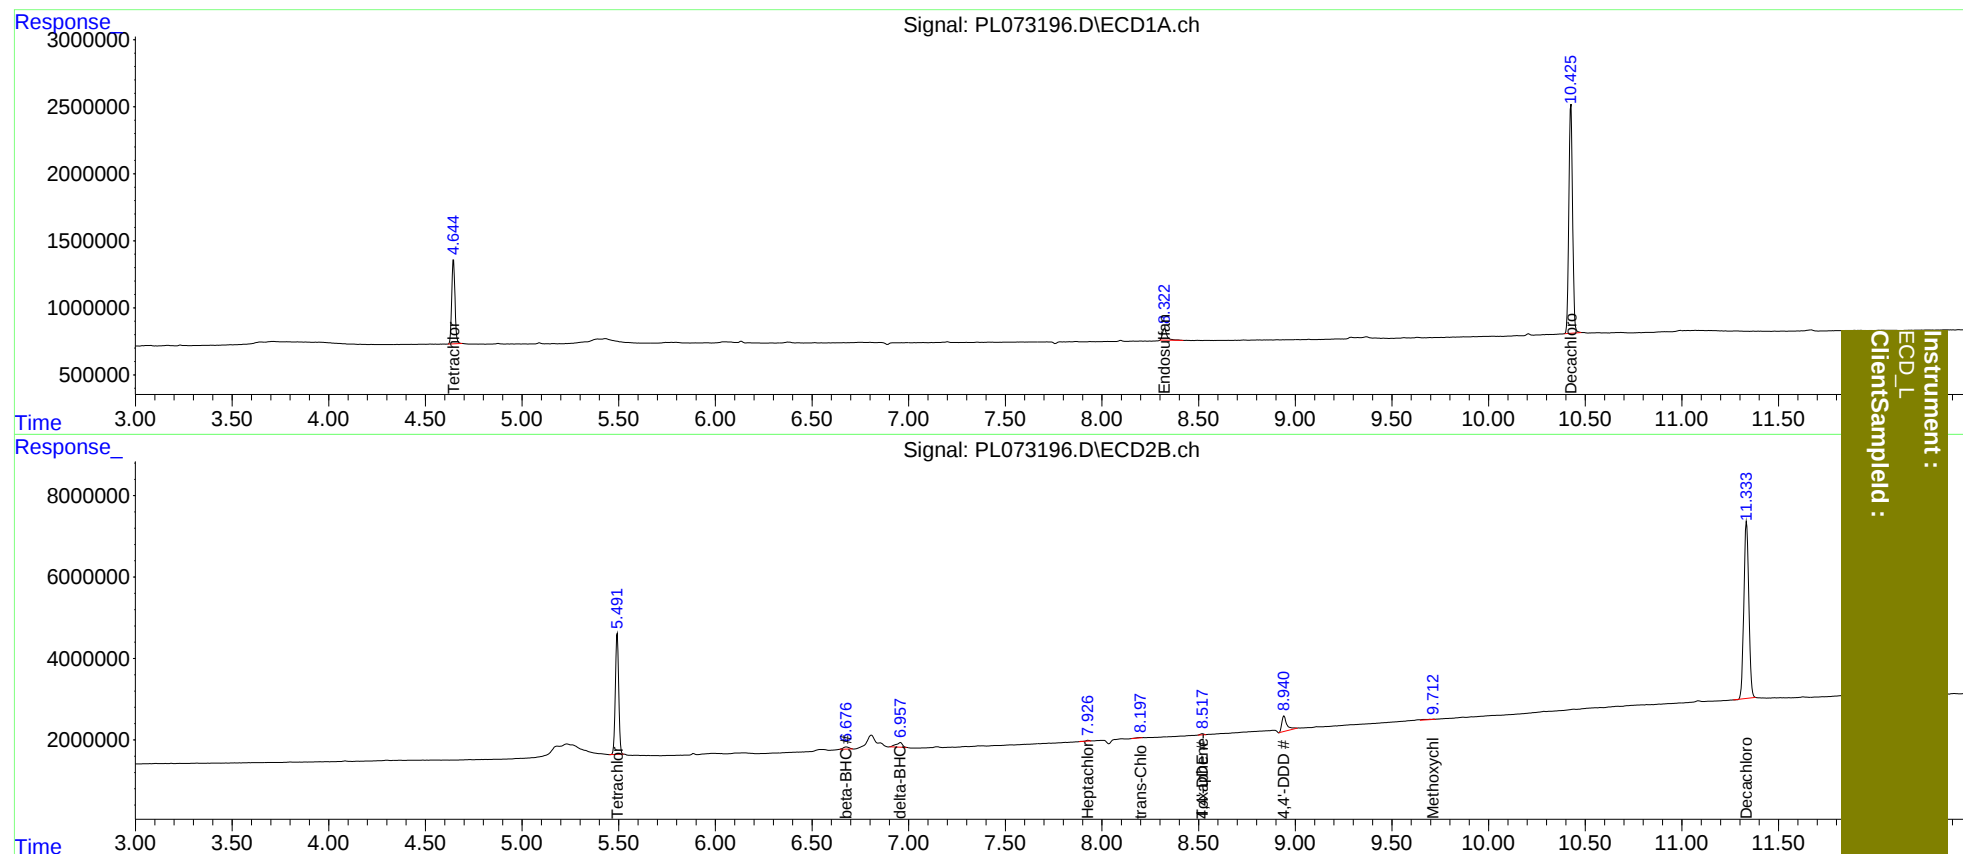


Instrument :
ECD_L
ClientSampled :
PIBLK242

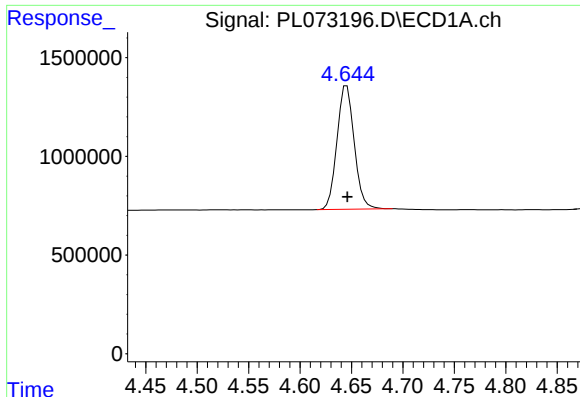

#1 Tetrachloro-m-xylene


R.T.: 4.645 min
Delta R.T.: 0.000 min
Response: 7320050
Conc: 21.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

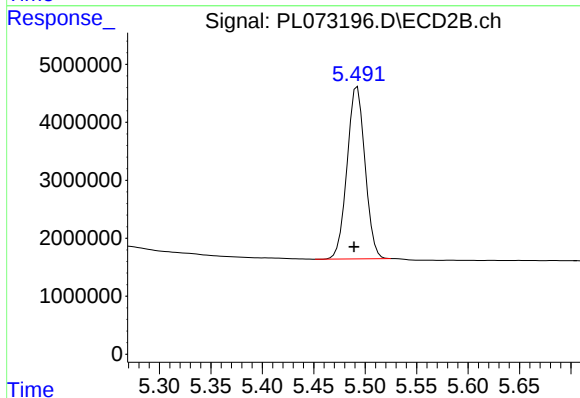


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.003 min
Response: 36066778
Conc: 23.10 ng/ml

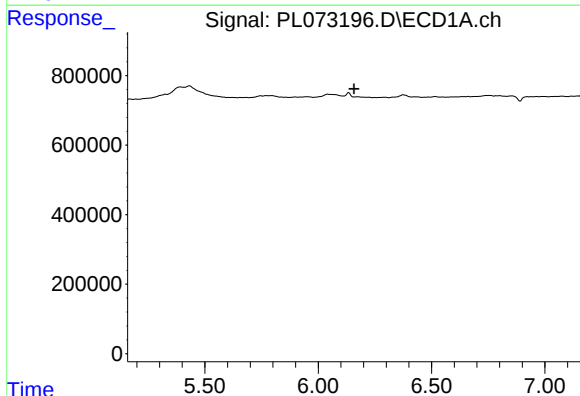


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

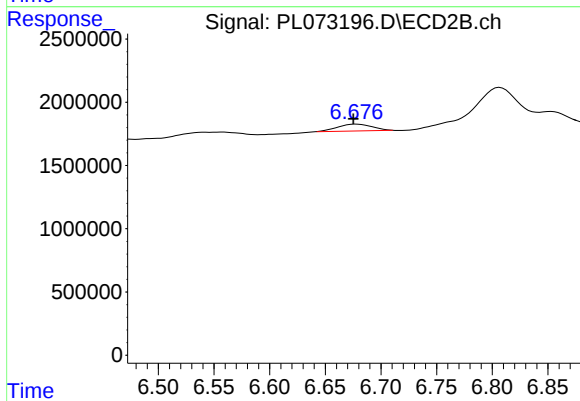

#6 beta-BHC


R.T.: 6.678 min
Delta R.T.: 0.002 min
Response: 1174817
Conc: 1.20 ng/ml

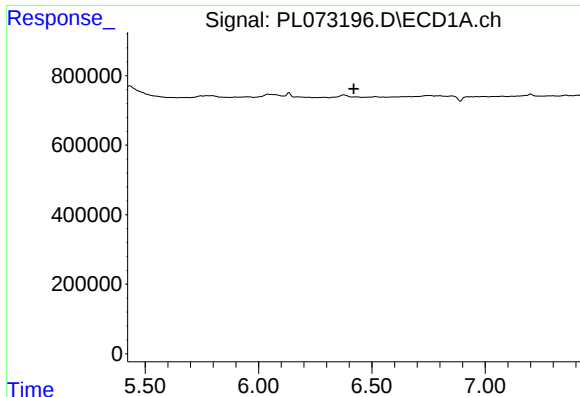

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

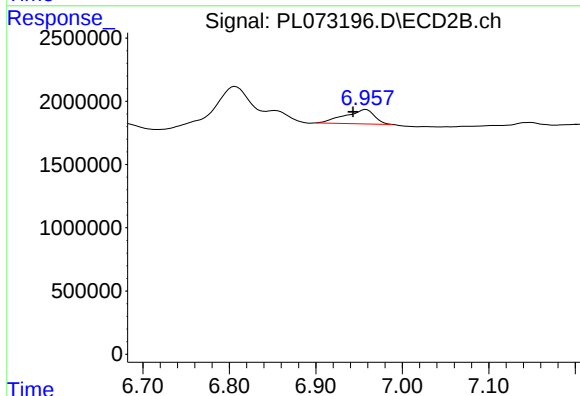


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.015 min
Response: 2663664
Conc: 1.38 ng/ml

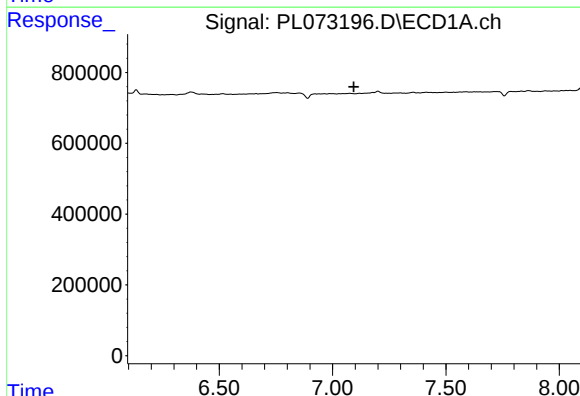


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.094 min
Response: 0
Conc: N.D.

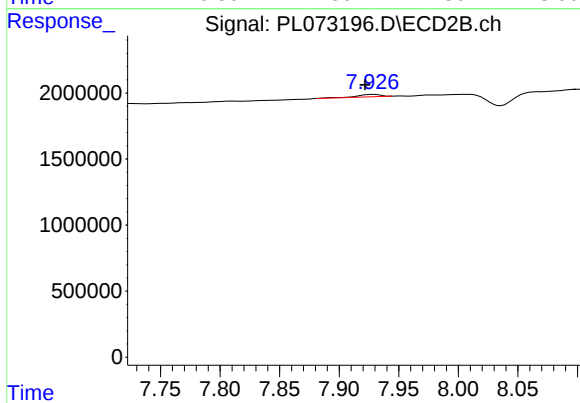

#8 Heptachlor epoxide


R.T.: 7.928 min
Delta R.T.: 0.006 min
Response: 251703
Conc: 0.15 ng/ml

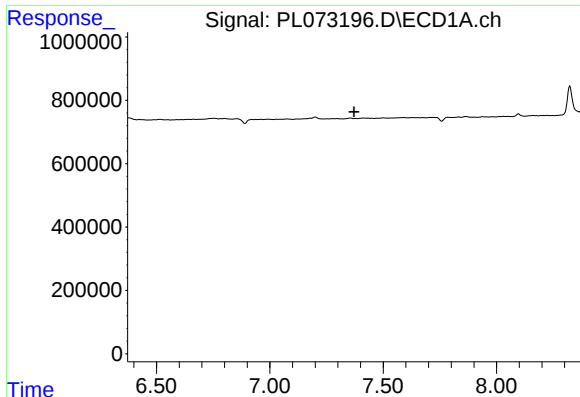

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

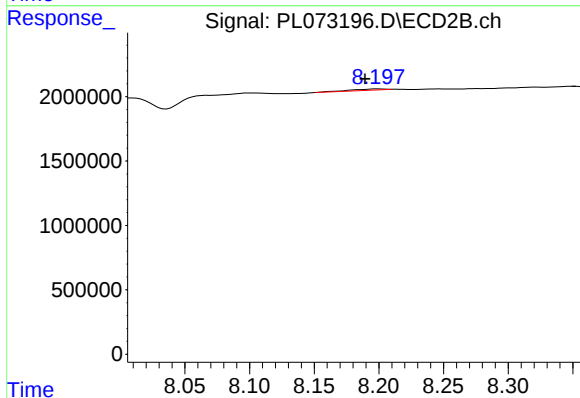


#10 trans-Chlordane

R.T.: 8.199 min
Delta R.T.: 0.010 min
Response: 183271
Conc: 0.11 ng/ml

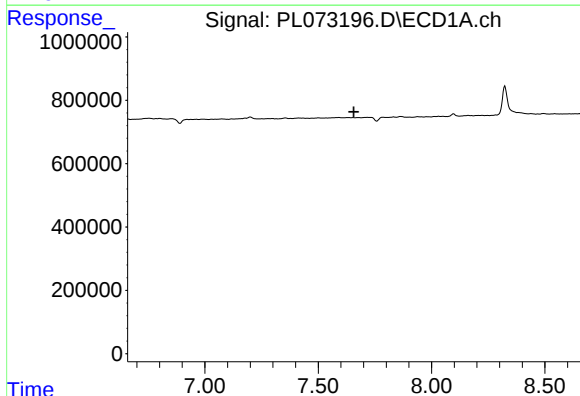


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.657 min
Response: 0
Conc: N.D.

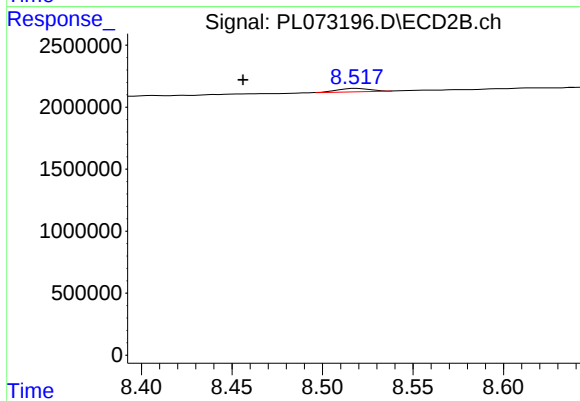

#12 4,4'-DDE


R.T.: 8.519 min
Delta R.T.: 0.063 min
Response: 335420
Conc: 0.22 ng/ml

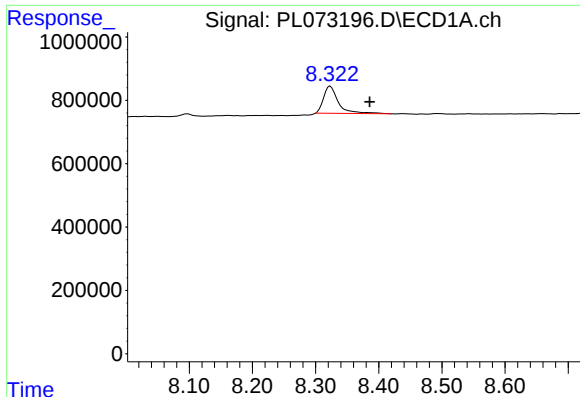

#15 Endosulfan II


R.T.: 8.323 min
Delta R.T.: -0.062 min
Response: 1386684
Conc: 2.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

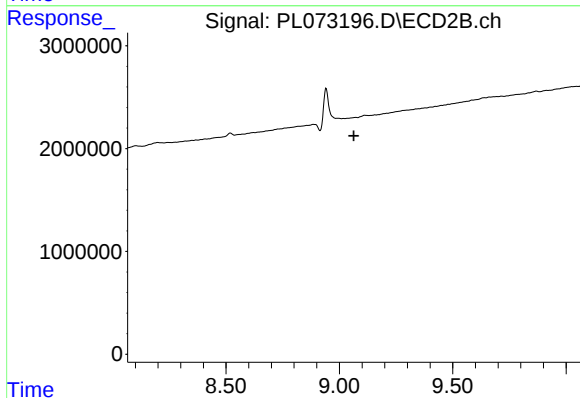


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

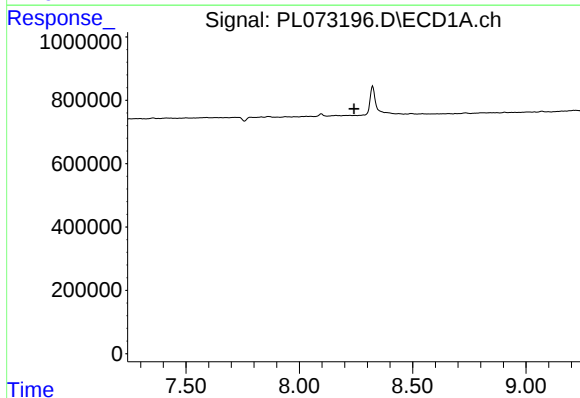


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

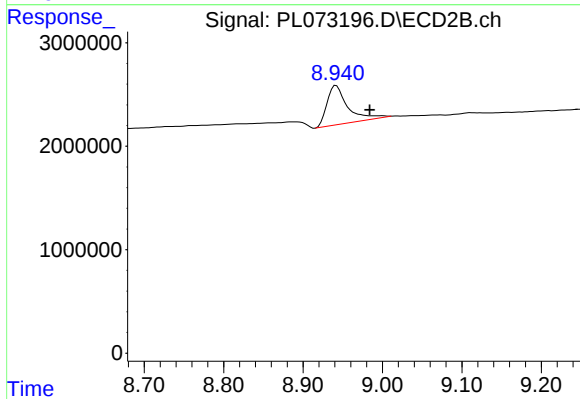

#16 4,4'-DDD


R.T.: 8.942 min
Delta R.T.: -0.042 min
Response: 6797648
Conc: 5.18 ng/ml

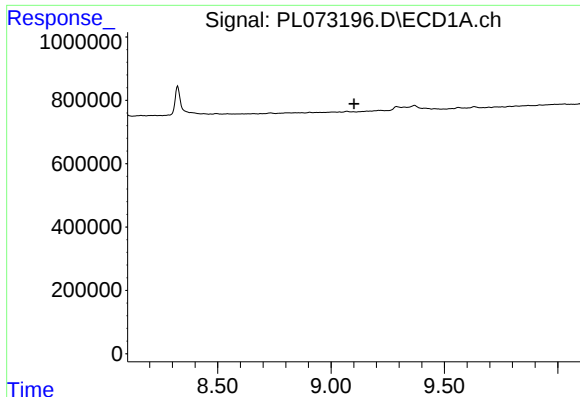

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

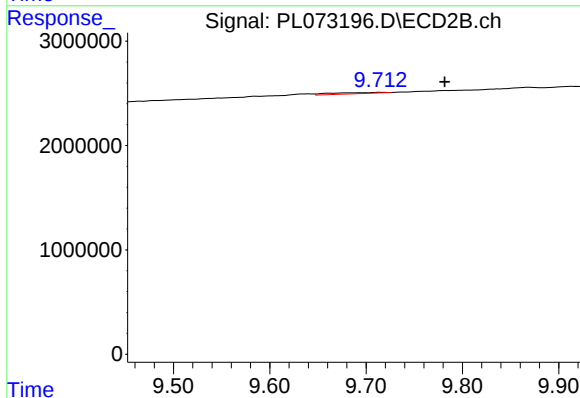


#20 Methoxychlor

R.T.: 9.715 min
Delta R.T.: -0.066 min
Response: 399884
Conc: 0.52 ng/ml

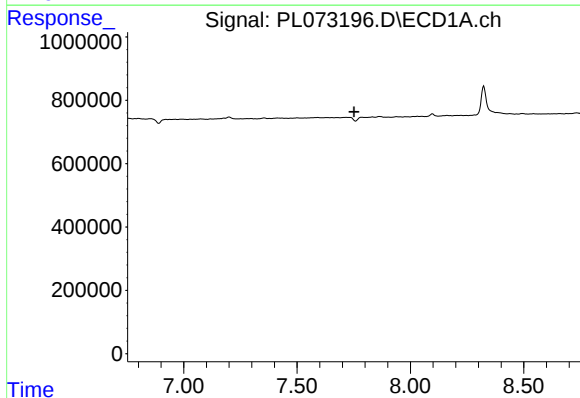


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.

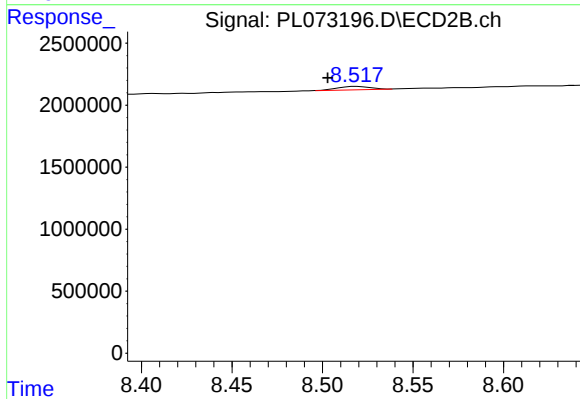

#22 Toxaphene-1


R.T.: 8.519 min
Delta R.T.: 0.016 min
Response: 335420
Conc: 34.86 ng/ml

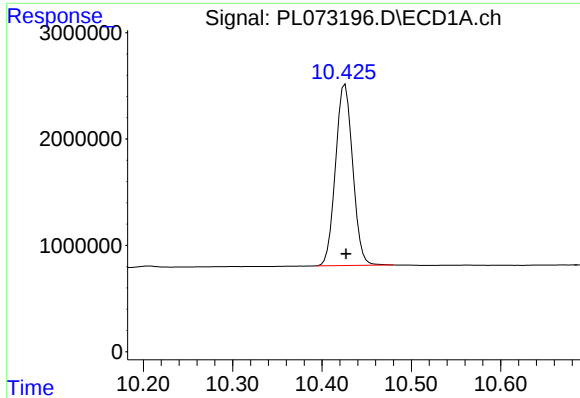

#27 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: 0.000 min
Response: 22790207
Conc: 47.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

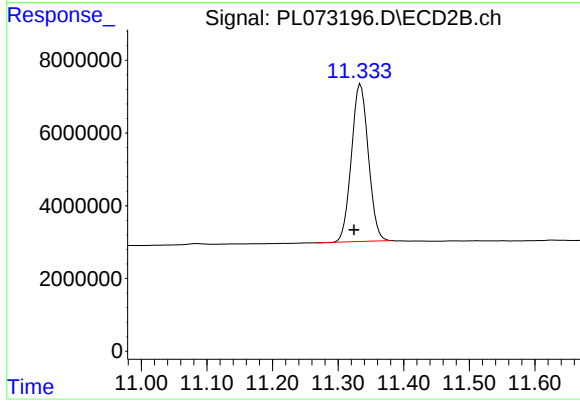

#27 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: 0.010 min
Response: 77518775
Conc: 47.96 ng/ml