

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030723\
 Data File : PL081289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2023 13:17
 Operator : AR\AJ
 Sample : 01825-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HH-TP1-0306

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/08/2023
 Supervised By : Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 19:33:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.338	2.663	46185272	42285863	21.377	20.894
2)	SA Decachlor...	8.765	7.791	34980665	33939294	22.945	17.718
Target Compounds							
17)	MA 4,4'-DDT	6.797	5.912	2152820	5358456	1.356m	3.340 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030723\
Data File : PL081289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2023 13:17
Operator : AR\AJ
Sample : 01825-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HH-TP1-0306


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/08/2023
Supervised By : Ankita Jodhani 03/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 19:33:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

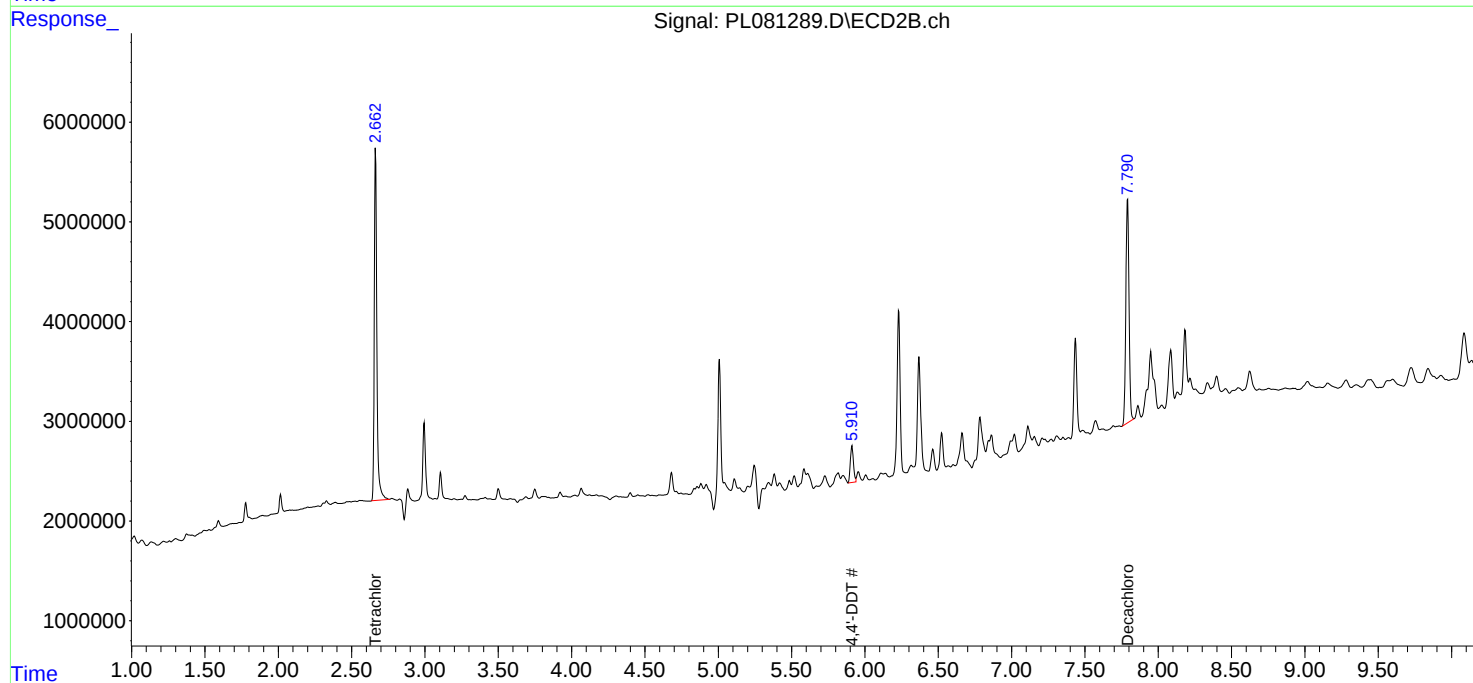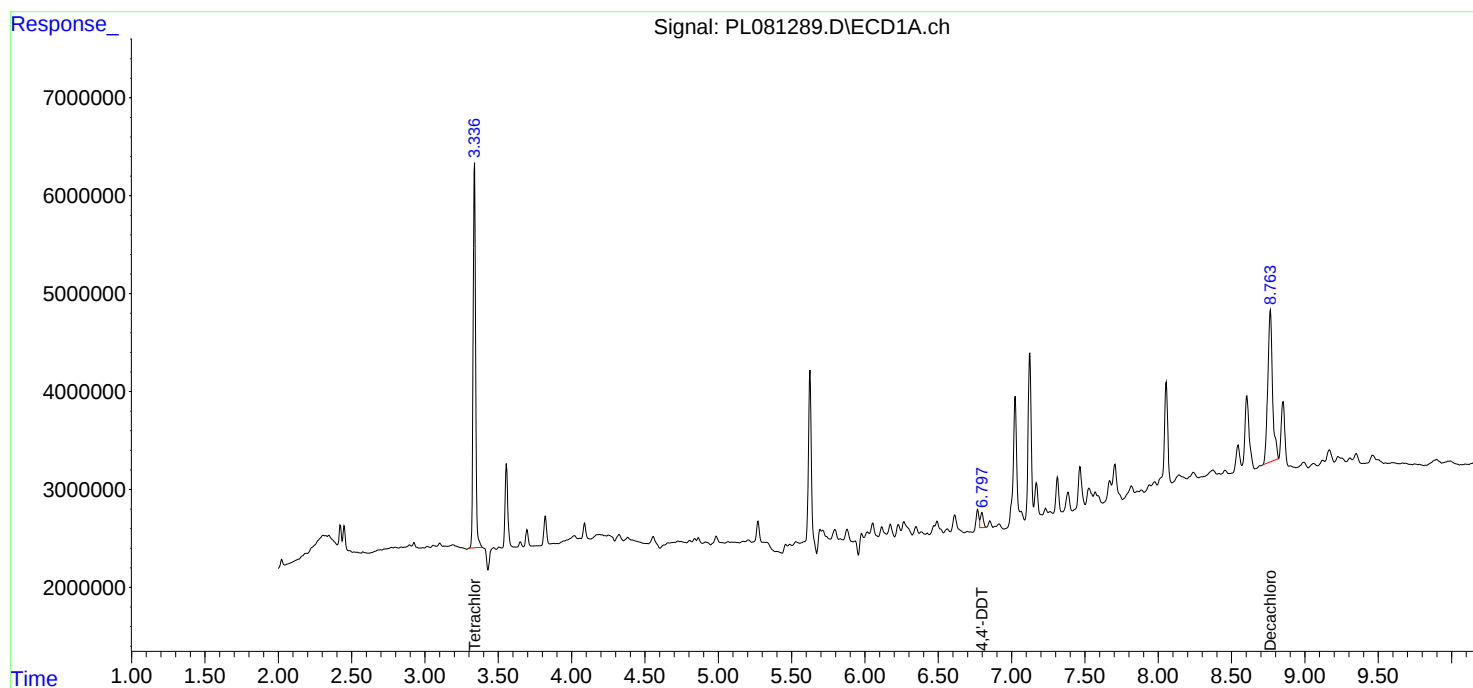

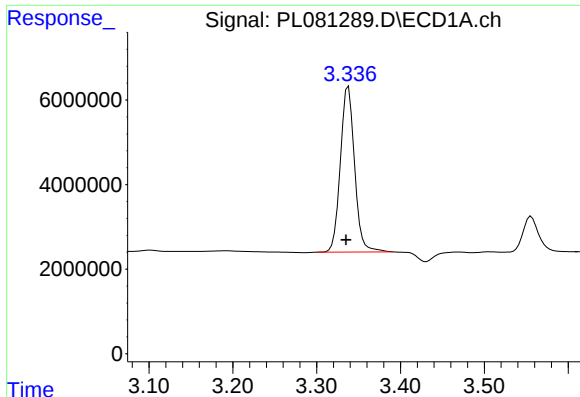


#1 Tetrachloro-m-xylene

R.T.: 3.338 min
Delta R.T.: 0.003 min
Response: 46185272
Conc: 21.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
HH-TP1-0306


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

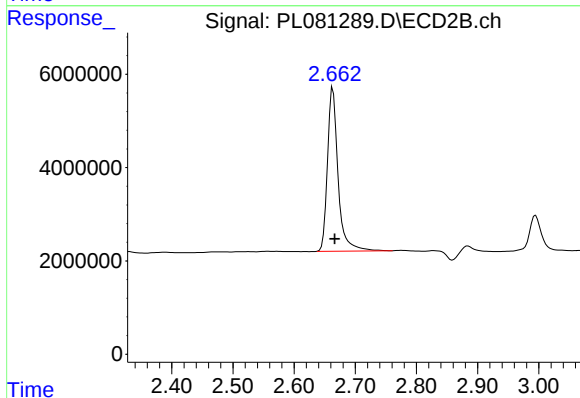


#1 Tetrachloro-m-xylene

R.T.: 2.663 min
Delta R.T.: -0.003 min
Response: 42285863
Conc: 20.89 ng/ml

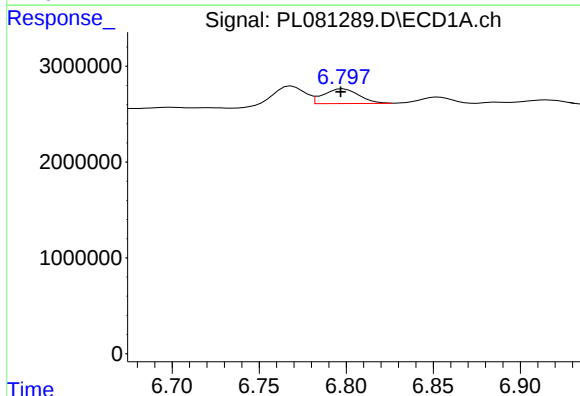


#17 4,4'-DDT

R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 2152820
Conc: 1.36 ng/ml m

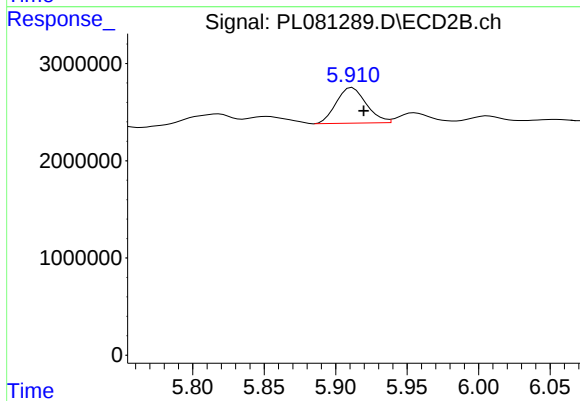

#17 4,4'-DDT

R.T.: 5.912 min
Delta R.T.: -0.008 min
Response: 5358456
Conc: 3.34 ng/ml

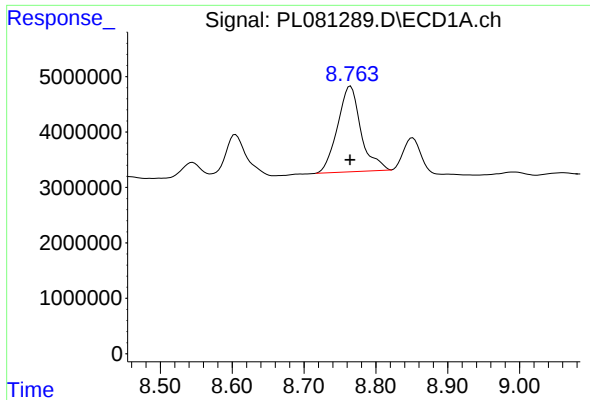


#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 34980665
Conc: 22.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
HH-TP1-0306

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/08/2023
Supervised By :Ankita Jodhani 03/08/2023

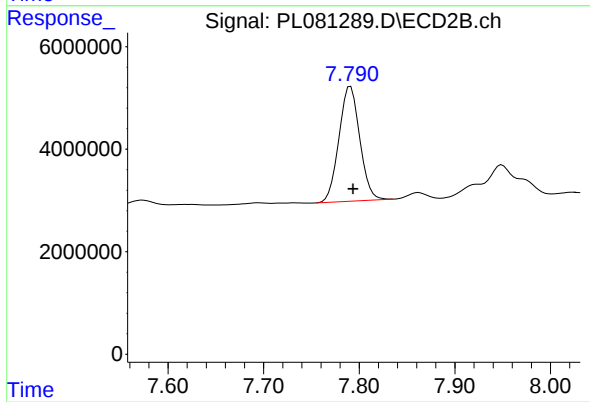

#28 Decachlorobiphenyl

R.T.: 7.791 min
Delta R.T.: -0.003 min
Response: 33939294
Conc: 17.72 ng/ml