

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030724\
 Data File : PL088436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2024 13:03
 Operator : AR\AJ
 Sample : PB159488BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB159488BL

Manual Integrations APPROVED

Reviewed By :Abdul
 Mirza

03/08/2024
 Supervised By :Ankita
 Jodhani

03/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 09:59:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.644	2.854	57593065	29407302	20.968m	20.967
28) SA Decachlor...	9.318	8.089	49795681	29296309	25.855m	23.008

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030724\
Data File : PL088436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2024 13:03
Operator : AR\AJ
Sample : PB159488BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB159488BL

Manual Integrations
APPROVED



Reviewed By : Abdul
Mirza


03/08/2024
Supervised By : Ankita
Jodhani

03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 09:59:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

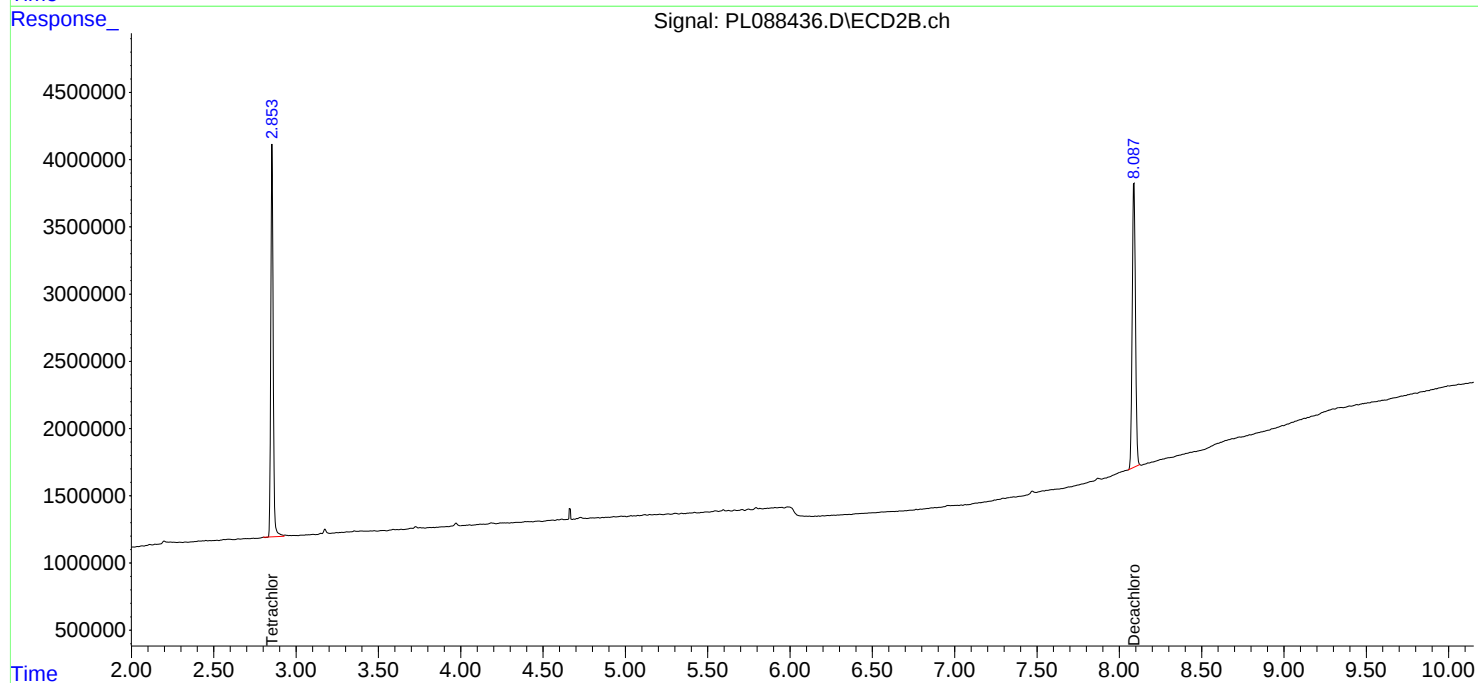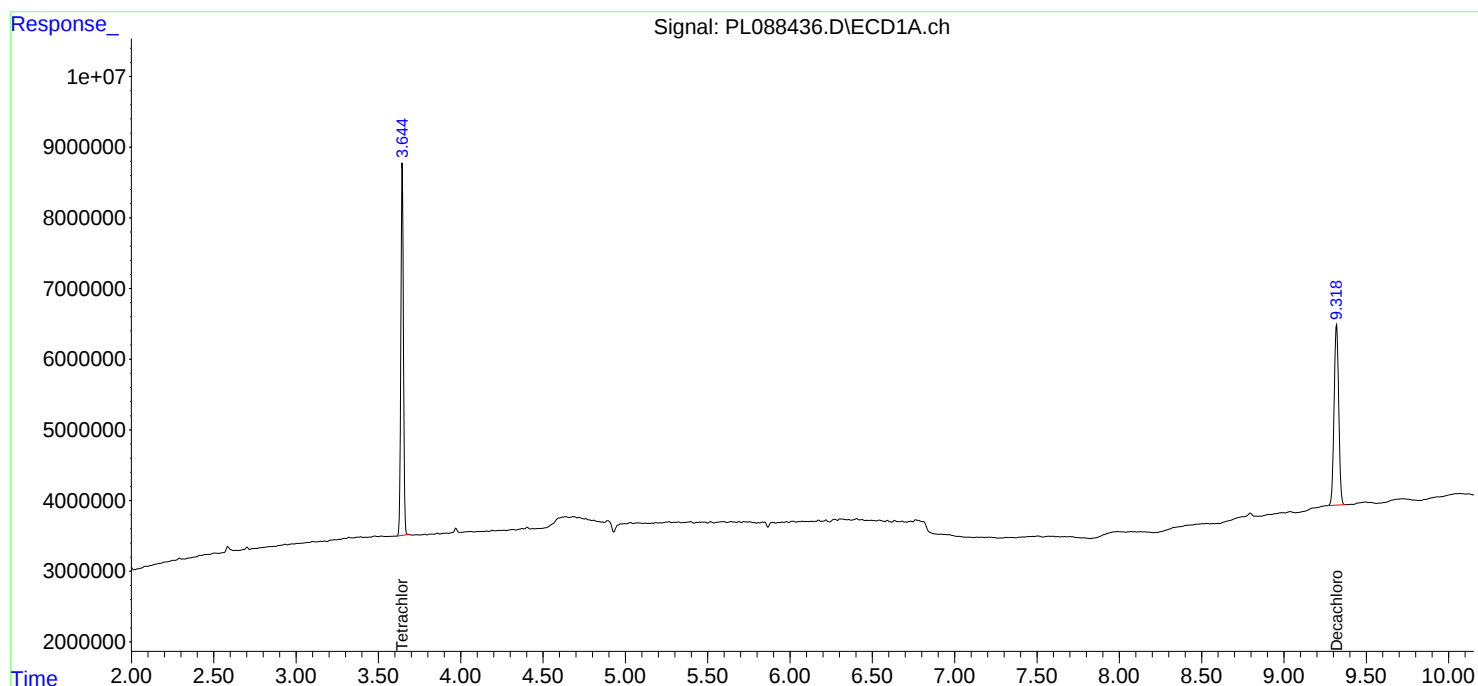

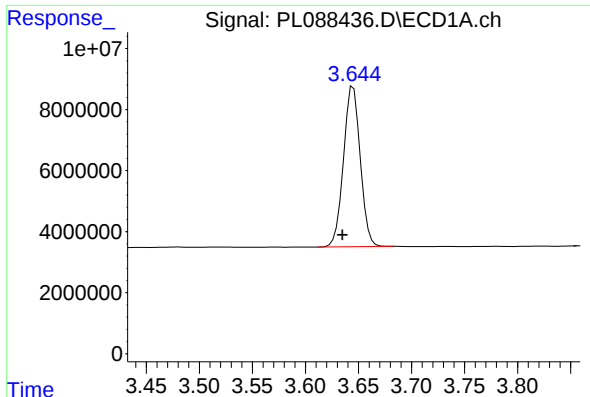

#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.009 min
Response: 57593065
Conc: 20.97 ng/ml


Instrument :
ECD_L
ClientSampleId :
PB159488BL

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza


03/08/2024
Supervised By :Ankita
Jodhani

03/08/2024

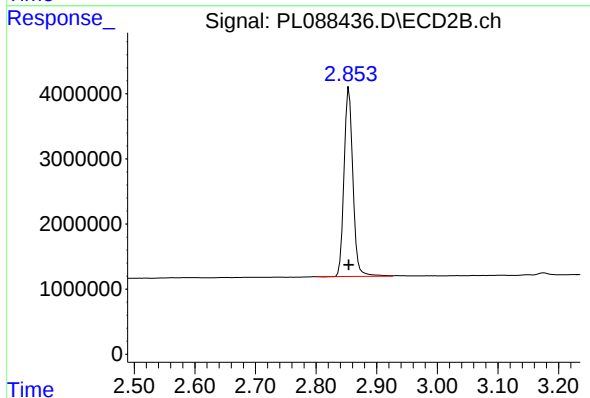


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.000 min
Response: 29407302
Conc: 20.97 ng/ml

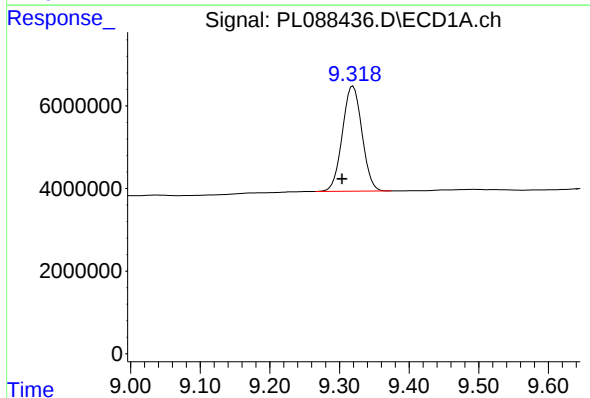

#28 Decachlorobiphenyl

R.T.: 9.318 min
Delta R.T.: 0.014 min
Response: 49795681
Conc: 25.86 ng/ml m

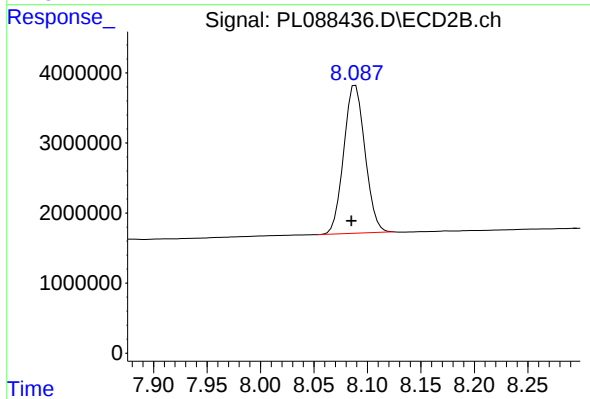

#28 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.004 min
Response: 29296309
Conc: 23.01 ng/ml