

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030724\
 Data File : PL088444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2024 14:57
 Operator : AR\AJ
 Sample : P1688-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/08/2024
 Supervised By :Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 21:53:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.854	51546931	27813853	18.767m	19.831
28) SA Decachlor...	9.302	8.082	37987694	24924065	19.724	19.575

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030724\
Data File : PL088444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2024 14:57
Operator : AR\AJ
Sample : P1688-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-5


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/08/2024
Supervised By : Ankita Jodhani 03/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 21:53:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

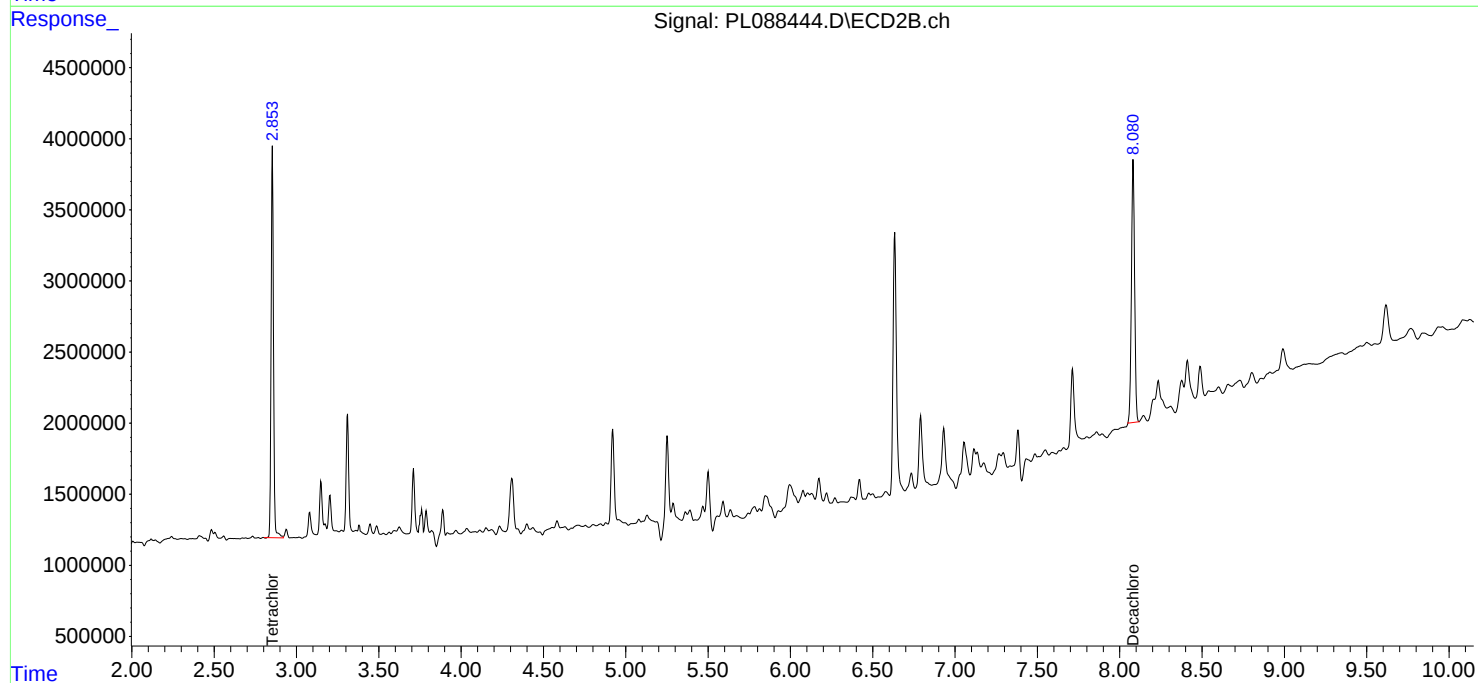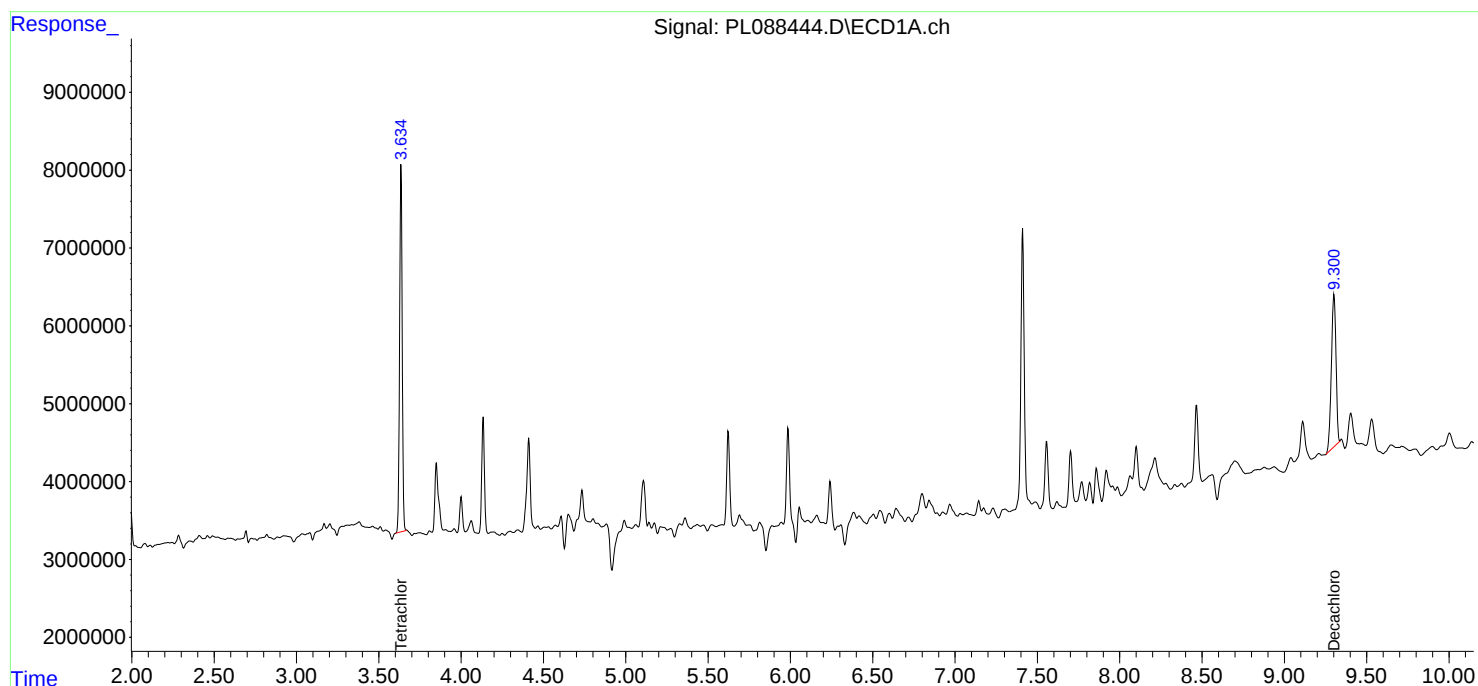

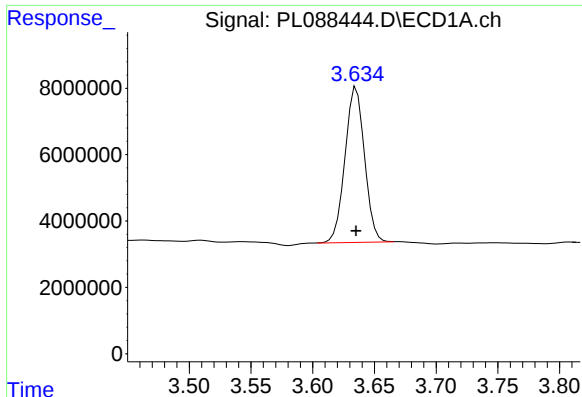


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 51546931
Conc: 18.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-5


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/08/2024
Supervised By :Ankita Jodhani 03/08/2024

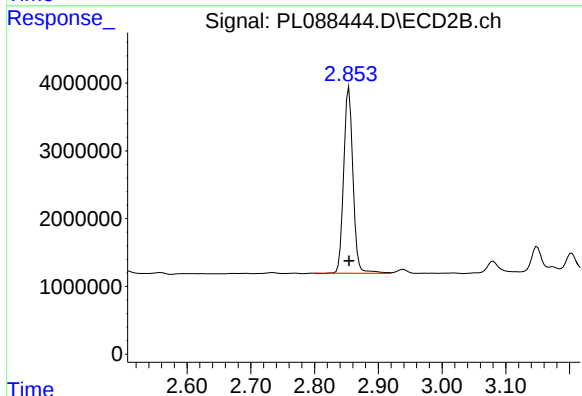


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.000 min
Response: 27813853
Conc: 19.83 ng/ml

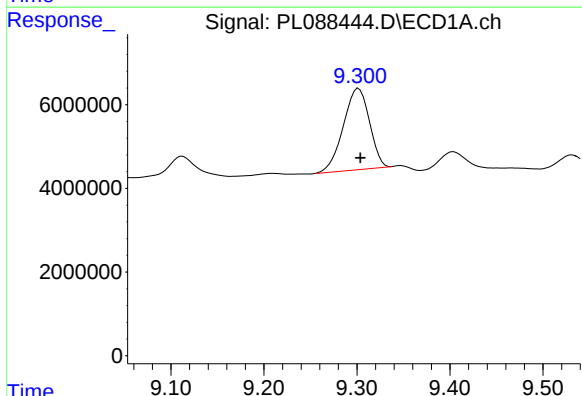

#28 Decachlorobiphenyl

R.T.: 9.302 min
Delta R.T.: -0.002 min
Response: 37987694
Conc: 19.72 ng/ml

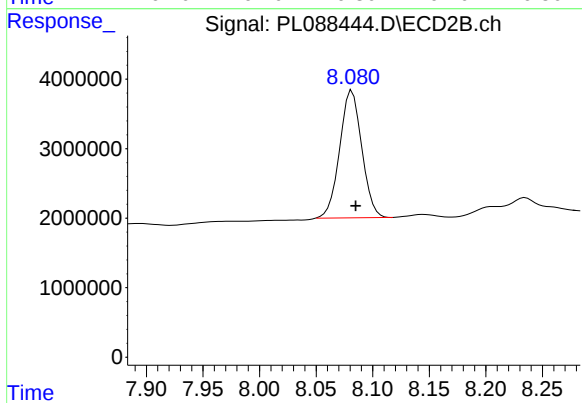

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: -0.003 min
Response: 24924065
Conc: 19.57 ng/ml