

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030819\
 Data File : PL045656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2019 00:47
 Operator : AJ\SJ
 Sample : K1761-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N4871

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 03:34:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.981	125.2E6	37222885	18.202	17.381
28)	SA Decachlor...	8.045	9.038	117.9E6	35239044	14.084	15.422
Target Compounds							
2)	A alpha-BHC	0.000	4.397f	0	1049867	N.D.	0.346 #
11)	B alpha-Chl...	5.317	0.000	57642244	0	5.944	N.D. #
26)	Chlordane-4	5.317	0.000	57642244	0	54.377	N.D. #
27)	Chlordane-5	0.000	6.973	0	1369020	N.D.	15.071 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030819\
Data File : PL045656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2019 00:47
Operator : AJ\SJ
Sample : K1761-01
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
N4871

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 03:34:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

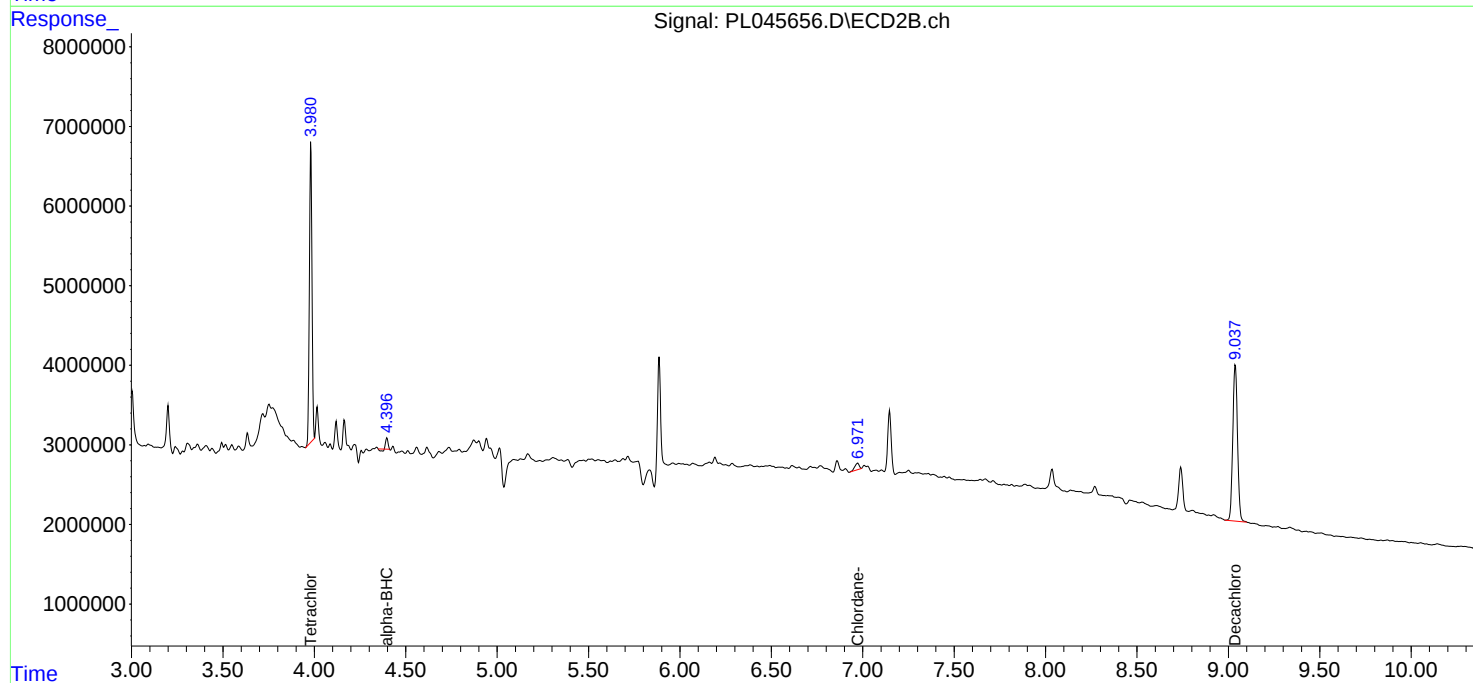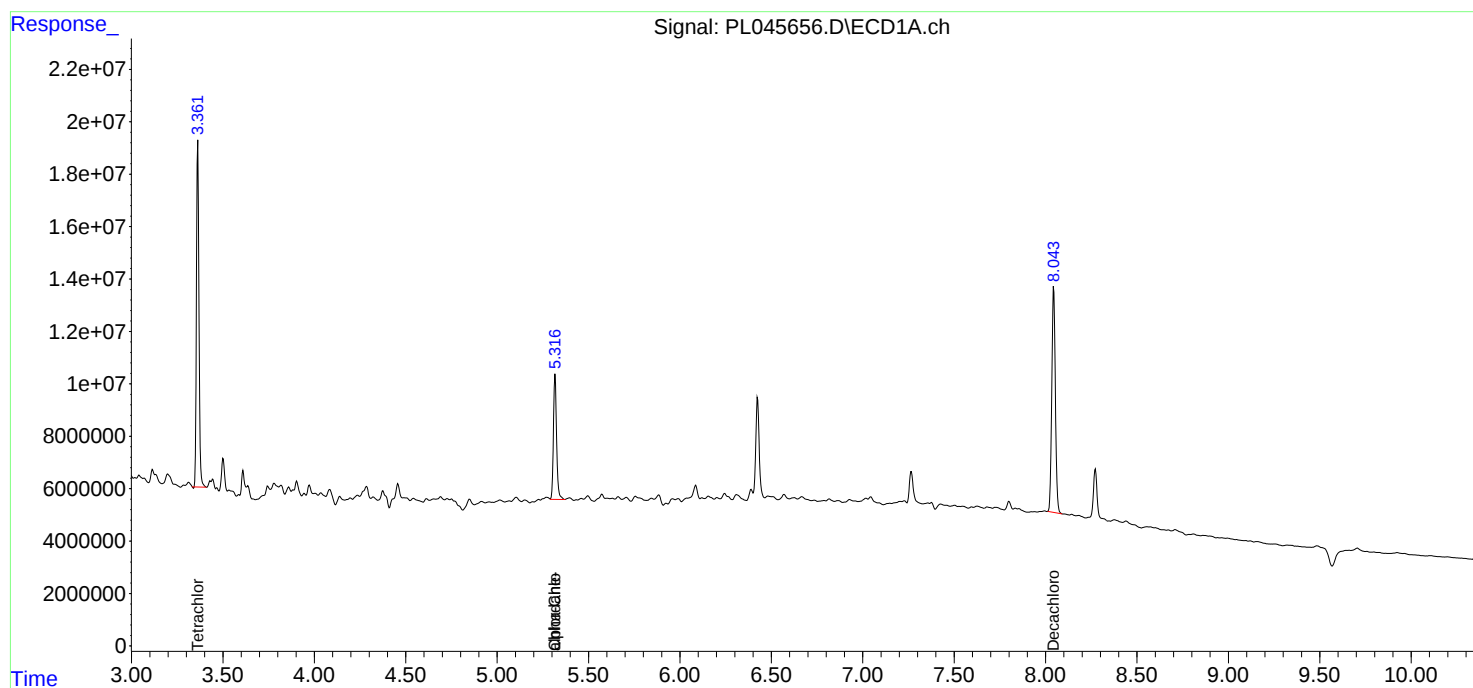


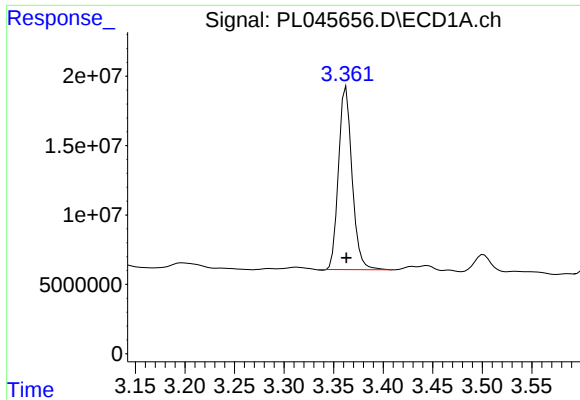

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 125214554
Conc: 18.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
N4871

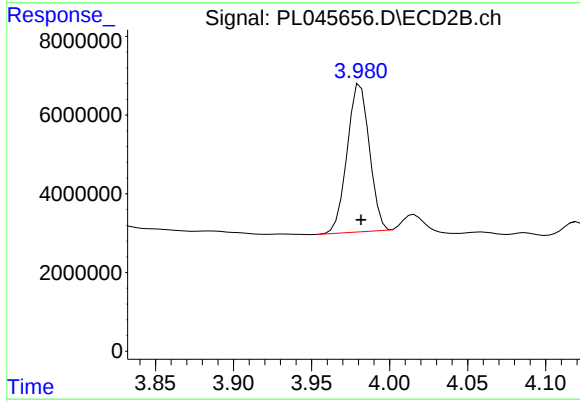


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 37222885
Conc: 17.38 ng/ml

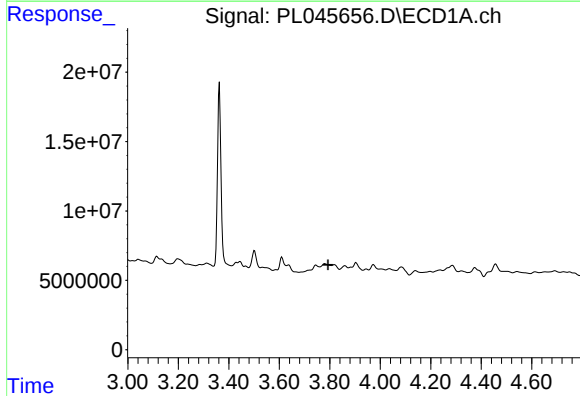


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.794 min
Response: 0
Conc: N.D.

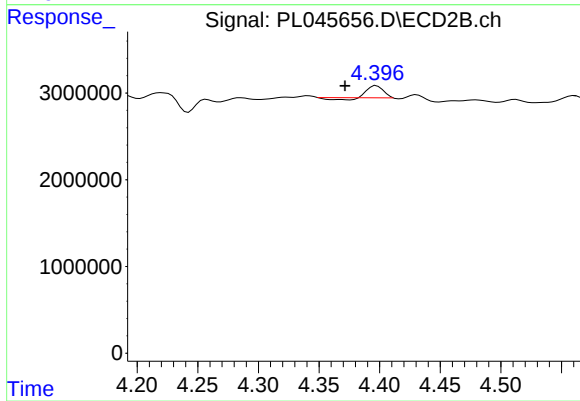

#2 alpha-BHC


R.T.: 4.397 min
Delta R.T.: 0.026 min
Response: 1049867
Conc: 0.35 ng/ml

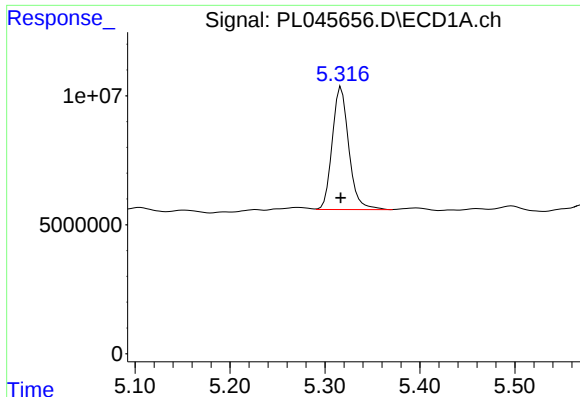

#11 alpha-Chlordane


R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 57642244
Conc: 5.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
N4871

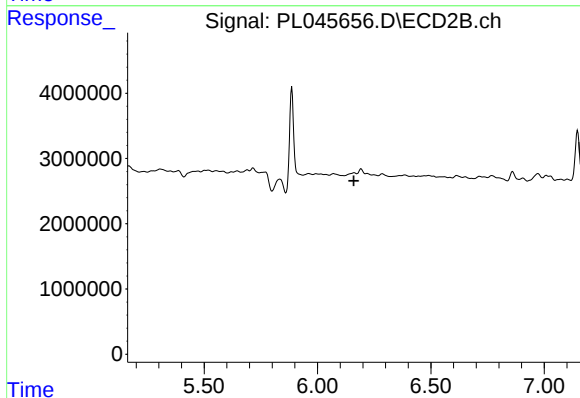


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

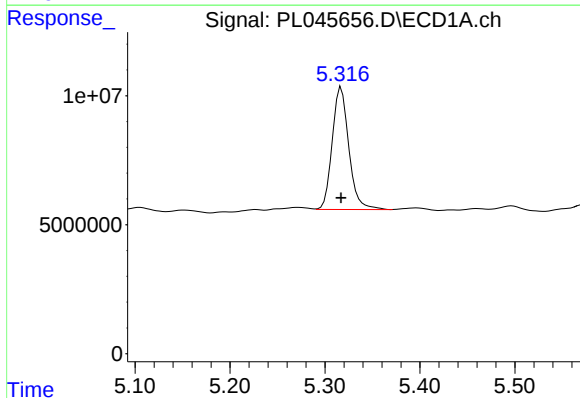

#26 Chlordane-4

R.T.: 5.317 min
Delta R.T.: 0.000 min
Response: 57642244
Conc: 54.38 ng/ml

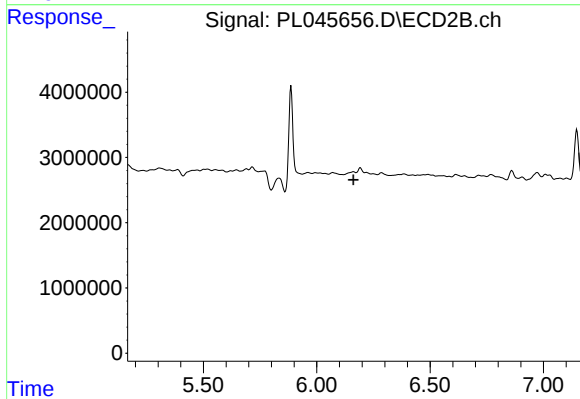

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

