

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030819\
 Data File : PL045610.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2019 11:09
 Operator : AJ\SJ
 Sample : K1764-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KITCHEN-SINK

Manual Integrations
 APPROVED

Sohil
 3/11/2019 10:34:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 21:54:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	130.4E6	40013188	18.952	18.684
28)	SA Decachlor...	8.043	9.036	118.4E6	35694775	14.147	15.622
Target Compounds							
3)	MA gamma-BHC...	4.071	4.653	21580203	2400657	2.135m	0.850m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030819\
Data File : PL045610.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2019 11:09
Operator : AJ\SJ
Sample : K1764-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
KITCHEN-SINK


Manual Integrations
APPROVED

Sohil
3/11/2019 10:34:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 21:54:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

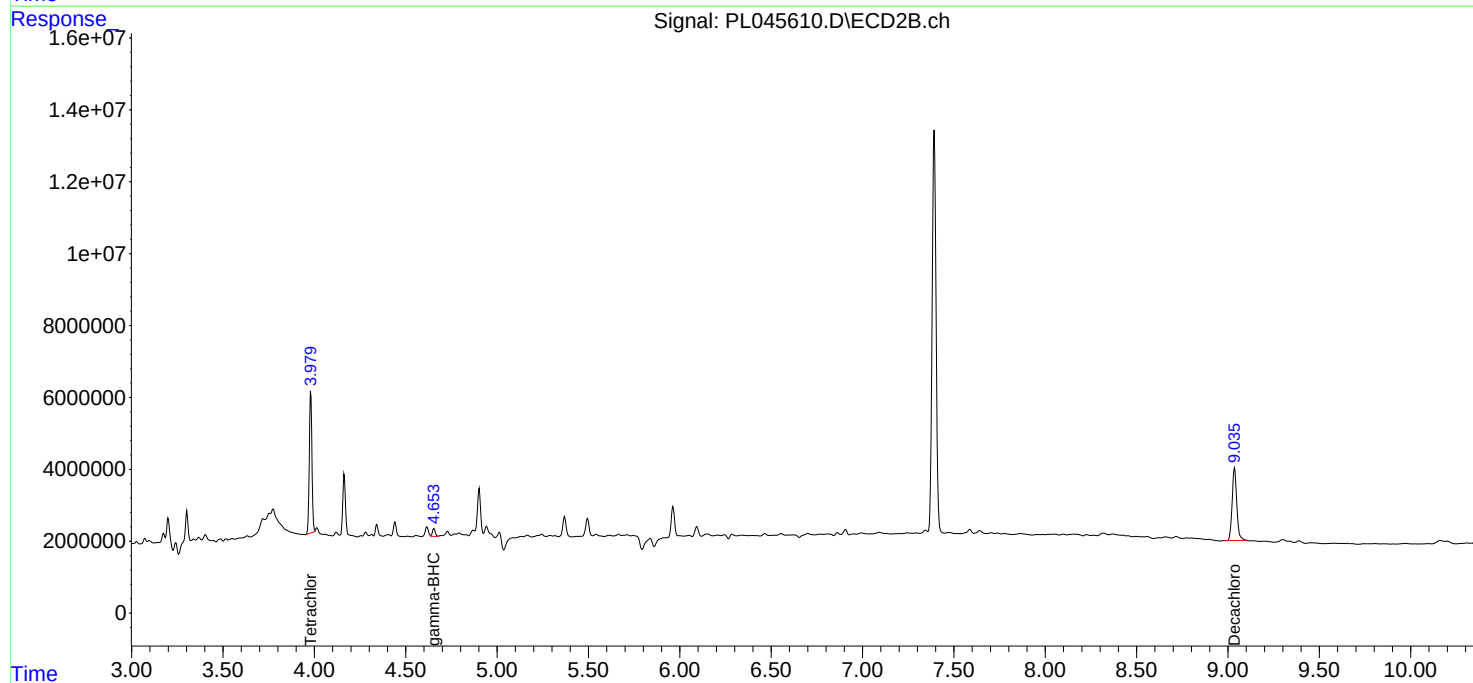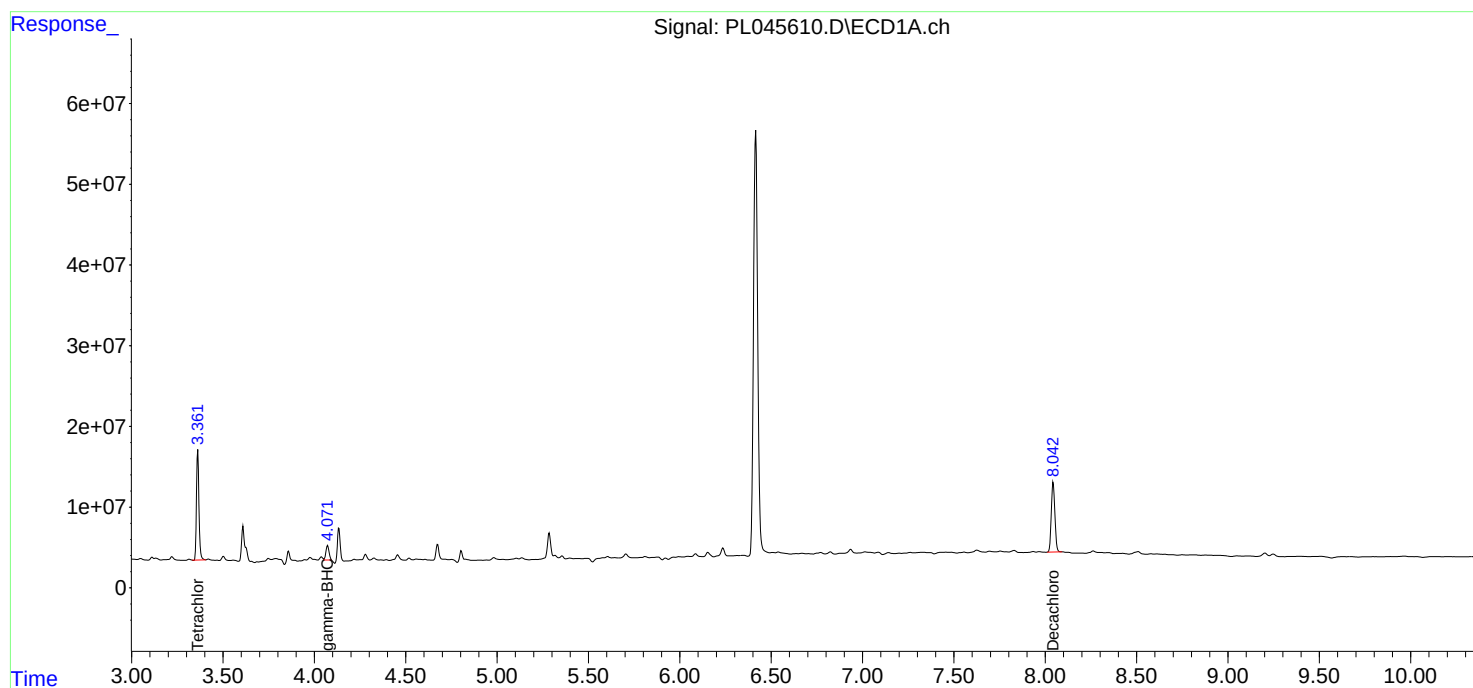

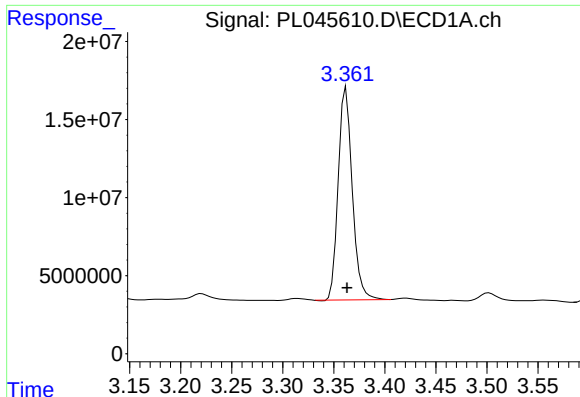


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 130373739
Conc: 18.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
KITCHEN-SINK


Manual Integrations
APPROVED

Sohil
3/11/2019 10:34:27 AM

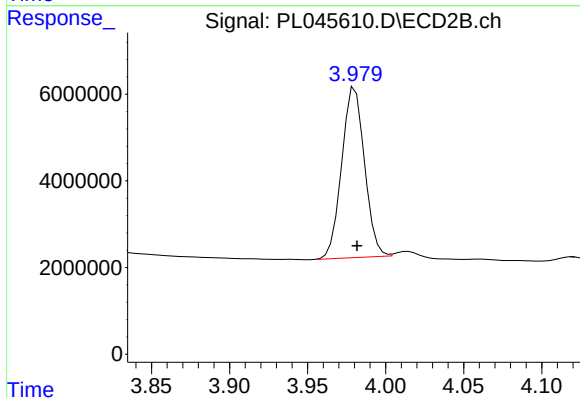


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 40013188
Conc: 18.68 ng/ml

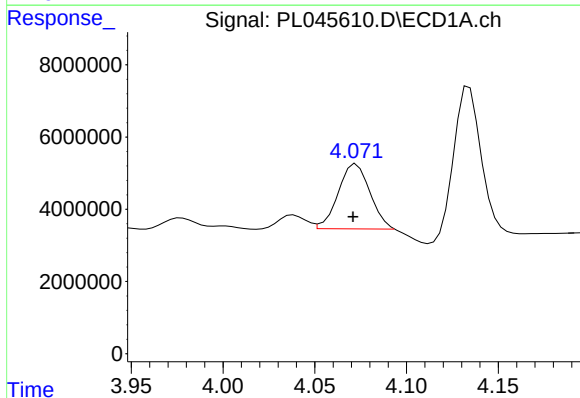


#3 gamma-BHC (Lindane)

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 21580203
Conc: 2.14 ng/ml m

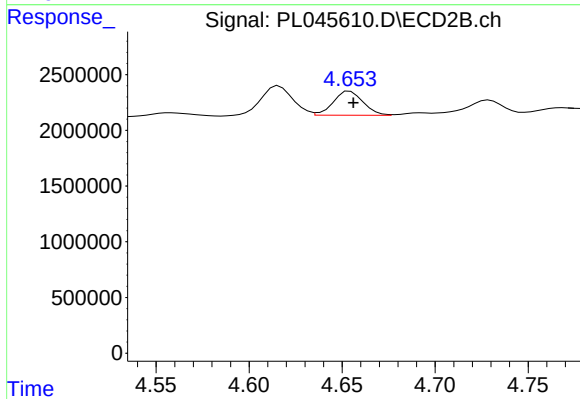

#3 gamma-BHC (Lindane)

R.T.: 4.653 min
Delta R.T.: -0.003 min
Response: 2400657
Conc: 0.85 ng/ml m

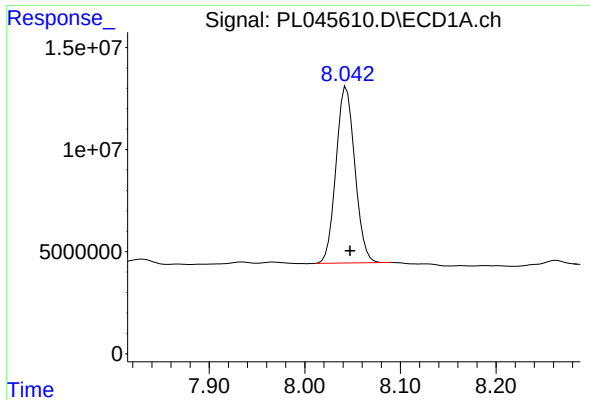


#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.004 min
Response: 118377879
Conc: 14.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
KITCHEN-SINK

Manual Integrations
APPROVED

Sohil
3/11/2019 10:34:27 AM

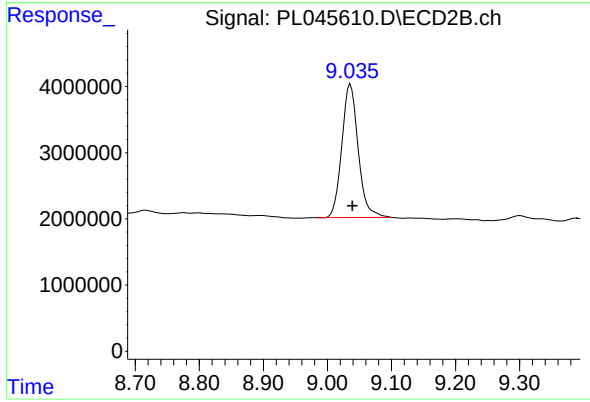

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: -0.003 min
Response: 35694775
Conc: 15.62 ng/ml