

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 09:15
 Operator : AR\AJ
 Sample : IBLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 11:52:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	59048982	47312977	20.082	19.053
28)	SA Decachlor...	8.139	9.250	49832677	40487067	17.957	18.432
Target Compounds							
6)	B beta-BHC	4.397	0.000	3880490	0	2.078	N.D. #
23)	Chlordane-1	4.309f	0.000	3747850	0	29.404	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 09:15
Operator : AR\AJ
Sample : IBLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 11:52:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

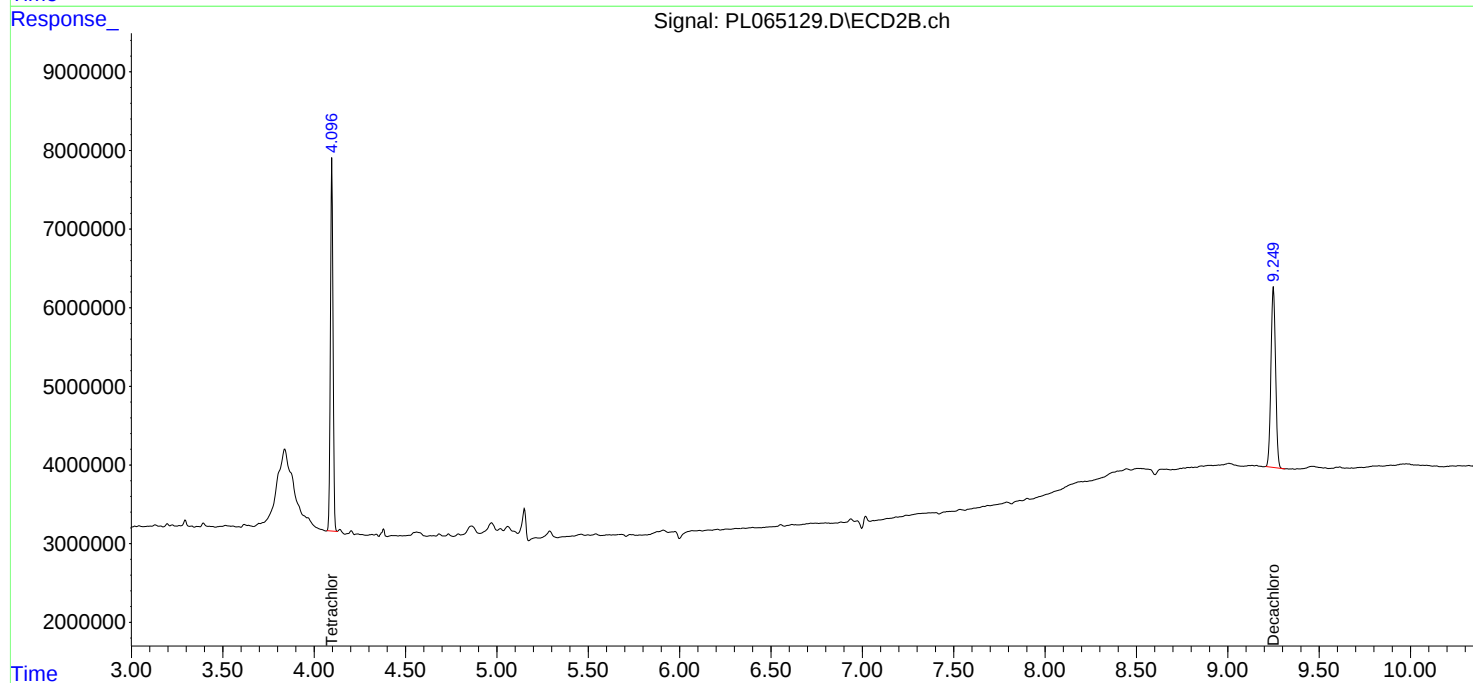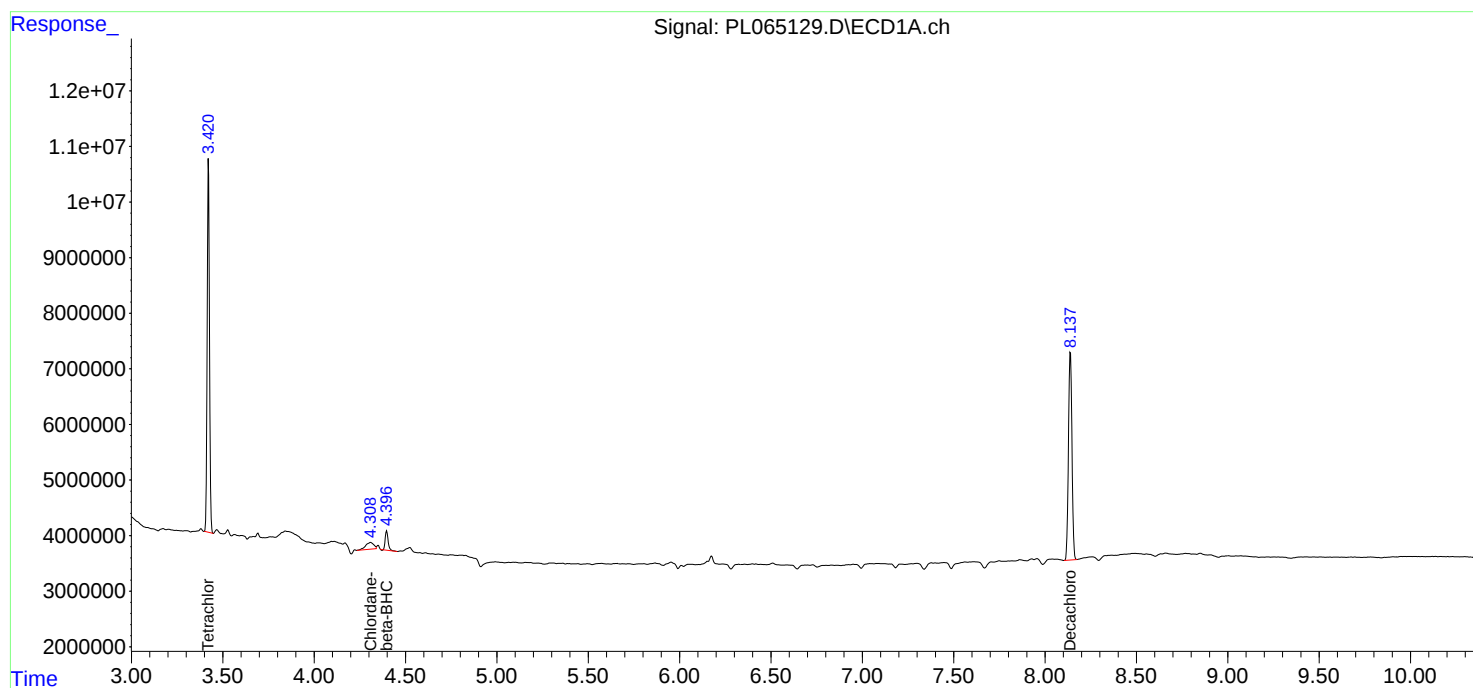


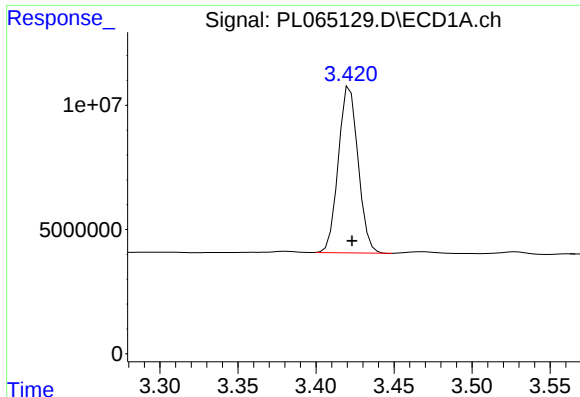

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 59048982
Conc: 20.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

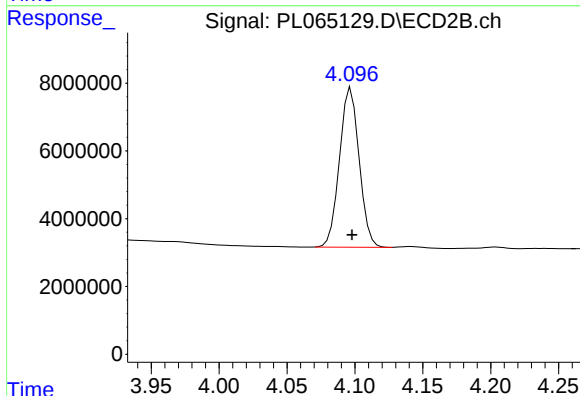


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 47312977
Conc: 19.05 ng/ml

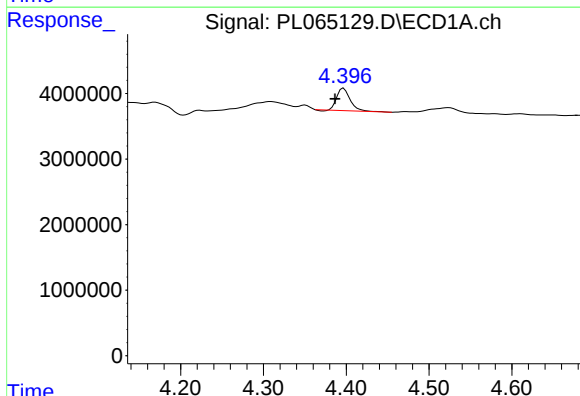


#6 beta-BHC

R.T.: 4.397 min
Delta R.T.: 0.010 min
Response: 3880490
Conc: 2.08 ng/ml

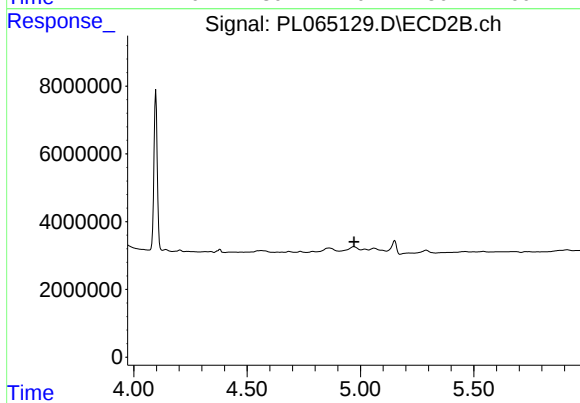

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.972 min
Response: 0
Conc: N.D.

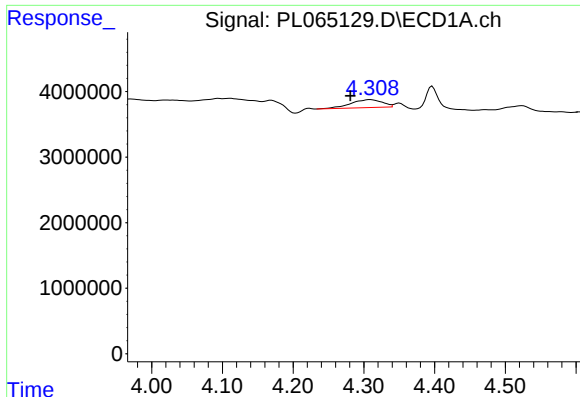

#23 Chlordane-1


R.T.: 4.309 min
Delta R.T.: 0.028 min
Response: 3747850
Conc: 29.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

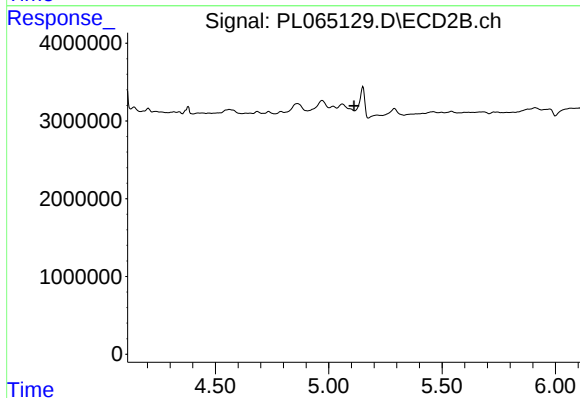


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

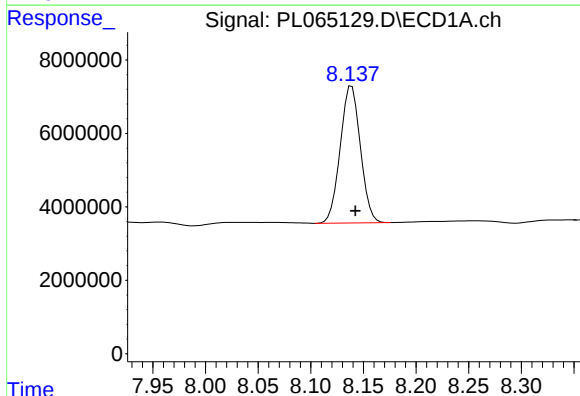

#28 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.003 min
Response: 49832677
Conc: 17.96 ng/ml

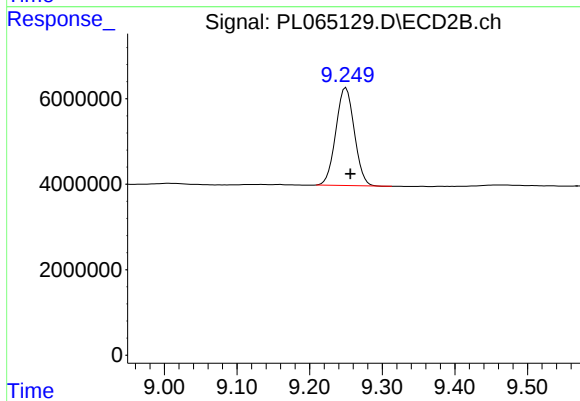

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 40487067
Conc: 18.43 ng/ml