

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 10:27
 Operator : AR\AJ
 Sample : M1551-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VEOLIA-VNJ-204

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 11:53:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	4.098	40953706	34299003	13.928	13.812
28)	SA Decachlor...	8.146	9.255	47862668	37608508	17.247	17.122
Target Compounds							
6)	B beta-BHC	4.358f	4.980	479056	5538808	0.256	3.622 #
9)	A Endosulfan I	5.480f	0.000	4969236	0	1.390	N.D. #
10)	B gamma-Chl...	5.322f	0.000	2578619	0	0.658	N.D. #
12)	B 4,4'-DDE	5.571	6.473	9444915	9708212	2.628	3.883 #
13)	MA Dieldrin	5.695	6.614f	7824876	5188206	2.115	2.025
14)	MA Endrin	5.956	0.000	1281194	0	0.373	N.D. #
16)	A 4,4'-DDD	0.000	6.972	0	2597522	N.D.	1.287 #
17)	MA 4,4'-DDT	6.318	0.000	6987414	0	2.506	N.D. #
18)	B Endrin al...	6.412f	0.000	2205634	0	0.860	N.D. #
19)	B Endosulfa...	6.604	0.000	3709624	0	1.097	N.D. #
20)	A Methoxychlor	6.849f	0.000	5380158	0	3.408	N.D. #
23)	Chlordane-1	4.285	0.000	5915358	0	46.410	N.D. #
25)	Chlordane-3	5.322f	0.000	2578619	0	6.464	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 10:27
Operator : AR\AJ
Sample : M1551-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 11:53:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

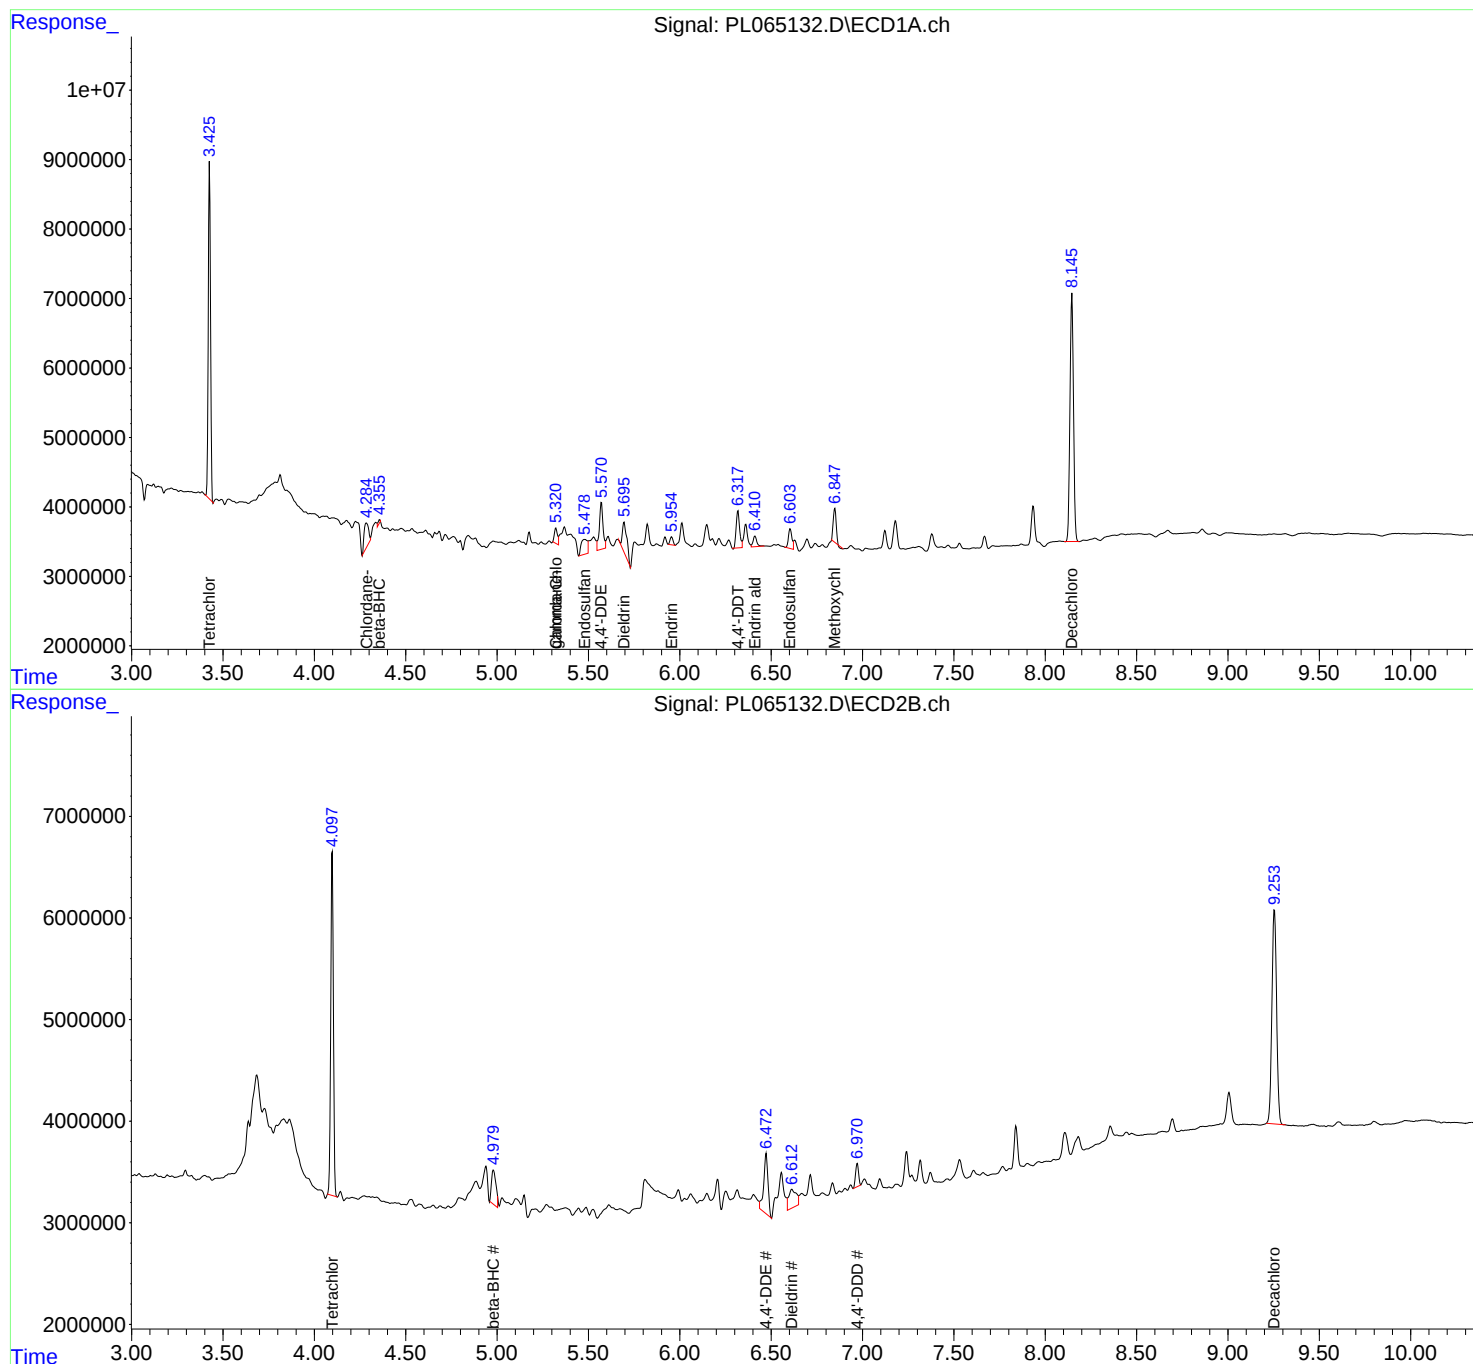


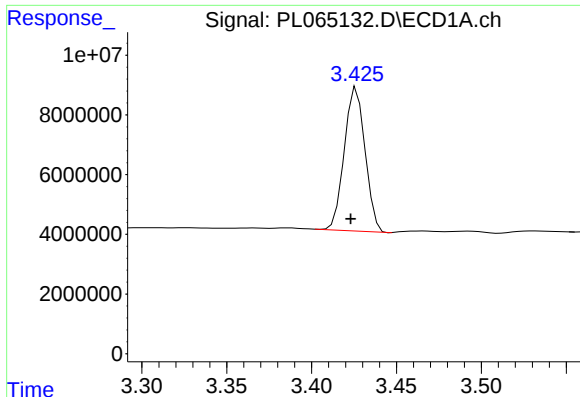

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: 0.004 min
Response: 40953706
Conc: 13.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

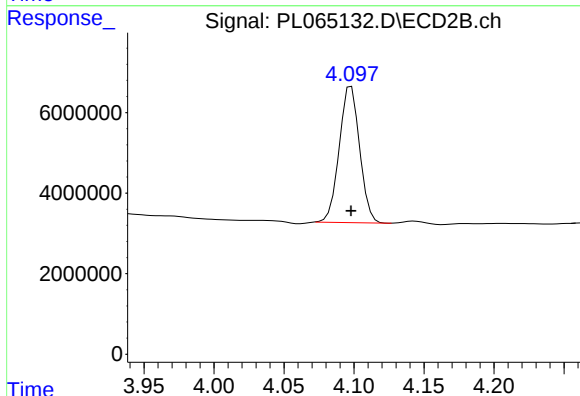


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 34299003
Conc: 13.81 ng/ml

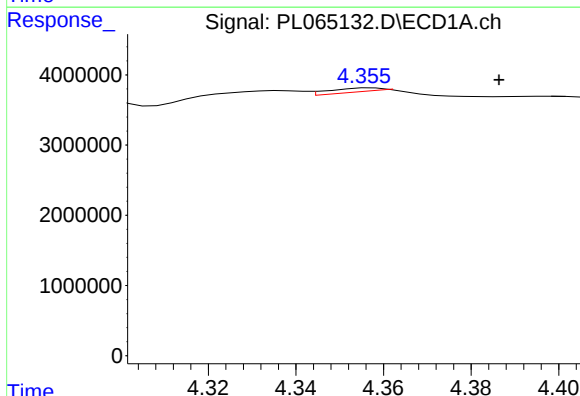


#6 beta-BHC

R.T.: 4.358 min
Delta R.T.: -0.029 min
Response: 479056
Conc: 0.26 ng/ml

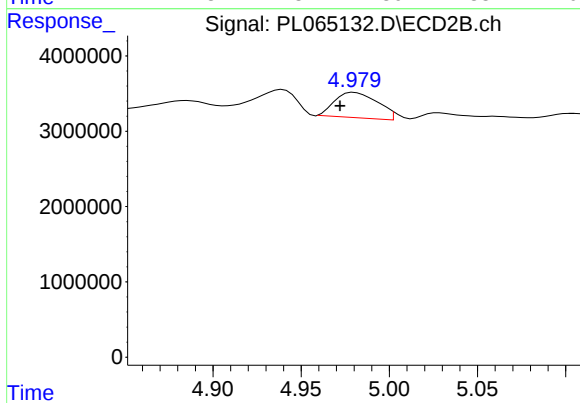

#6 beta-BHC


R.T.: 4.980 min
Delta R.T.: 0.008 min
Response: 5538808
Conc: 3.62 ng/ml

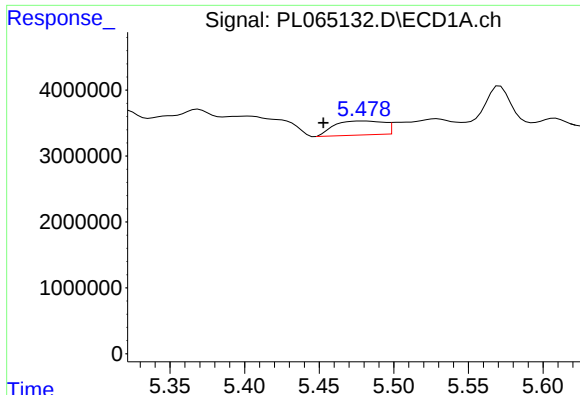

#9 Endosulfan I


R.T.: 5.480 min
Delta R.T.: 0.027 min
Response: 4969236
Conc: 1.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

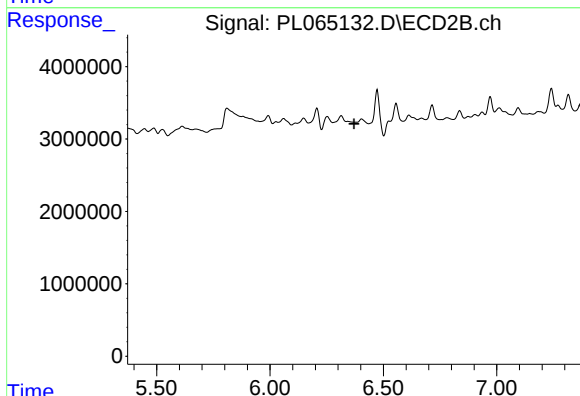


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.371 min
Response: 0
Conc: N.D.

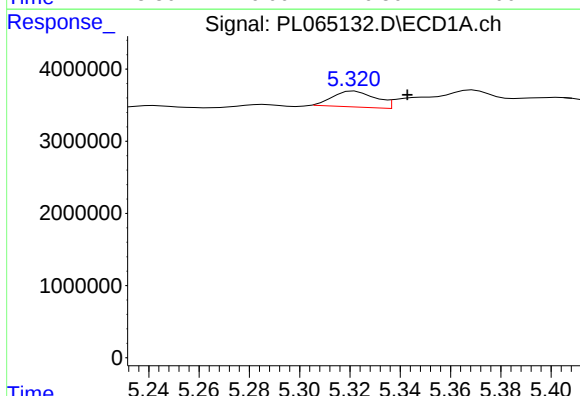


#10 gamma-Chlordane

R.T.: 5.322 min
Delta R.T.: -0.021 min
Response: 2578619
Conc: 0.66 ng/ml

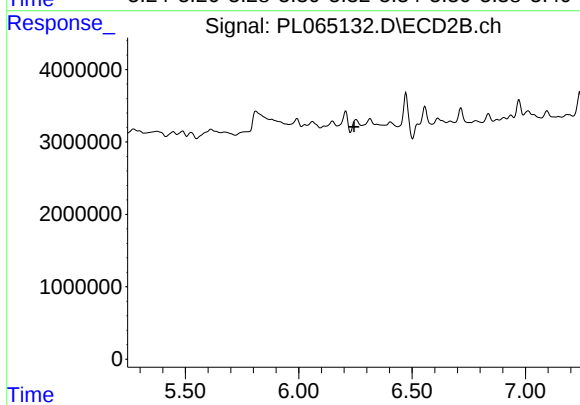

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

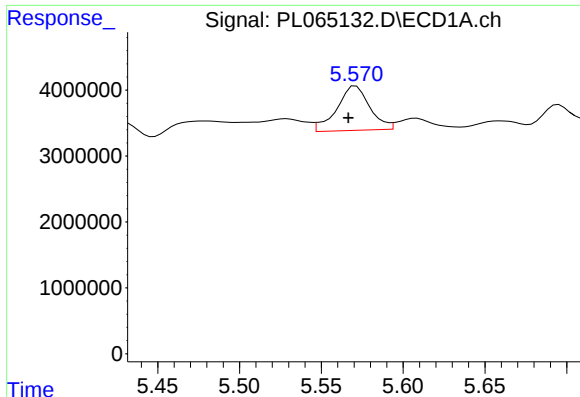

#12 4,4'-DDE


R.T.: 5.571 min
Delta R.T.: 0.005 min
Response: 9444915
Conc: 2.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

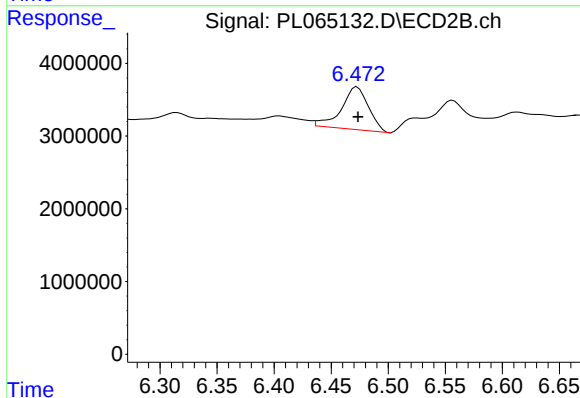


#12 4,4'-DDE

R.T.: 6.473 min
Delta R.T.: 0.000 min
Response: 9708212
Conc: 3.88 ng/ml

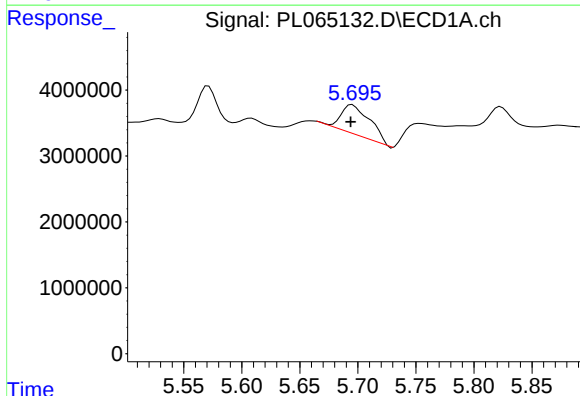


#13 Dieldrin

R.T.: 5.695 min
Delta R.T.: 0.001 min
Response: 7824876
Conc: 2.12 ng/ml

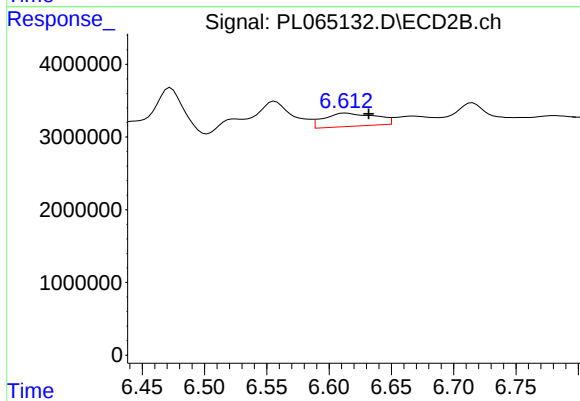

#13 Dieldrin


R.T.: 6.614 min
Delta R.T.: -0.018 min
Response: 5188206
Conc: 2.03 ng/ml

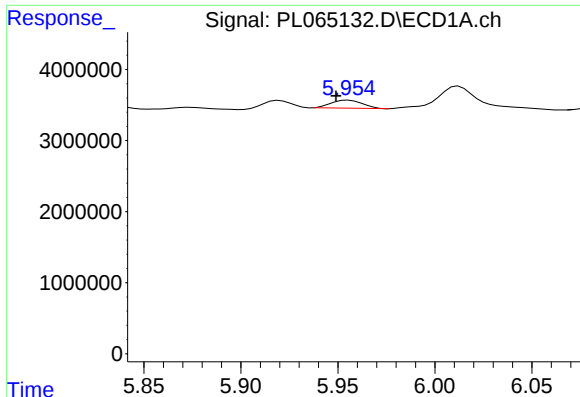

#14 Endrin


R.T.: 5.956 min
Delta R.T.: 0.007 min
Response: 1281194
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

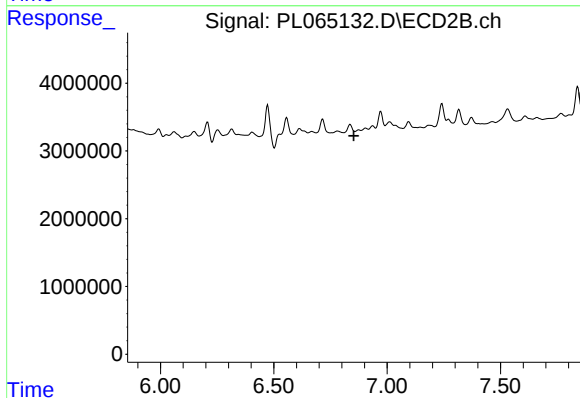


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

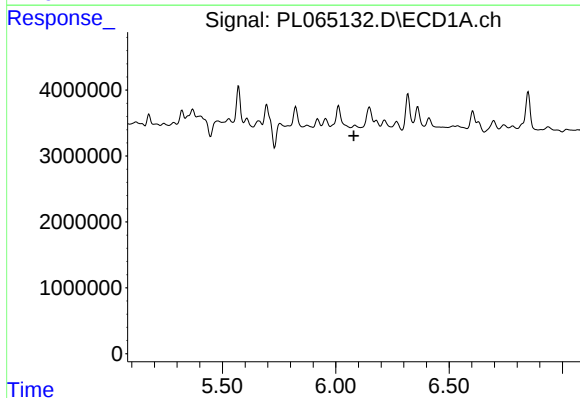


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.079 min
Response: 0
Conc: N.D.

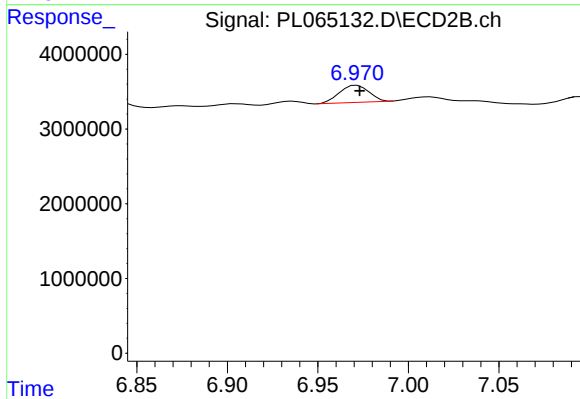

#16 4,4'-DDD


R.T.: 6.972 min
Delta R.T.: -0.002 min
Response: 2597522
Conc: 1.29 ng/ml

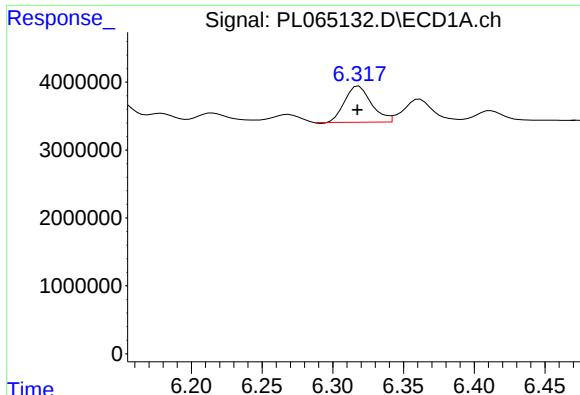

#17 4,4'-DDT


R.T.: 6.318 min
Delta R.T.: 0.001 min
Response: 6987414
Conc: 2.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

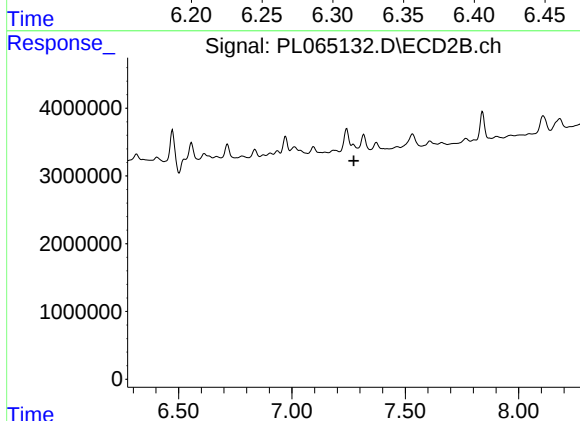


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

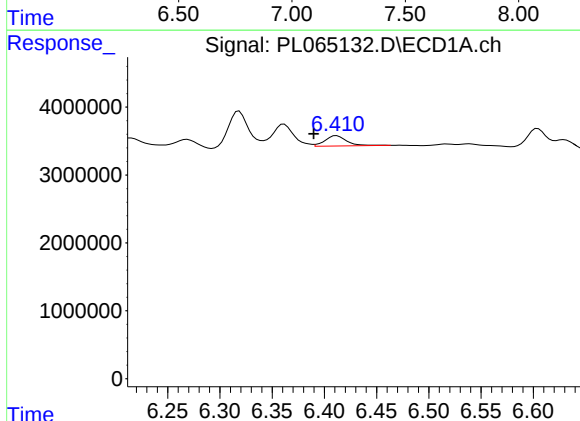


#18 Endrin aldehyde

R.T.: 6.412 min
Delta R.T.: 0.022 min
Response: 2205634
Conc: 0.86 ng/ml

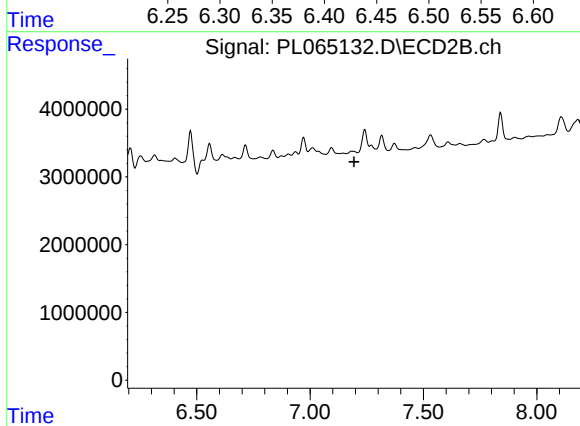

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.194 min
Response: 0
Conc: N.D.

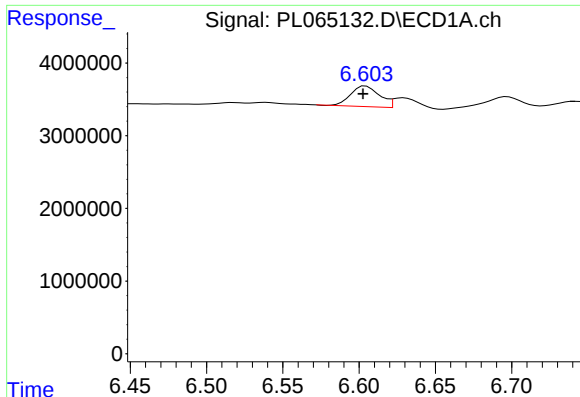

#19 Endosulfan Sulfate


R.T.: 6.604 min
Delta R.T.: 0.002 min
Response: 3709624
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

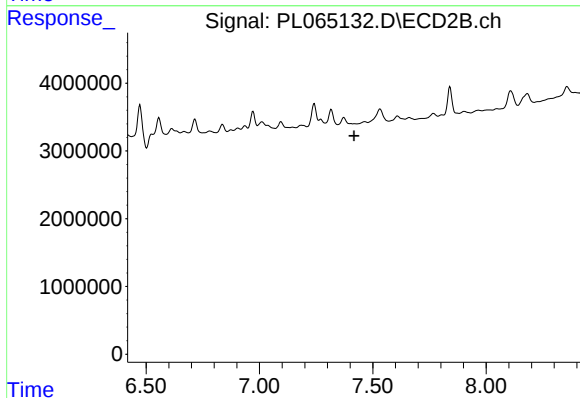


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

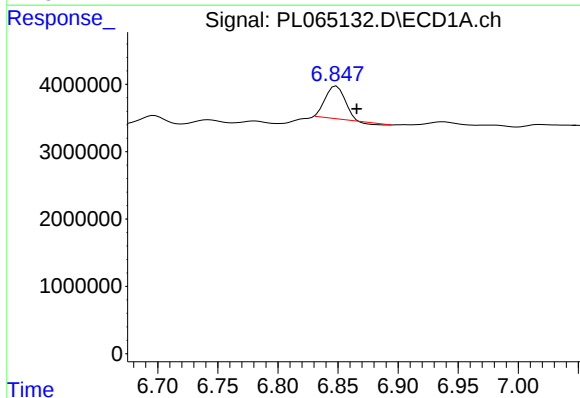


#20 Methoxychlor

R.T.: 6.849 min
Delta R.T.: -0.017 min
Response: 5380158
Conc: 3.41 ng/ml

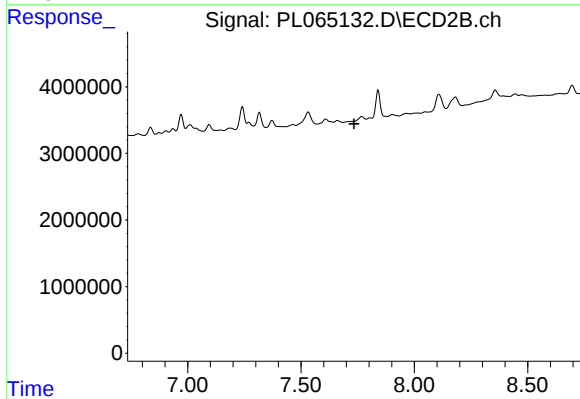

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.734 min
Response: 0
Conc: N.D.

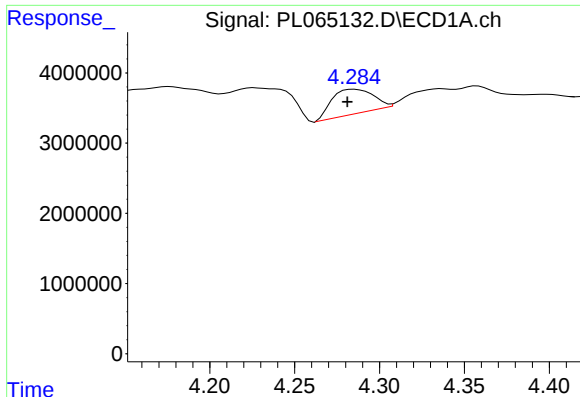

#23 Chlordane-1


R.T.: 4.285 min
Delta R.T.: 0.004 min
Response: 5915358
Conc: 46.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

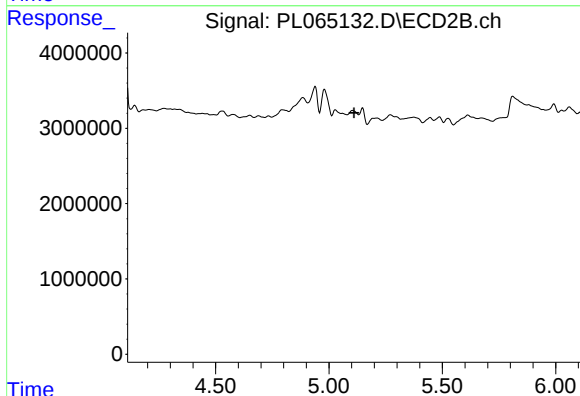


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

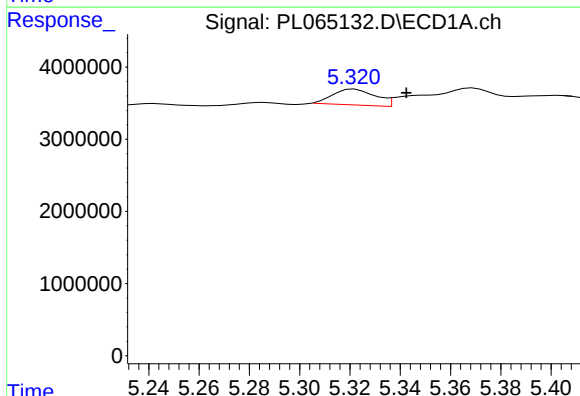


#25 Chlordane-3

R.T.: 5.322 min
Delta R.T.: -0.021 min
Response: 2578619
Conc: 6.46 ng/ml

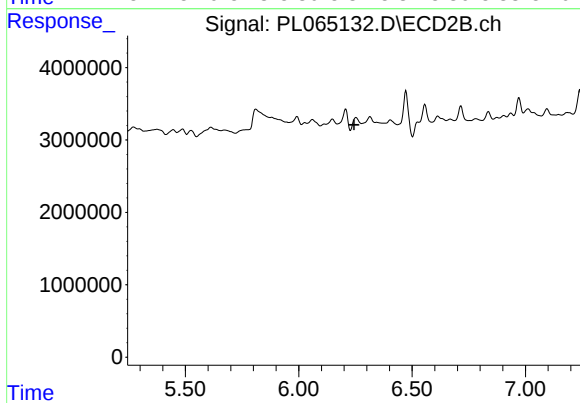

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.244 min
Response: 0
Conc: N.D.

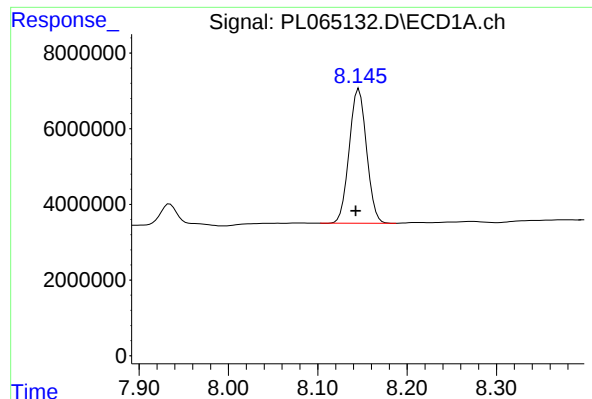

#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: 0.004 min
Response: 47862668
Conc: 17.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

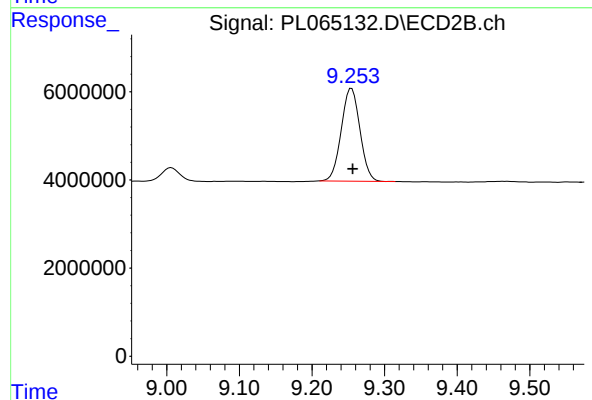

#28 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.002 min
Response: 37608508
Conc: 17.12 ng/ml