

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 10:56
 Operator : AR\AJ
 Sample : M1554-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HA-2A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 11:53:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	66436331	53890139	22.594	21.702
28)	SA Decachlor...	8.139	9.250	40702827	32446371	14.667	14.772
Target Compounds							
6)	B beta-BHC	4.398	0.000	1179797	0	0.632	N.D. #
9)	A Endosulfan I	5.473f	0.000	1129142	0	0.316	N.D. #
12)	B 4,4'-DDE	5.546f	0.000	50872600	0	14.154	N.D. #
15)	B Endosulfa...	6.211	0.000	954436	0	0.304	N.D. #
16)	A 4,4'-DDD	6.095f	0.000	6083550	0	2.044	N.D. #
17)	MA 4,4'-DDT	0.000	7.262	0	8323104	N.D.	4.247 #
18)	B Endrin al...	6.404	0.000	2517497	0	0.982	N.D. #
27)	Chlordane-5	6.211f	0.000	954436	0	7.350	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 10:56
Operator : AR\AJ
Sample : M1554-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HA-2A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 11:53:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

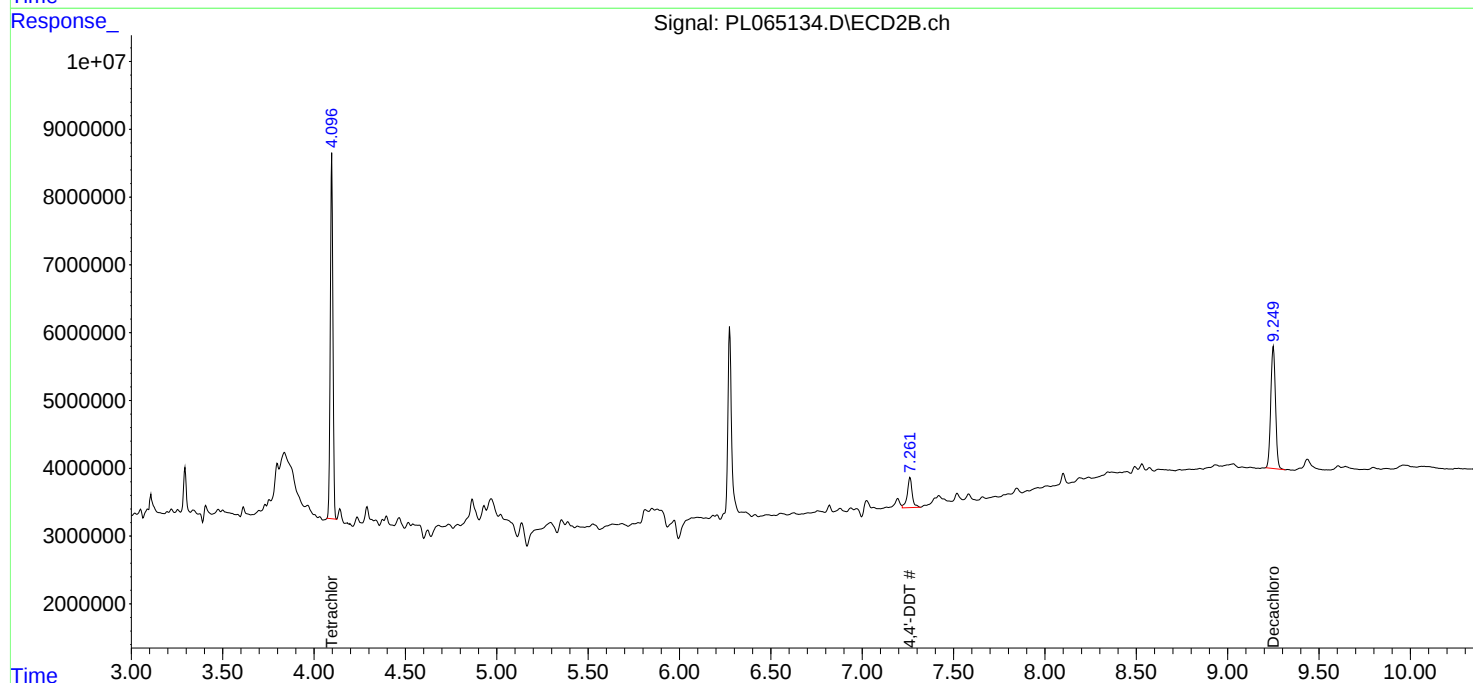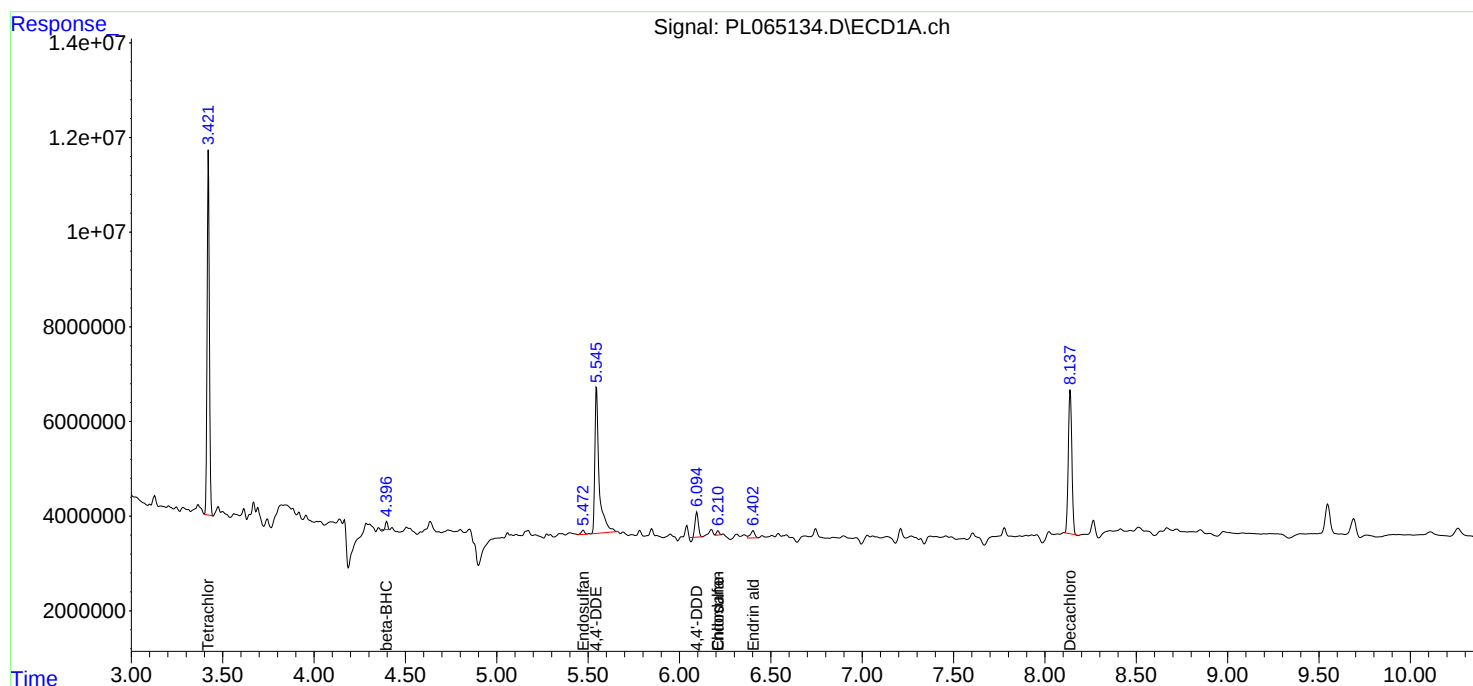


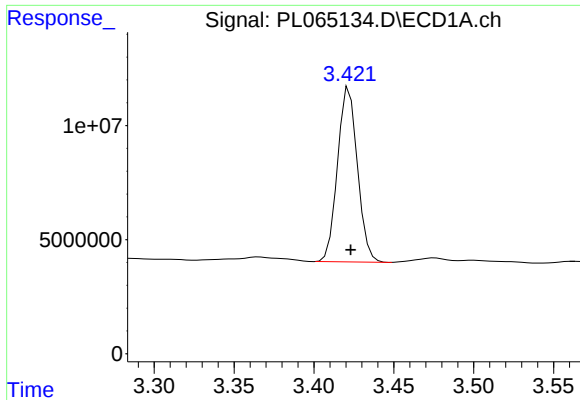

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 66436331
Conc: 22.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-2A

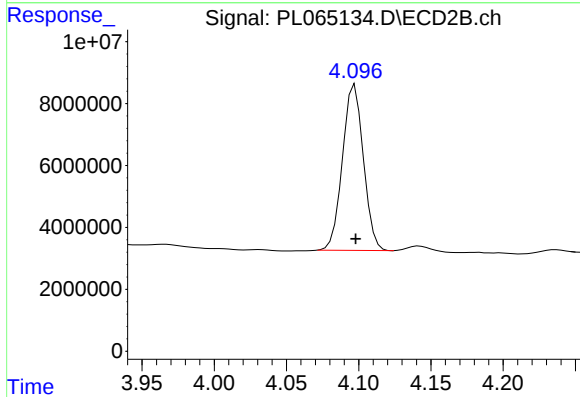


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 53890139
Conc: 21.70 ng/ml

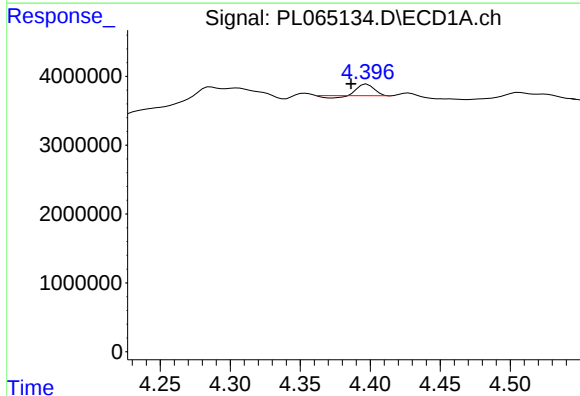


#6 beta-BHC

R.T.: 4.398 min
Delta R.T.: 0.011 min
Response: 1179797
Conc: 0.63 ng/ml

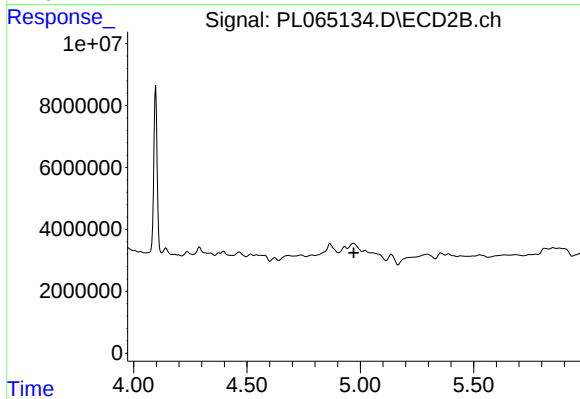

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.972 min
Response: 0
Conc: N.D.

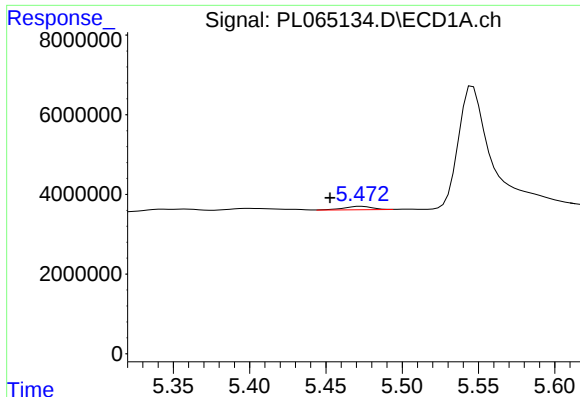

#9 Endosulfan I


R.T.: 5.473 min
Delta R.T.: 0.021 min
Response: 1129142
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-2A

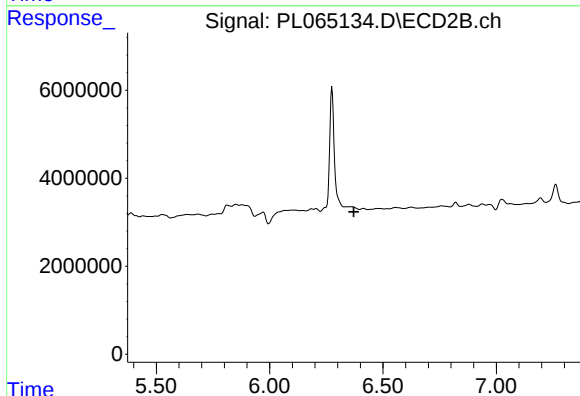


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.371 min
Response: 0
Conc: N.D.

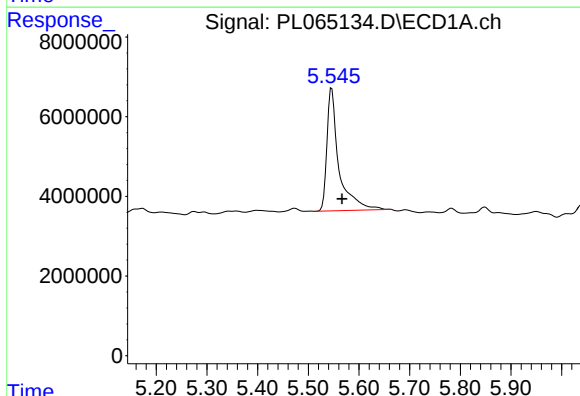


#12 4,4'-DDE

R.T.: 5.546 min
Delta R.T.: -0.020 min
Response: 50872600
Conc: 14.15 ng/ml

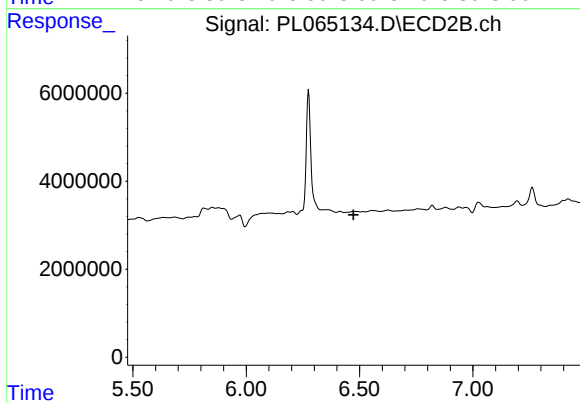

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

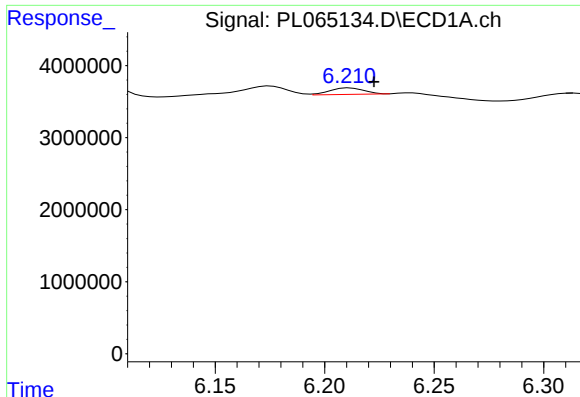

#15 Endosulfan II


R.T.: 6.211 min
Delta R.T.: -0.011 min
Response: 954436
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-2A

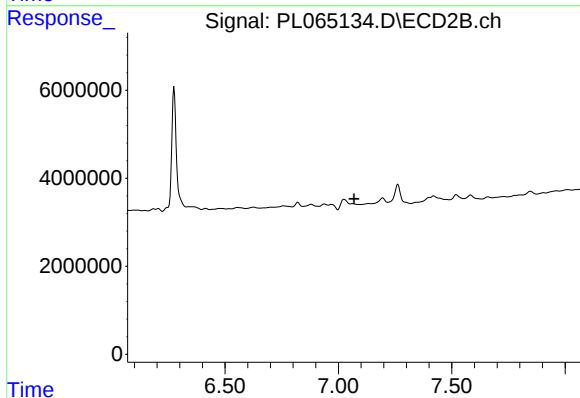


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

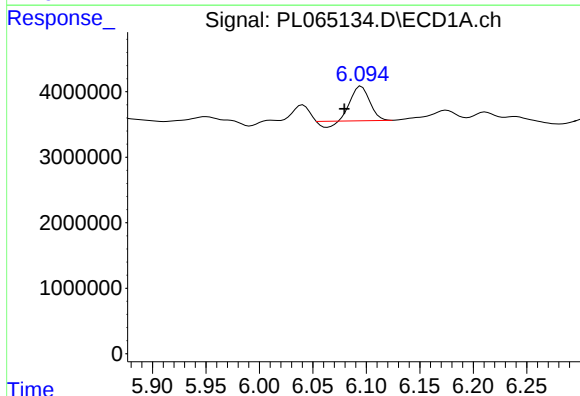


#16 4,4'-DDD

R.T.: 6.095 min
Delta R.T.: 0.016 min
Response: 6083550
Conc: 2.04 ng/ml

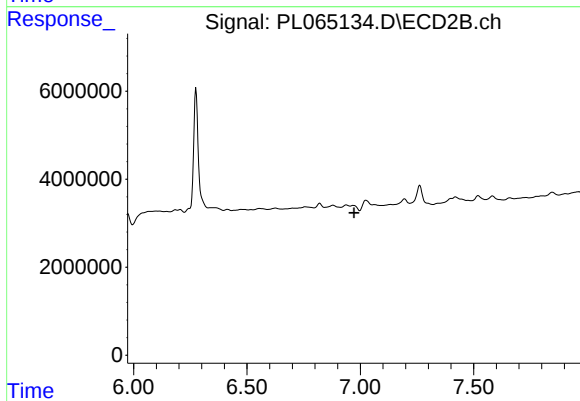

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.973 min
Response: 0
Conc: N.D.

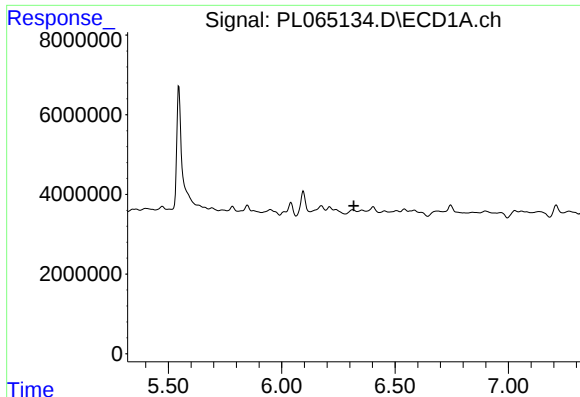

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HA-2A

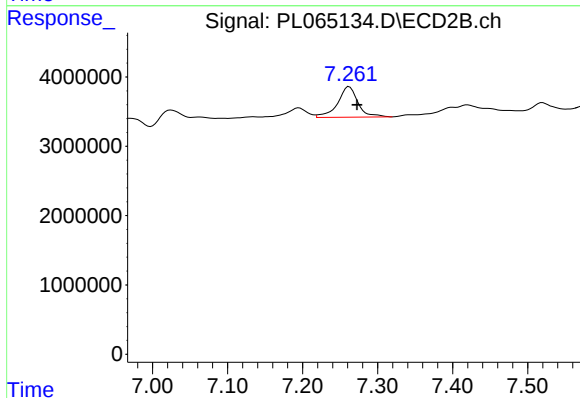


#17 4,4'-DDT

R.T.: 7.262 min
Delta R.T.: -0.010 min
Response: 8323104
Conc: 4.25 ng/ml

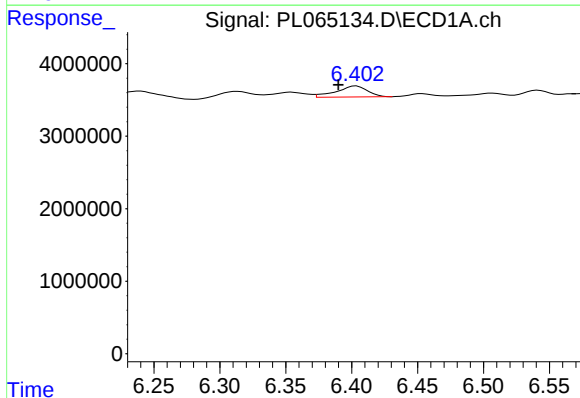


#18 Endrin aldehyde

R.T.: 6.404 min
Delta R.T.: 0.014 min
Response: 2517497
Conc: 0.98 ng/ml

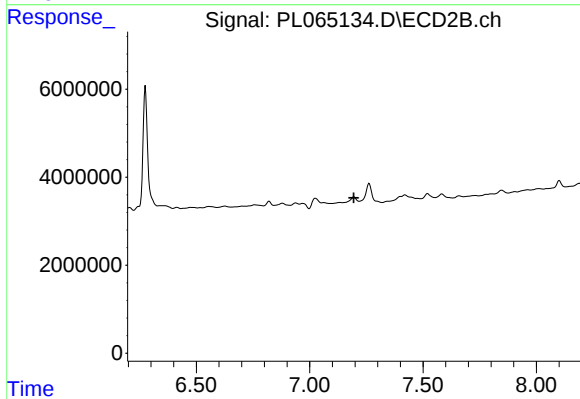

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.194 min
Response: 0
Conc: N.D.

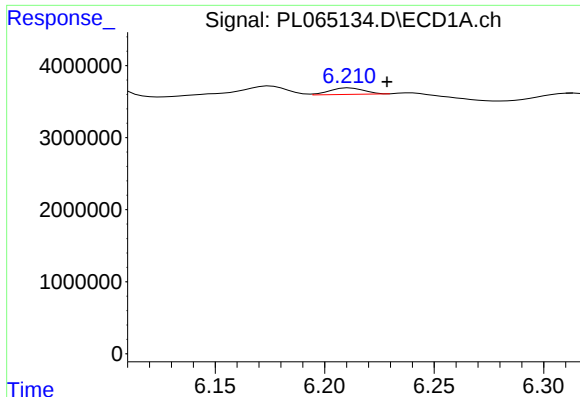

#27 Chlordane-5


R.T.: 6.211 min
Delta R.T.: -0.017 min
Response: 954436
Conc: 7.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-2A

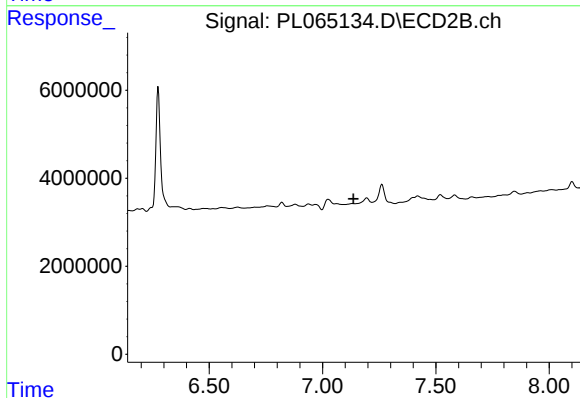


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.137 min
Response: 0
Conc: N.D.

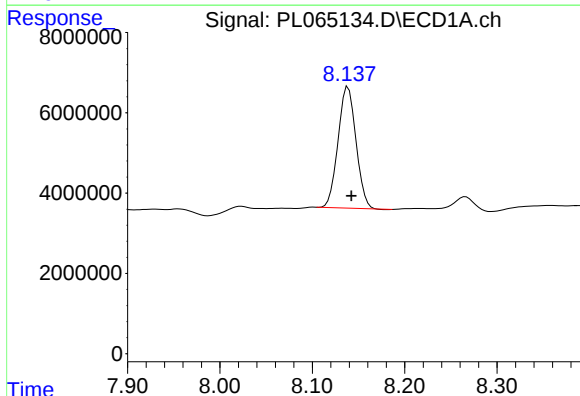

#28 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.004 min
Response: 40702827
Conc: 14.67 ng/ml

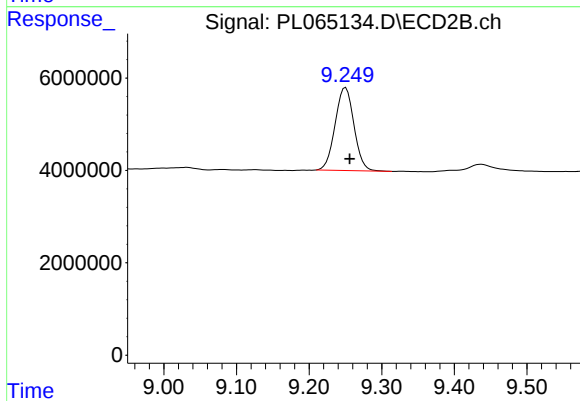

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 32446371
Conc: 14.77 ng/ml