

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030821\  
 Data File : PL065136.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 08 Mar 2021 11:24  
 Operator : AR\AJ  
 Sample : M1565-03  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 TP-2

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 08 11:54:12 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL030521.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Mar 05 02:26:14 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.421  | 4.097 | 50258605 | 41668178 | 17.092 | 16.780 |
| 28)                         | SA Decachlor... | 8.138  | 9.249 | 30901595 | 23864802 | 11.135 | 10.865 |
|                             |                 |        |       |          |          |        |        |
| Target Compounds            |                 |        |       |          |          |        |        |
| 9)                          | A Endosulfan I  | 5.472f | 0.000 | 1808985  | 0        | 0.506  | N.D. # |
| 12)                         | B 4,4'-DDE      | 5.561  | 0.000 | 1232917  | 0        | 0.343  | N.D. # |
| 13)                         | MA Dieldrin     | 5.690  | 0.000 | 2808623  | 0        | 0.759  | N.D. # |
| 14)                         | MA Endrin       | 5.952  | 0.000 | 1276844  | 0        | 0.372  | N.D. # |
| 16)                         | A 4,4'-DDD      | 6.091  | 0.000 | 2487161  | 0        | 0.835  | N.D. # |
| 17)                         | MA 4,4'-DDT     | 6.311  | 0.000 | 1428428  | 0        | 0.512  | N.D. # |
| 23)                         | Chlordane-1     | 4.282  | 0.000 | 437906   | 0        | 3.436  | N.D. # |
| -----                       |                 |        |       |          |          |        |        |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030821\  
Data File : PL065136.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 08 Mar 2021 11:24  
Operator : AR\AJ  
Sample : M1565-03  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
TP-2

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 08 11:54:12 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL030521.M  
Quant Title : GC Extractables  
QLast Update : Fri Mar 05 02:26:14 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

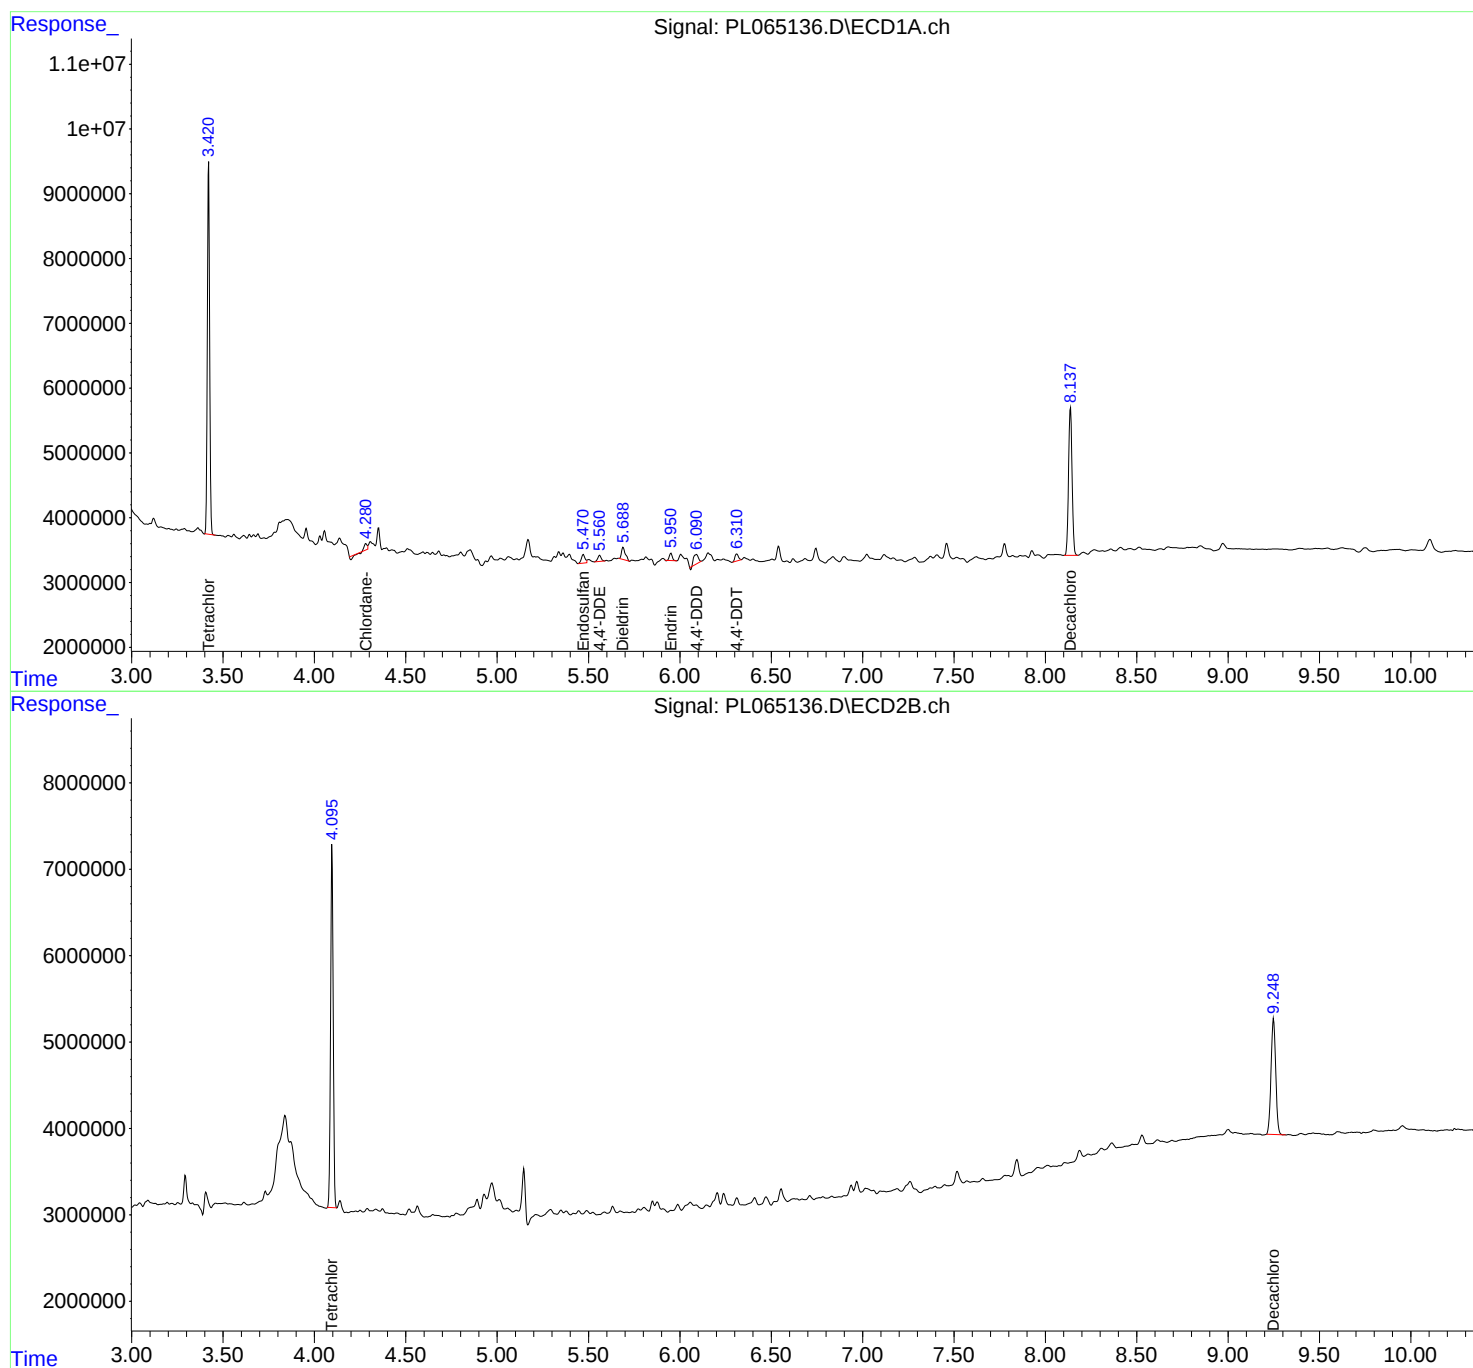


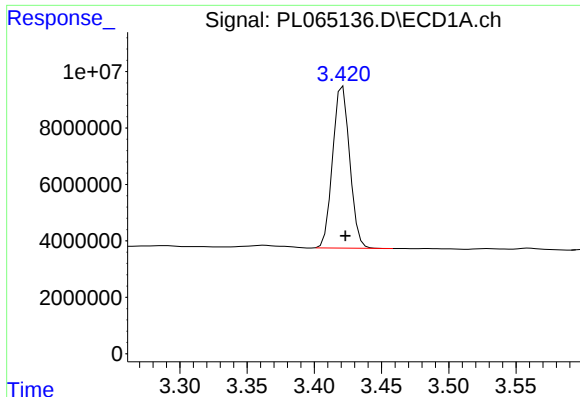

#1 Tetrachloro-m-xylene


R.T.: 3.421 min  
Delta R.T.: -0.002 min  
Response: 50258605  
Conc: 17.09 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-2

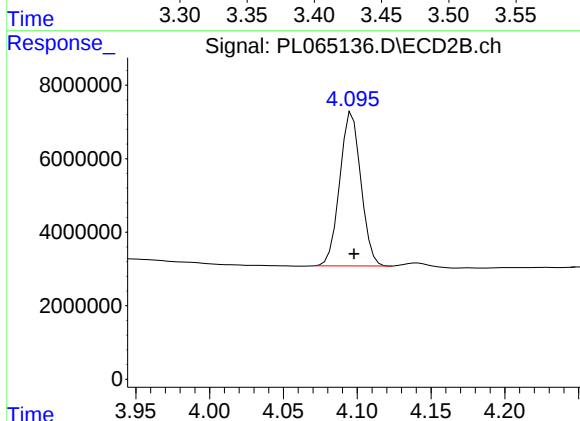


#1 Tetrachloro-m-xylene

R.T.: 4.097 min  
Delta R.T.: -0.001 min  
Response: 41668178  
Conc: 16.78 ng/ml

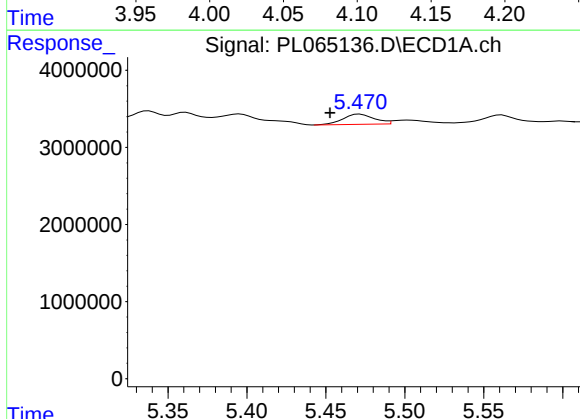


#9 Endosulfan I

R.T.: 5.472 min  
Delta R.T.: 0.019 min  
Response: 1808985  
Conc: 0.51 ng/ml

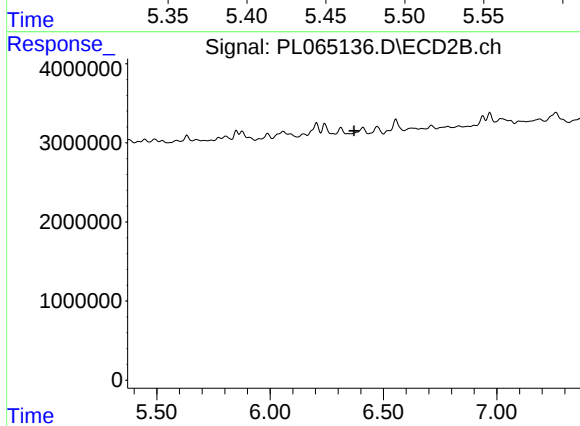

#9 Endosulfan I


R.T.: 0.000 min  
Exp R.T.: 6.371 min  
Response: 0  
Conc: N.D.

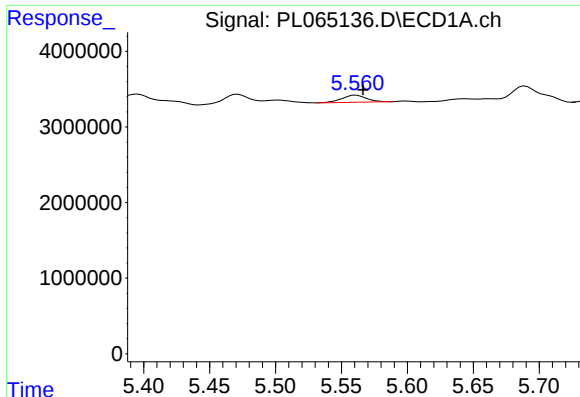

#12 4,4'-DDE


R.T.: 5.561 min  
Delta R.T.: -0.005 min  
Response: 1232917  
Conc: 0.34 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-2

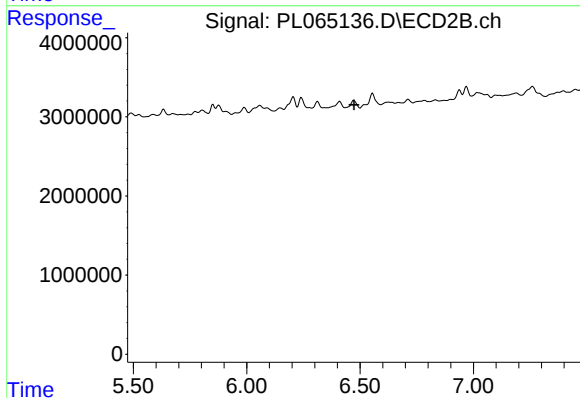


#12 4,4'-DDE

R.T.: 0.000 min  
Exp R.T. : 6.474 min  
Response: 0  
Conc: N.D.

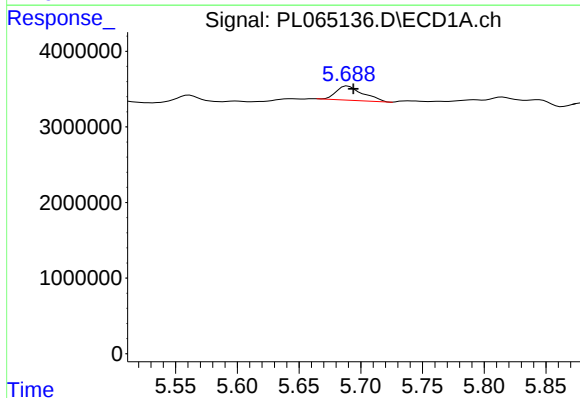


#13 Dieldrin

R.T.: 5.690 min  
Delta R.T.: -0.004 min  
Response: 2808623  
Conc: 0.76 ng/ml

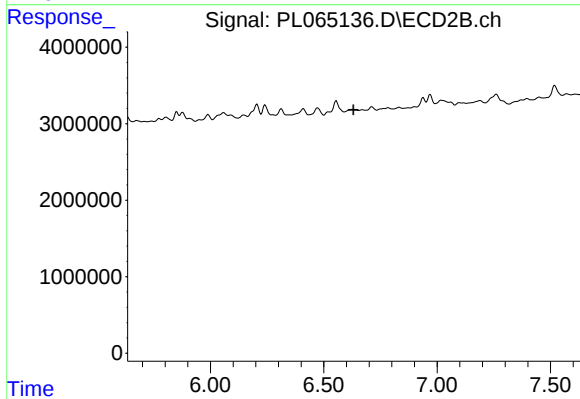

#13 Dieldrin


R.T.: 0.000 min  
Exp R.T. : 6.632 min  
Response: 0  
Conc: N.D.

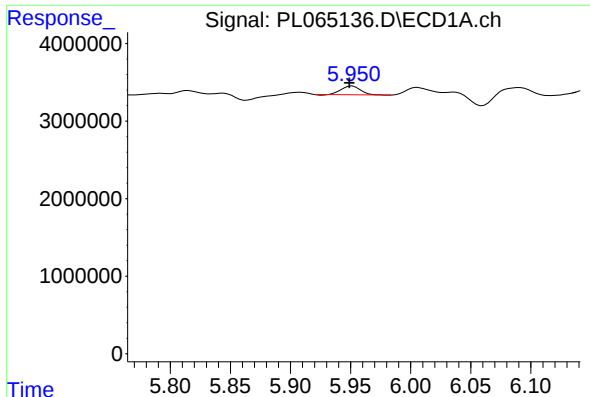

#14 Endrin


R.T.: 5.952 min  
Delta R.T.: 0.003 min  
Response: 1276844  
Conc: 0.37 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-2

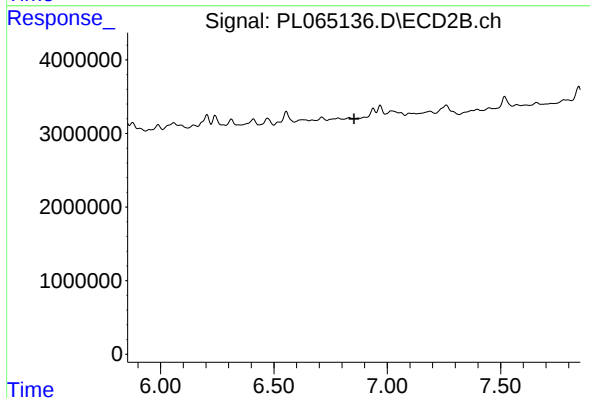


#14 Endrin

R.T.: 0.000 min  
Exp R.T. : 6.853 min  
Response: 0  
Conc: N.D.

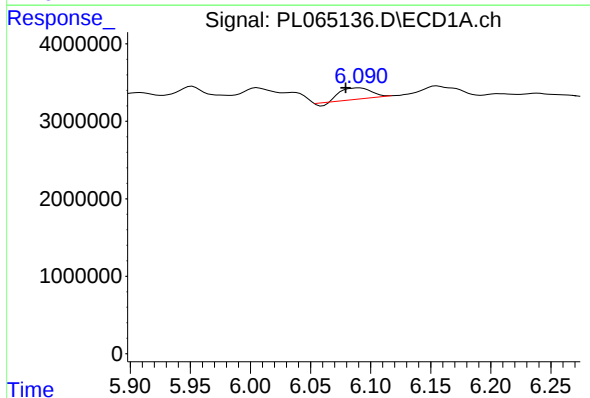


#16 4,4'-DDD

R.T.: 6.091 min  
Delta R.T.: 0.012 min  
Response: 2487161  
Conc: 0.84 ng/ml

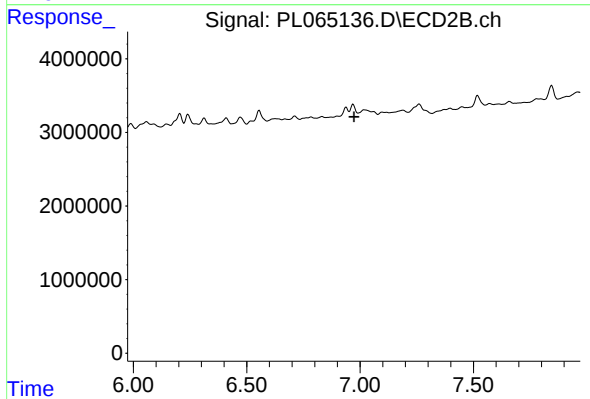

#16 4,4'-DDD


R.T.: 0.000 min  
Exp R.T. : 6.973 min  
Response: 0  
Conc: N.D.

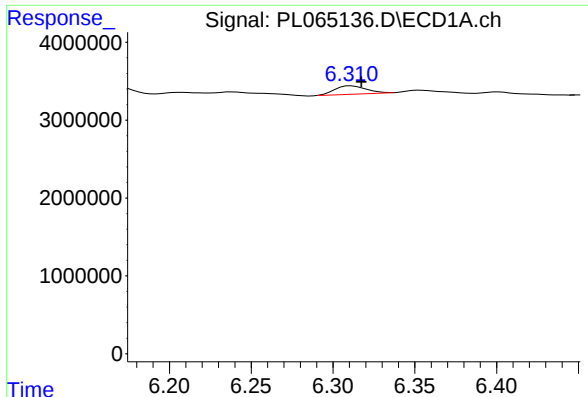

#17 4,4'-DDT


R.T.: 6.311 min  
Delta R.T.: -0.006 min  
Response: 1428428  
Conc: 0.51 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-2

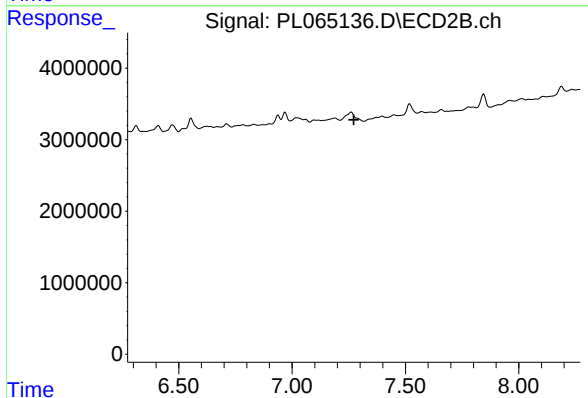


#17 4,4'-DDT

R.T.: 0.000 min  
Exp R.T. : 7.273 min  
Response: 0  
Conc: N.D.

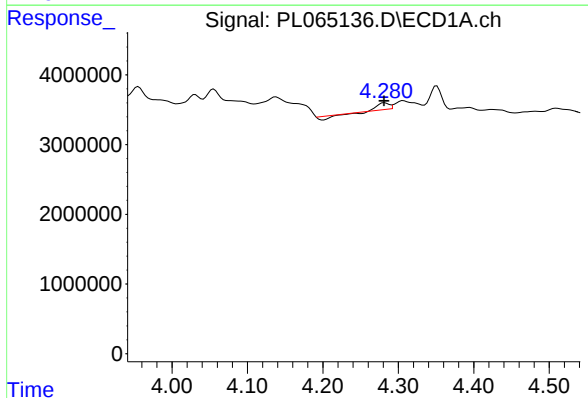


#23 Chlordane-1

R.T.: 4.282 min  
Delta R.T.: 0.000 min  
Response: 437906  
Conc: 3.44 ng/ml

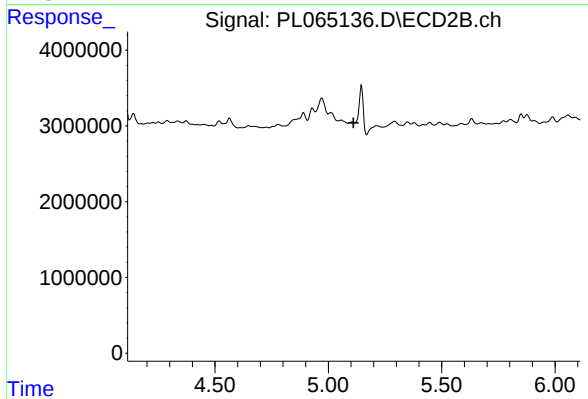

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T. : 5.112 min  
Response: 0  
Conc: N.D.

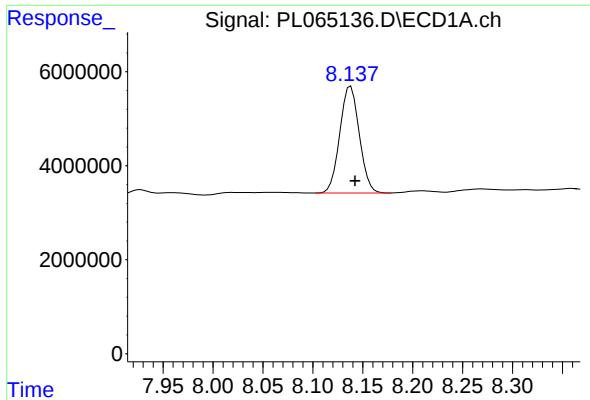

#28 Decachlorobiphenyl

R.T.: 8.138 min  
Delta R.T.: -0.004 min  
Response: 30901595  
Conc: 11.14 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-2

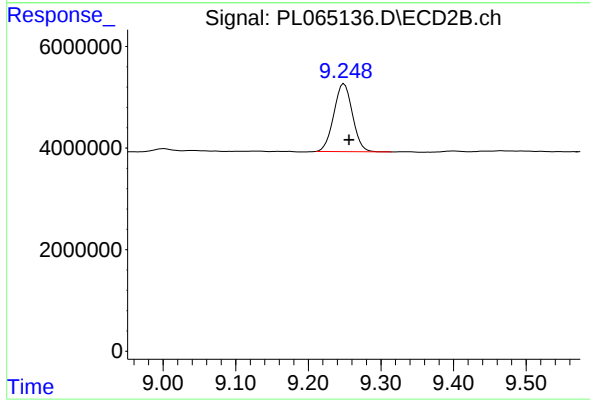

#28 Decachlorobiphenyl

R.T.: 9.249 min  
Delta R.T.: -0.007 min  
Response: 23864802  
Conc: 10.86 ng/ml