

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 10:27
 Operator : AR\AJ
 Sample : M1551-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VEOLIA-VNJ-204

Manual Integrations
 APPROVED

Ankita
 3/9/2021 2:03:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 11:53:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427	4.098	40953706	34299003	13.928	13.812
28)	SA Decachlor...	8.146	9.255	47862668	37608508	17.247	17.122
Target Compounds							
12)	B 4,4'-DDE	5.570	6.471	6210407	5340668	1.728m	2.136m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 10:27
Operator : AR\AJ
Sample : M1551-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204


Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 11:53:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

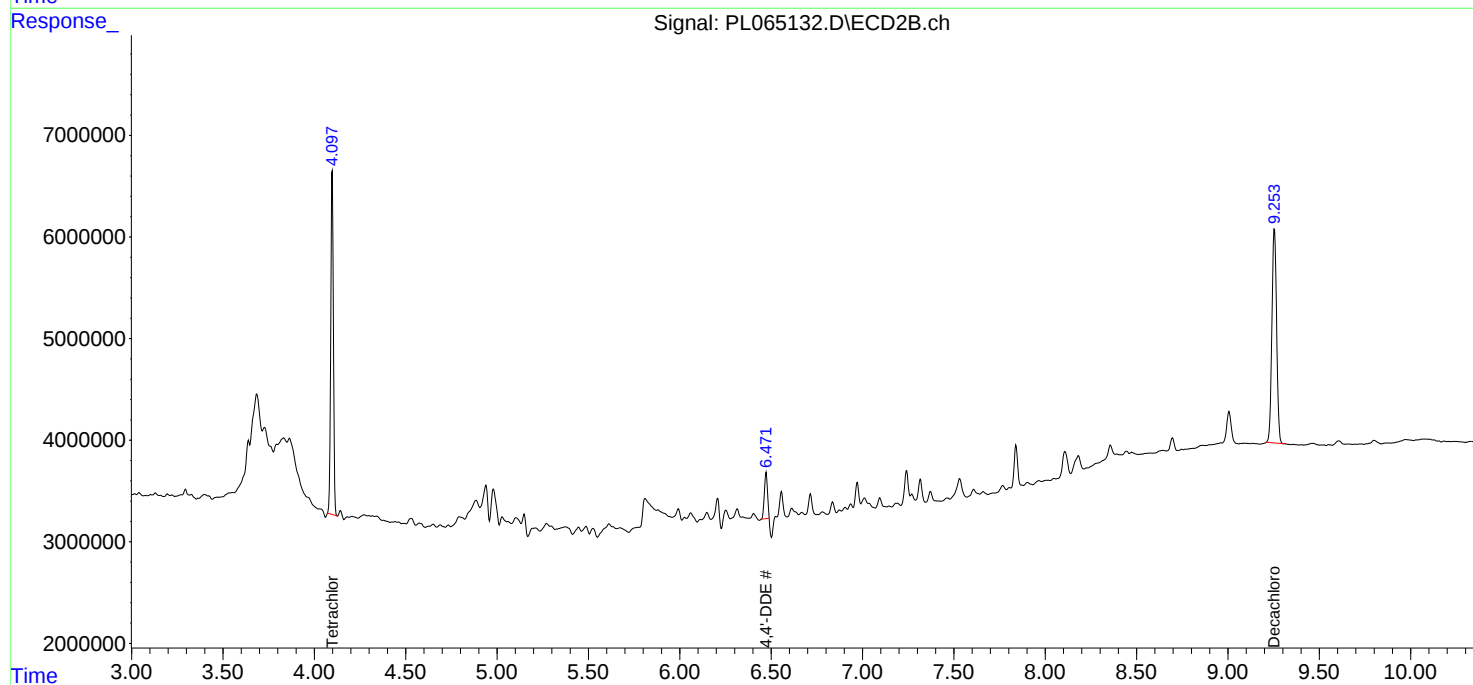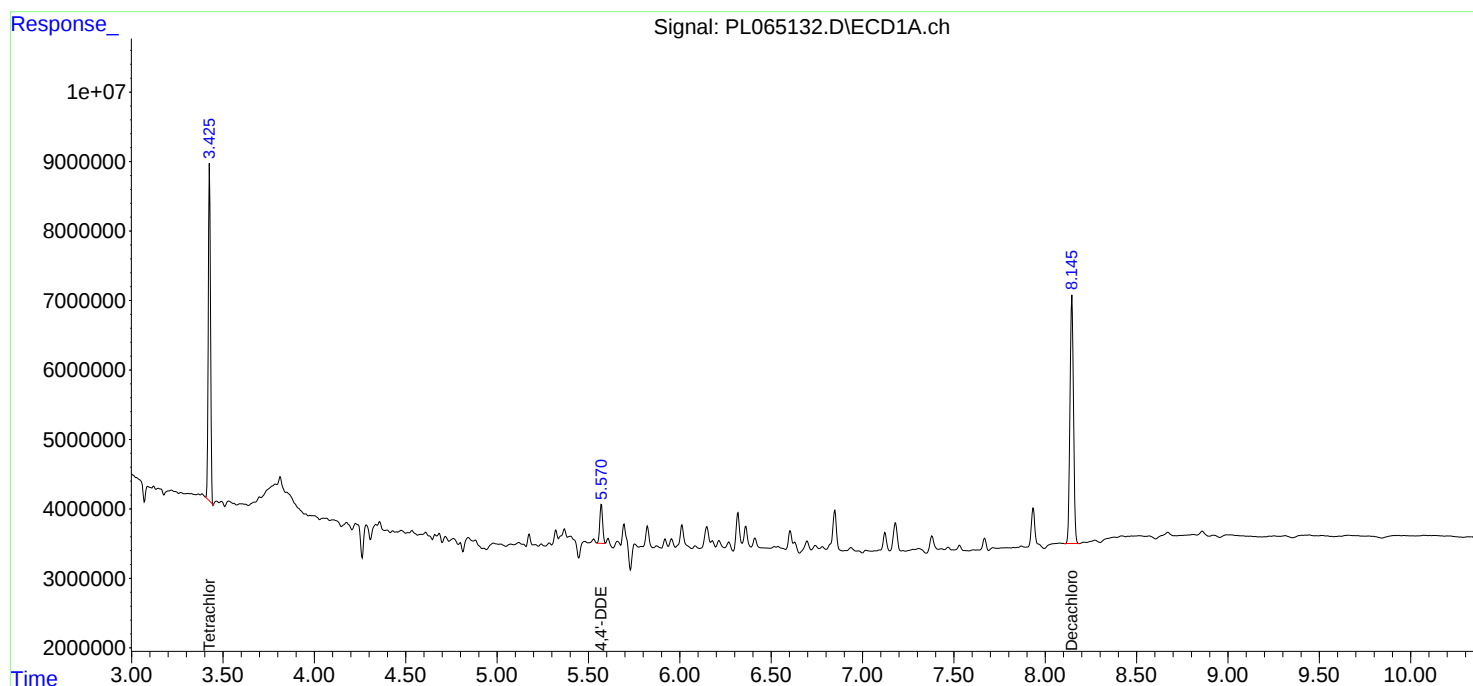

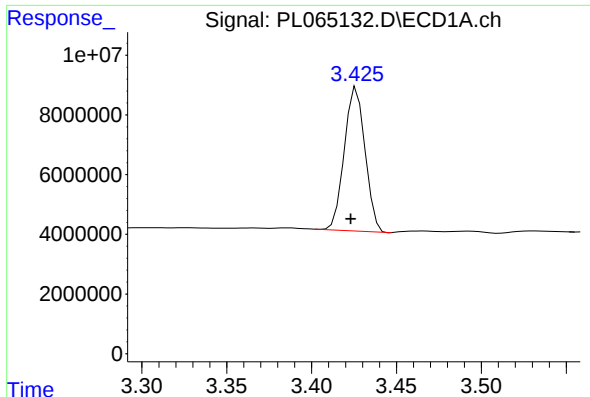


#1 Tetrachloro-m-xylene

R.T.: 3.427 min
Delta R.T.: 0.004 min
Response: 40953706
Conc: 13.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204


Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:49 PM

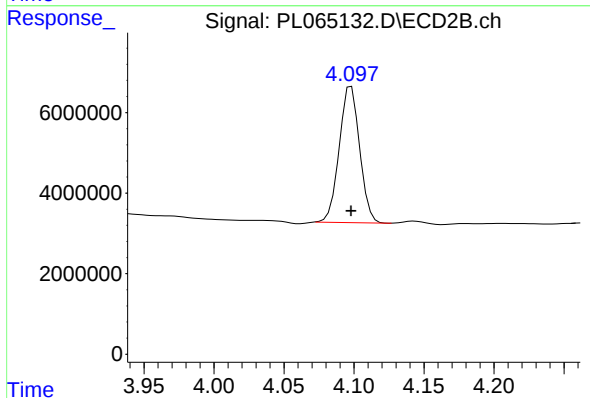


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 34299003
Conc: 13.81 ng/ml

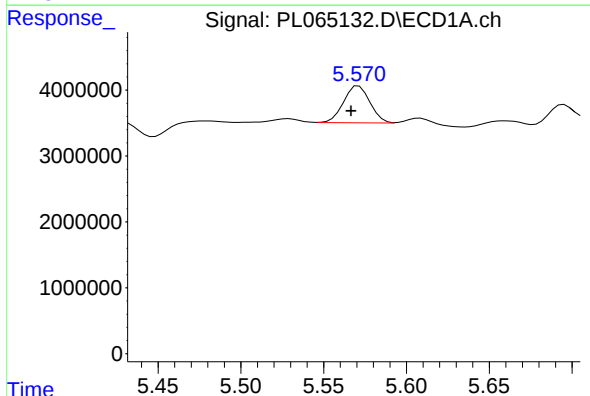


#12 4,4'-DDE

R.T.: 5.570 min
Delta R.T.: 0.003 min
Response: 6210407
Conc: 1.73 ng/ml m

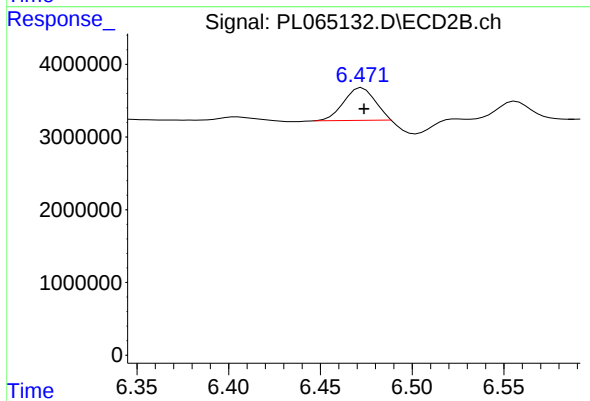

#12 4,4'-DDE

R.T.: 6.471 min
Delta R.T.: -0.002 min
Response: 5340668
Conc: 2.14 ng/ml m

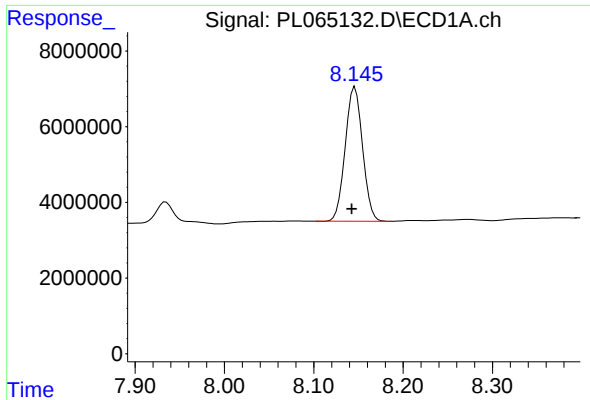


#28 Decachlorobiphenyl

R.T.: 8.146 min
Delta R.T.: 0.004 min
Response: 47862668
Conc: 17.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-VNJ-204

Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:49 PM

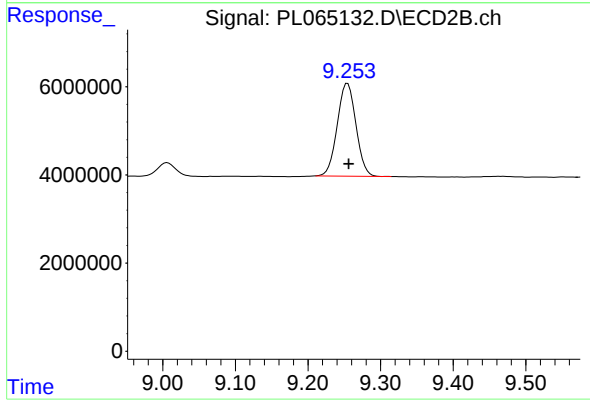

#28 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.002 min
Response: 37608508
Conc: 17.12 ng/ml