

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 10:56
 Operator : AR\AJ
 Sample : M1554-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HA-2A

Manual Integrations
 APPROVED

Ankita
 3/9/2021 2:03:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 11:53:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	66436331	53890139	22.594	21.702
28)	SA Decachlor...	8.139	9.250	40702827	32446371	14.667	14.772
Target Compounds							
17)	MA 4,4'-DDT	6.312	7.262	1526630	8323104	0.548m	4.247 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 10:56
Operator : AR\AJ
Sample : M1554-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
HA-2A


Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 11:53:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

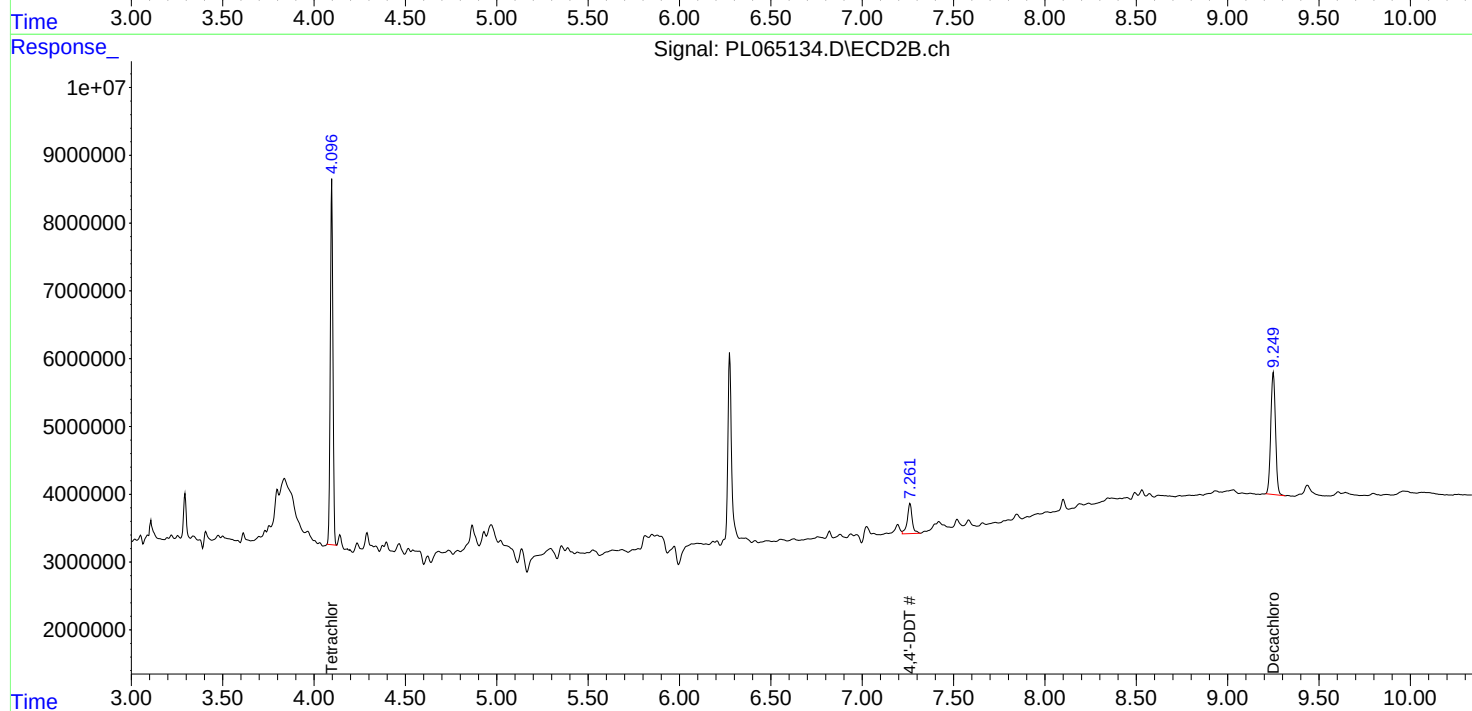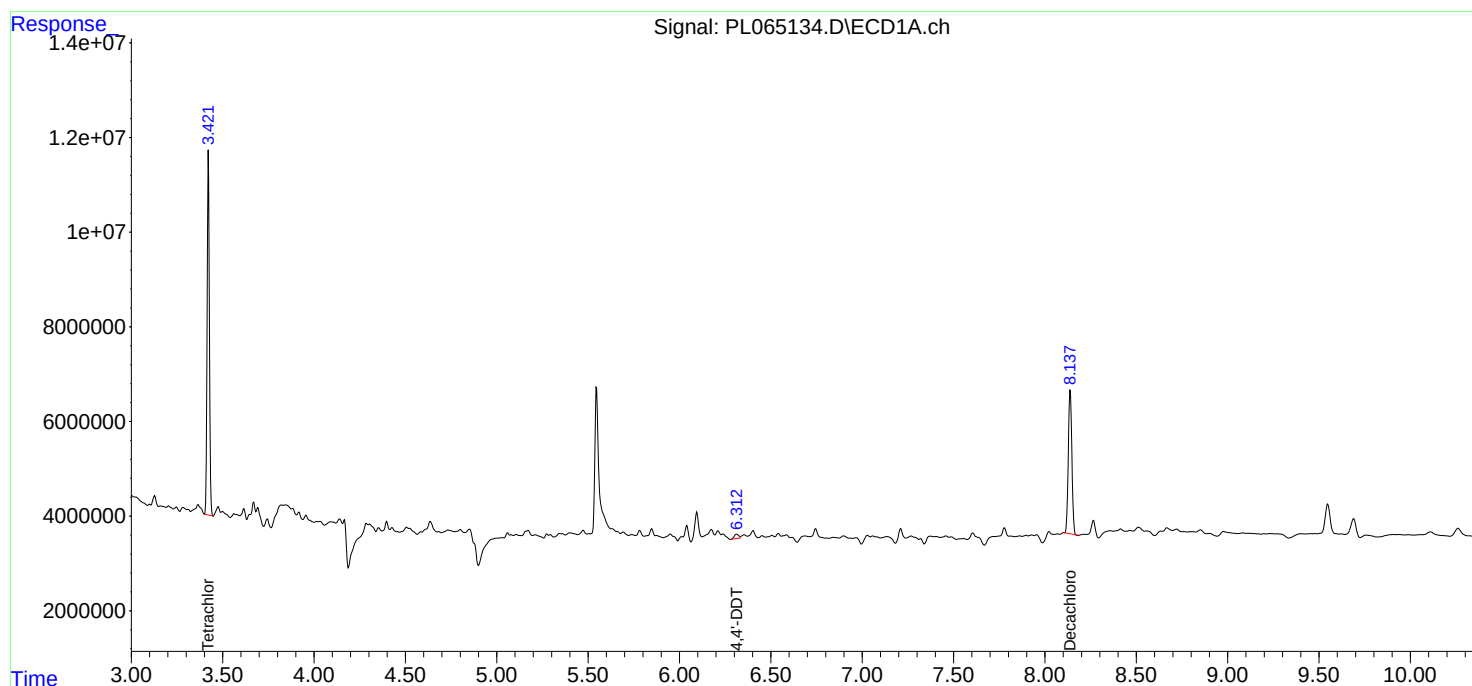

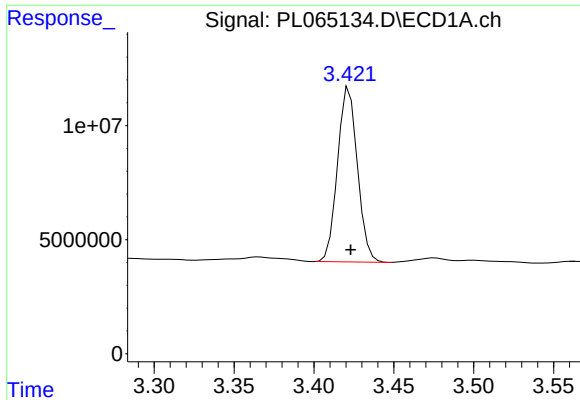


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 66436331
Conc: 22.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-2A


Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:54 PM

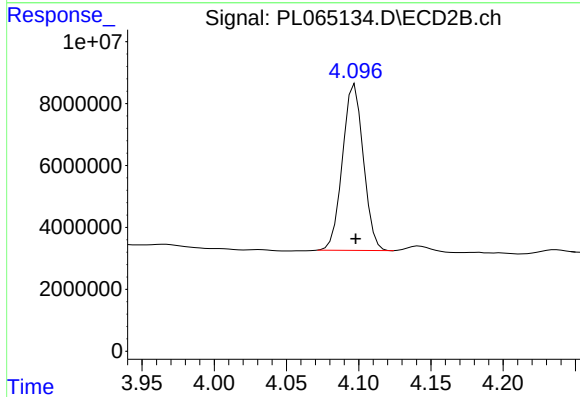


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 53890139
Conc: 21.70 ng/ml

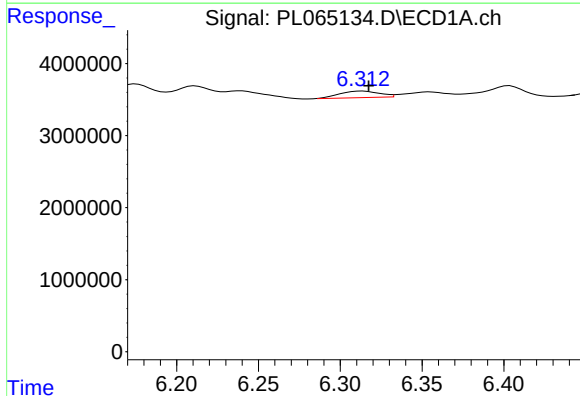


#17 4,4'-DDT

R.T.: 6.312 min
Delta R.T.: -0.005 min
Response: 1526630
Conc: 0.55 ng/ml m

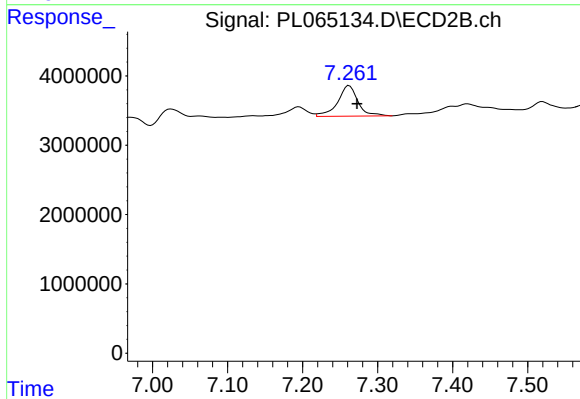

#17 4,4'-DDT

R.T.: 7.262 min
Delta R.T.: -0.010 min
Response: 8323104
Conc: 4.25 ng/ml

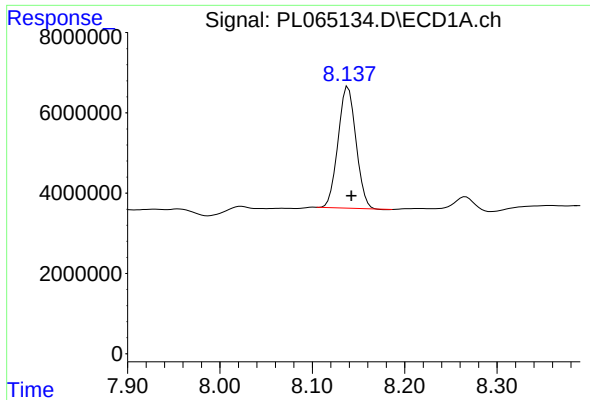


#28 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.004 min
Response: 40702827
Conc: 14.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-2A

Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:54 PM

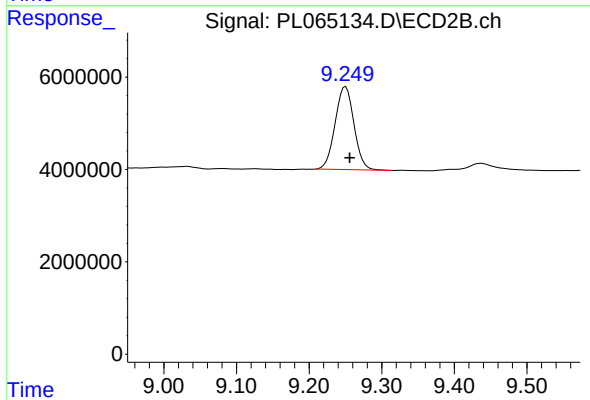

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 32446371
Conc: 14.77 ng/ml