

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 11:38
 Operator : AR\AJ
 Sample : M1565-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 13:15:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.096	31337201	26878131	10.657	10.824
28)	SA Decachlor...	8.138	9.250	30154039	22127323	10.866	10.074
Target Compounds							
12)	B 4,4'-DDE	5.563	6.470	6245058	4993870	1.737	1.998



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 11:38
Operator : AR\AJ
Sample : M1565-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 13:15:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

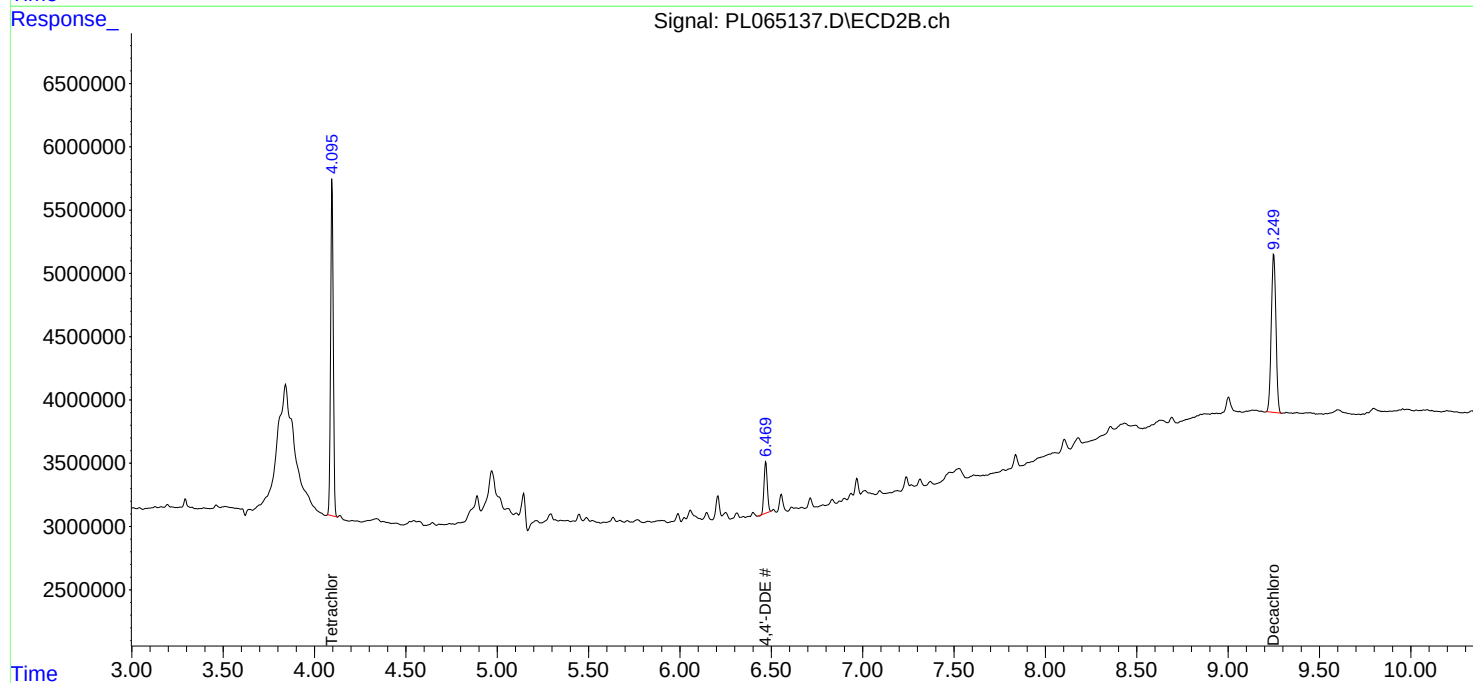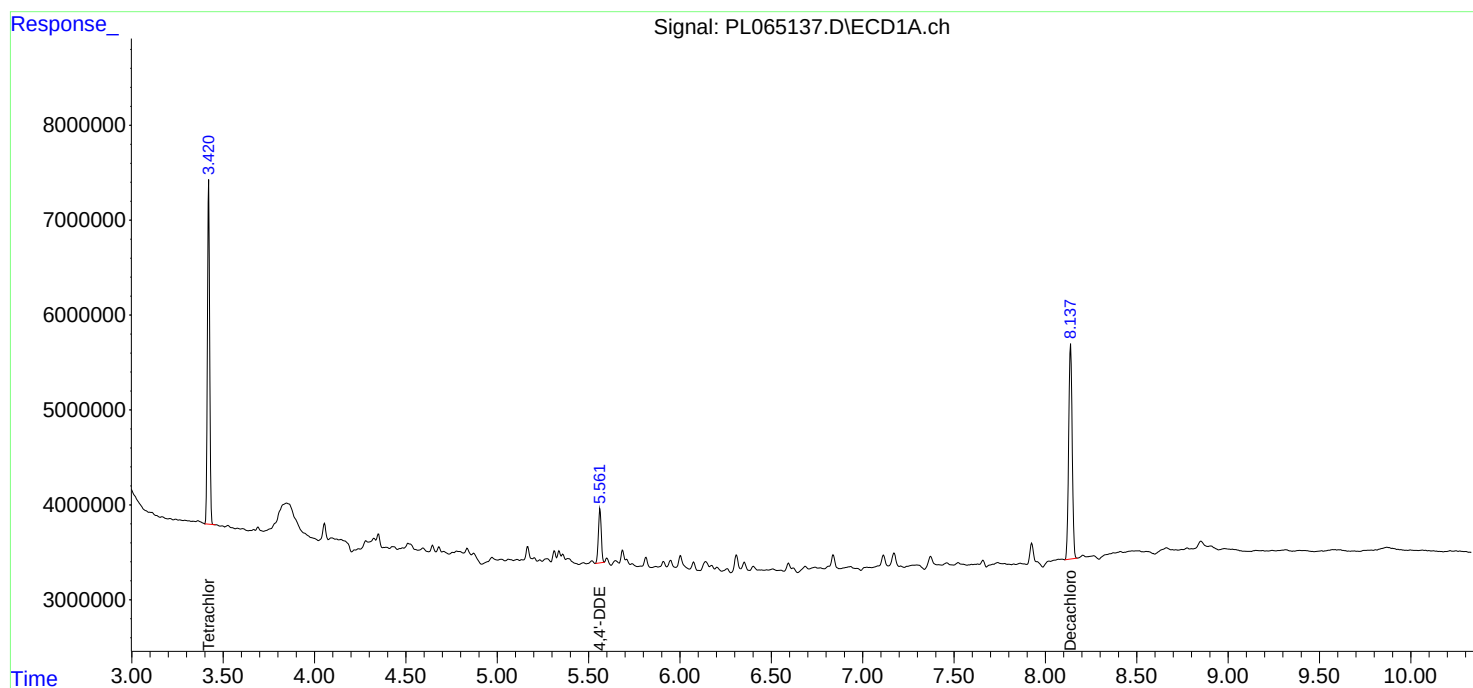


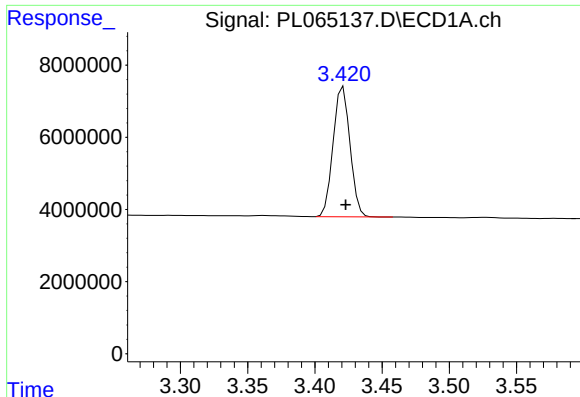

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: -0.002 min
Response: 31337201
Conc: 10.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

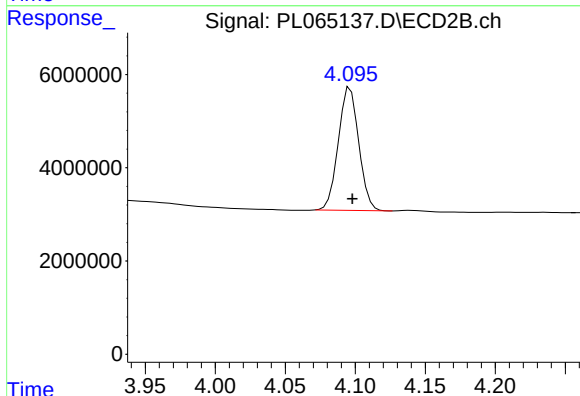


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.002 min
Response: 26878131
Conc: 10.82 ng/ml

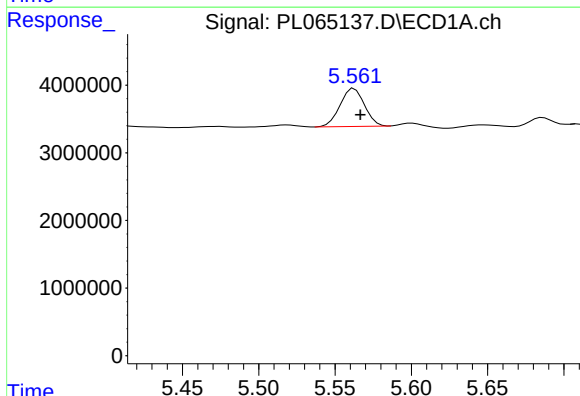


#12 4,4'-DDE

R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 6245058
Conc: 1.74 ng/ml

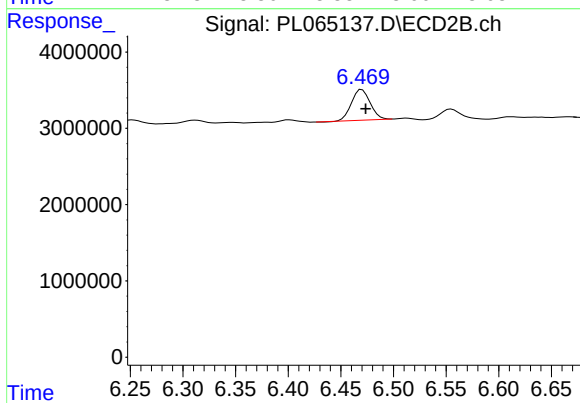

#12 4,4'-DDE


R.T.: 6.470 min
Delta R.T.: -0.004 min
Response: 4993870
Conc: 2.00 ng/ml

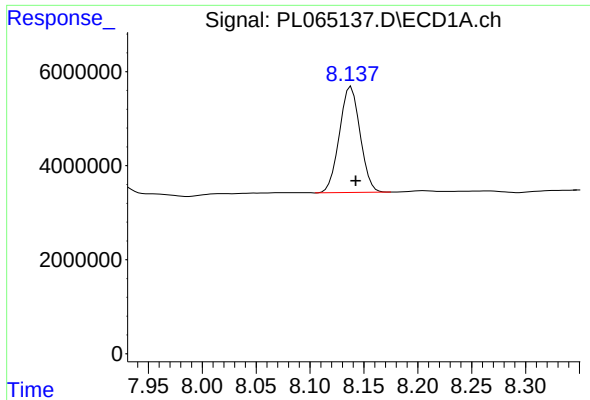

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 30154039
Conc: 10.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

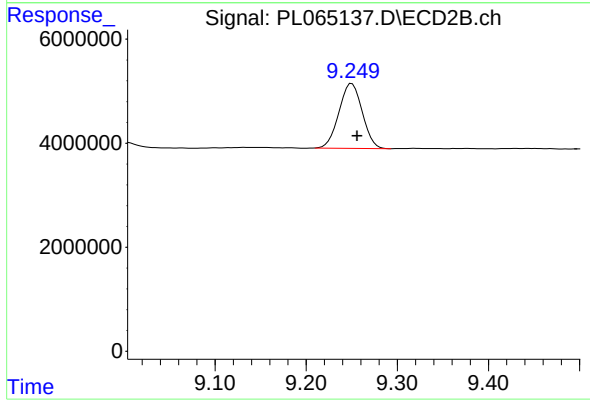

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 22127323
Conc: 10.07 ng/ml