

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 12:07
 Operator : AR\AJ
 Sample : M1567-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-02-030421

Manual Integrations
 APPROVED

Ankita
 3/9/2021 2:03:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 13:15:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	34466988	28451723	11.722	11.458
28)	SA Decachlor...	8.138	9.250	36641863	29437838	13.204	13.402
Target Compounds							
11)	B alpha-Chl...	5.396	6.313	3879672	5337787	1.012m	1.931 #
17)	MA 4,4'-DDT	6.311	7.266	4263391	1576290	1.529	0.804m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 12:07
Operator : AR\AJ
Sample : M1567-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PL-02-030421


Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 13:15:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

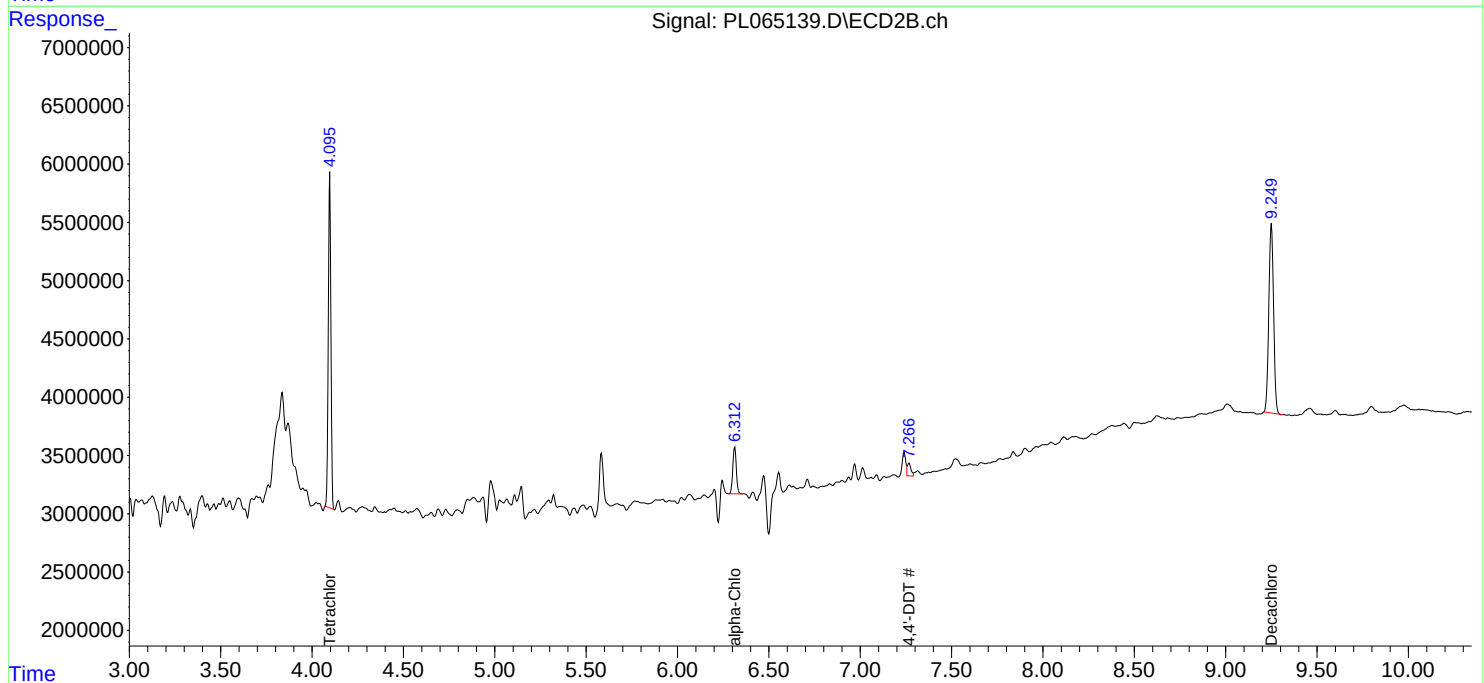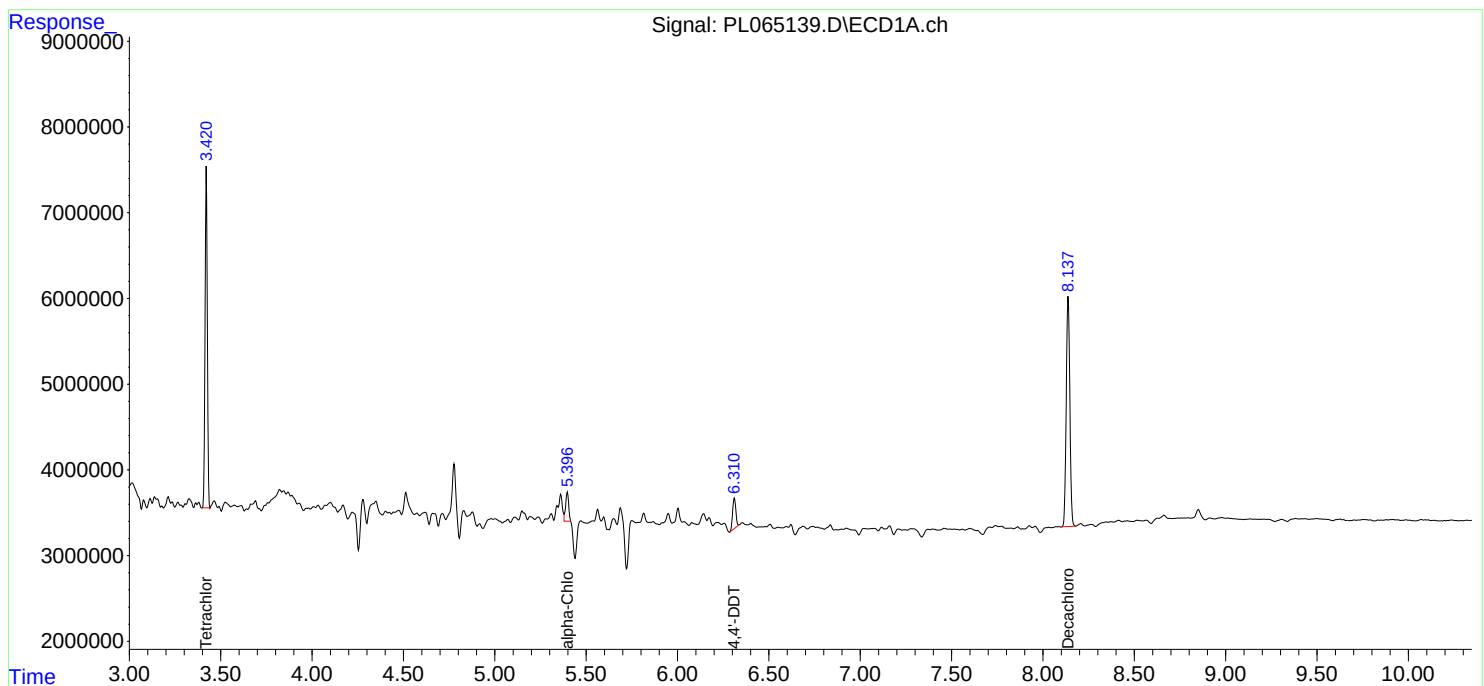

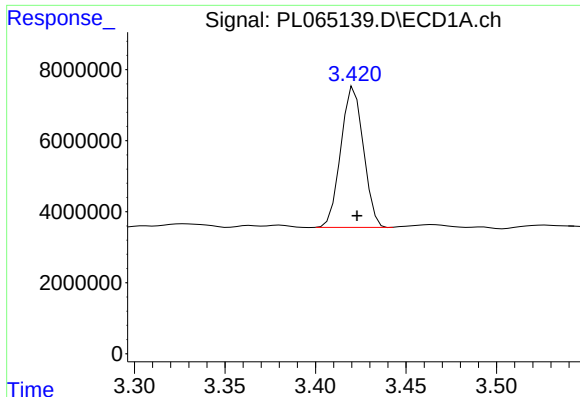


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 34466988
Conc: 11.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-030421


Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:58 PM

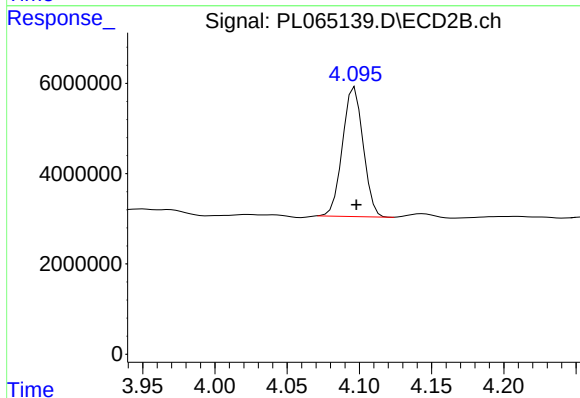


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.001 min
Response: 28451723
Conc: 11.46 ng/ml

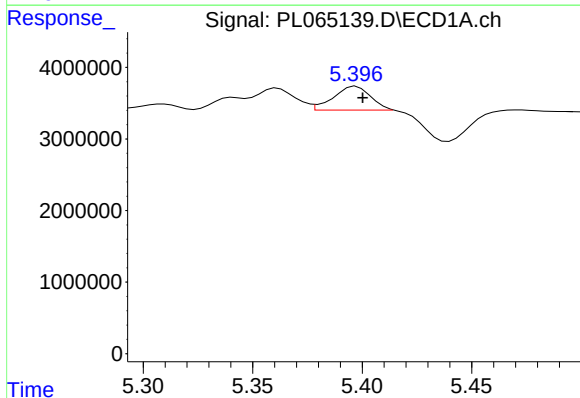


#11 alpha-Chlordane

R.T.: 5.396 min
Delta R.T.: -0.004 min
Response: 3879672
Conc: 1.01 ng/ml m

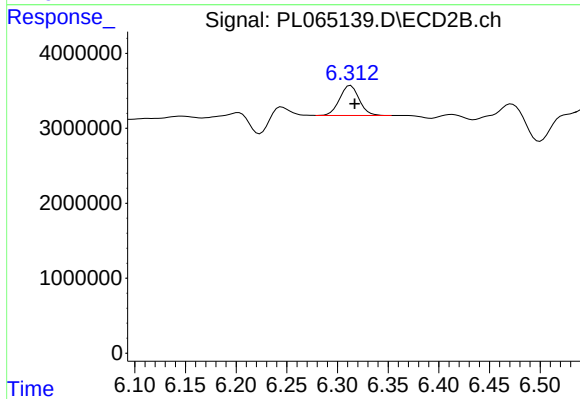

#11 alpha-Chlordane

R.T.: 6.313 min
Delta R.T.: -0.004 min
Response: 5337787
Conc: 1.93 ng/ml

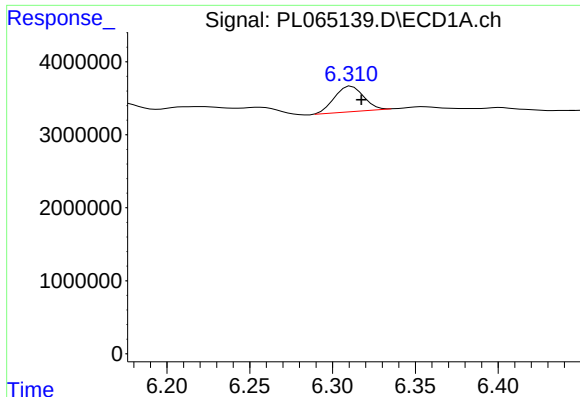


#17 4,4'-DDT

R.T.: 6.311 min
Delta R.T.: -0.006 min
Response: 4263391
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-030421


Manual Integrations
APPROVED

Ankita
3/9/2021 2:03:58 PM

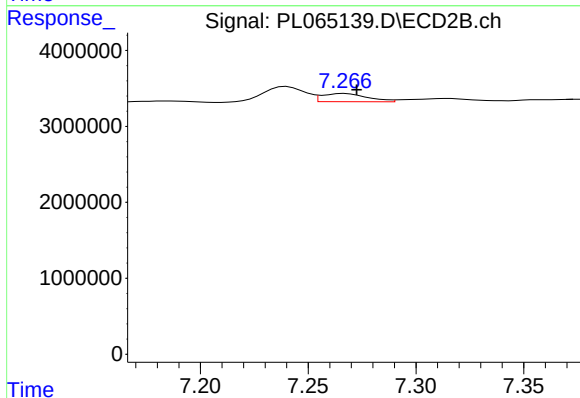


#17 4,4'-DDT

R.T.: 7.266 min
Delta R.T.: -0.007 min
Response: 1576290
Conc: 0.80 ng/ml m

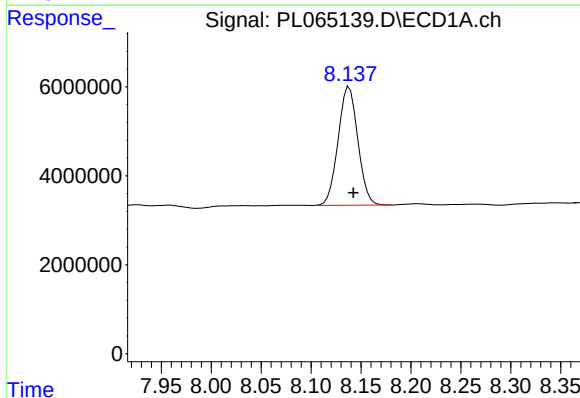

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.004 min
Response: 36641863
Conc: 13.20 ng/ml

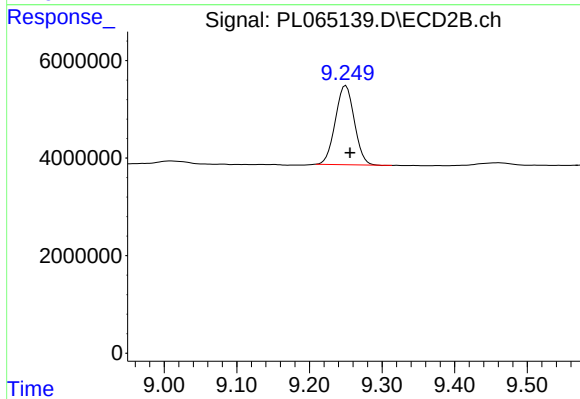

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.006 min
Response: 29437838
Conc: 13.40 ng/ml