

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 15:29
 Operator : AR\AJ
 Sample : M1579-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-02-030521

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:07:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	33250605	27098346	11.308	10.913
28)	SA Decachlor...	8.140	9.251	34041234	29424409	12.267	13.396
Target Compounds							
12)	B 4,4'-DDE	5.564	6.471	3876185	3323638	1.078	1.329


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 15:29
Operator : AR\AJ
Sample : M1579-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HR-02-030521

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:07:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

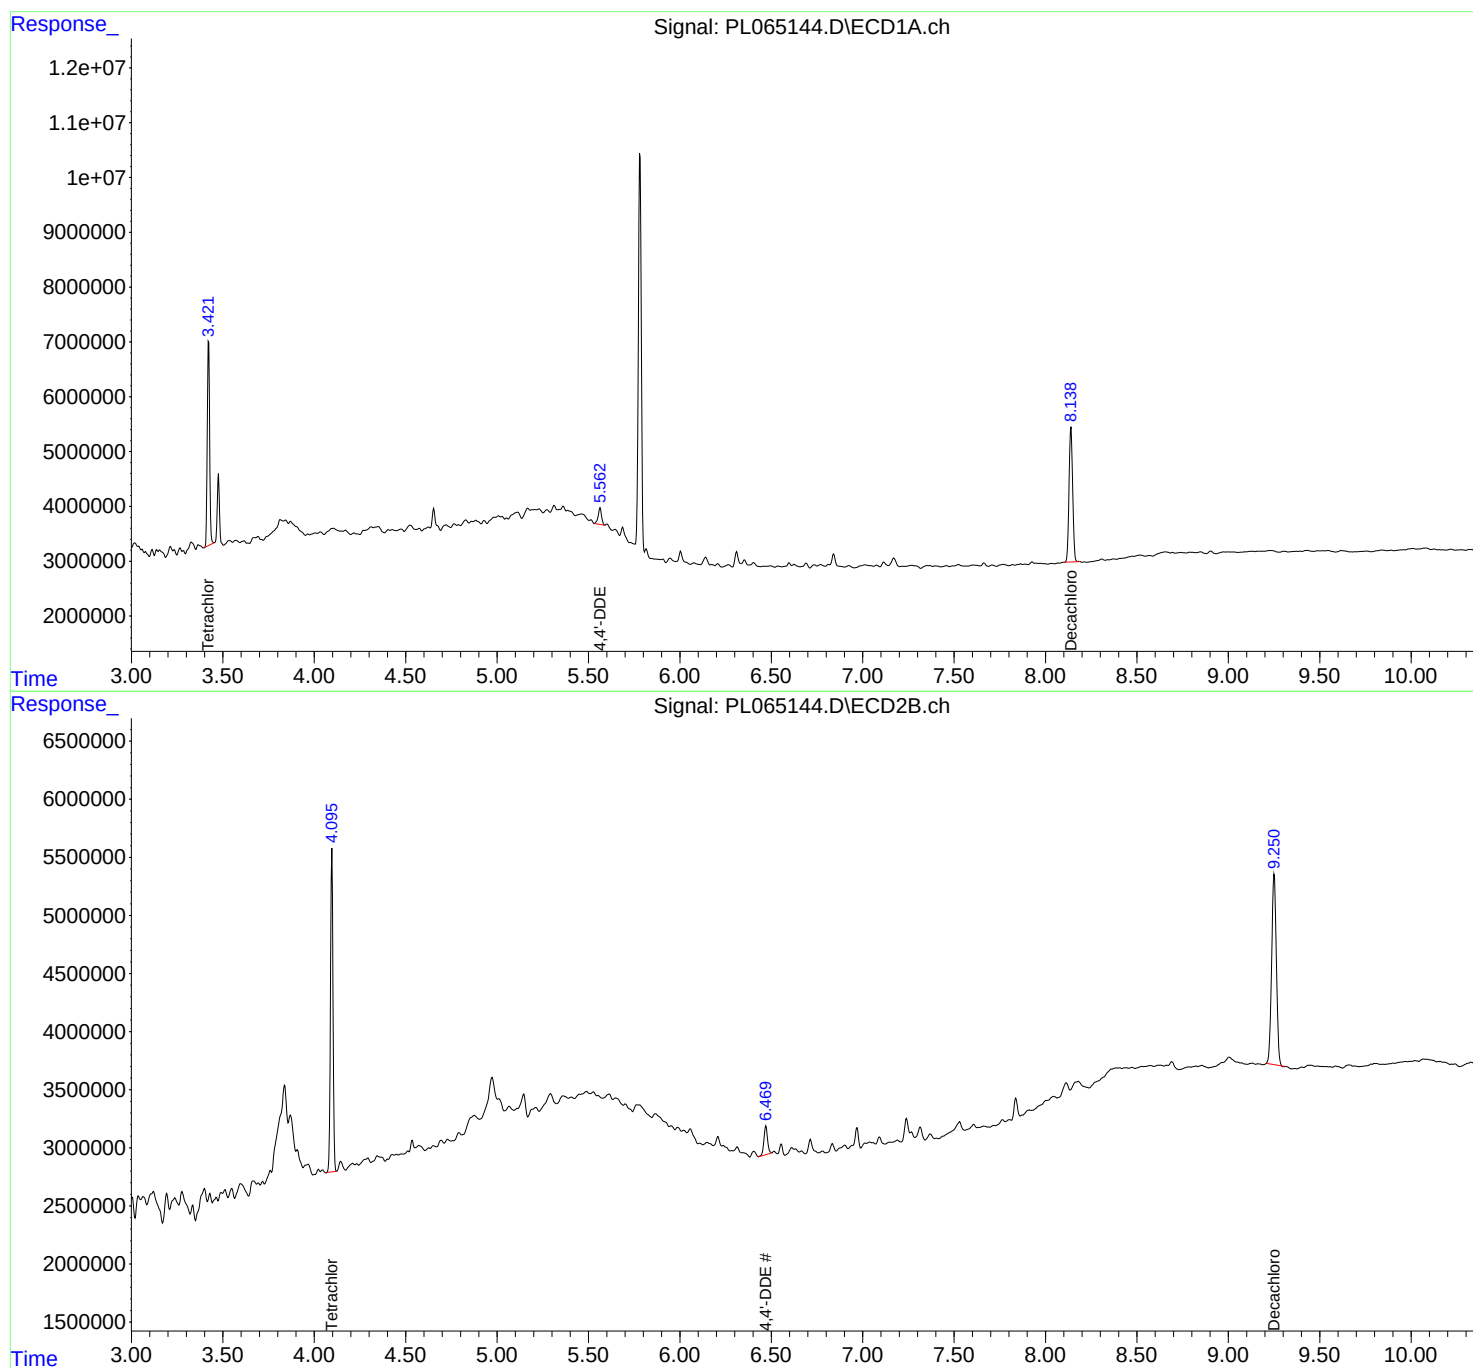


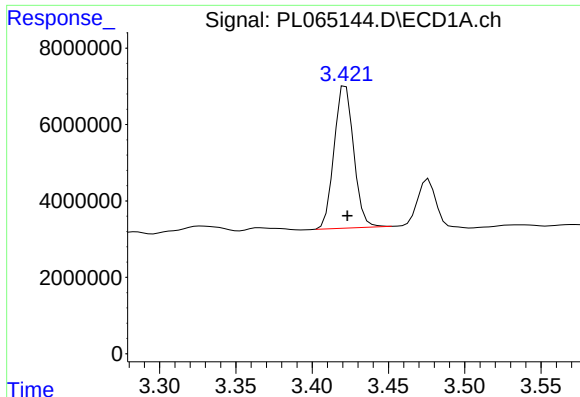

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 33250605
Conc: 11.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-02-030521

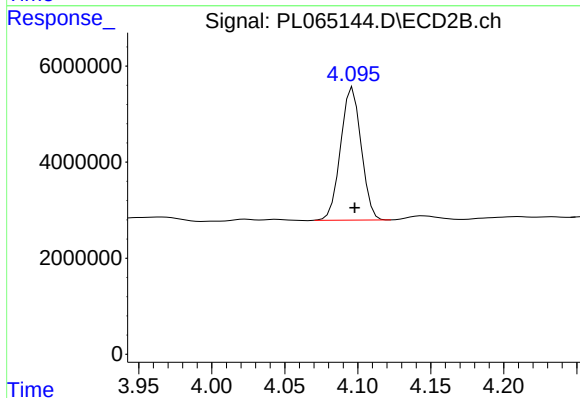


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.001 min
Response: 27098346
Conc: 10.91 ng/ml

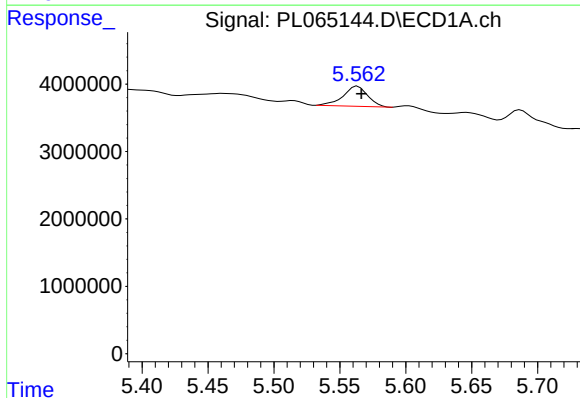


#12 4,4'-DDE

R.T.: 5.564 min
Delta R.T.: -0.003 min
Response: 3876185
Conc: 1.08 ng/ml

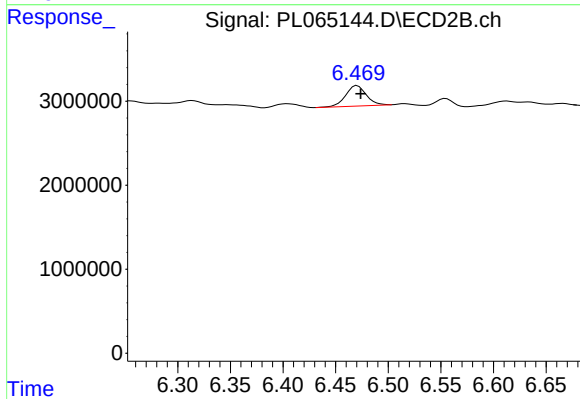

#12 4,4'-DDE


R.T.: 6.471 min
Delta R.T.: -0.003 min
Response: 3323638
Conc: 1.33 ng/ml

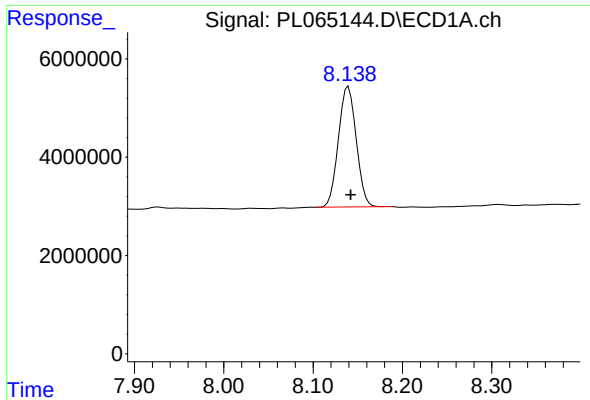

#28 Decachlorobiphenyl

R.T.: 8.140 min
Delta R.T.: -0.003 min
Response: 34041234
Conc: 12.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-02-030521

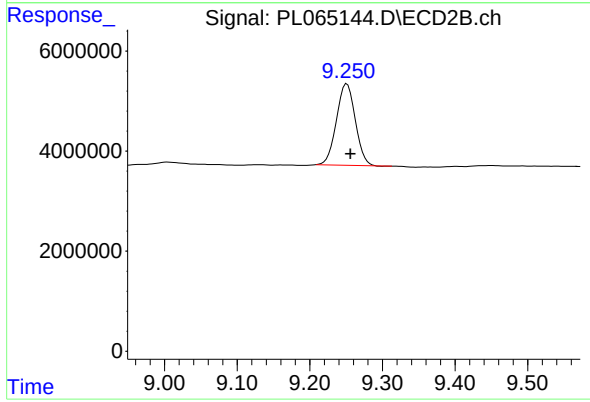

#28 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.005 min
Response: 29424409
Conc: 13.40 ng/ml