

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 16:11
 Operator : AR\AJ
 Sample : M1582-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VEOLIA-72-11991

Manual Integrations
 APPROVED

Ankita
 3/9/2021 2:04:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:08:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.422	4.097	53699753	44321791	18.263	17.849
28) SA Decachlor...	8.139	9.251	25626658	21283665	9.235	9.690
Target Compounds						
6) B beta-BHC	4.391	4.973	3105199	4440895	1.663m	2.904m#
12) B 4,4'-DDE	5.562	6.469	5262465	2825457	1.464m	1.130m
17) MA 4,4'-DDT	6.314	7.266	2508339	5479129	0.900	2.795 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 16:11
Operator : AR\AJ
Sample : M1582-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VEOLIA-72-11991


Manual Integrations
APPROVED

Ankita
3/9/2021 2:04:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:08:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

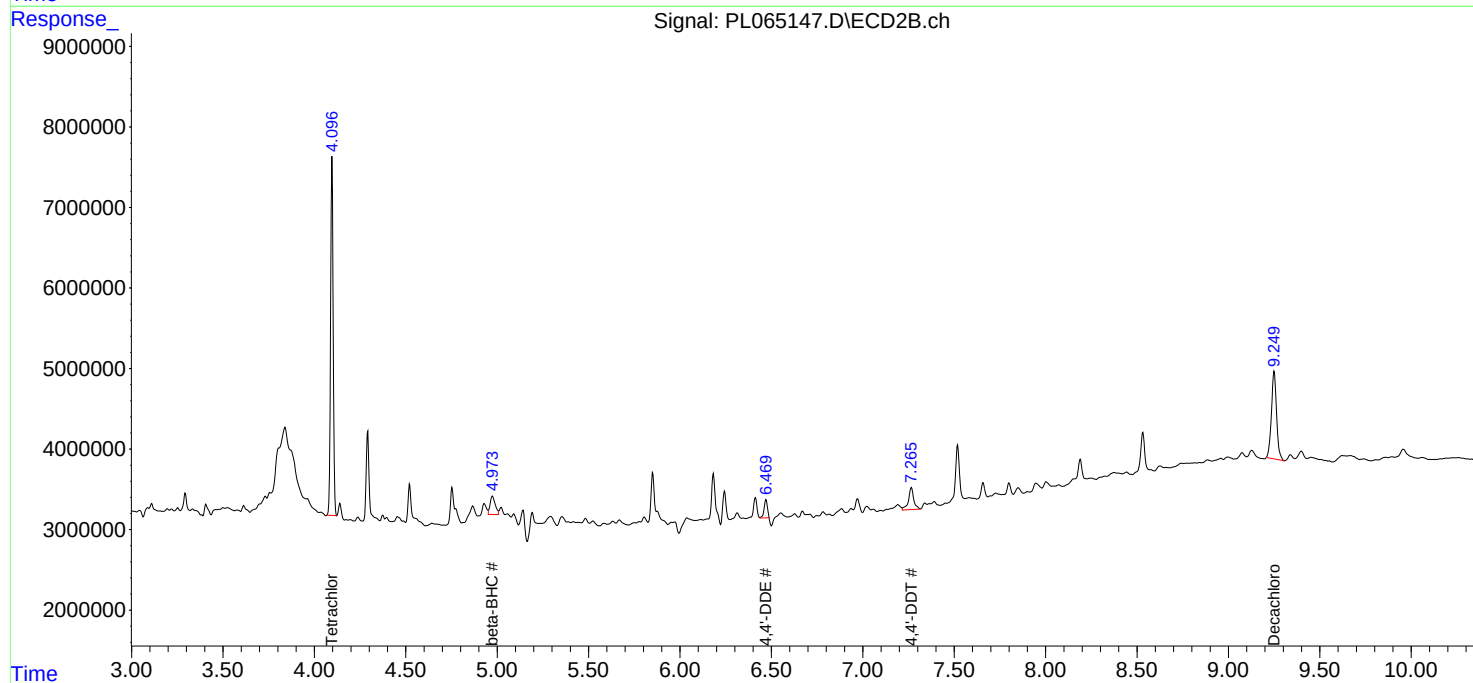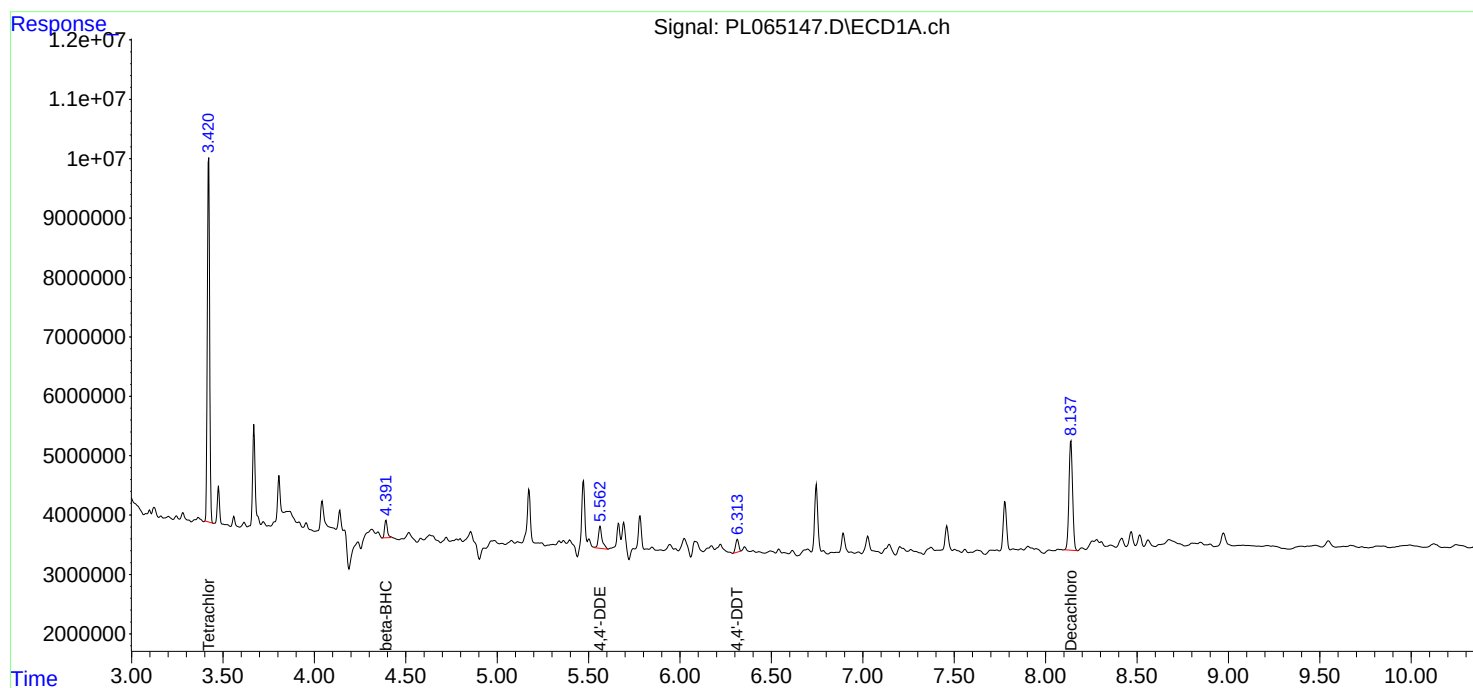

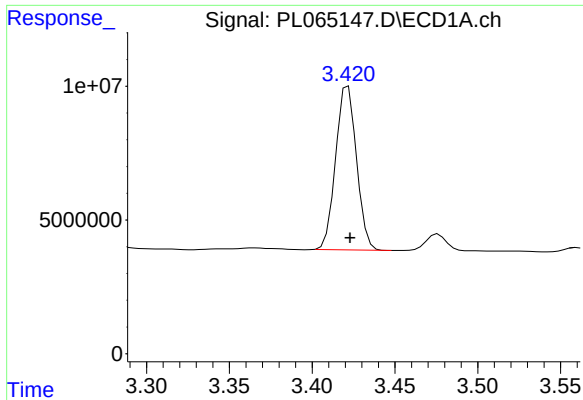


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 53699753
Conc: 18.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-72-11991


Manual Integrations
APPROVED

Ankita
3/9/2021 2:04:00 PM

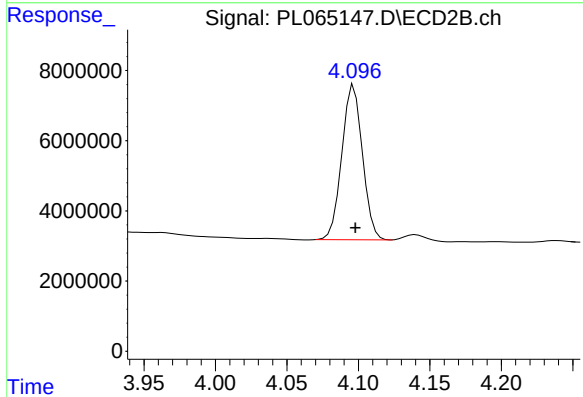


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.001 min
Response: 44321791
Conc: 17.85 ng/ml

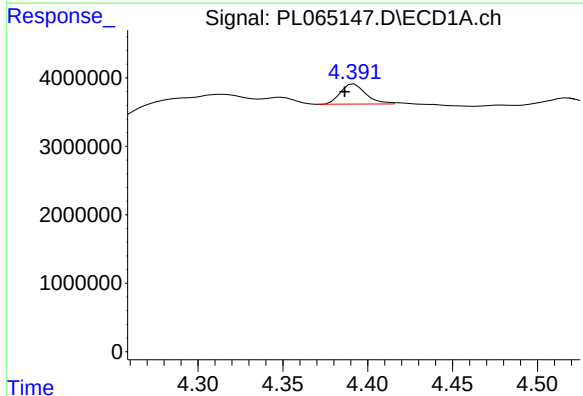


#6 beta-BHC

R.T.: 4.391 min
Delta R.T.: 0.004 min
Response: 3105199
Conc: 1.66 ng/ml m

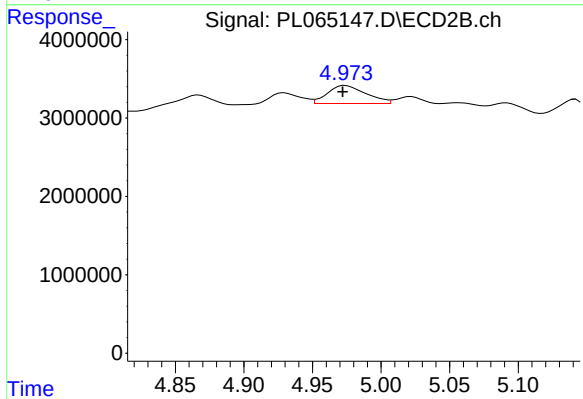

#6 beta-BHC

R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 4440895
Conc: 2.90 ng/ml m

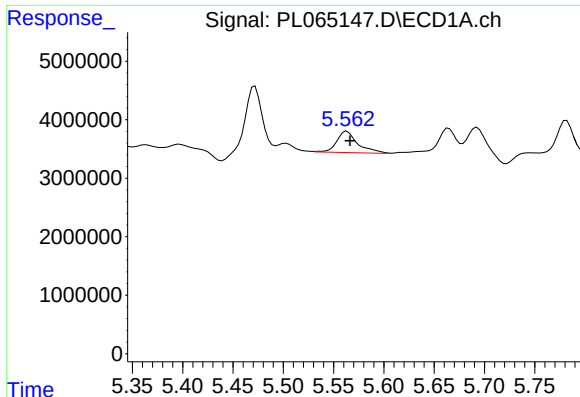


#12 4,4'-DDE

R.T.: 5.562 min
Delta R.T.: -0.005 min
Response: 5262465
Conc: 1.46 ng/ml m

Instrument :
ECD_L
ClientSampleId :
VEOLIA-72-11991


Manual Integrations
APPROVED

Ankita
3/9/2021 2:04:00 PM

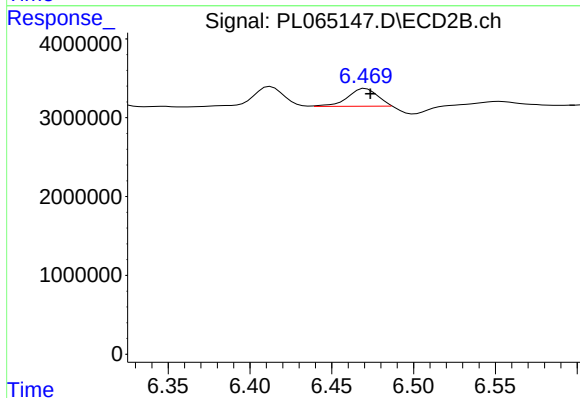


#12 4,4'-DDE

R.T.: 6.469 min
Delta R.T.: -0.005 min
Response: 2825457
Conc: 1.13 ng/ml m

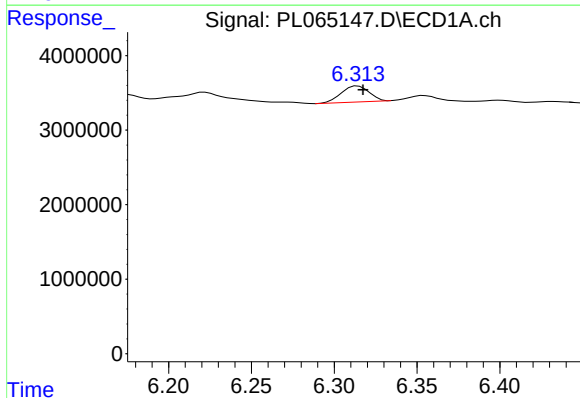


#17 4,4'-DDT

R.T.: 6.314 min
Delta R.T.: -0.003 min
Response: 2508339
Conc: 0.90 ng/ml

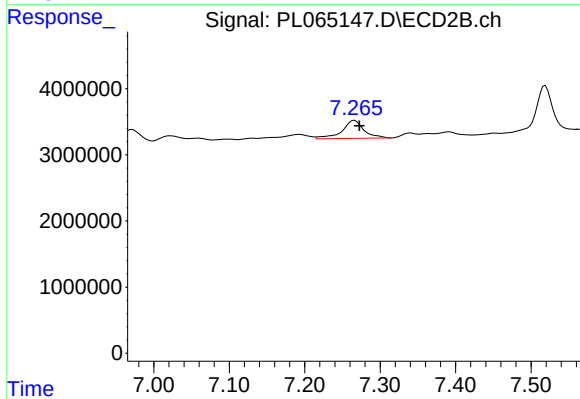

#17 4,4'-DDT

R.T.: 7.266 min
Delta R.T.: -0.007 min
Response: 5479129
Conc: 2.80 ng/ml

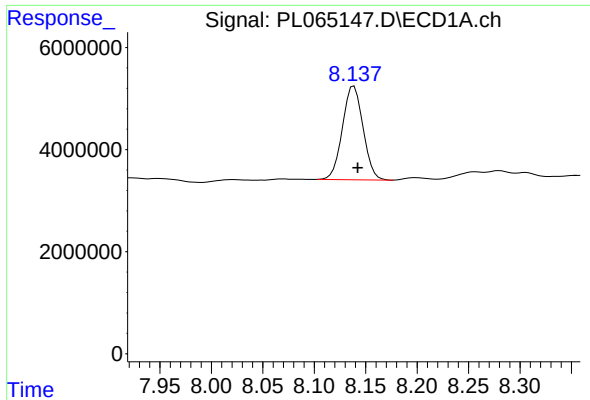


#28 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.004 min
Response: 25626658
Conc: 9.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
VEOLIA-72-11991

Manual Integrations
APPROVED

Ankita
3/9/2021 2:04:00 PM

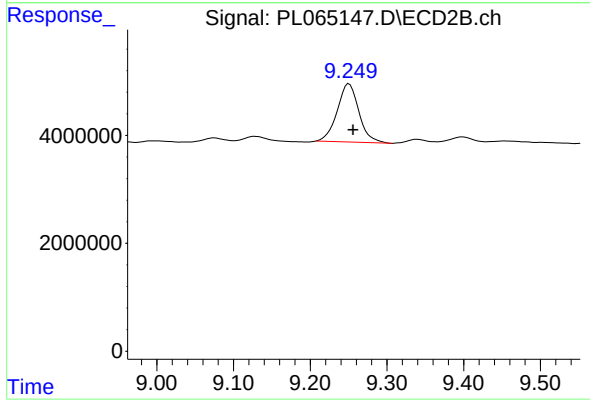

#28 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.005 min
Response: 21283665
Conc: 9.69 ng/ml