

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
 Data File : PL065150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2021 16:54
 Operator : AR\AJ
 Sample : M1590-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-EF-01-018-ABCD

Manual Integrations
 APPROVED

Ankita
 3/9/2021 2:04:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:09:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	35946874	31127284	12.225	12.535
28)	SA Decachlor...	8.139	9.251	38543377	31052494	13.889	14.137
Target Compounds							
11)	B alpha-Chl...	5.397	6.313	1975318	3507259	0.515	1.269 #
17)	MA 4,4'-DDT	6.313	7.268	4453185	2355957	1.597	1.202m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030821\
Data File : PL065150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2021 16:54
Operator : AR\AJ
Sample : M1590-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-EF-01-018-ABCD


Manual Integrations
APPROVED

Ankita
3/9/2021 2:04:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:09:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

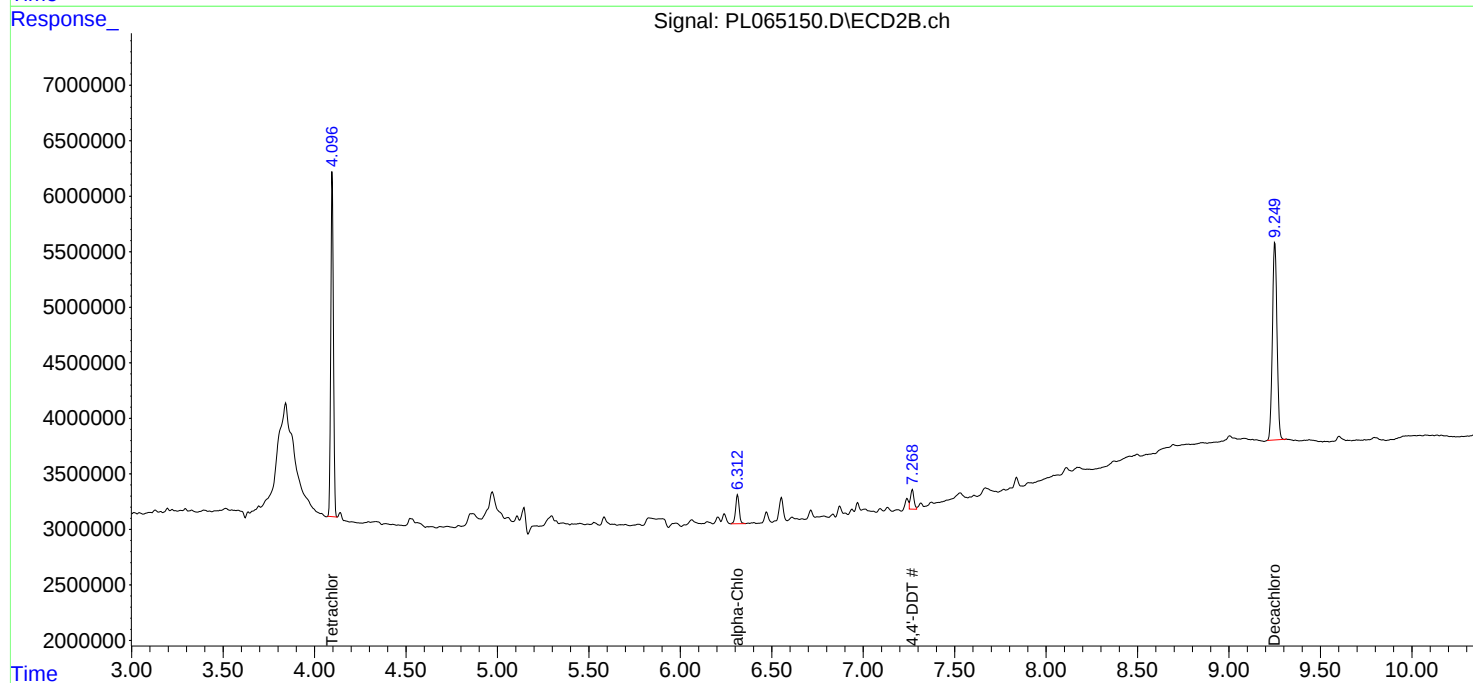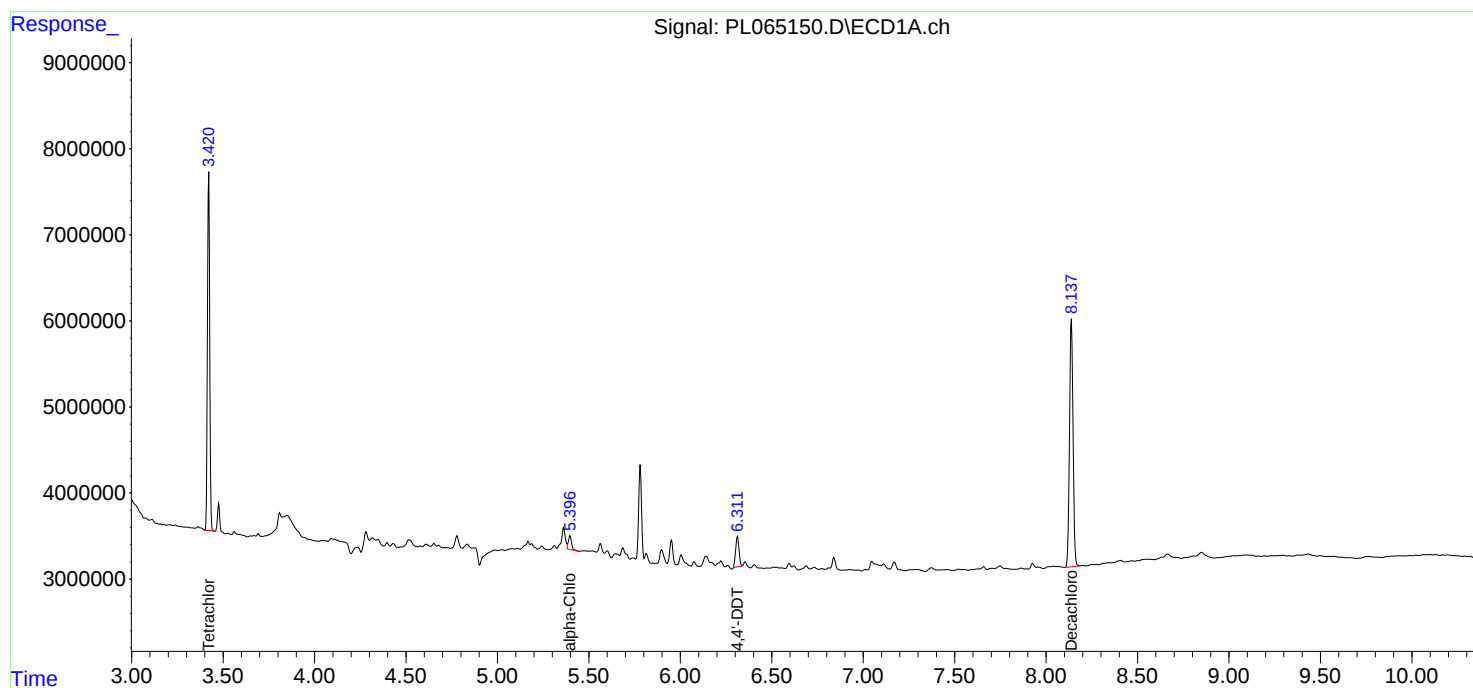

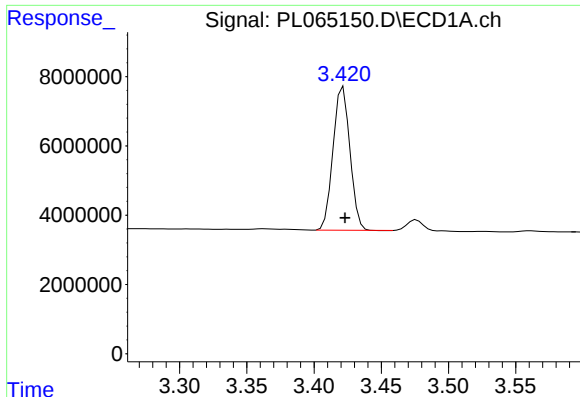


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.001 min
Response: 35946874
Conc: 12.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-018-ABCD


Manual Integrations
APPROVED

Ankita
3/9/2021 2:04:04 PM

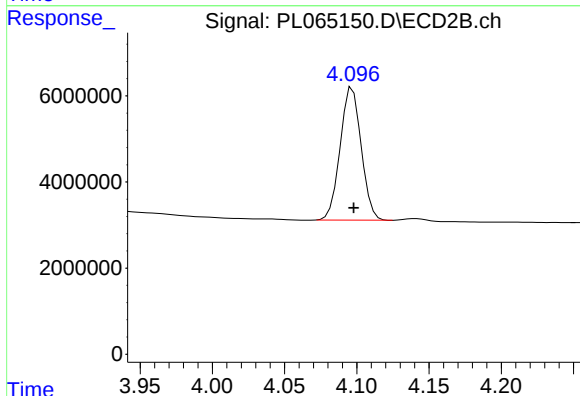


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 31127284
Conc: 12.54 ng/ml

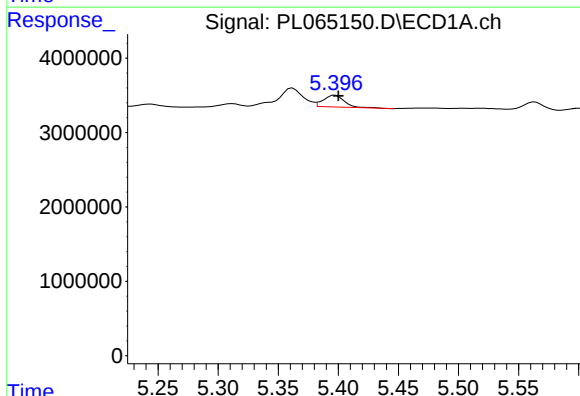


#11 alpha-Chlordane

R.T.: 5.397 min
Delta R.T.: -0.003 min
Response: 1975318
Conc: 0.52 ng/ml

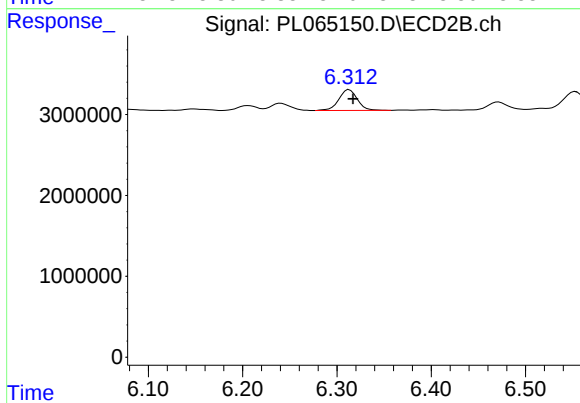

#11 alpha-Chlordane

R.T.: 6.313 min
Delta R.T.: -0.004 min
Response: 3507259
Conc: 1.27 ng/ml

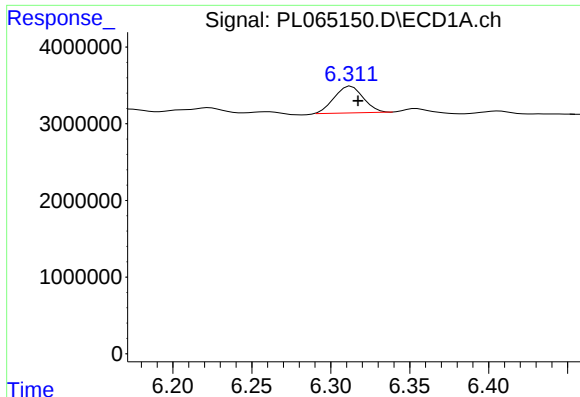


#17 4,4'-DDT

R.T.: 6.313 min
Delta R.T.: -0.004 min
Response: 4453185
Conc: 1.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-EF-01-018-ABCD


Manual Integrations
APPROVED

Ankita
3/9/2021 2:04:04 PM

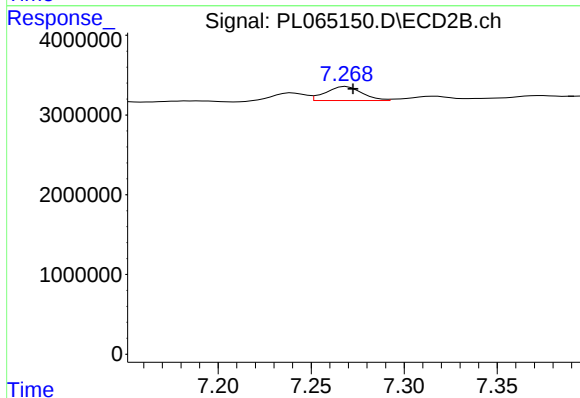


#17 4,4'-DDT

R.T.: 7.268 min
Delta R.T.: -0.005 min
Response: 2355957
Conc: 1.20 ng/ml m

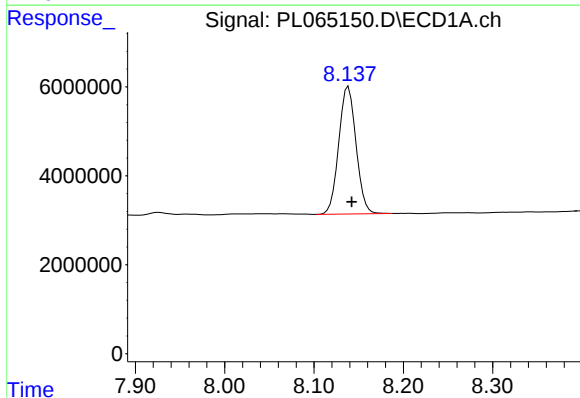

#28 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.004 min
Response: 38543377
Conc: 13.89 ng/ml

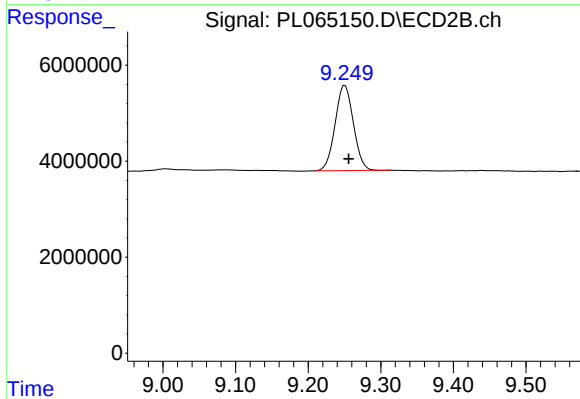

#28 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.005 min
Response: 31052494
Conc: 14.14 ng/ml