

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030822\
 Data File : PL073217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 19:24
 Operator : AR\AJ
 Sample : N1775-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 05:51:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.491	6896596	33821740	20.054	21.665
27)	SA Decachlor...	10.421	11.329	19999566	68573795	41.595	42.426
Target Compounds							
2)	A alpha-BHC	0.000	6.026f	0	224467	N.D.	0.116
3)	MA gamma-BHC...	0.000	6.454	0	322645	N.D.	0.170
6)	B beta-BHC	0.000	6.667	0	731504	N.D.	0.748
7)	B delta-BHC	0.000	6.955	0	2109398	N.D.	1.091
8)	B Heptachlo...	0.000	7.964f	0	560326	N.D.	0.329
15)	B Endosulfa...	8.320f	0.000	633660	0	1.352	N.D. #
16)	A 4,4'-DDD	0.000	8.938f	0	3825458	N.D.	2.913
20)	A Methoxychlor	0.000	9.712f	0	151474	N.D.	0.198
21)	B Endrin ke...	0.000	9.950	0	492772	N.D.	0.348
26)	Toxaphene-5	0.000	9.868	0	6501	N.D.	0.383


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030822\
Data File : PL073217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 19:24
Operator : AR\AJ
Sample : N1775-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 05:51:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

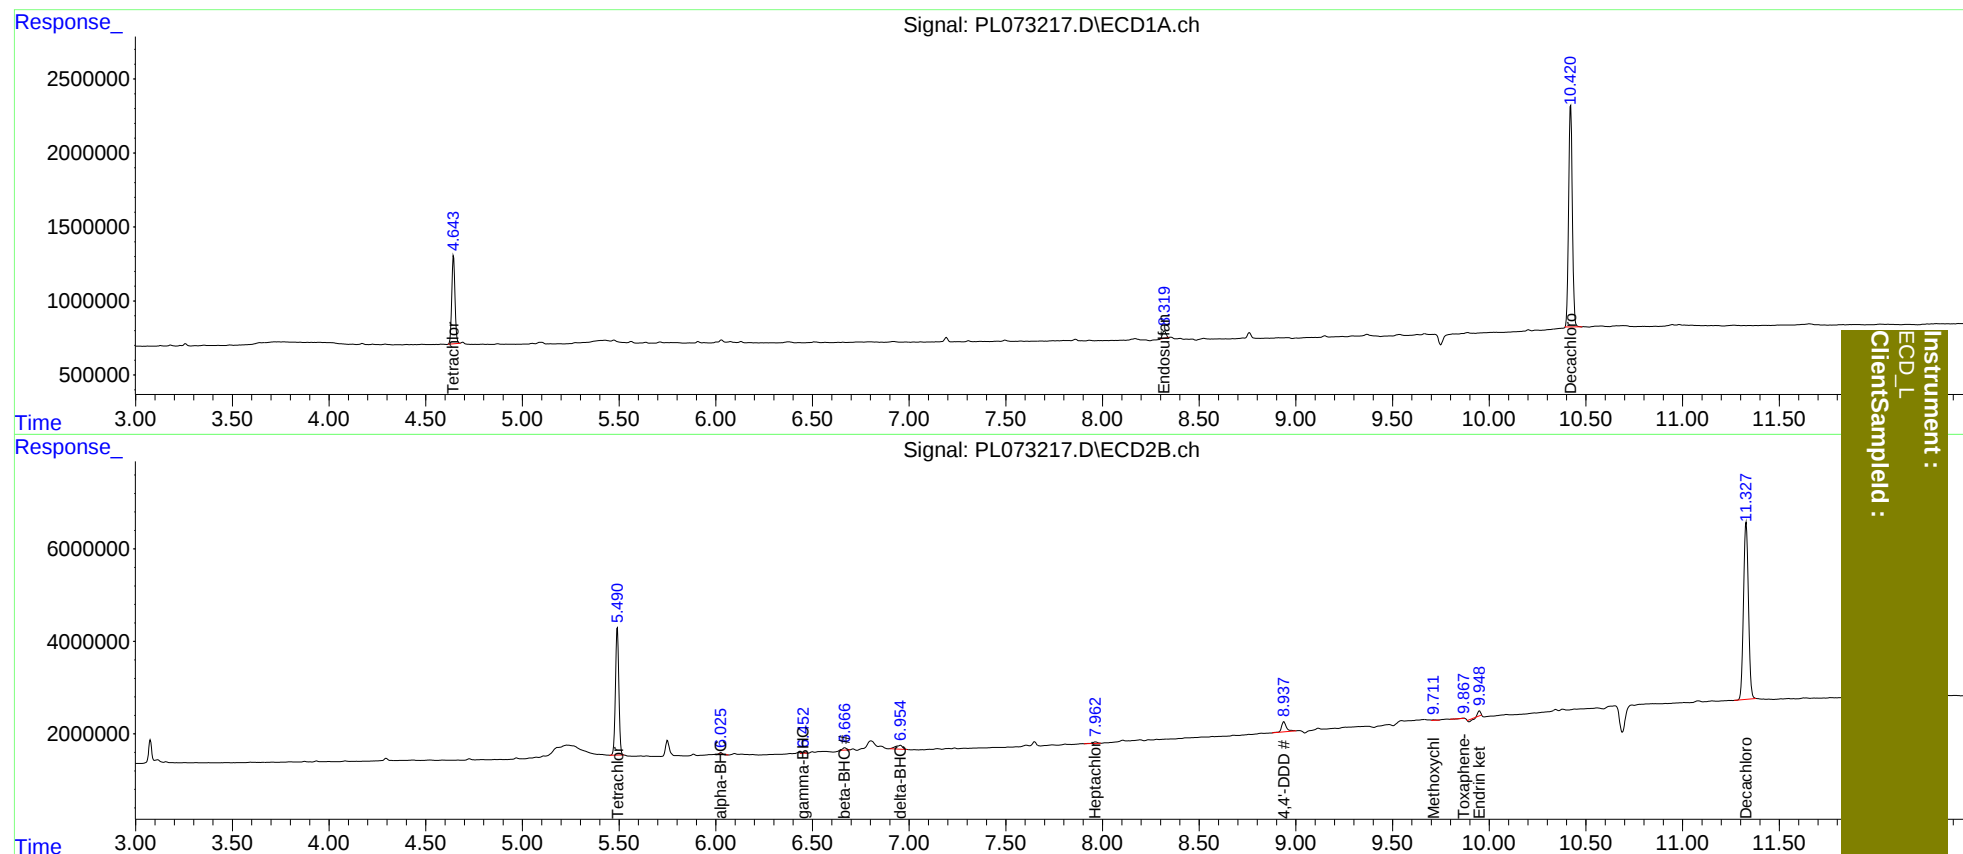


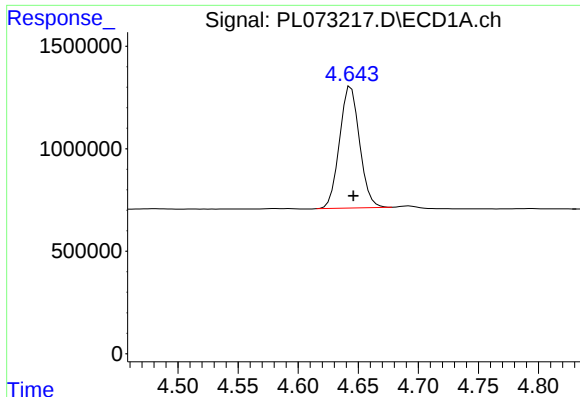

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 6896596
Conc: 20.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

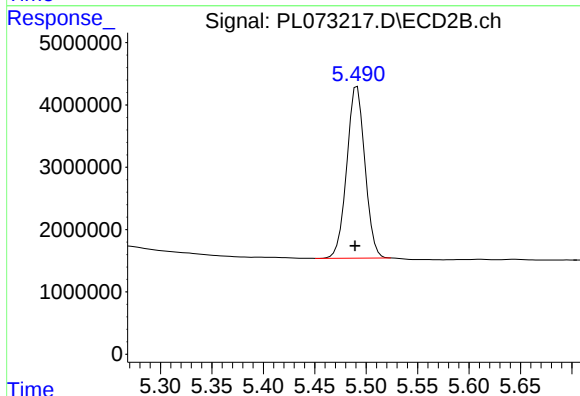


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.002 min
Response: 33821740
Conc: 21.66 ng/ml

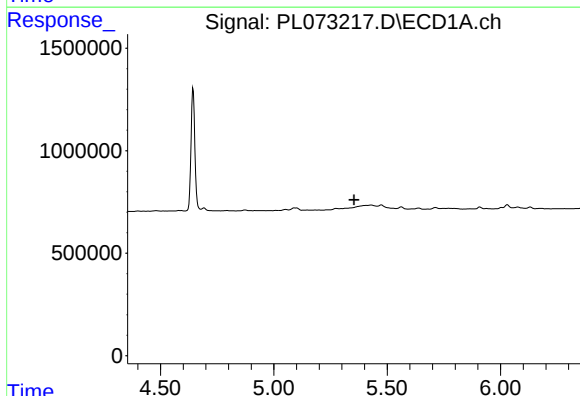


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

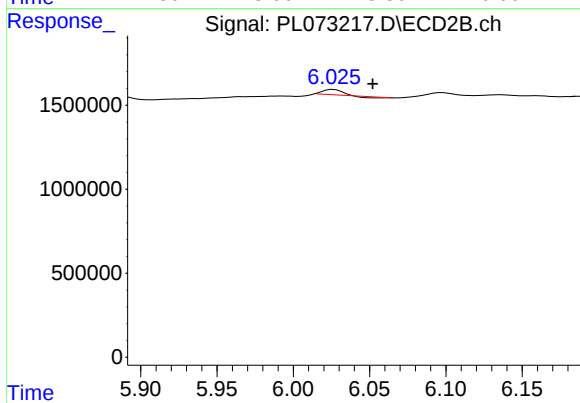

#2 alpha-BHC


R.T.: 6.026 min
Delta R.T.: -0.026 min
Response: 224467
Conc: 0.12 ng/ml

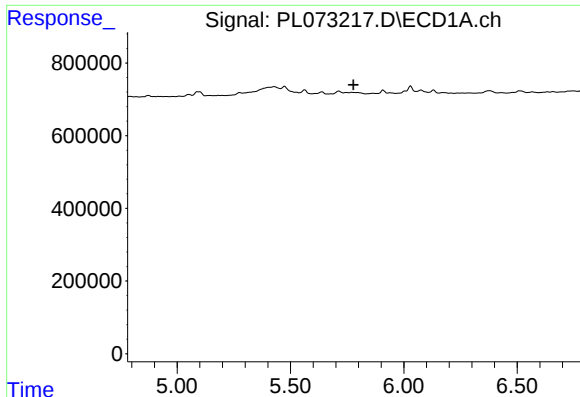

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 5.778 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

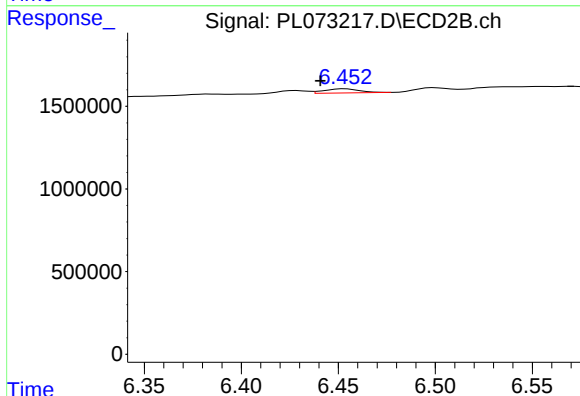


#3 gamma-BHC (Lindane)

R.T.: 6.454 min
Delta R.T.: 0.013 min
Response: 322645
Conc: 0.17 ng/ml

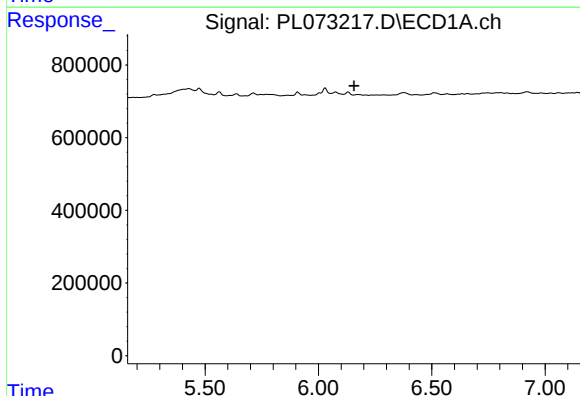


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

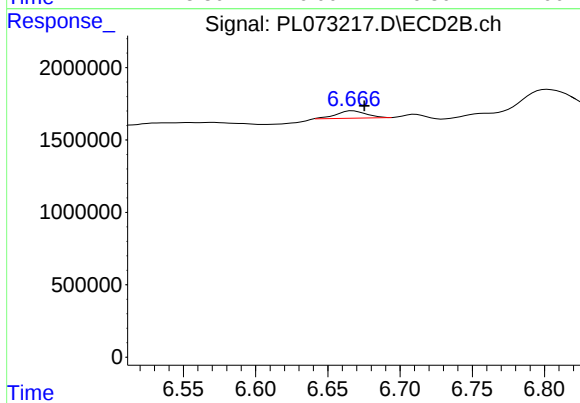

#6 beta-BHC


R.T.: 6.667 min
Delta R.T.: -0.008 min
Response: 731504
Conc: 0.75 ng/ml

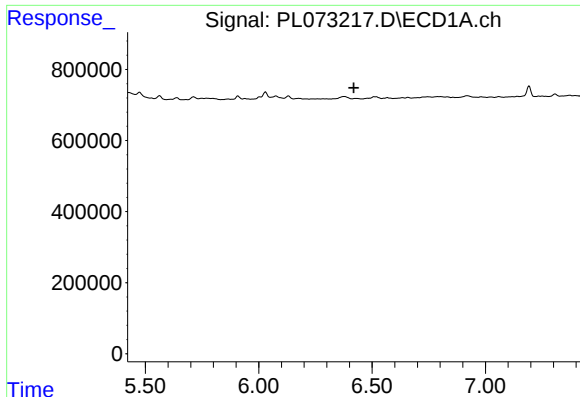

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

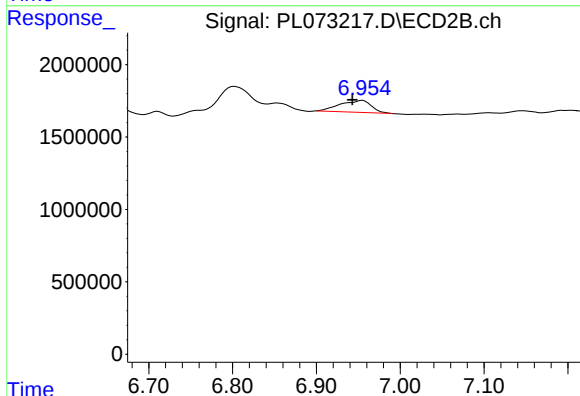


#7 delta-BHC

R.T.: 6.955 min
Delta R.T.: 0.012 min
Response: 2109398
Conc: 1.09 ng/ml

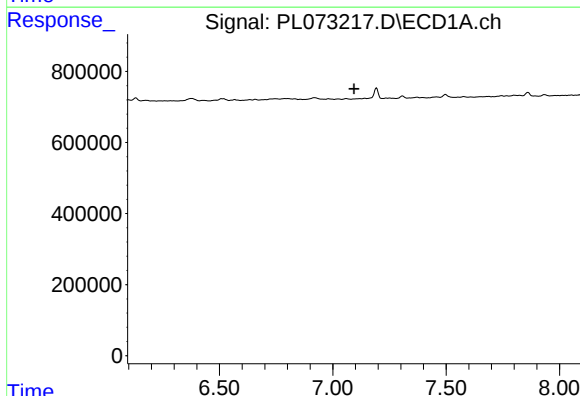


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.094 min
Response: 0
Conc: N.D.

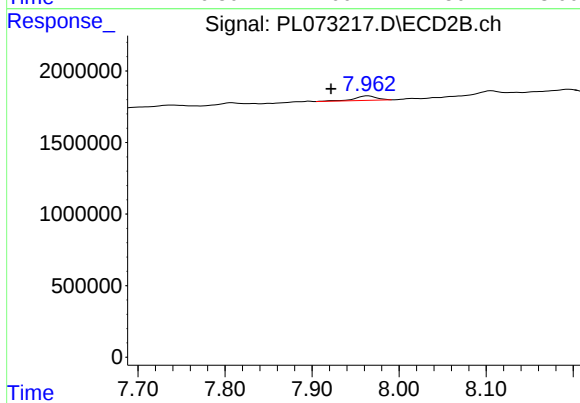

#8 Heptachlor epoxide


R.T.: 7.964 min
Delta R.T.: 0.042 min
Response: 560326
Conc: 0.33 ng/ml

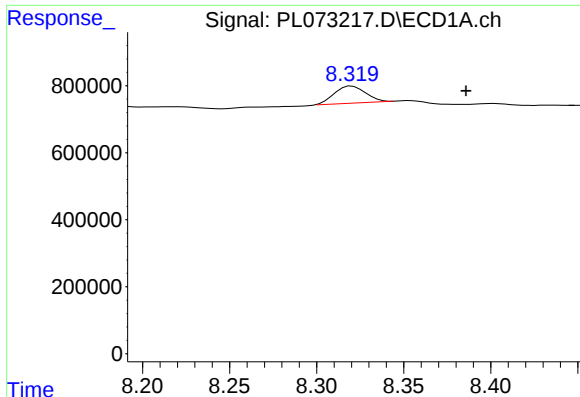

#15 Endosulfan II


R.T.: 8.320 min
Delta R.T.: -0.066 min
Response: 633660
Conc: 1.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

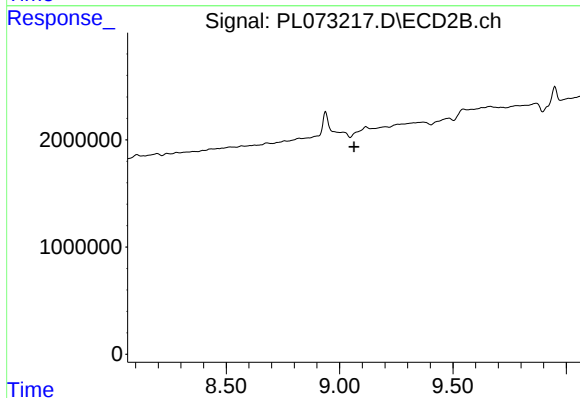


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

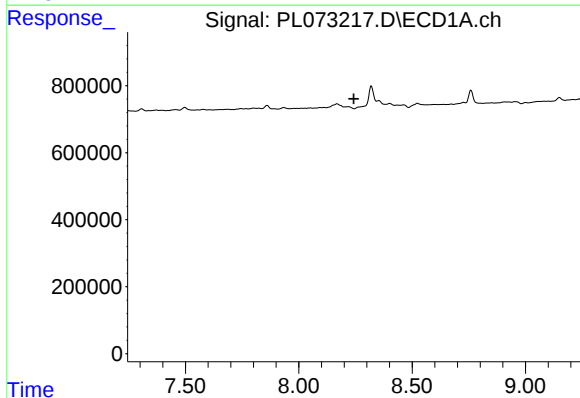


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

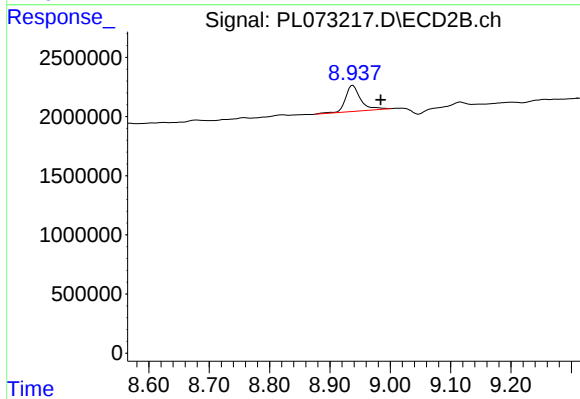

#16 4,4'-DDD


R.T.: 8.938 min
Delta R.T.: -0.046 min
Response: 3825458
Conc: 2.91 ng/ml

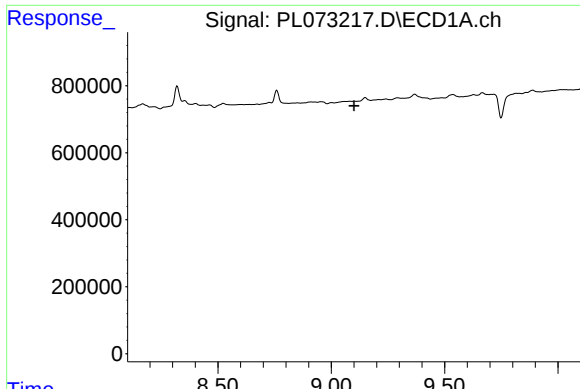

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

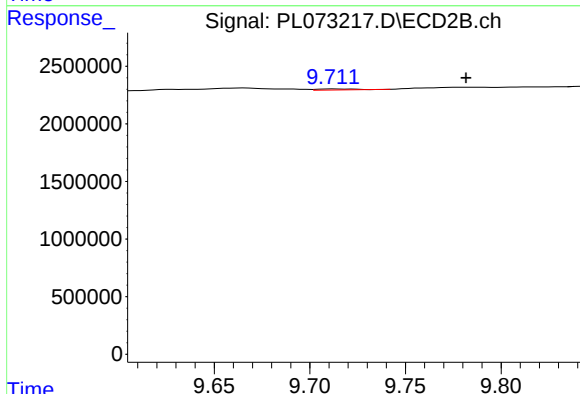


#20 Methoxychlor

R.T.: 9.712 min
Delta R.T.: -0.070 min
Response: 151474
Conc: 0.20 ng/ml

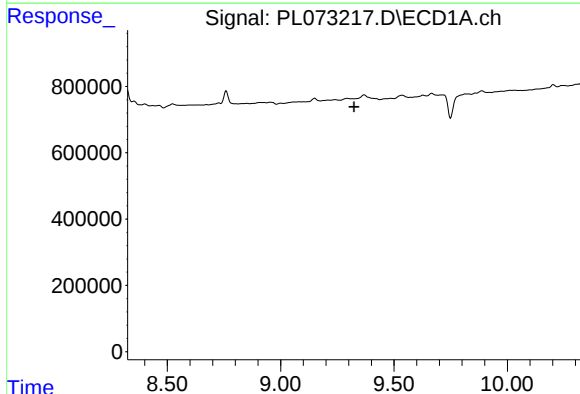


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.324 min
Response: 0
Conc: N.D.

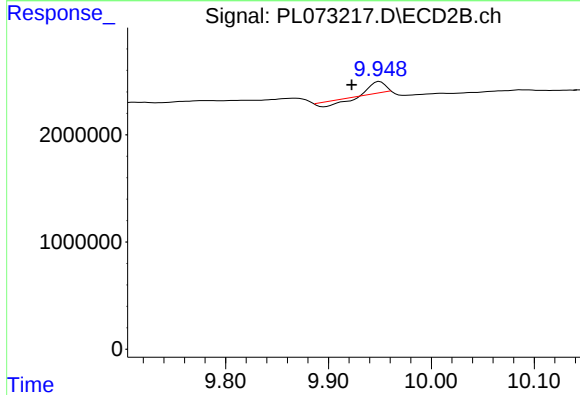

#21 Endrin ketone


R.T.: 9.950 min
Delta R.T.: 0.027 min
Response: 492772
Conc: 0.35 ng/ml

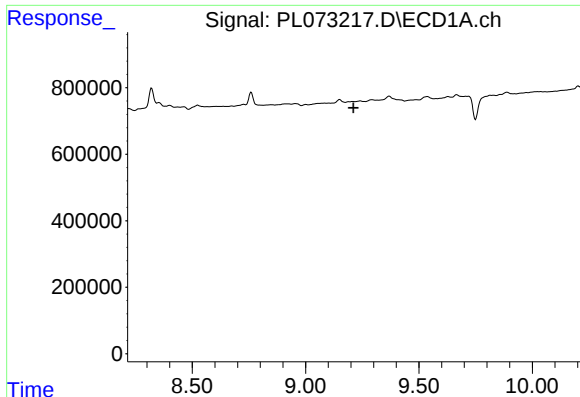

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 9.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

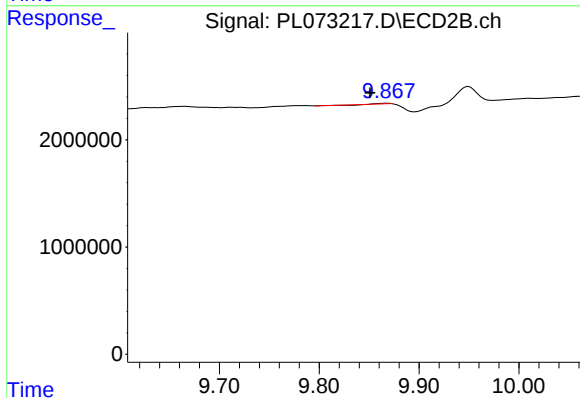


#26 Toxaphene-5

R.T.: 9.868 min
Delta R.T.: 0.017 min
Response: 6501
Conc: 0.38 ng/ml

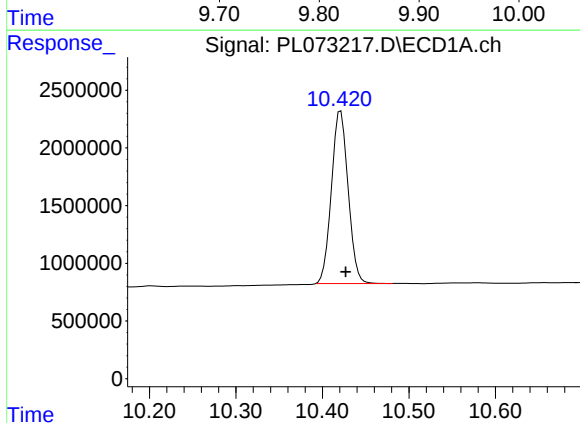

#27 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: -0.006 min
Response: 19999566
Conc: 41.60 ng/ml

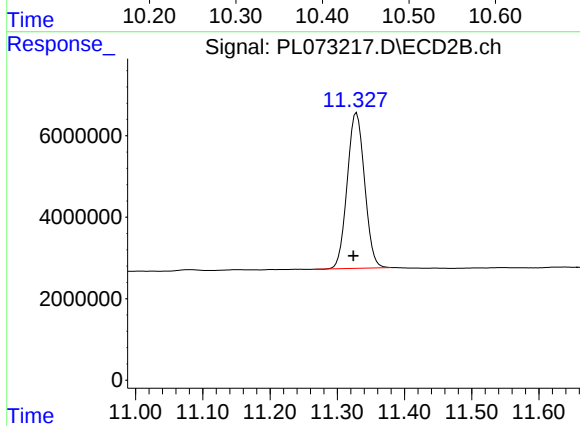

#27 Decachlorobiphenyl

R.T.: 11.329 min
Delta R.T.: 0.004 min
Response: 68573795
Conc: 42.43 ng/ml