

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030822\
 Data File : PL073225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 21:36
 Operator : AR\AJ
 Sample : N1775-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 05:54:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.492	6491957	31594895	18.878	20.238
27)	SA Decachlor...	10.422	11.330	16871255	57744964	35.089	35.726
Target Compounds							
2)	A alpha-BHC	0.000	6.098f	0	561334	N.D.	0.290
6)	B beta-BHC	0.000	6.669	0	643991	N.D.	0.658
7)	B delta-BHC	0.000	6.938	0	1562918	N.D.	0.808
15)	B Endosulfa...	8.321f	0.000	802721	0	1.713	N.D. #
16)	A 4,4'-DDD	0.000	8.939f	0	4097462	N.D.	3.120
20)	A Methoxychlor	0.000	9.727f	0	113126	N.D.	0.148
21)	B Endrin ke...	0.000	9.951	0	10487	N.D.	<MDL

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030822\
Data File : PL073225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 21:36
Operator : AR\AJ
Sample : N1775-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 05:54:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

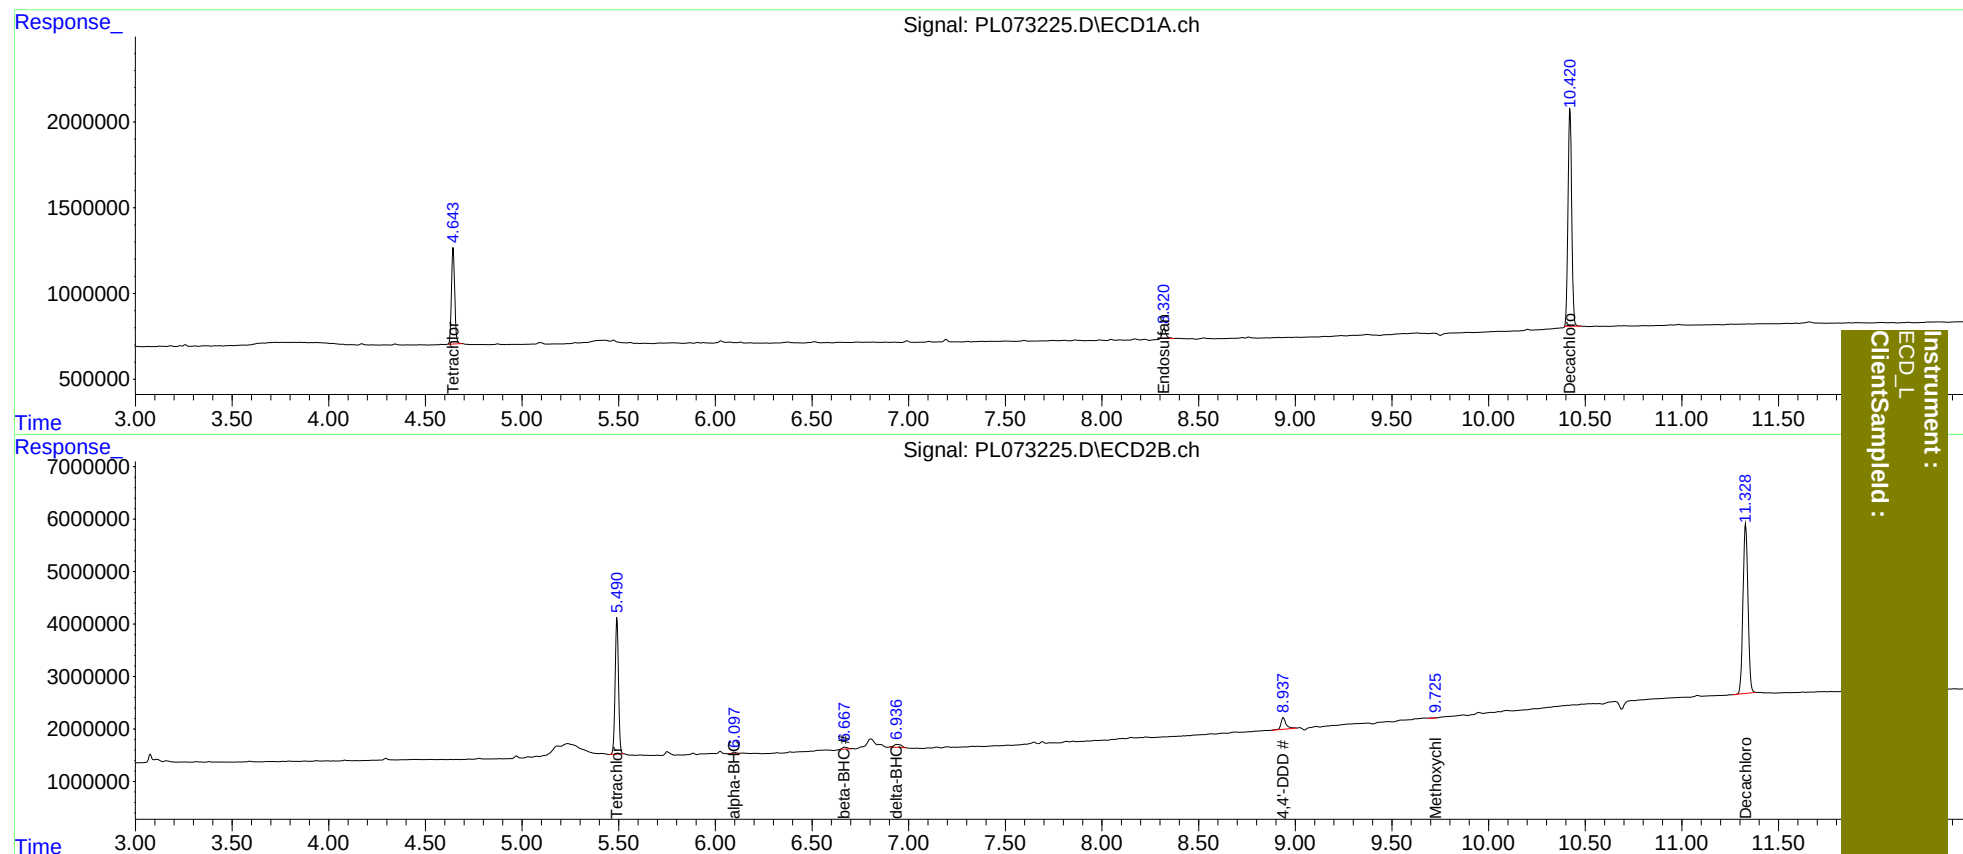


Instrument :
ECD_L
ClientSampled :
N1775-19

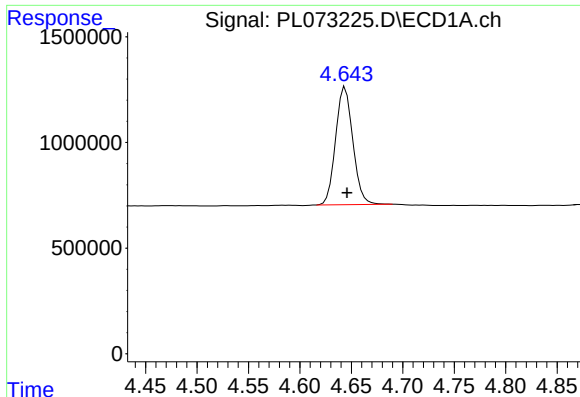

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 6491957
Conc: 18.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

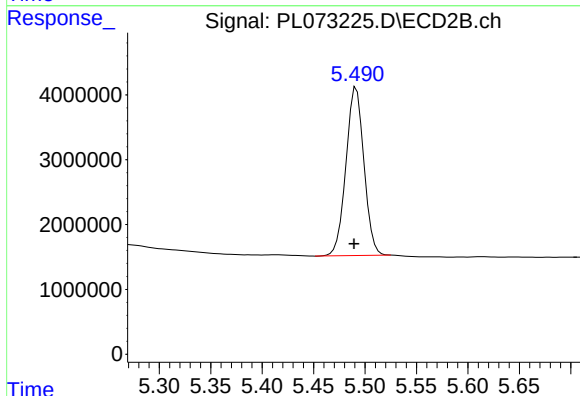


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.002 min
Response: 31594895
Conc: 20.24 ng/ml

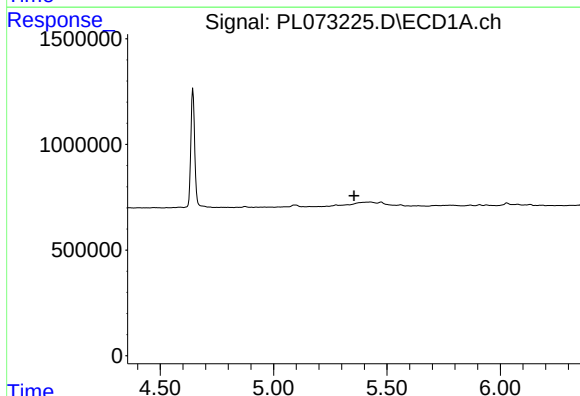


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

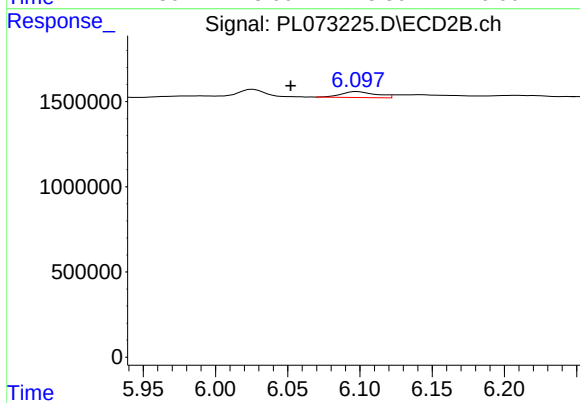

#2 alpha-BHC


R.T.: 6.098 min
Delta R.T.: 0.046 min
Response: 561334
Conc: 0.29 ng/ml

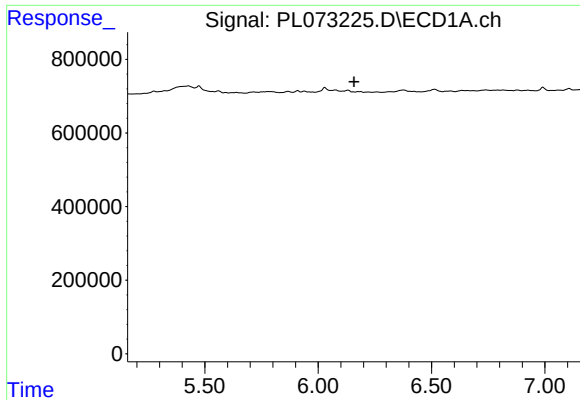

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

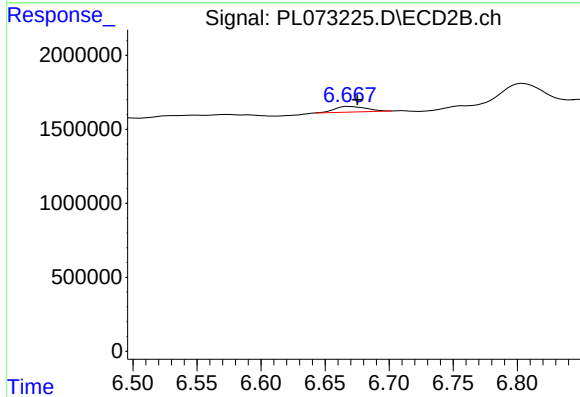


#6 beta-BHC

R.T.: 6.669 min
Delta R.T.: -0.007 min
Response: 643991
Conc: 0.66 ng/ml

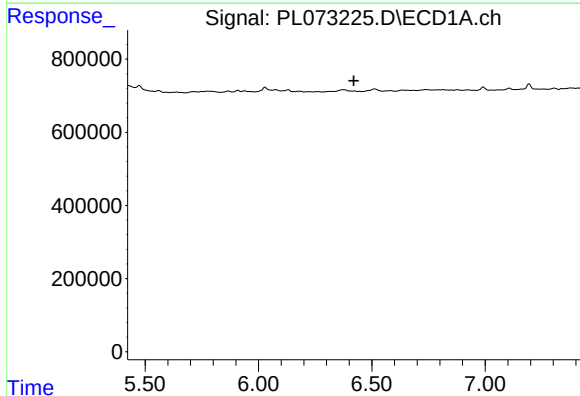


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

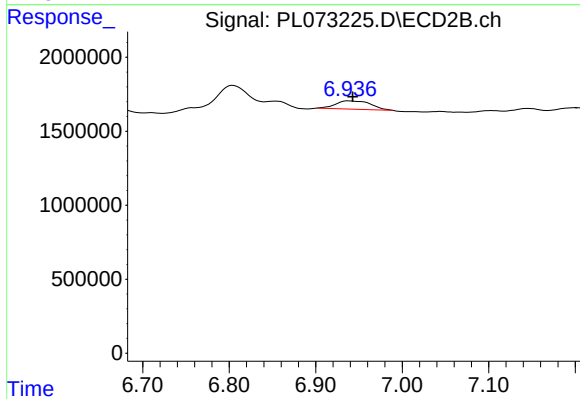

#7 delta-BHC


R.T.: 6.938 min
Delta R.T.: -0.005 min
Response: 1562918
Conc: 0.81 ng/ml

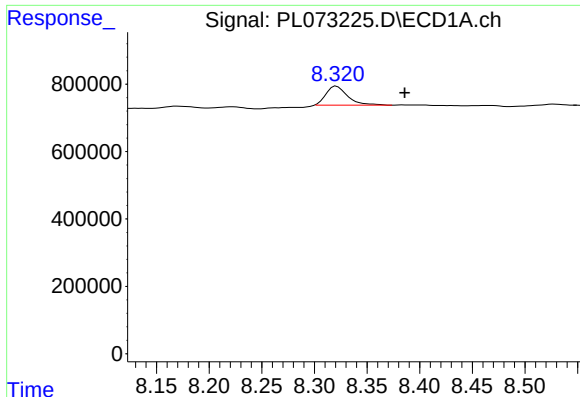

#15 Endosulfan II


R.T.: 8.321 min
Delta R.T.: -0.065 min
Response: 802721
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

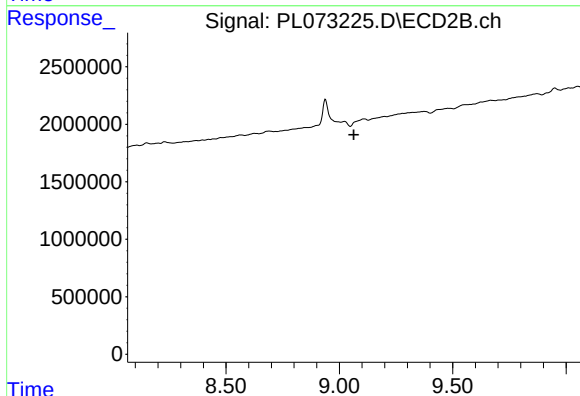


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

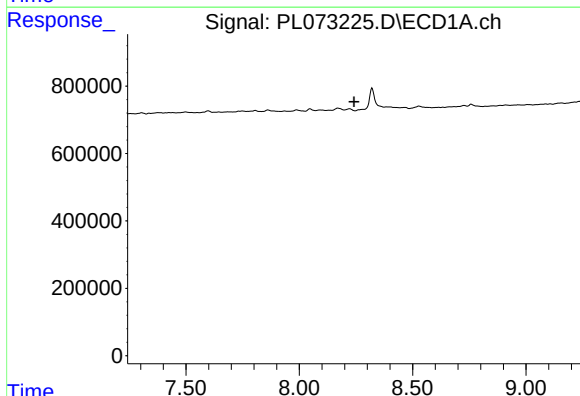


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

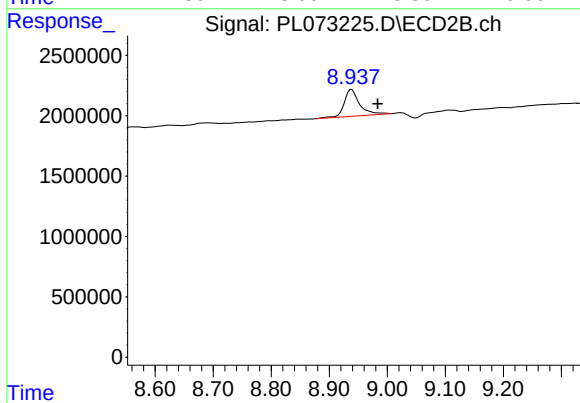

#16 4,4'-DDD


R.T.: 8.939 min
Delta R.T.: -0.045 min
Response: 4097462
Conc: 3.12 ng/ml

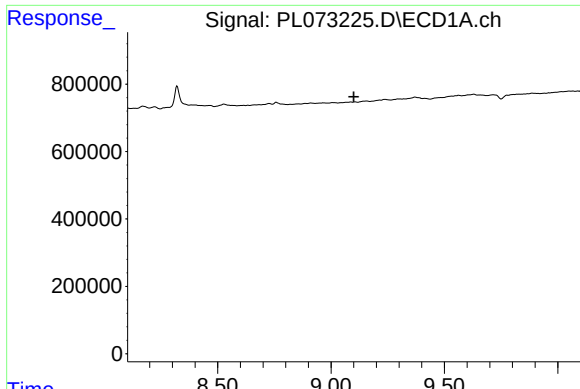

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

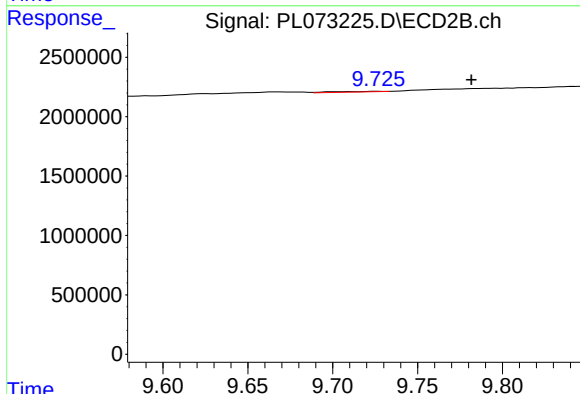


#20 Methoxychlor

R.T.: 9.727 min
Delta R.T.: -0.055 min
Response: 113126
Conc: 0.15 ng/ml

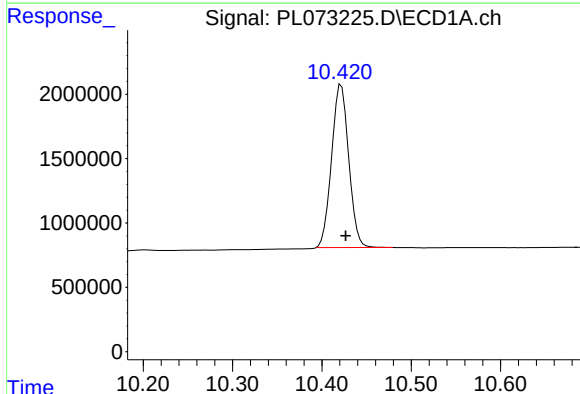

#27 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.005 min
Response: 16871255
Conc: 35.09 ng/ml

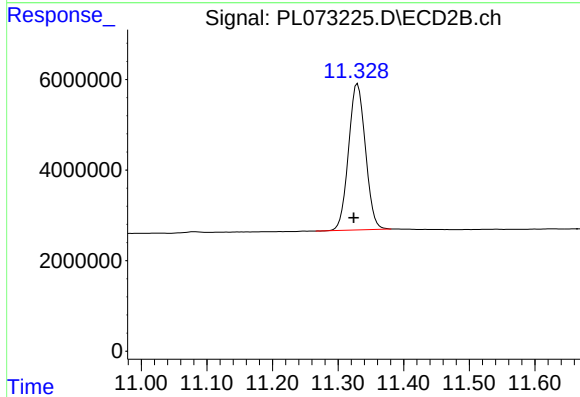

#27 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: 0.006 min
Response: 57744964
Conc: 35.73 ng/ml