

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030822\
 Data File : PL073231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2022 23:15
 Operator : AR\AJ
 Sample : PIBLK246
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 05:56:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.491	7360871	35128941	21.405	22.502
27)	SA Decachlor...	10.422	11.329	22736471	77653808	47.287	48.044
Target Compounds							
6)	B beta-BHC	0.000	6.676	0	772360	N.D.	0.789
7)	B delta-BHC	0.000	6.958	0	2431257	N.D.	1.257
8)	B Heptachlo...	0.000	7.926	0	1577159	N.D.	0.927
10)	B trans-Chl...	0.000	8.219	0	462851	N.D.	0.265
11)	B cis-Chlor...	0.000	8.219f	0	462851	N.D.	0.271
12)	B 4,4'-DDE	0.000	8.516f	0	8536965	N.D.	5.640
14)	MA Endrin	8.094	0.000	2343063	0	5.764	N.D. #
15)	B Endosulfa...	8.321f	8.994f	755827	1087834	1.613	0.751 #
16)	A 4,4'-DDD	0.000	8.994	0	1087834	N.D.	0.828
20)	A Methoxychlor	0.000	9.723f	0	64310	N.D.	<MDL
22)	Toxaphene-1	0.000	8.516	0	8536965	N.D.	887.357
23)	Toxaphene-2	0.000	8.994	0	1087834	N.D.	51.976


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030822\
Data File : PL073231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2022 23:15
Operator : AR\AJ
Sample : PIBLK246
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 05:56:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

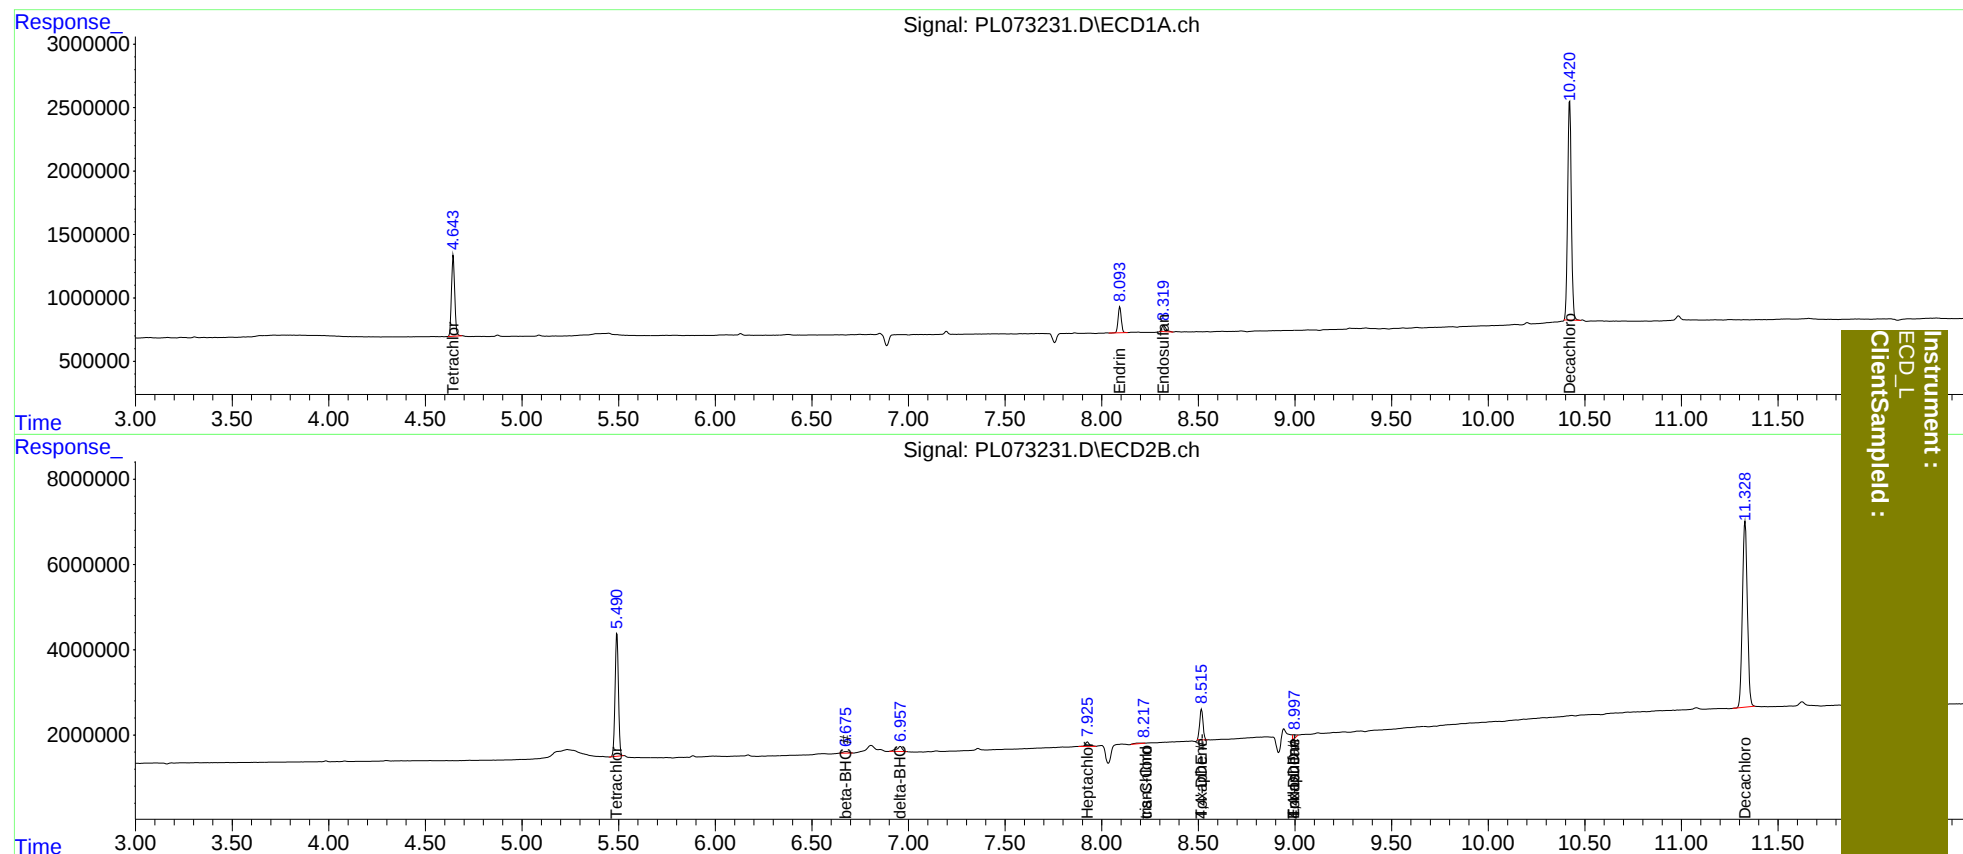


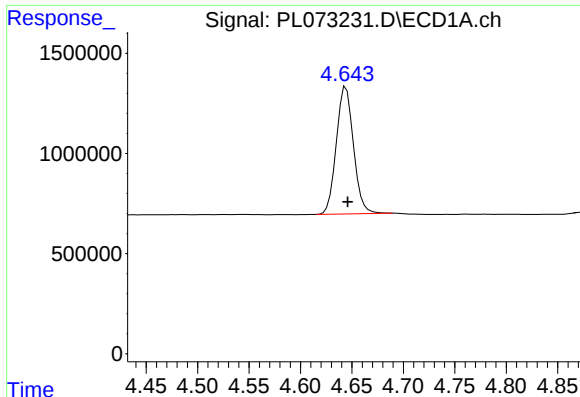

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 7360871
Conc: 21.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

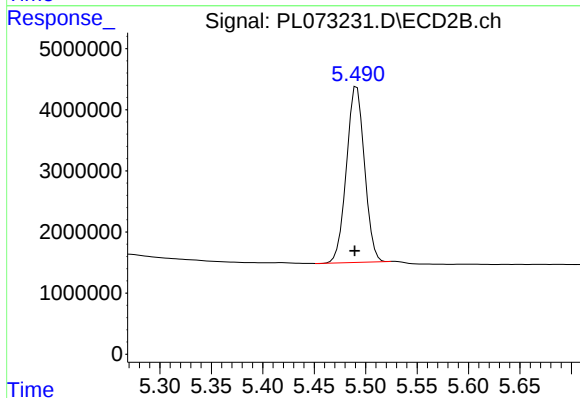


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.002 min
Response: 35128941
Conc: 22.50 ng/ml

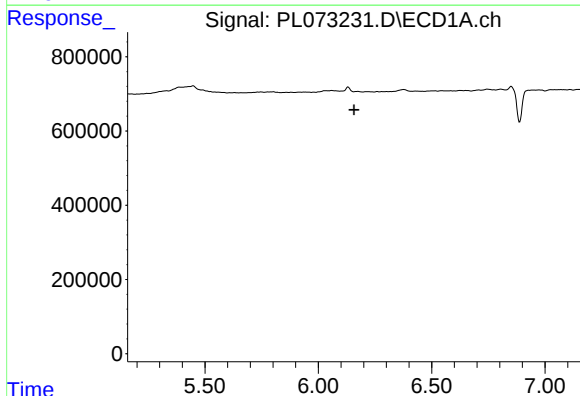


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

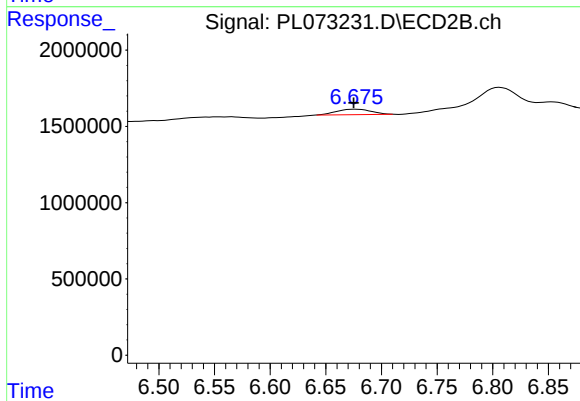

#6 beta-BHC


R.T.: 6.676 min
Delta R.T.: 0.001 min
Response: 772360
Conc: 0.79 ng/ml

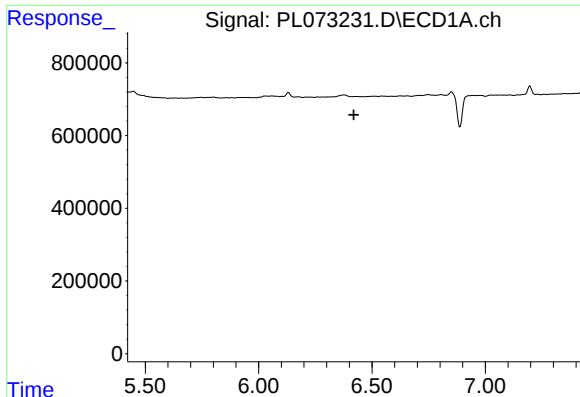

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

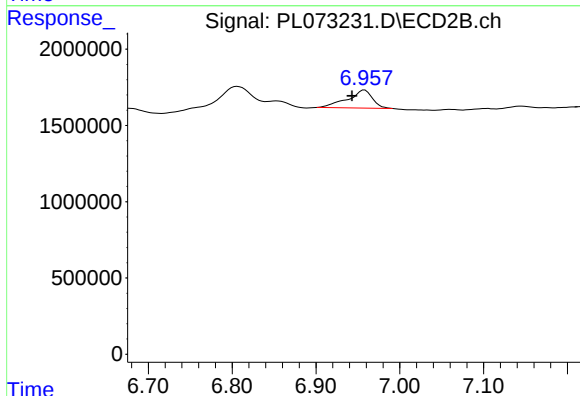


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.015 min
Response: 2431257
Conc: 1.26 ng/ml

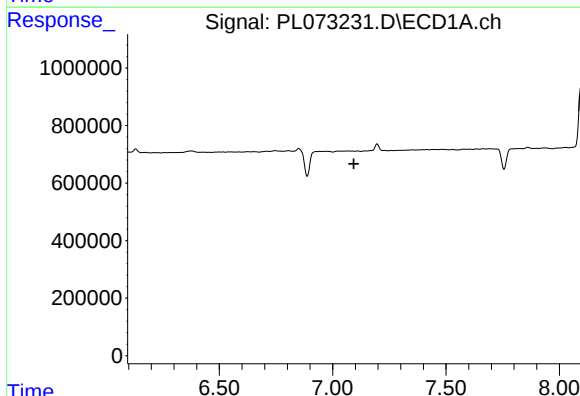


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.094 min
Response: 0
Conc: N.D.

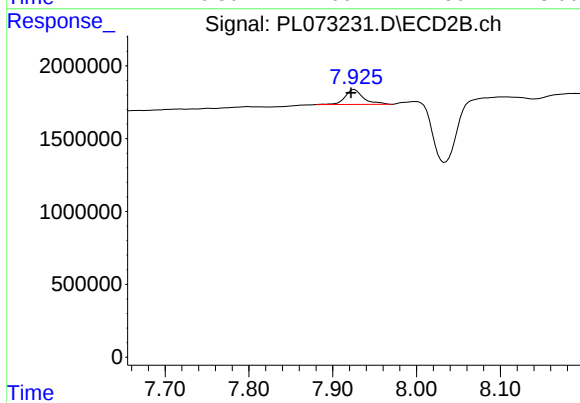

#8 Heptachlor epoxide


R.T.: 7.926 min
Delta R.T.: 0.004 min
Response: 1577159
Conc: 0.93 ng/ml

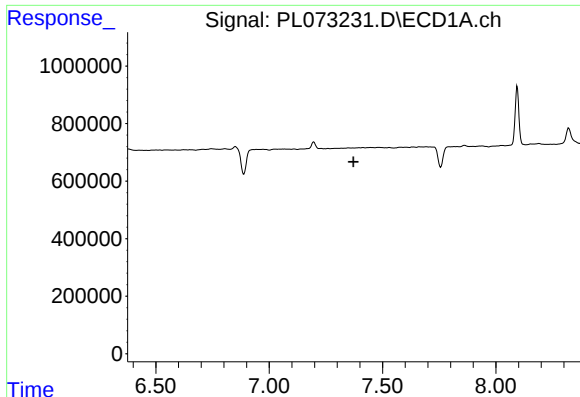

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

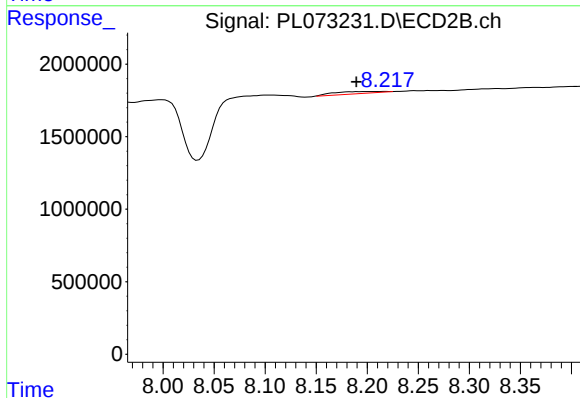


#10 trans-Chlordane

R.T.: 8.219 min
Delta R.T.: 0.029 min
Response: 462851
Conc: 0.27 ng/ml

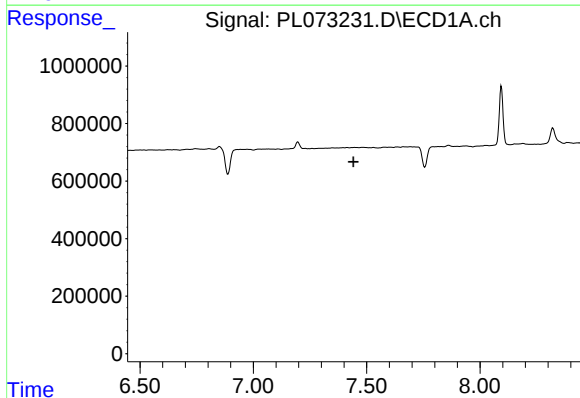


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.442 min
Response: 0
Conc: N.D.

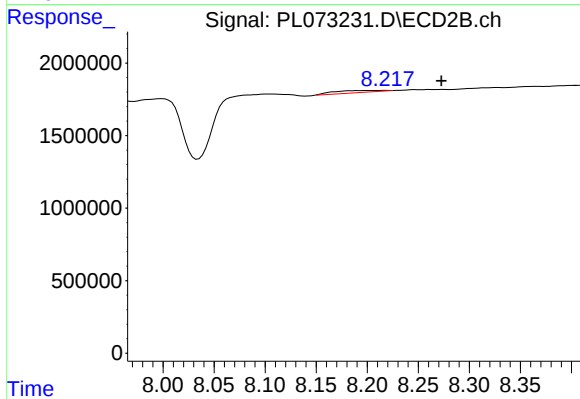

#11 cis-Chlordane


R.T.: 8.219 min
Delta R.T.: -0.054 min
Response: 462851
Conc: 0.27 ng/ml

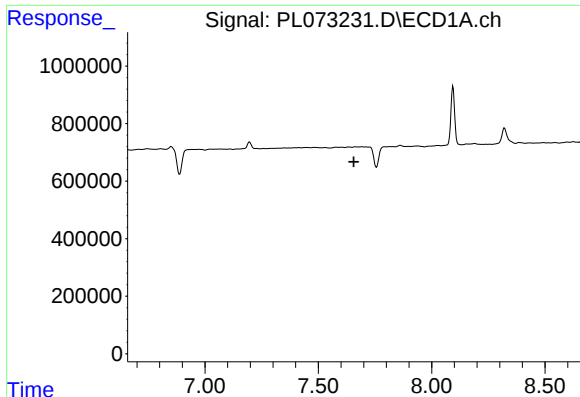

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.657 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

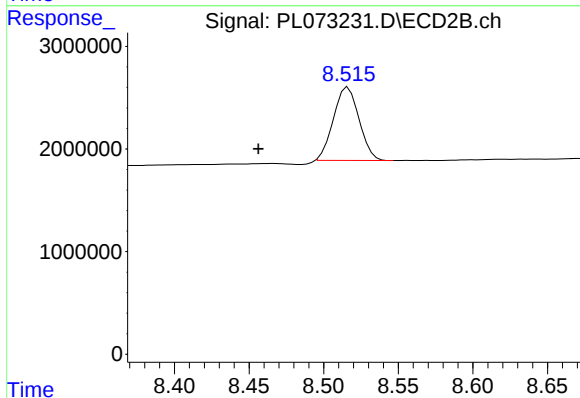


#12 4,4'-DDE

R.T.: 8.516 min
Delta R.T.: 0.060 min
Response: 8536965
Conc: 5.64 ng/ml

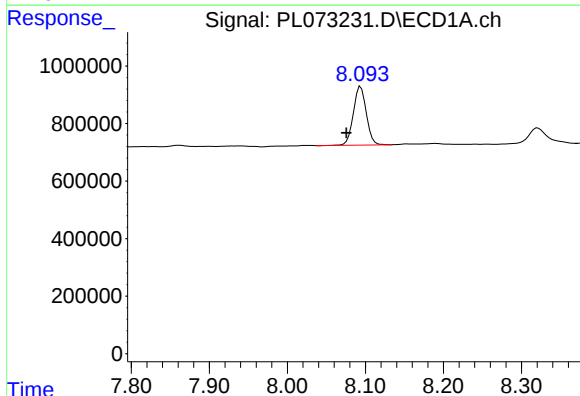


#14 Endrin

R.T.: 8.094 min
Delta R.T.: 0.019 min
Response: 2343063
Conc: 5.76 ng/ml

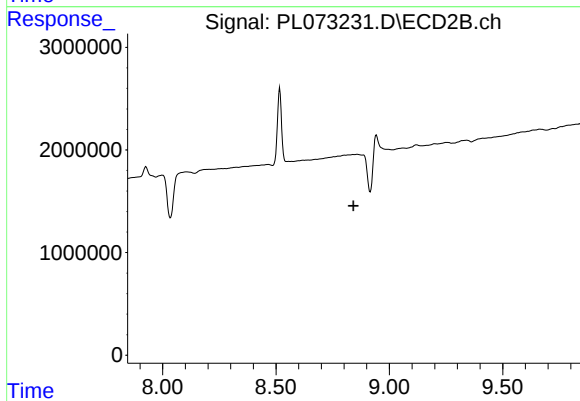

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.842 min
Response: 0
Conc: N.D.

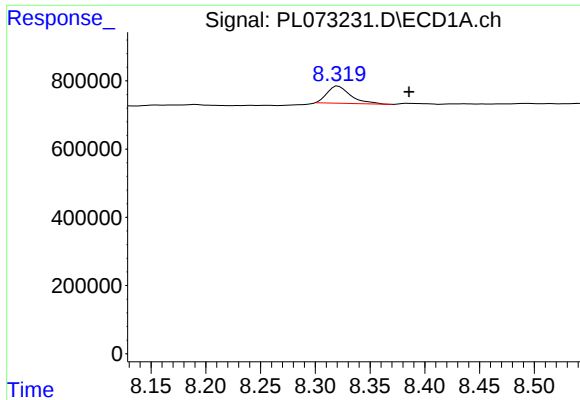

#15 Endosulfan II


R.T.: 8.321 min
Delta R.T.: -0.065 min
Response: 755827
Conc: 1.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

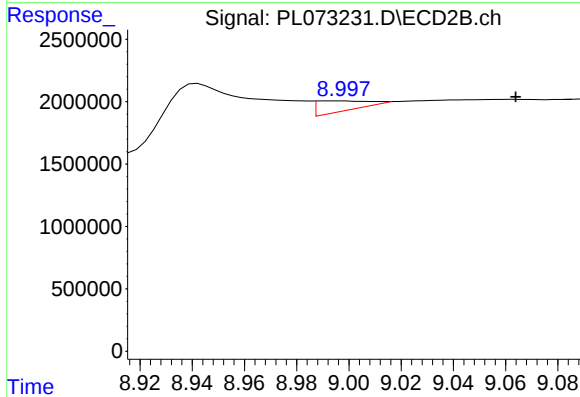


#15 Endosulfan II

R.T.: 8.994 min
Delta R.T.: -0.070 min
Response: 1087834
Conc: 0.75 ng/ml

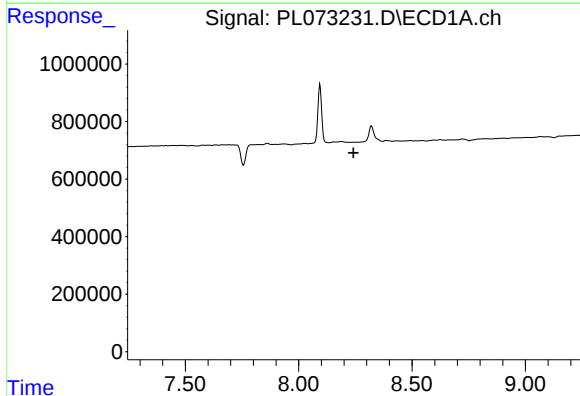


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

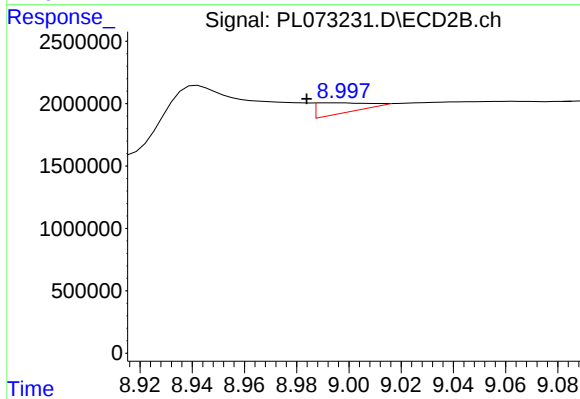

#16 4,4'-DDD


R.T.: 8.994 min
Delta R.T.: 0.010 min
Response: 1087834
Conc: 0.83 ng/ml

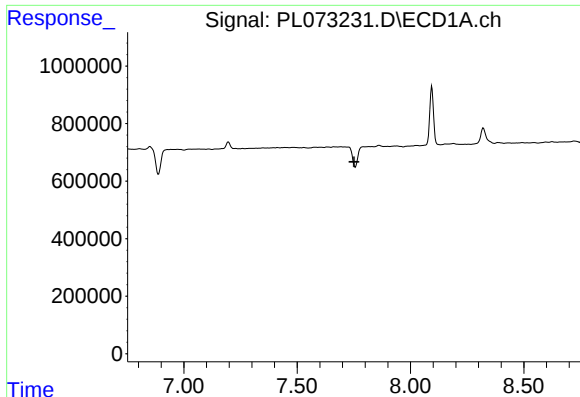

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

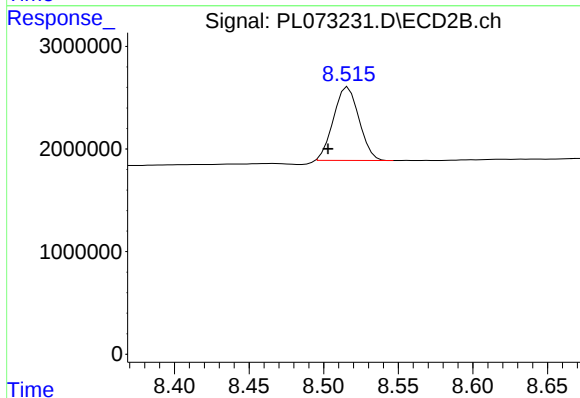


#22 Toxaphene-1

R.T.: 8.516 min
Delta R.T.: 0.014 min
Response: 8536965
Conc: 887.36 ng/ml

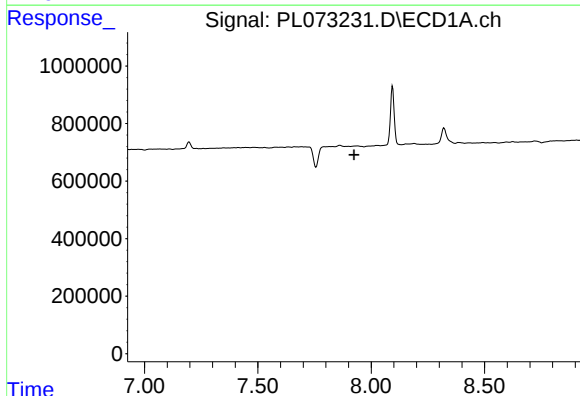


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 7.925 min
Response: 0
Conc: N.D.

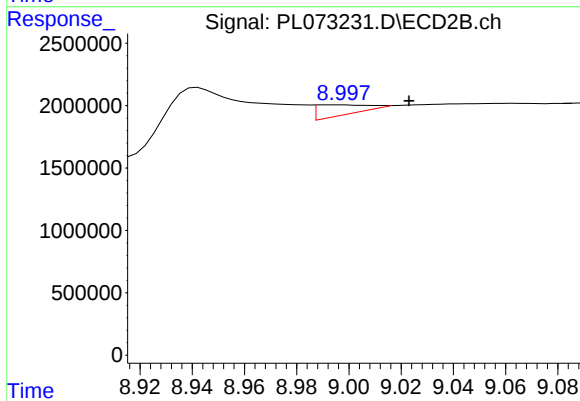

#23 Toxaphene-2


R.T.: 8.994 min
Delta R.T.: -0.029 min
Response: 1087834
Conc: 51.98 ng/ml

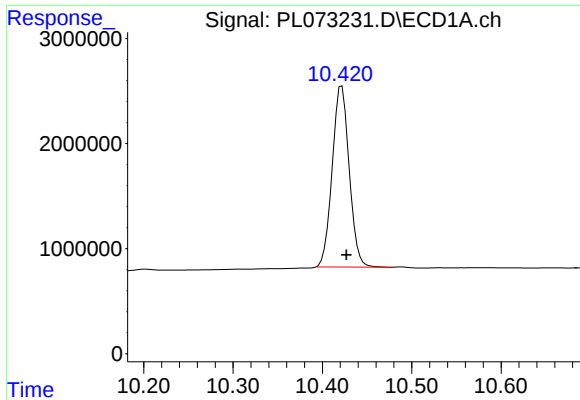

#27 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.005 min
Response: 22736471
Conc: 47.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

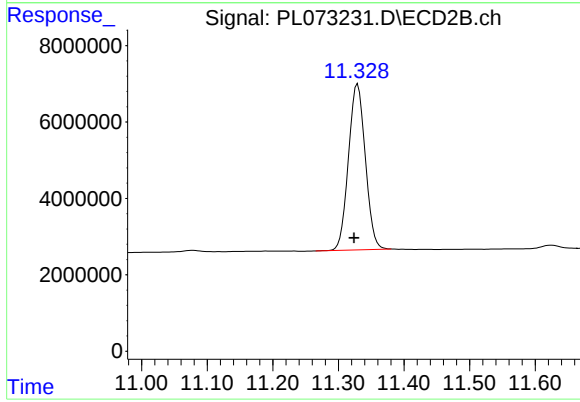

#27 Decachlorobiphenyl

R.T.: 11.329 min
Delta R.T.: 0.005 min
Response: 77653808
Conc: 48.04 ng/ml