

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030823\
 Data File : PL081321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2023 15:27
 Operator : AR\AJ
 Sample : 01829-10 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SS-10-20230306

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/09/2023
 Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 20:34:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.338	2.660	3776425	2616595	1.748	1.293m#
2) SA Decachlor...	8.767	7.787	5975691	1943104	3.920m	1.014 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030823\
Data File : PL081321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2023 15:27
Operator : AR\AJ
Sample : 01829-10 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SS-10-20230306


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 20:34:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

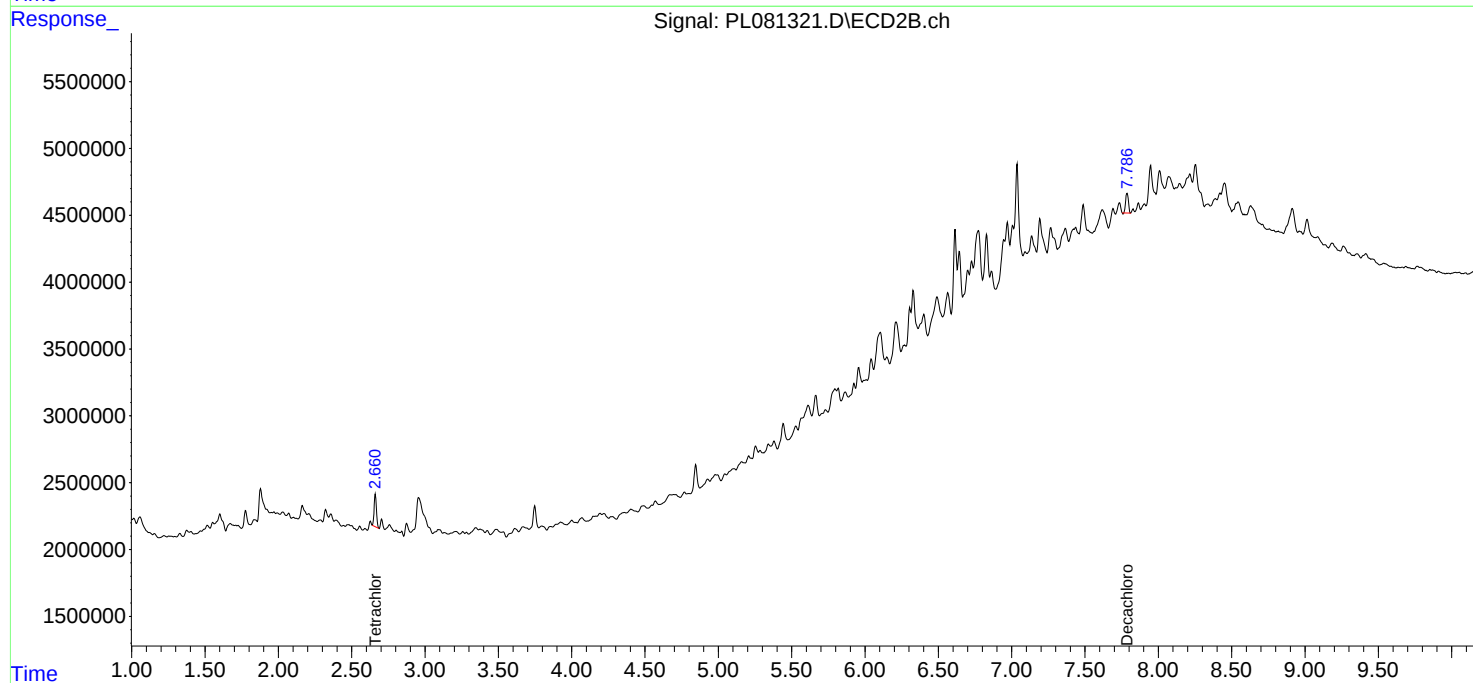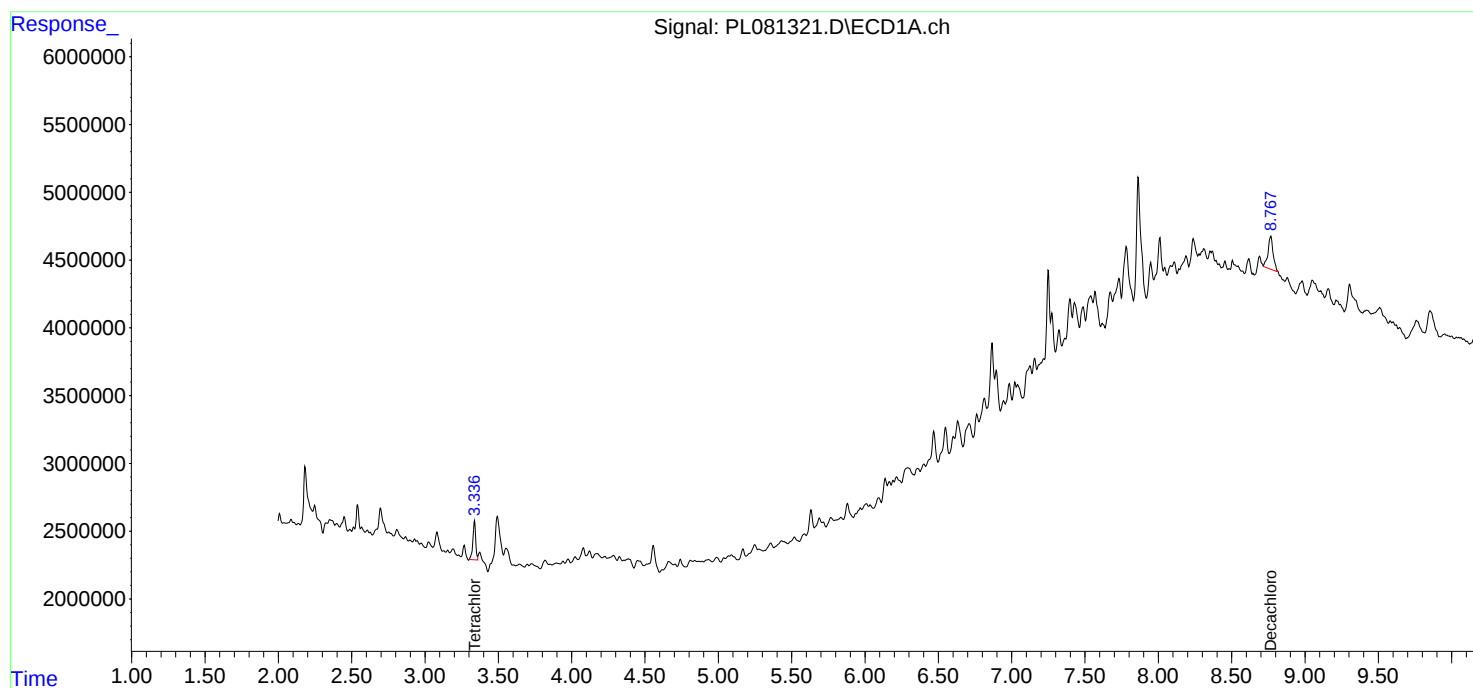

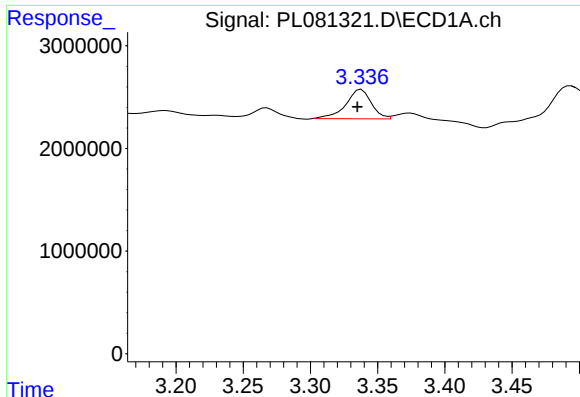


#1 Tetrachloro-m-xylene

R.T.: 3.338 min
Delta R.T.: 0.003 min
Response: 3776425
Conc: 1.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
SS-10-20230306


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

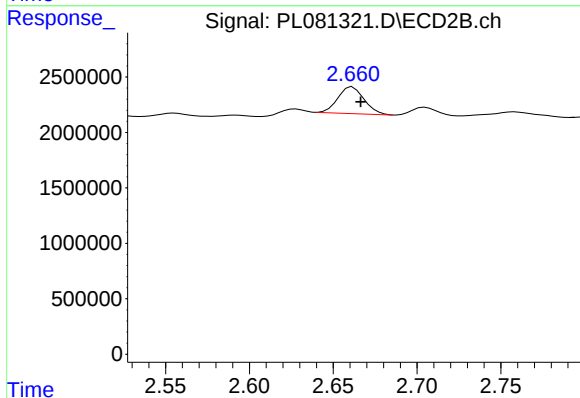


#1 Tetrachloro-m-xylene

R.T.: 2.660 min
Delta R.T.: -0.006 min
Response: 2616595
Conc: 1.29 ng/ml m

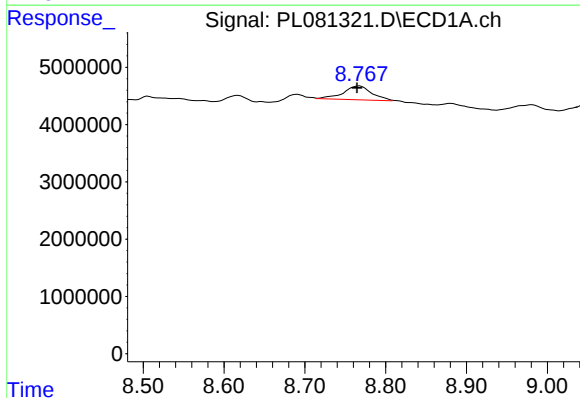

#28 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: 0.002 min
Response: 5975691
Conc: 3.92 ng/ml m

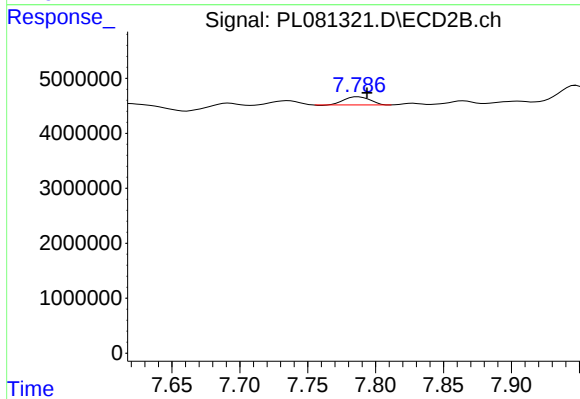

#28 Decachlorobiphenyl

R.T.: 7.787 min
Delta R.T.: -0.007 min
Response: 1943104
Conc: 1.01 ng/ml