

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030823\
 Data File : PL081324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2023 16:30
 Operator : AR\AJ
 Sample : 01829-13 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SS-11-20230306

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 20:38:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	2.664	2297521	2255196	1.063	1.114
28)	SA Decachlor...	8.758	7.788	3116709	2538666	2.044	1.325 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030823\
Data File : PL081324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2023 16:30
Operator : AR\AJ
Sample : 01829-13 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SS-11-20230306

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 20:38:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

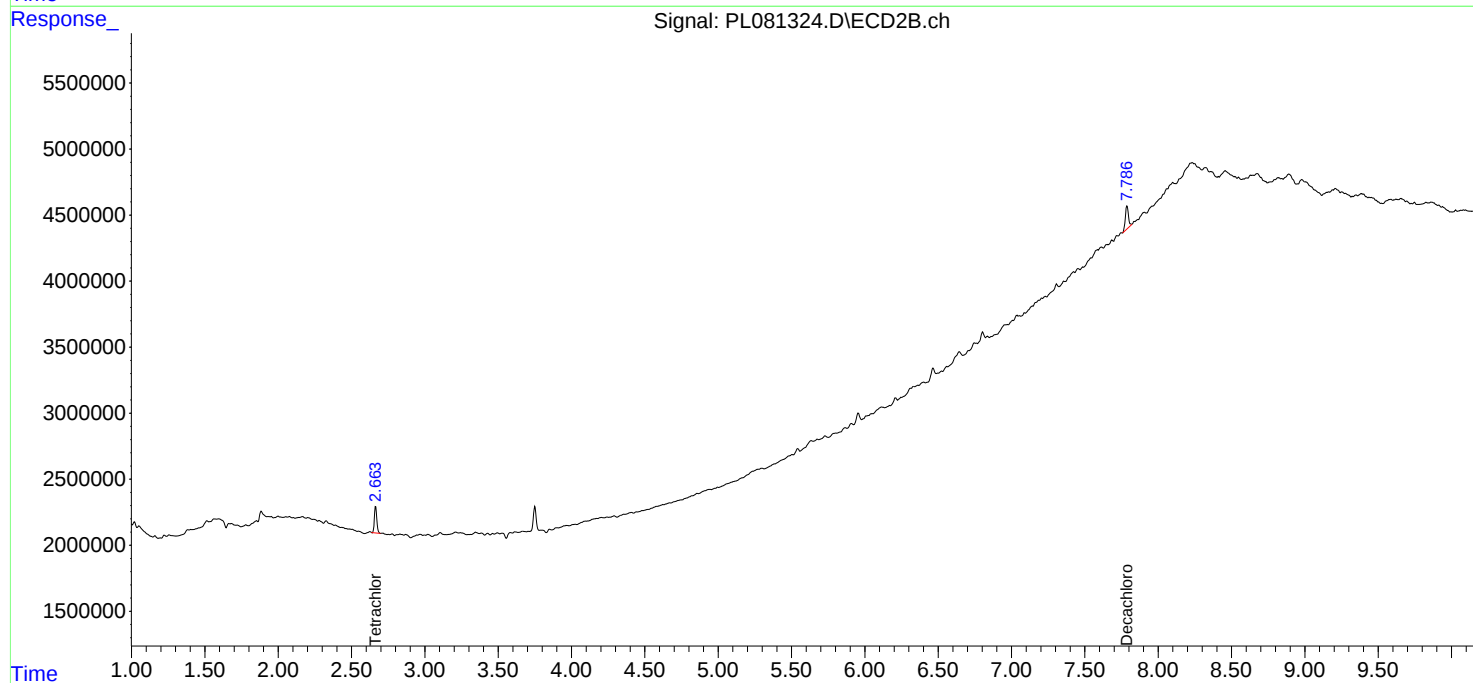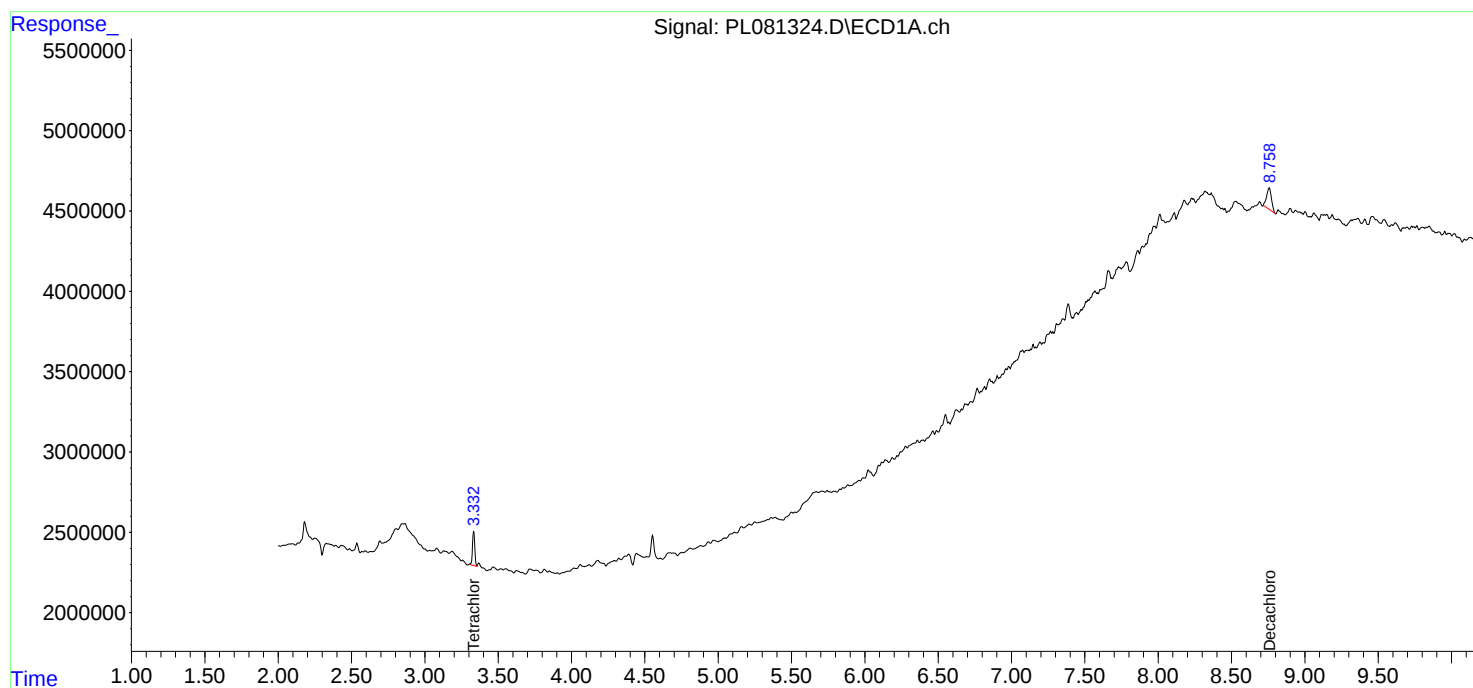


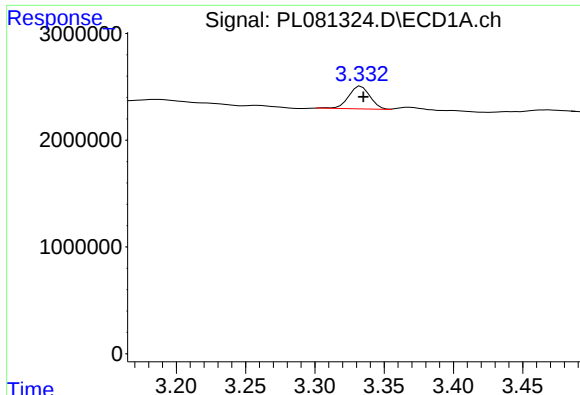

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.002 min
Response: 2297521
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
SS-11-20230306

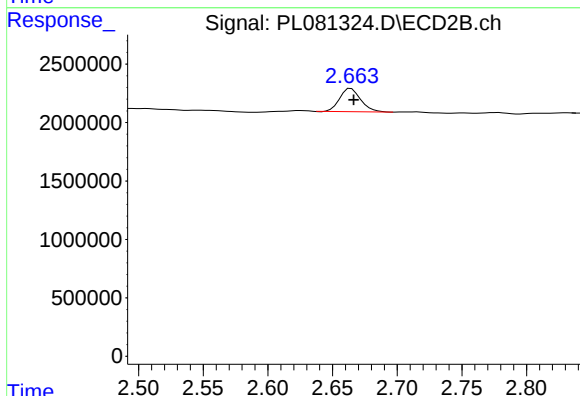


#1 Tetrachloro-m-xylene

R.T.: 2.664 min
Delta R.T.: -0.002 min
Response: 2255196
Conc: 1.11 ng/ml

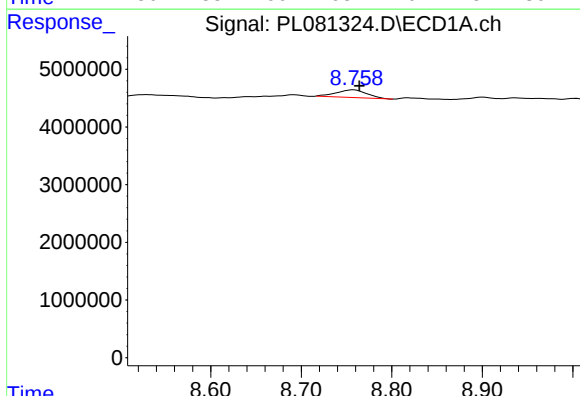

#28 Decachlorobiphenyl

R.T.: 8.758 min
Delta R.T.: -0.006 min
Response: 3116709
Conc: 2.04 ng/ml

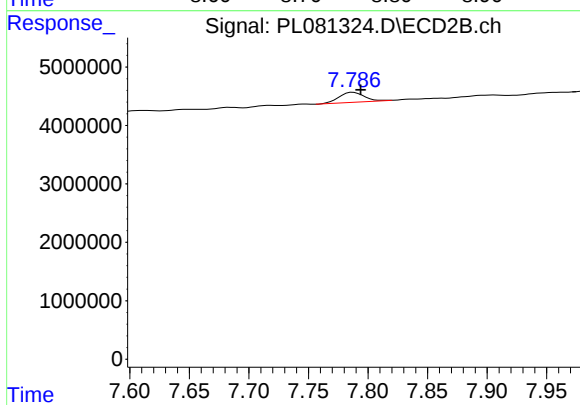

#28 Decachlorobiphenyl

R.T.: 7.788 min
Delta R.T.: -0.006 min
Response: 2538666
Conc: 1.33 ng/ml