

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030920\
 Data File : PL057145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2020 14:02
 Operator : AJ\MA
 Sample : L1803-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N38129

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 00:37:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	176.1E6	39068893	20.662	18.312
28)	SA Decachlor...	8.205	8.979	129.0E6	28348612	13.350	13.342
Target Compounds							
3)	MA gamma-BHC...	4.187	0.000	29731126	0	2.164	N.D. #
4)	MA Heptachlor	4.466f	5.138	105.0E6	2006354	7.732	0.645 #
7)	B delta-BHC	0.000	5.000	0	19544885	N.D.	8.027 #
11)	B alpha-Chl...	5.446	0.000	53404136	0	4.347	N.D. #
15)	B Endosulfa...	6.292	6.870f	10001546	4774009	0.926	1.701 #
23)	Chlordane-1	4.347f	4.938	5554945	3885494	18.276	48.443 #
26)	Chlordane-4	5.446	0.000	53404136	0	58.112	N.D. #
27)	Chlordane-5	6.292	0.000	10001546	0	27.535	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030920\
Data File : PL057145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2020 14:02
Operator : AJ\MA
Sample : L1803-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
N38129

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 00:37:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

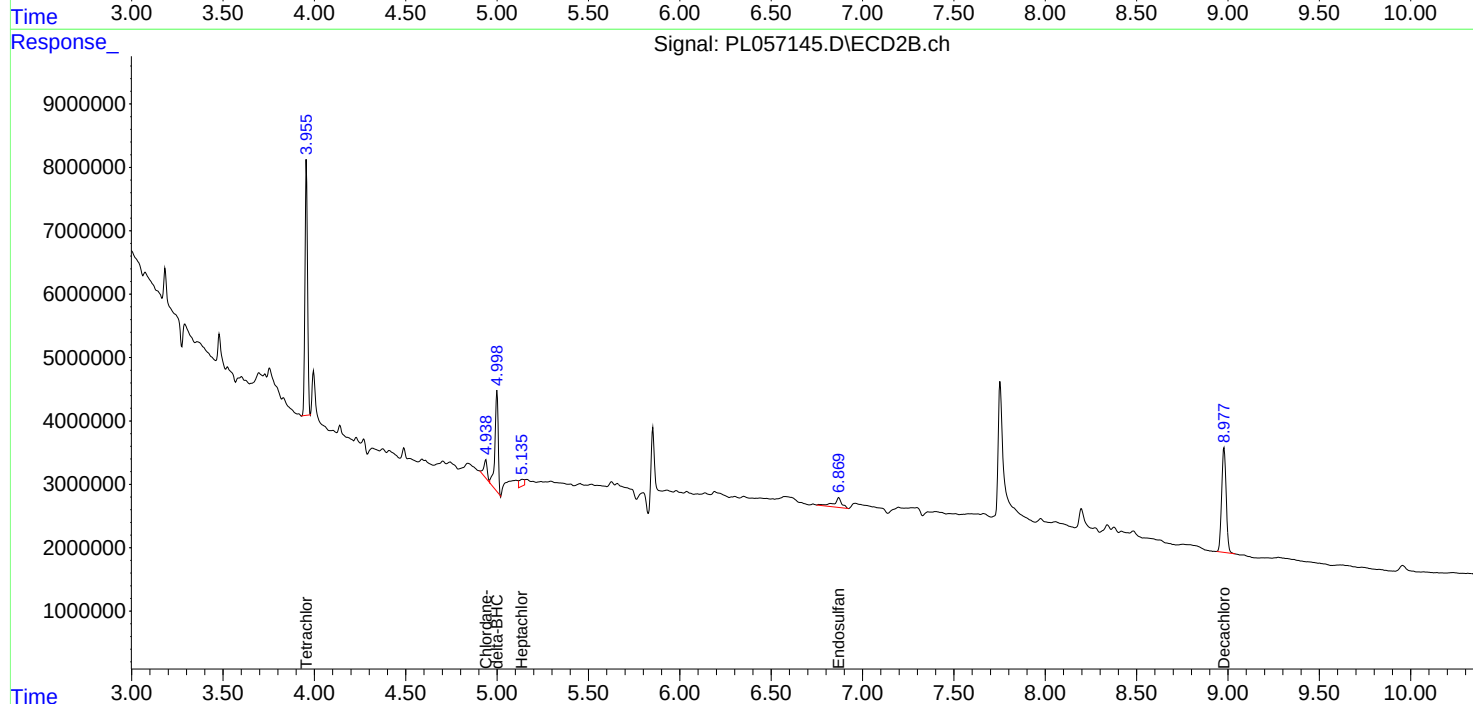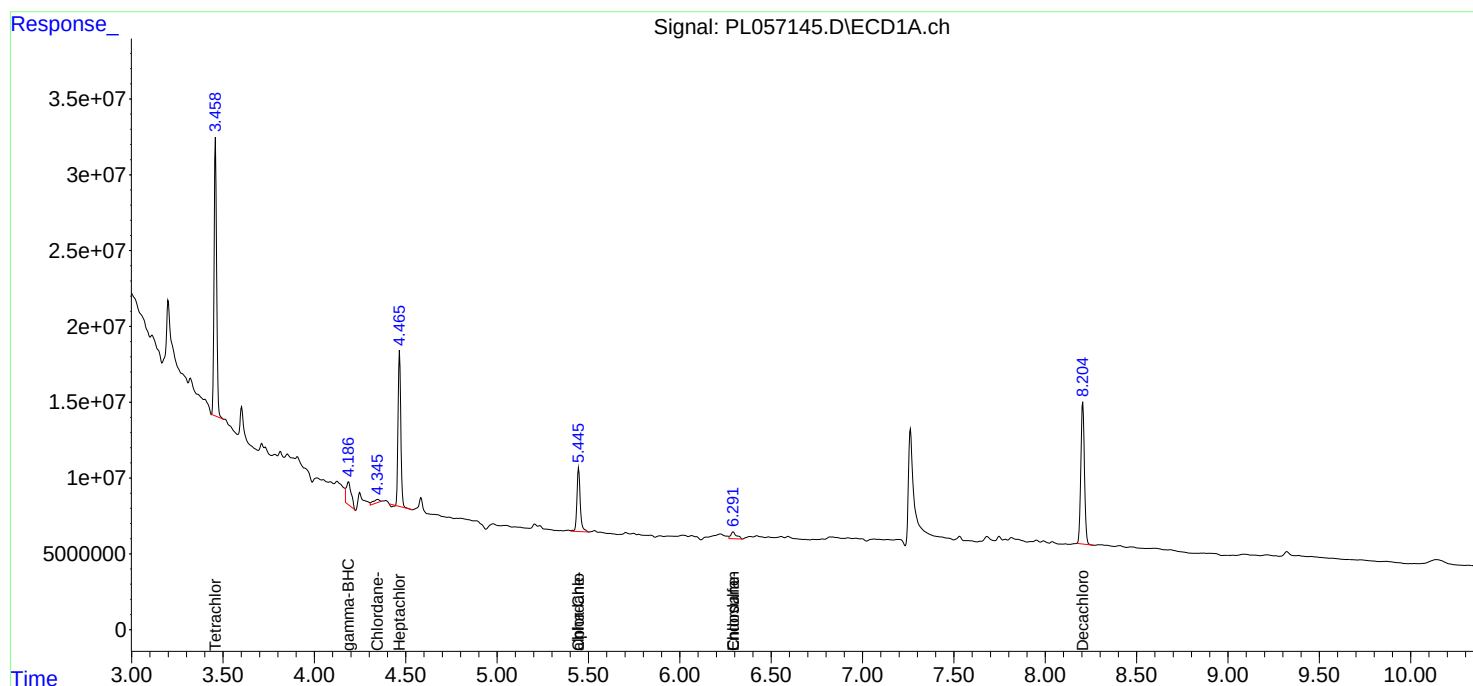


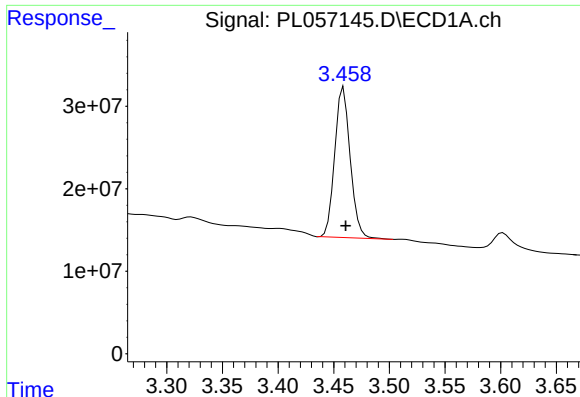

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 176089805
Conc: 20.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
N38129

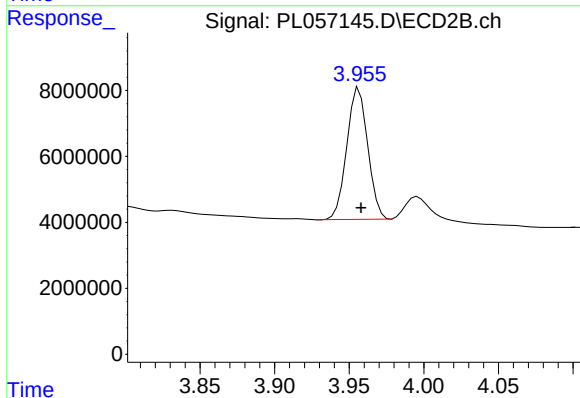


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 39068893
Conc: 18.31 ng/ml

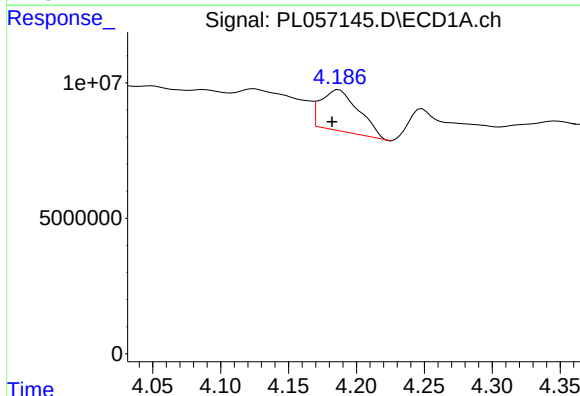


#3 gamma-BHC (Lindane)

R.T.: 4.187 min
Delta R.T.: 0.005 min
Response: 29731126
Conc: 2.16 ng/ml

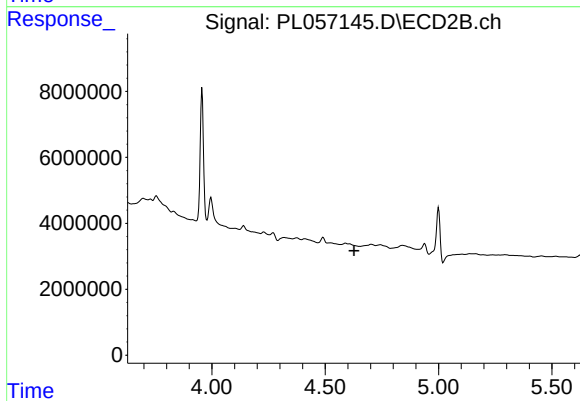

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.627 min
Response: 0
Conc: N.D.

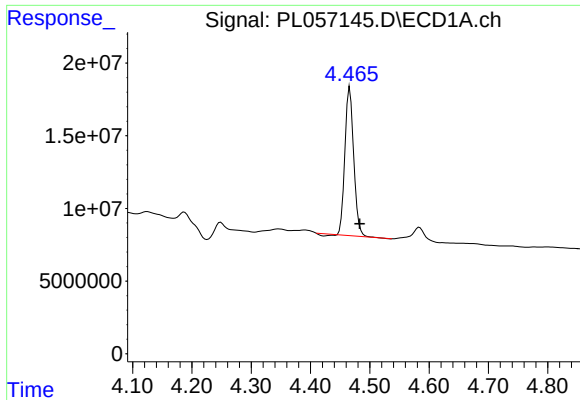

#4 Heptachlor


R.T.: 4.466 min
Delta R.T.: -0.017 min
Response: 105026379
Conc: 7.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
N38129

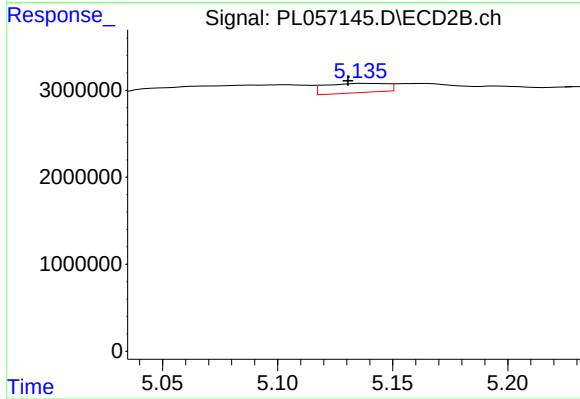


#4 Heptachlor

R.T.: 5.138 min
Delta R.T.: 0.007 min
Response: 2006354
Conc: 0.64 ng/ml

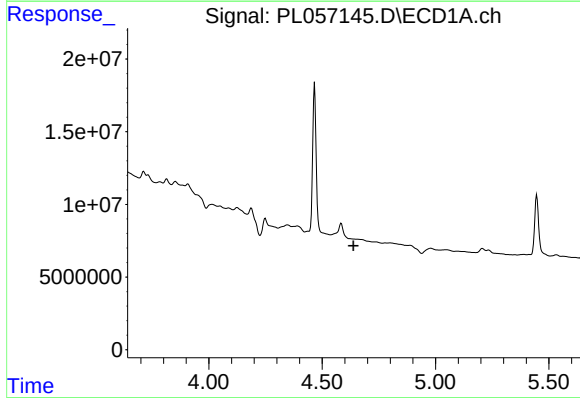


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.638 min
Response: 0
Conc: N.D.

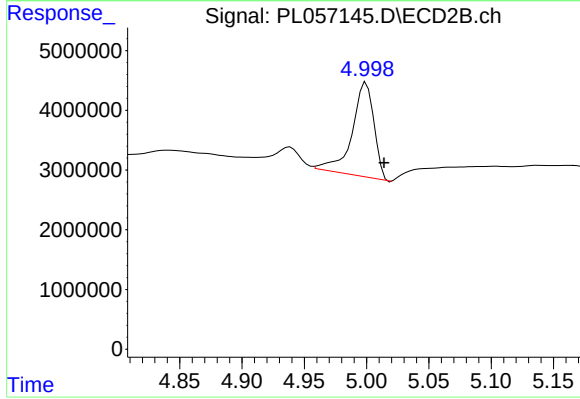

#7 delta-BHC


R.T.: 5.000 min
Delta R.T.: -0.014 min
Response: 19544885
Conc: 8.03 ng/ml

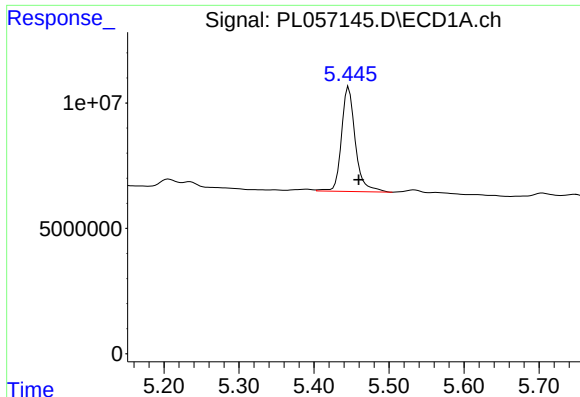

#11 alpha-Chlordane


R.T.: 5.446 min
Delta R.T.: -0.013 min
Response: 53404136
Conc: 4.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
N38129

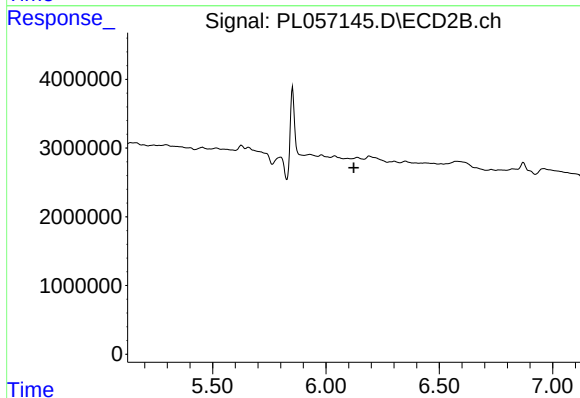


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.123 min
Response: 0
Conc: N.D.

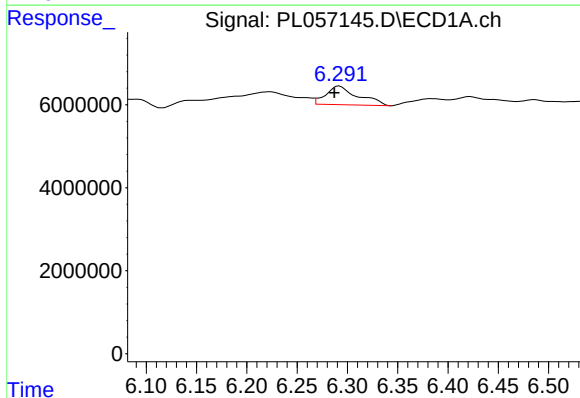


#15 Endosulfan II

R.T.: 6.292 min
Delta R.T.: 0.005 min
Response: 10001546
Conc: 0.93 ng/ml

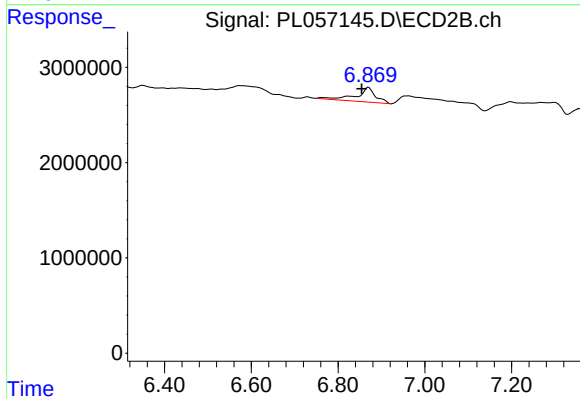

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.015 min
Response: 4774009
Conc: 1.70 ng/ml

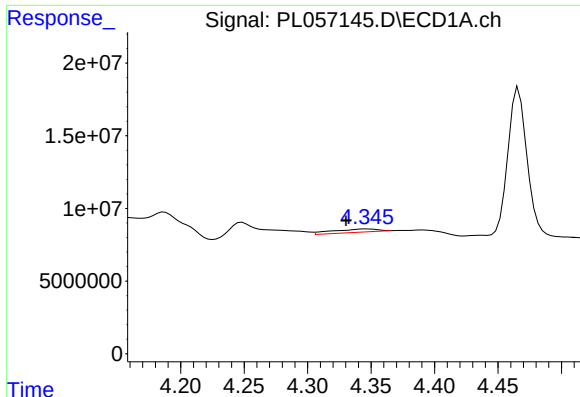

#23 Chlordane-1


R.T.: 4.347 min
Delta R.T.: 0.016 min
Response: 5554945
Conc: 18.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
N38129

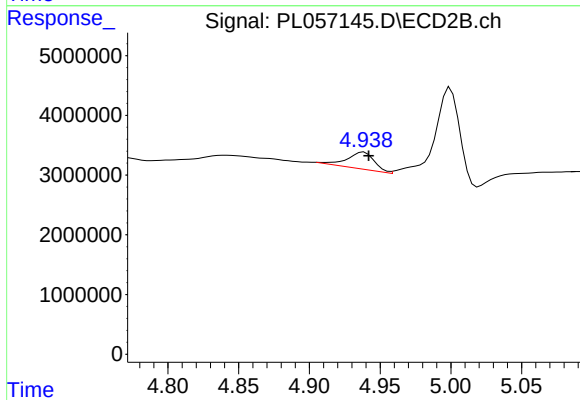


#23 Chlordane-1

R.T.: 4.938 min
Delta R.T.: -0.004 min
Response: 3885494
Conc: 48.44 ng/ml

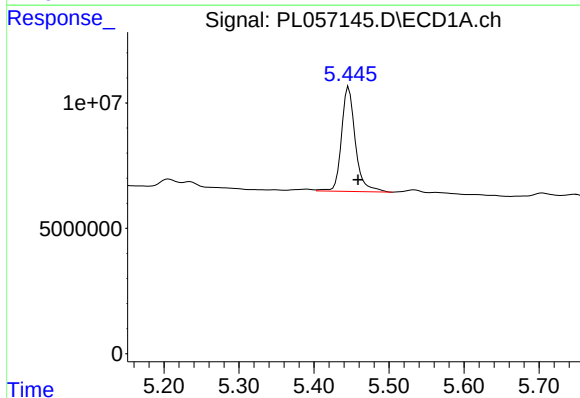


#26 Chlordane-4

R.T.: 5.446 min
Delta R.T.: -0.012 min
Response: 53404136
Conc: 58.11 ng/ml

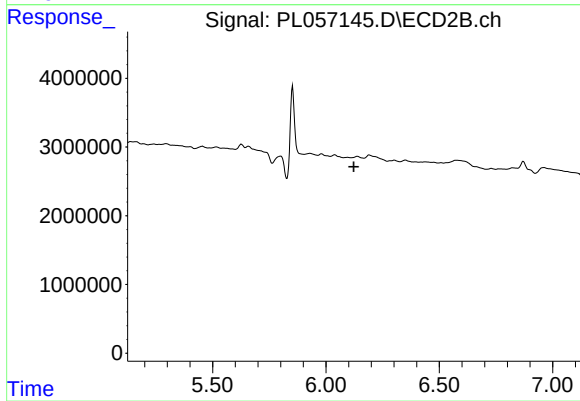

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.123 min
Response: 0
Conc: N.D.

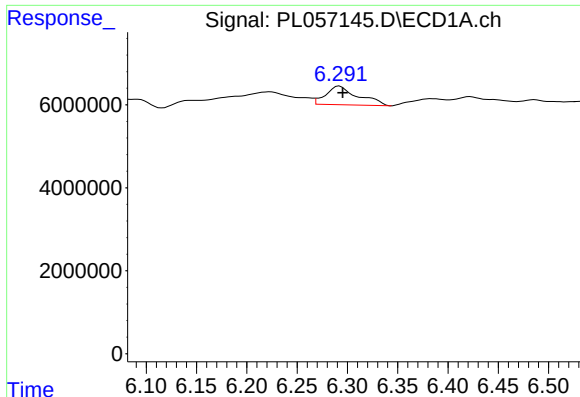

#27 Chlordane-5


R.T.: 6.292 min
Delta R.T.: -0.003 min
Response: 10001546
Conc: 27.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
N38129

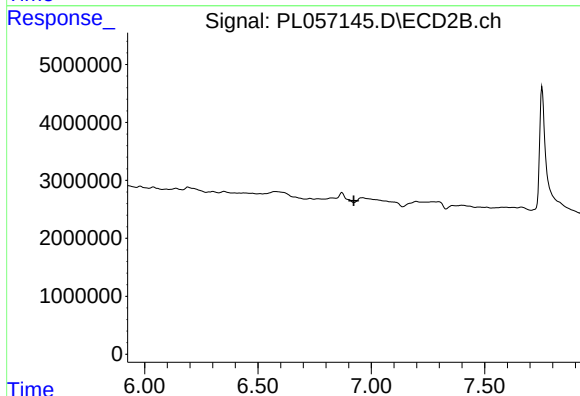


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.923 min
Response: 0
Conc: N.D.

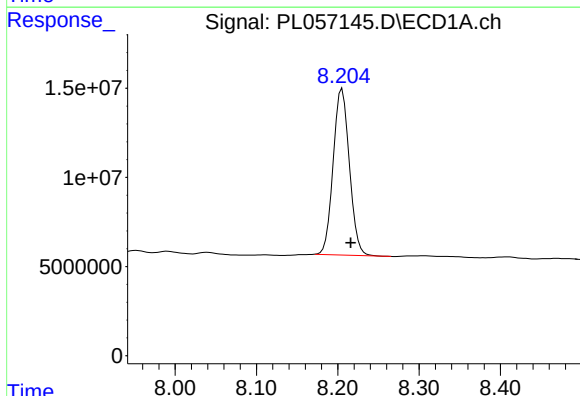

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.011 min
Response: 129029836
Conc: 13.35 ng/ml

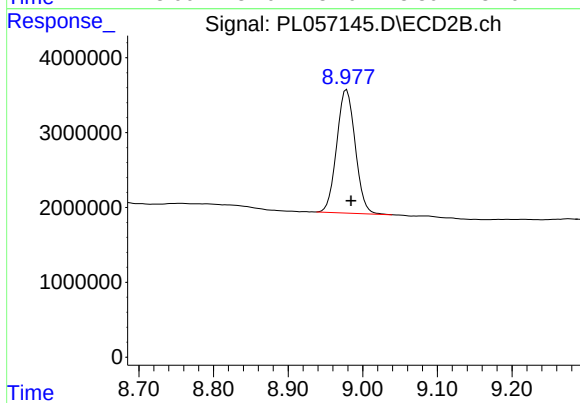

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.006 min
Response: 28348612
Conc: 13.34 ng/ml