

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030920\
 Data File : PL057149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2020 15:00
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 00:38:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	183.1E6	44857897	21.483	21.025
28)	SA Decachlor...	8.206	8.980	192.2E6	42573487	19.888	20.037
Target Compounds							
4)	MA Heptachlor	0.000	5.140	0	6360724	N.D.	2.044 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030920\
Data File : PL057149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2020 15:00
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 00:38:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

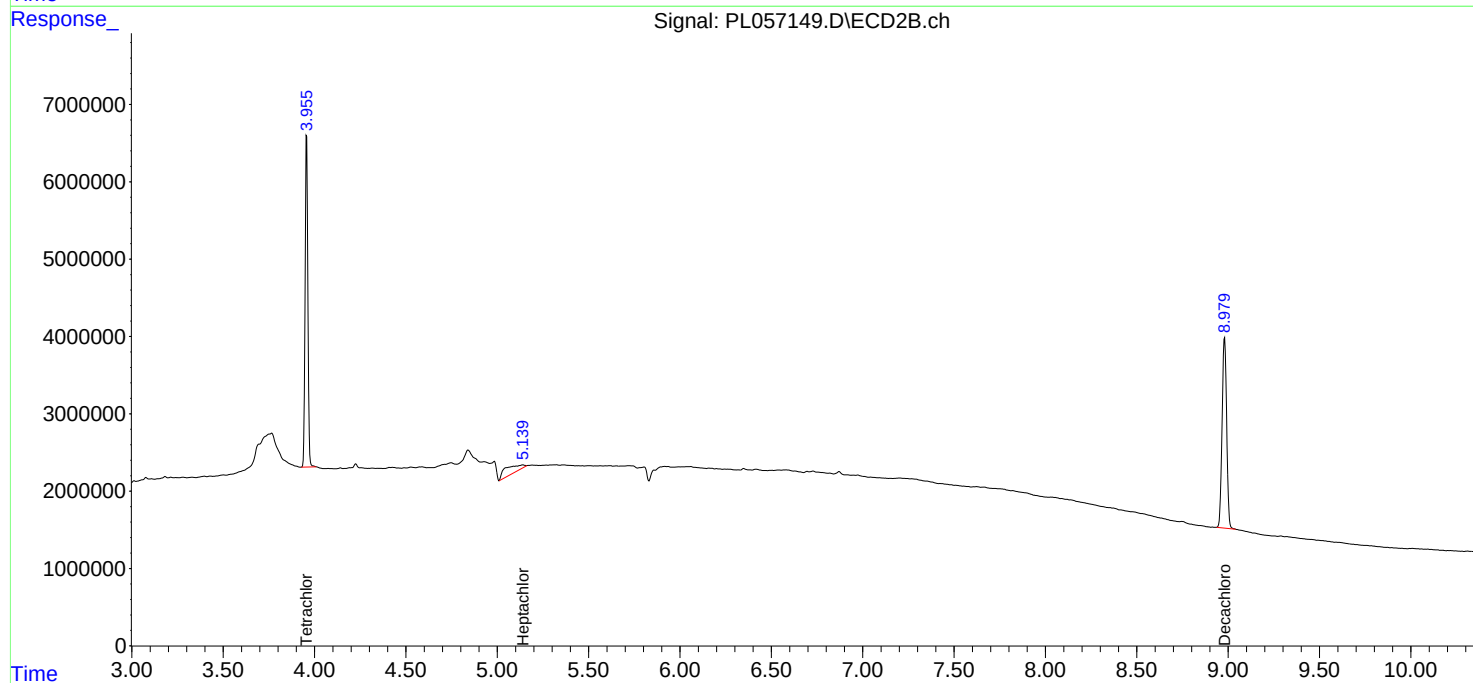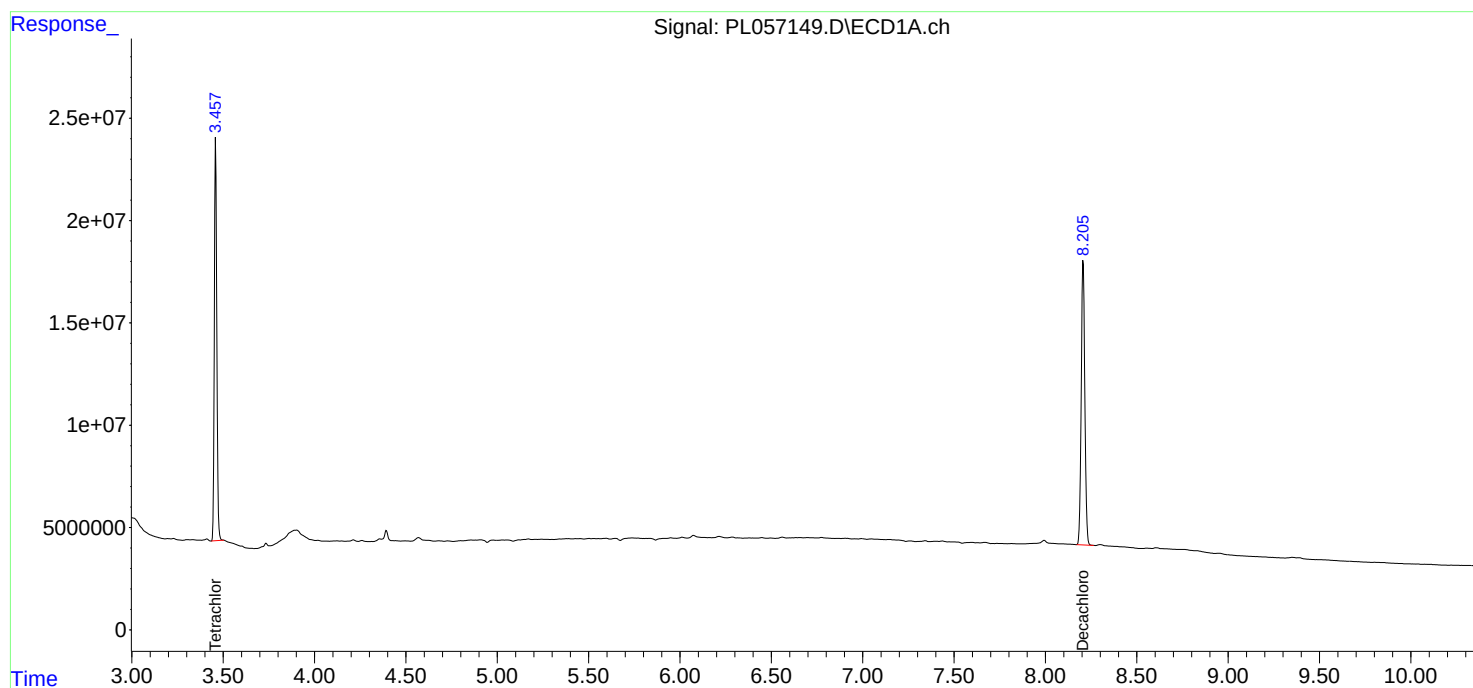


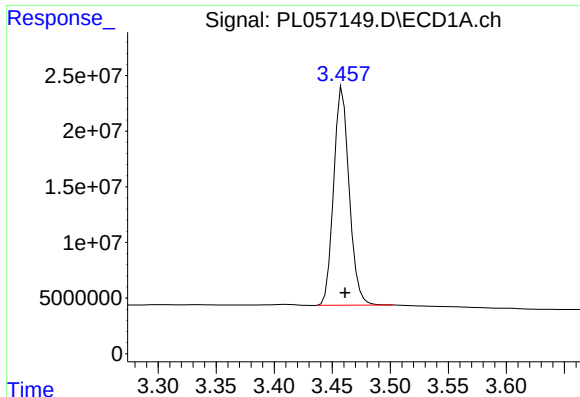

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 183082383
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

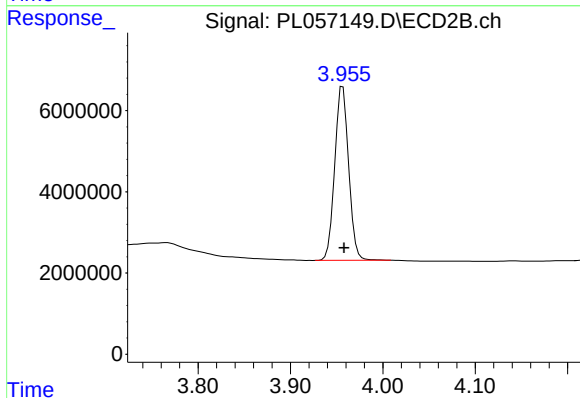


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 44857897
Conc: 21.03 ng/ml

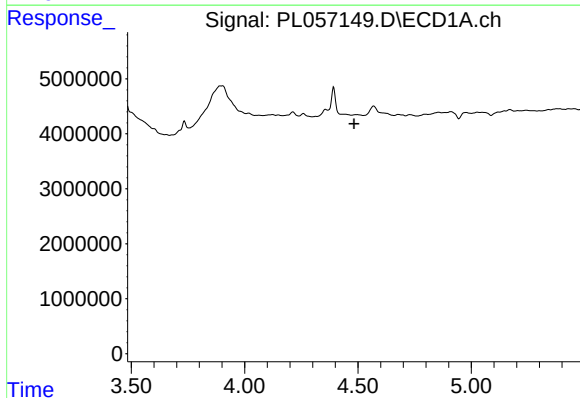


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

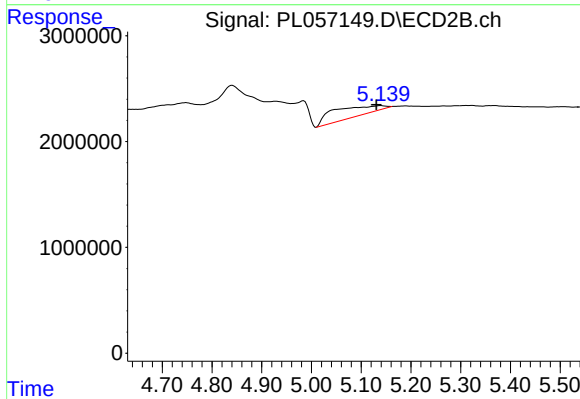

#4 Heptachlor


R.T.: 5.140 min
Delta R.T.: 0.010 min
Response: 6360724
Conc: 2.04 ng/ml

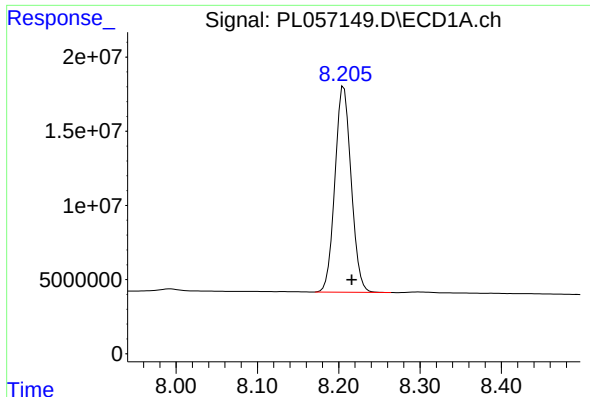

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.010 min
Response: 192216208
Conc: 19.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

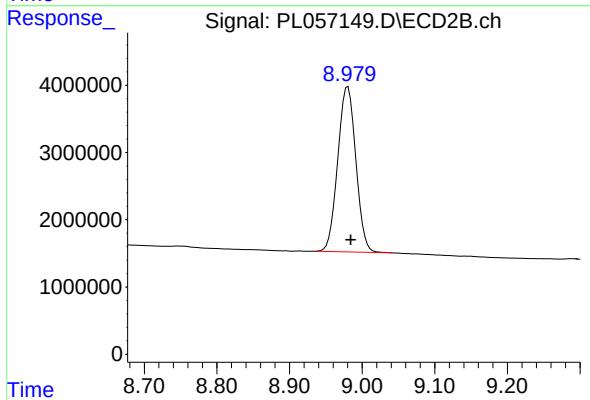

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.004 min
Response: 42573487
Conc: 20.04 ng/ml