

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
 Data File : PL073249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 19:46
 Operator : AR\AJ
 Sample : N1816-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 04:52:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.492	6971593	33869041	20.273	21.695
27)	SA Decachlor...	10.422	11.332	20812245	71393060	43.285	44.170
Target Compounds							
2)	A alpha-BHC	0.000	6.027f	0	395724	N.D.	0.205
6)	B beta-BHC	0.000	6.668	0	712378	N.D.	0.728
7)	B delta-BHC	0.000	6.954	0	2083451	N.D.	1.078
8)	B Heptachlo...	0.000	7.966f	0	240135	N.D.	0.141
9)	A Endosulfan I	0.000	8.365f	0	178244	N.D.	0.112
15)	B Endosulfa...	8.321f	0.000	604997	0	1.291	N.D. #
16)	A 4,4'-DDD	0.000	8.940f	0	2782712	N.D.	2.119
20)	A Methoxychlor	0.000	9.723f	0	415901	N.D.	0.543

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
Data File : PL073249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 19:46
Operator : AR\AJ
Sample : N1816-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 04:52:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

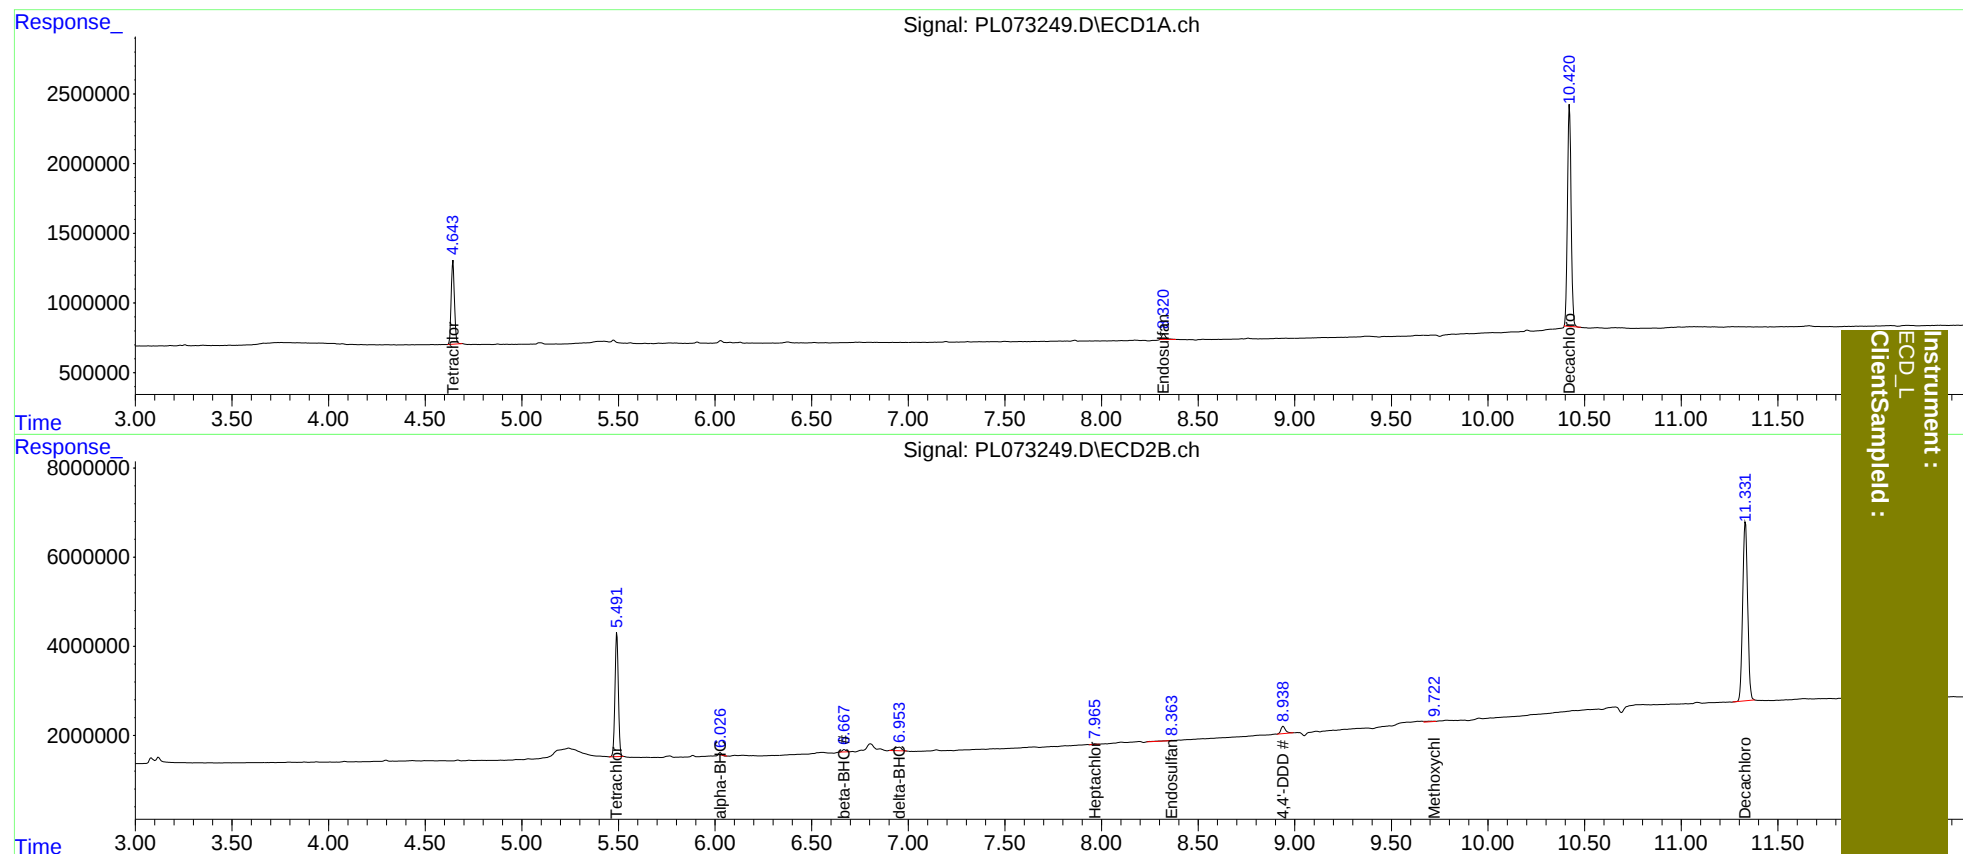


Instrument :
ECD_L
ClientSampled :
N1816-04

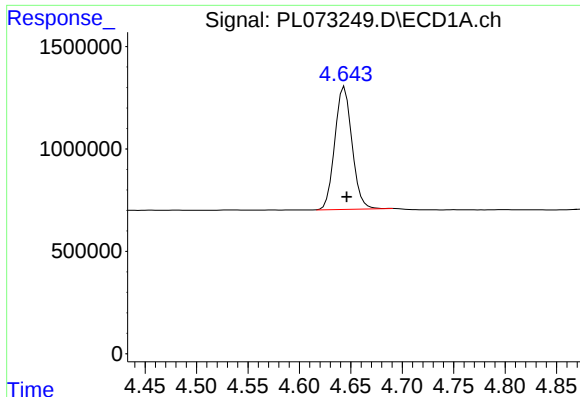

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 6971593
Conc: 20.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

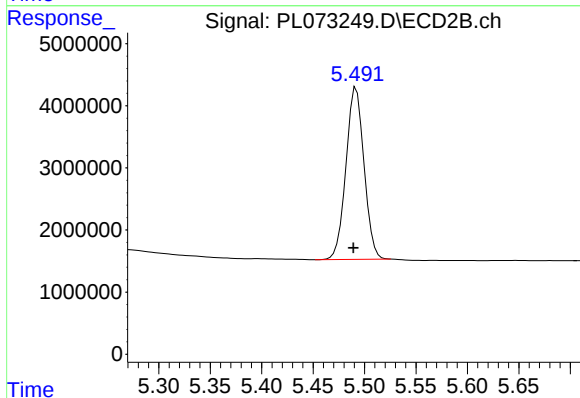


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.003 min
Response: 33869041
Conc: 21.69 ng/ml

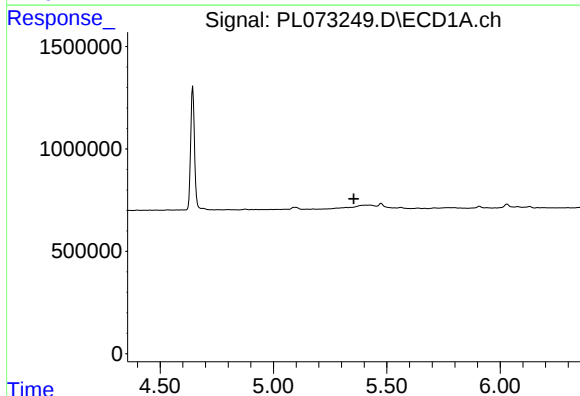


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

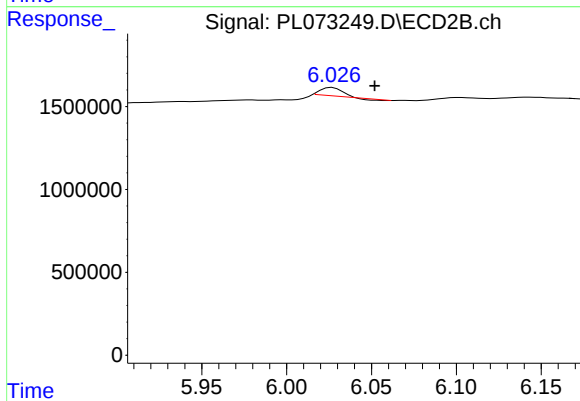

#2 alpha-BHC


R.T.: 6.027 min
Delta R.T.: -0.025 min
Response: 395724
Conc: 0.20 ng/ml

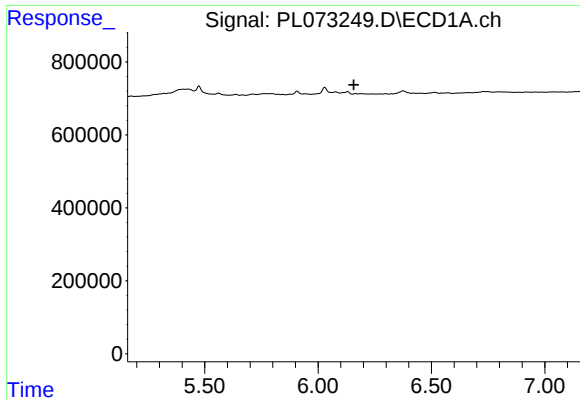

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

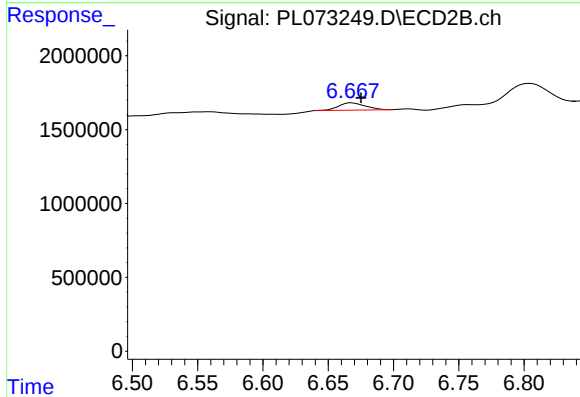


#6 beta-BHC

R.T.: 6.668 min
Delta R.T.: -0.007 min
Response: 712378
Conc: 0.73 ng/ml

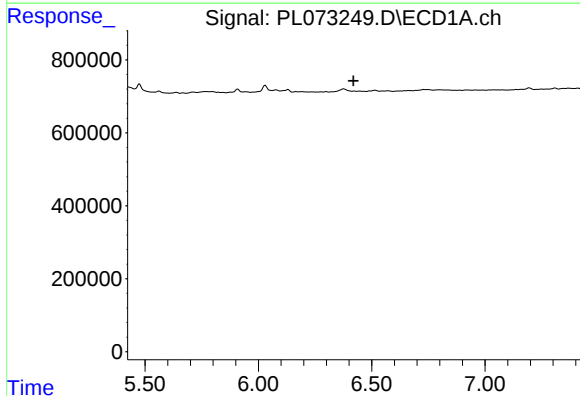


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

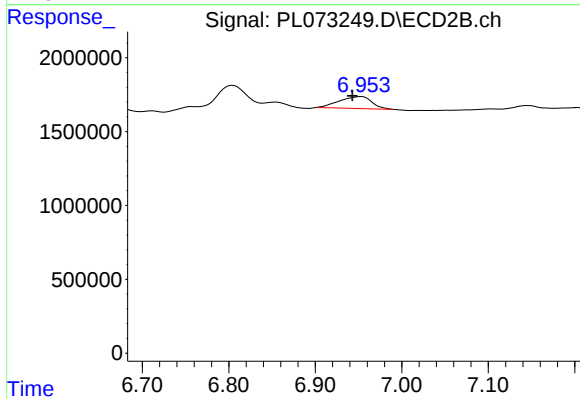

#7 delta-BHC


R.T.: 6.954 min
Delta R.T.: 0.011 min
Response: 2083451
Conc: 1.08 ng/ml

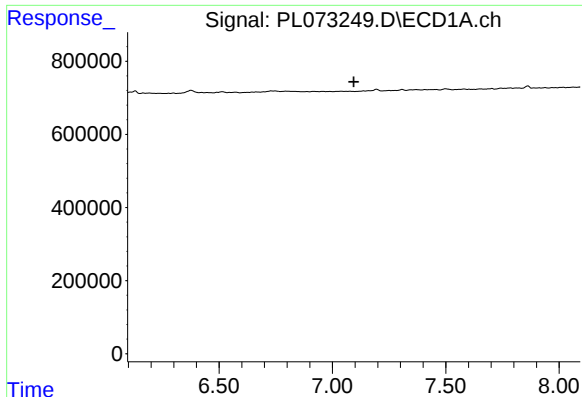

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

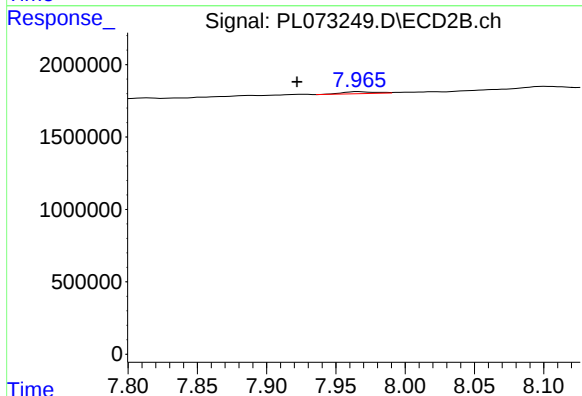


#8 Heptachlor epoxide

R.T.: 7.966 min
Delta R.T.: 0.045 min
Response: 240135
Conc: 0.14 ng/ml

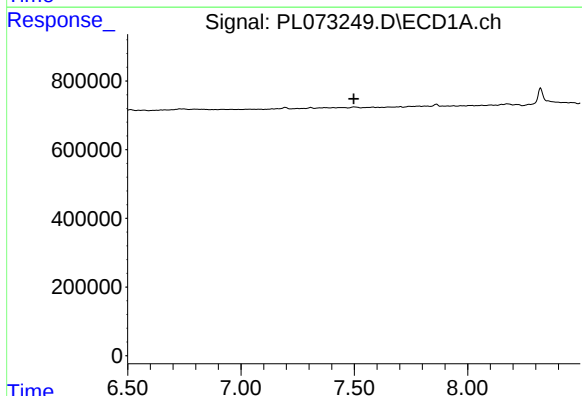


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.497 min
Response: 0
Conc: N.D.

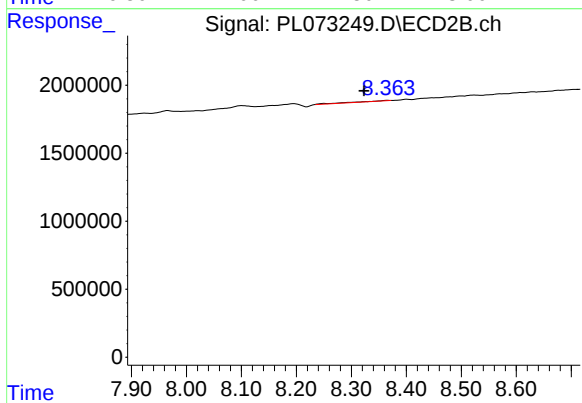

#9 Endosulfan I


R.T.: 8.365 min
Delta R.T.: 0.042 min
Response: 178244
Conc: 0.11 ng/ml

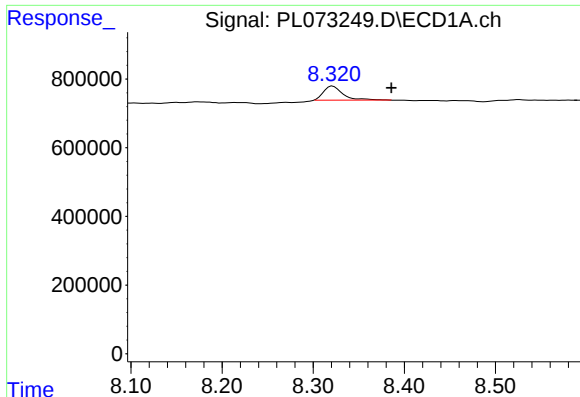

#15 Endosulfan II


R.T.: 8.321 min
Delta R.T.: -0.064 min
Response: 604997
Conc: 1.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

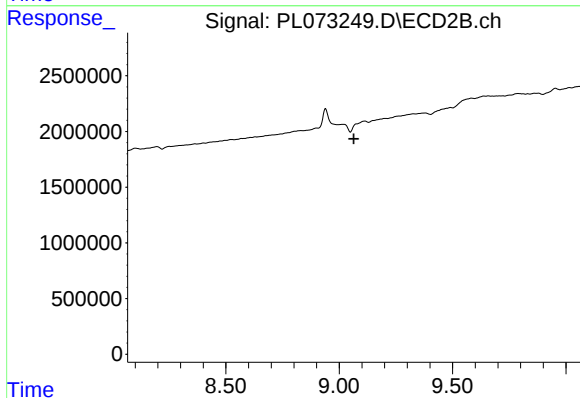


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

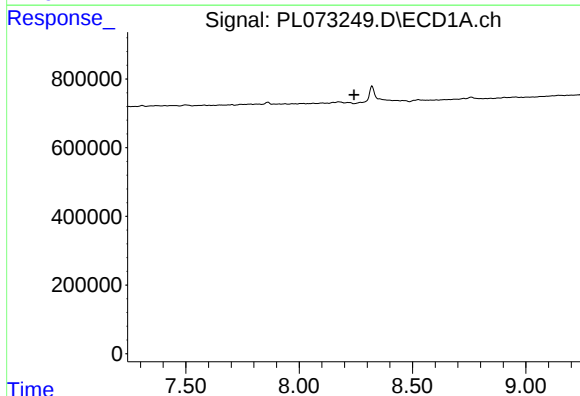


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

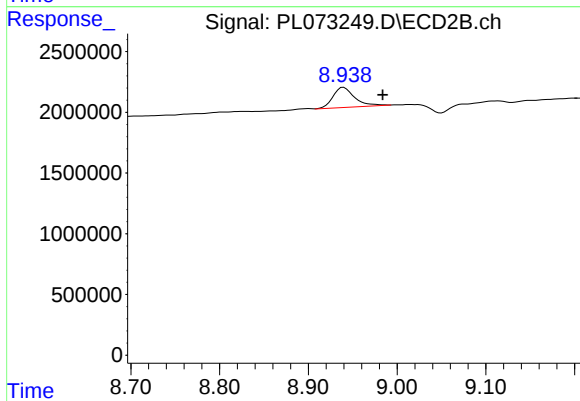

#16 4,4'-DDD


R.T.: 8.940 min
Delta R.T.: -0.044 min
Response: 2782712
Conc: 2.12 ng/ml

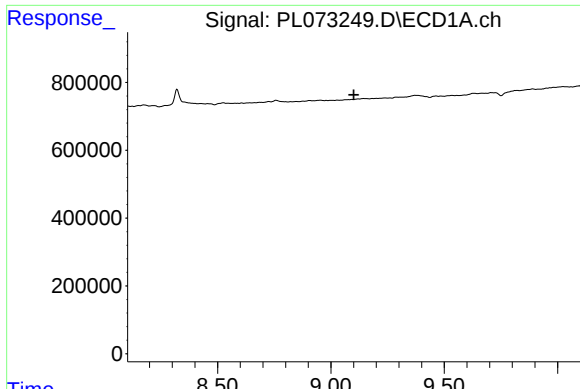

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

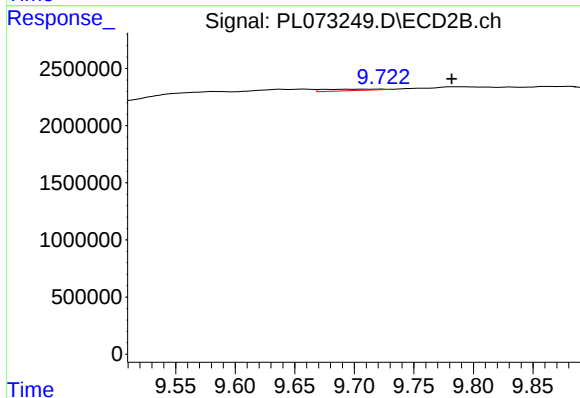


#20 Methoxychlor

R.T.: 9.723 min
Delta R.T.: -0.058 min
Response: 415901
Conc: 0.54 ng/ml

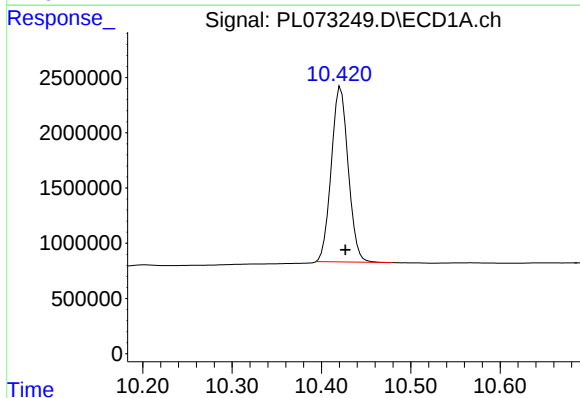

#27 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.005 min
Response: 20812245
Conc: 43.29 ng/ml

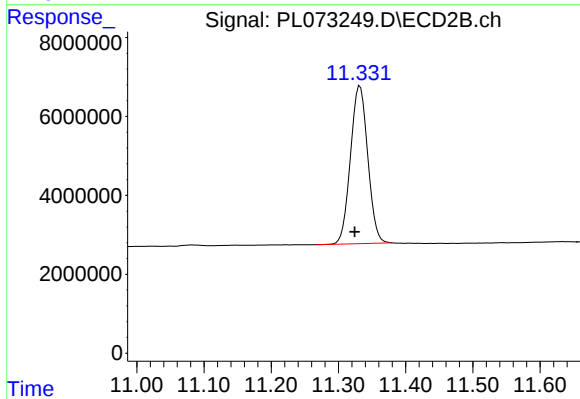

#27 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.008 min
Response: 71393060
Conc: 44.17 ng/ml