

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
 Data File : PL073252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 20:35
 Operator : AR\AJ
 Sample : N1816-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 04:53:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.493	7041115	34355005	20.475	22.006
27)	SA Decachlor...	10.422	11.332	19433405	66472999	40.418	41.126
Target Compounds							
2)	A alpha-BHC	0.000	6.028	0	360050	N.D.	0.186
6)	B beta-BHC	0.000	6.674	0	334022	N.D.	0.341
7)	B delta-BHC	0.000	6.954	0	2015555	N.D.	1.042
15)	B Endosulfa...	8.322f	0.000	729906	0	1.558	N.D. #
16)	A 4,4'-DDD	0.000	8.940f	0	2794016	N.D.	2.127
20)	A Methoxychlor	0.000	9.718f	0	83582	N.D.	0.109


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
Data File : PL073252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 20:35
Operator : AR\AJ
Sample : N1816-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 04:53:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

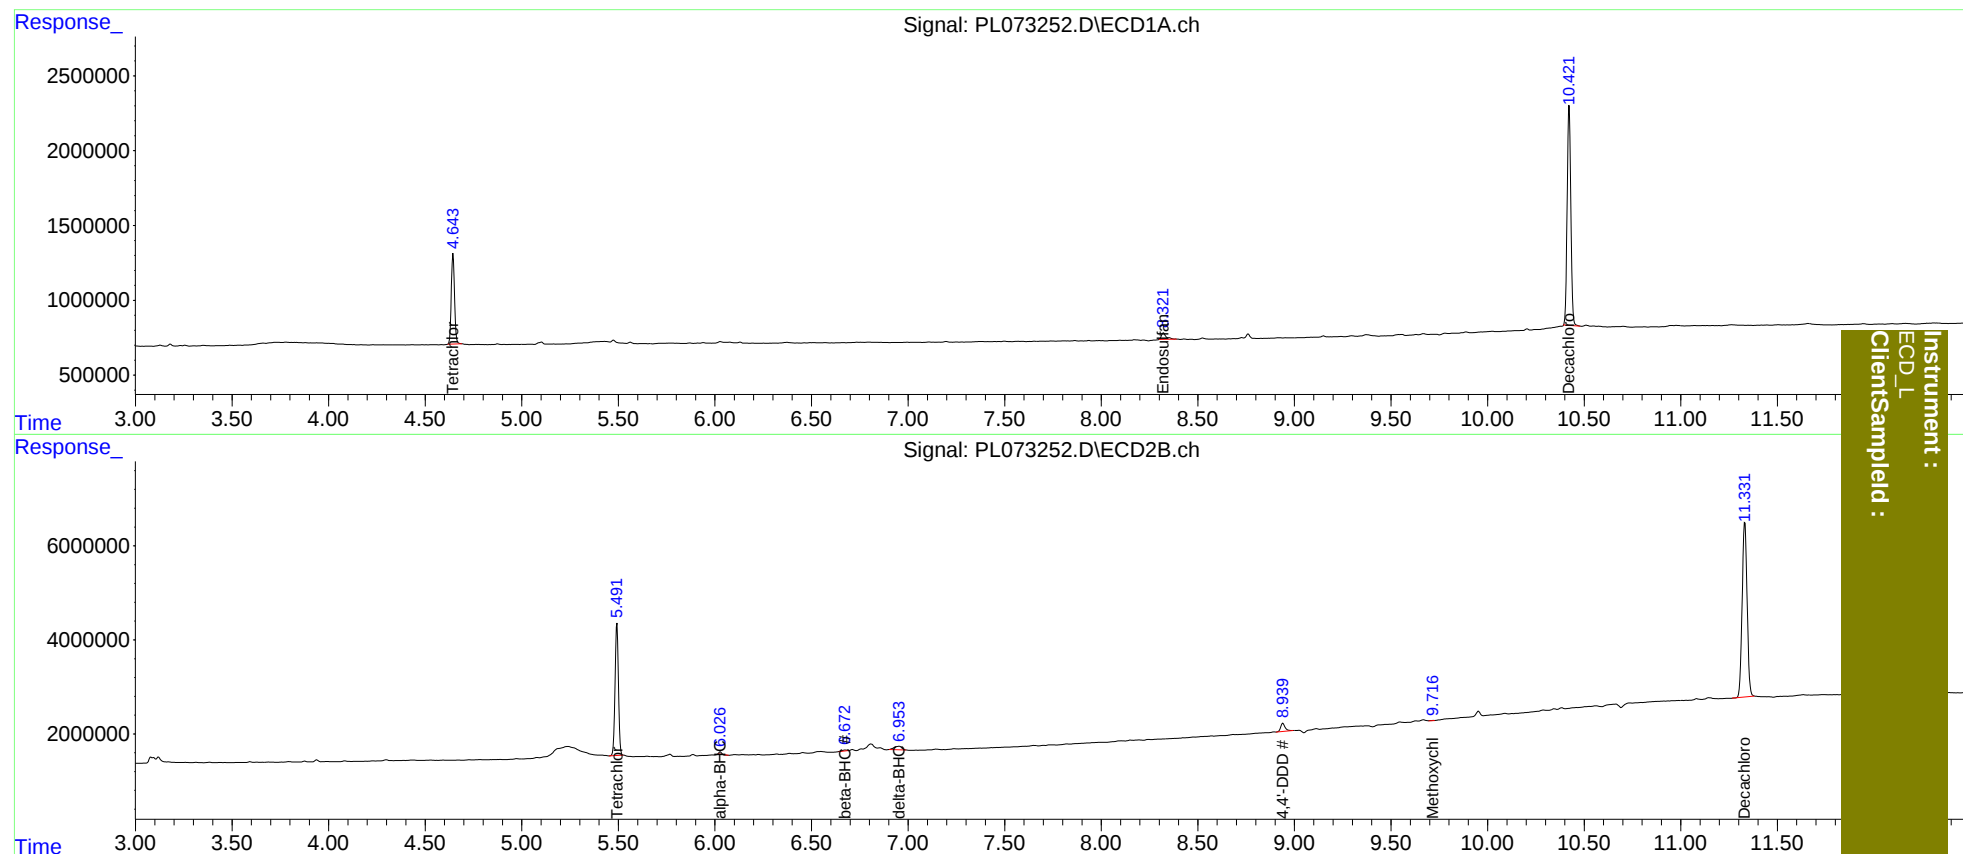


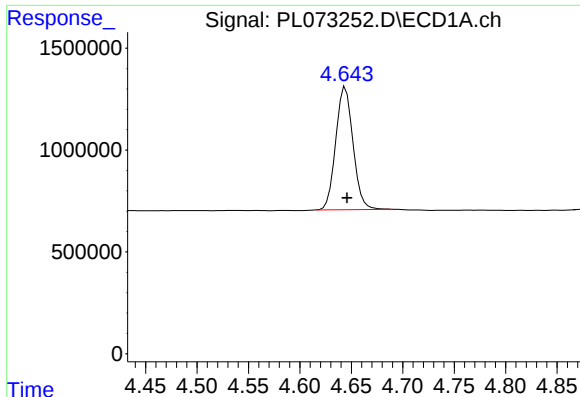

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 7041115
Conc: 20.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

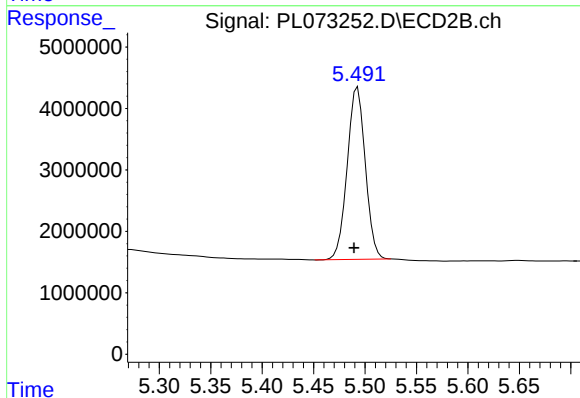


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.003 min
Response: 34355005
Conc: 22.01 ng/ml

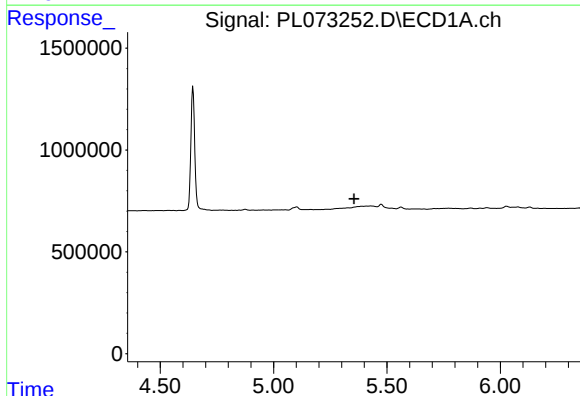


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

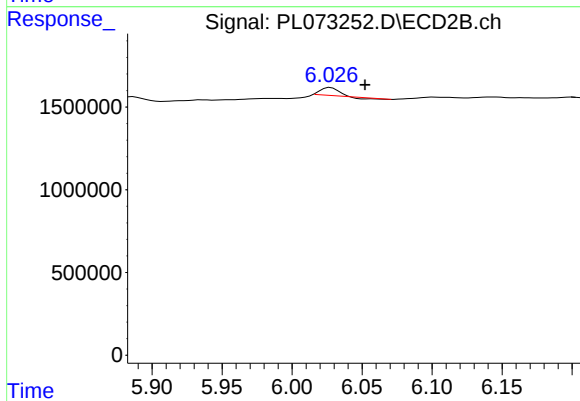

#2 alpha-BHC


R.T.: 6.028 min
Delta R.T.: -0.024 min
Response: 360050
Conc: 0.19 ng/ml

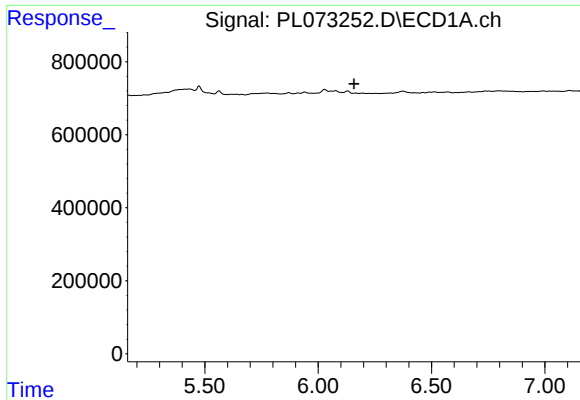

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

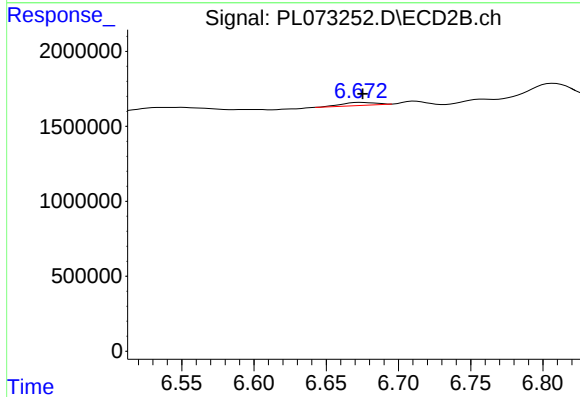


#6 beta-BHC

R.T.: 6.674 min
Delta R.T.: -0.002 min
Response: 334022
Conc: 0.34 ng/ml

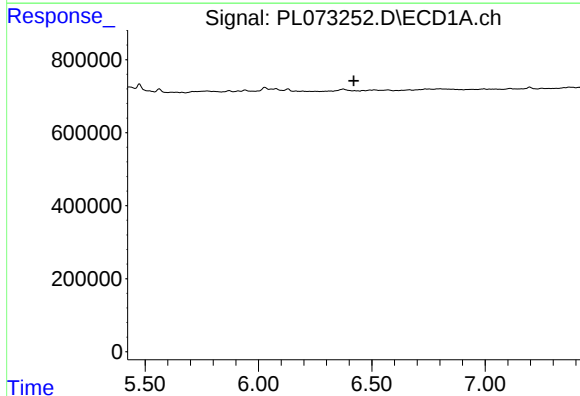


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

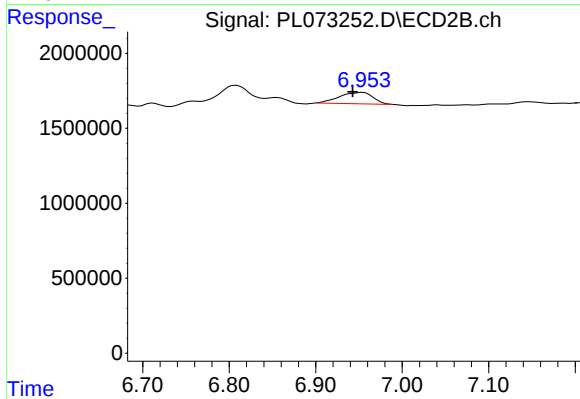

#7 delta-BHC


R.T.: 6.954 min
Delta R.T.: 0.011 min
Response: 2015555
Conc: 1.04 ng/ml

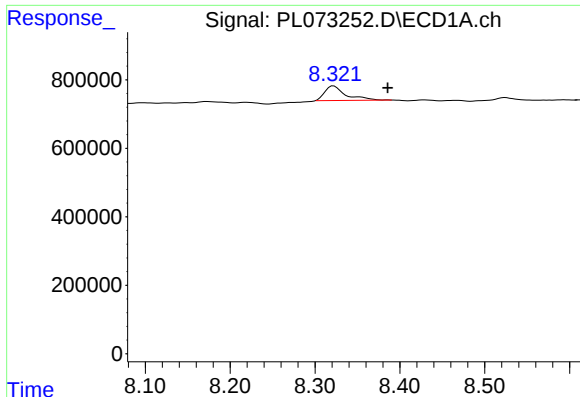

#15 Endosulfan II


R.T.: 8.322 min
Delta R.T.: -0.064 min
Response: 729906
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

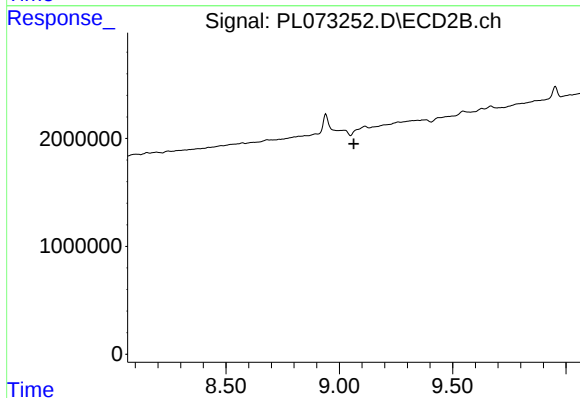


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

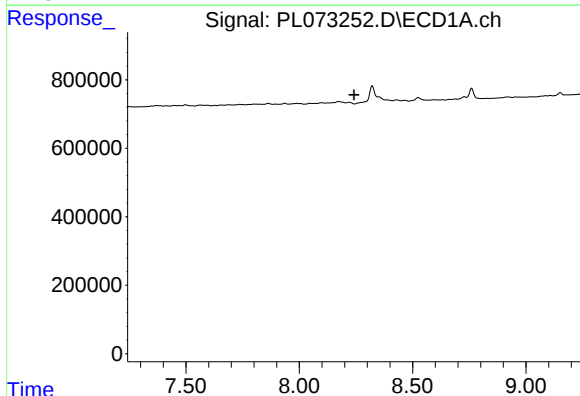


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

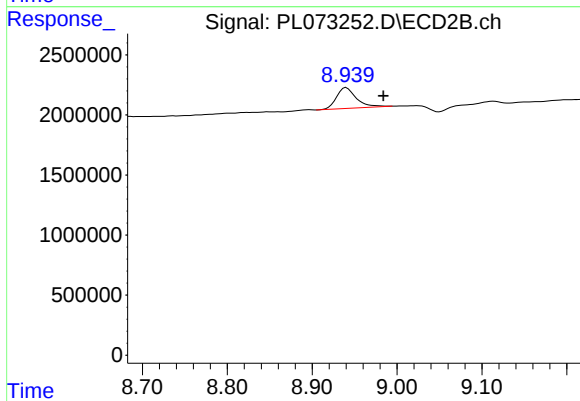

#16 4,4'-DDD


R.T.: 8.940 min
Delta R.T.: -0.044 min
Response: 2794016
Conc: 2.13 ng/ml

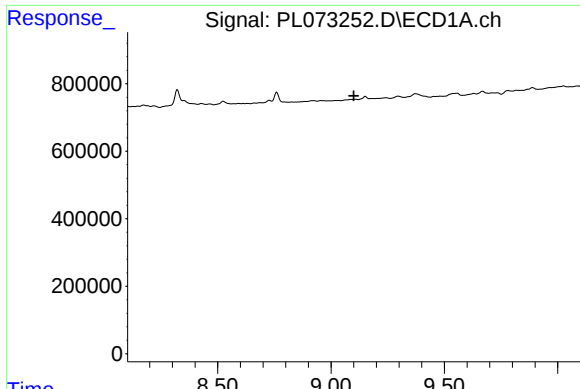

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

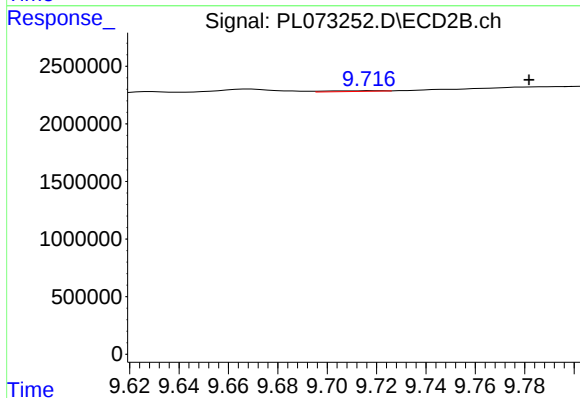


#20 Methoxychlor

R.T.: 9.718 min
Delta R.T.: -0.063 min
Response: 83582
Conc: 0.11 ng/ml

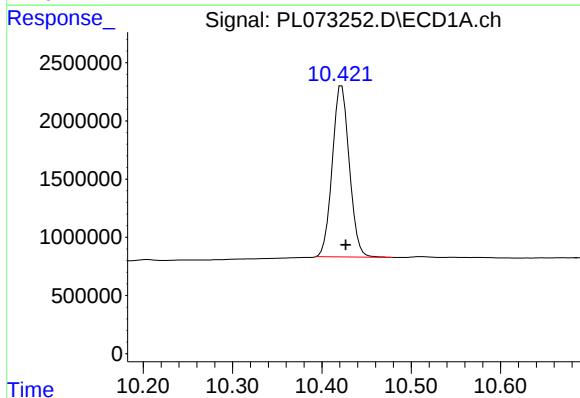

#27 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.005 min
Response: 19433405
Conc: 40.42 ng/ml

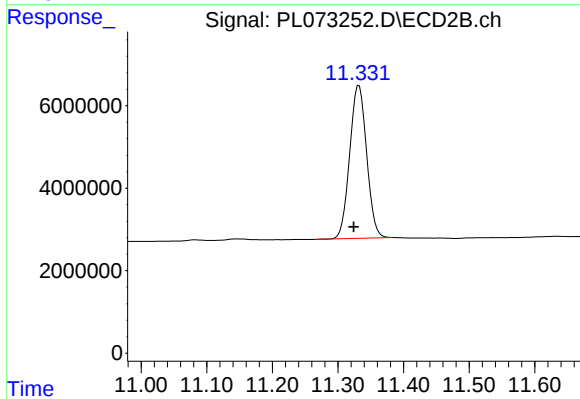

#27 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.008 min
Response: 66472999
Conc: 41.13 ng/ml