

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
 Data File : PL073260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 23:33
 Operator : AR\AJ
 Sample : N1816-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 04:55:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.493	6976939	34090131	20.288	21.837
27)	SA Decachlor...	10.422	11.331	19548261	67295104	40.656	41.635
Target Compounds							
2)	A alpha-BHC	0.000	6.027	0	682985	N.D.	0.353
3)	MA gamma-BHC...	0.000	6.455	0	239936	N.D.	0.127
6)	B beta-BHC	0.000	6.676	0	268837	N.D.	0.275
7)	B delta-BHC	0.000	6.953	0	1908597	N.D.	0.987
8)	B Heptachlo...	0.000	7.853f	0	239496	N.D.	0.141
15)	B Endosulfa...	8.322f	0.000	467210	0	0.997	N.D. #
16)	A 4,4'-DDD	0.000	8.940f	0	2797027	N.D.	2.130
20)	A Methoxychlor	0.000	9.720f	0	107147	N.D.	0.140
21)	B Endrin ke...	0.000	9.952	0	328611	N.D.	0.232
26)	Toxaphene-5	0.000	9.867	0	194299	N.D.	11.447


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
Data File : PL073260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 23:33
Operator : AR\AJ
Sample : N1816-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 04:55:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

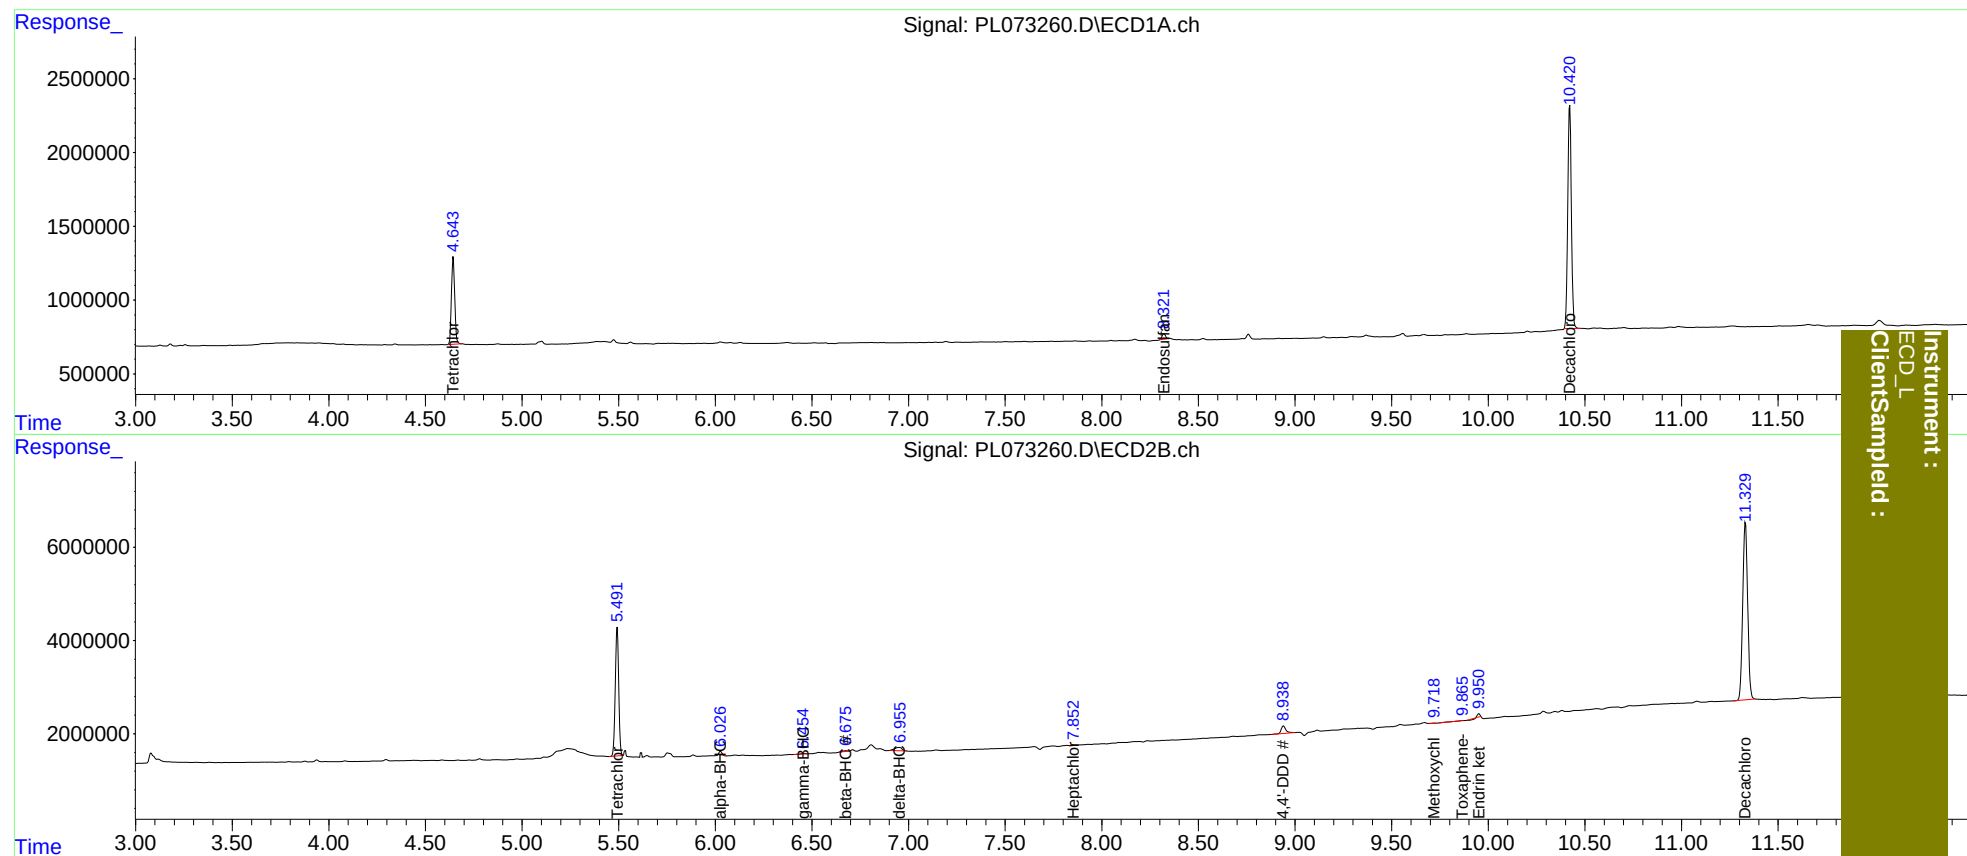


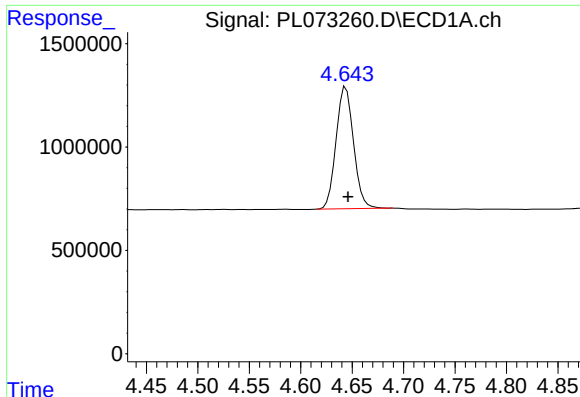

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 6976939
Conc: 20.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

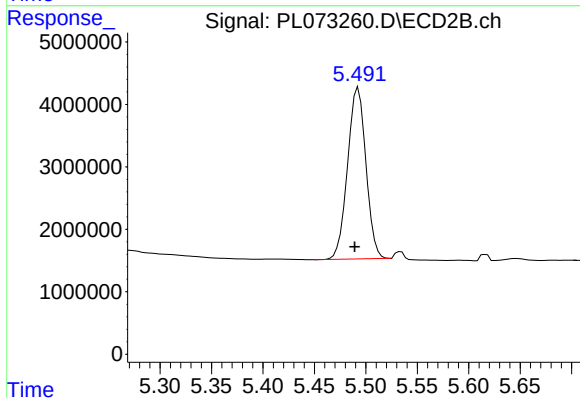


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.003 min
Response: 34090131
Conc: 21.84 ng/ml

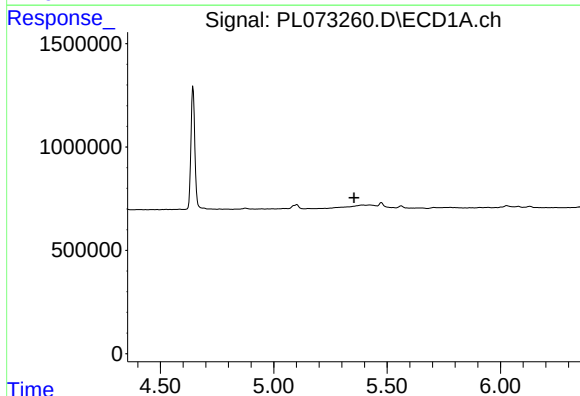


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

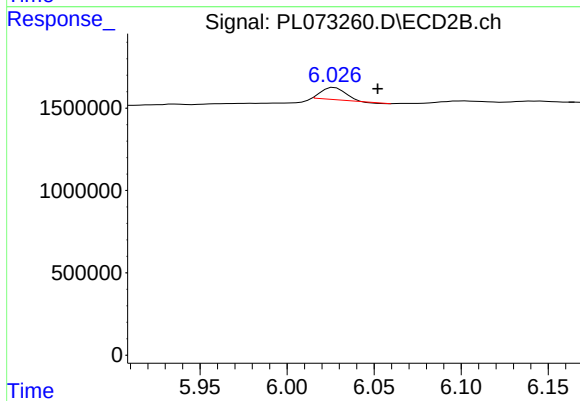

#2 alpha-BHC


R.T.: 6.027 min
Delta R.T.: -0.025 min
Response: 682985
Conc: 0.35 ng/ml

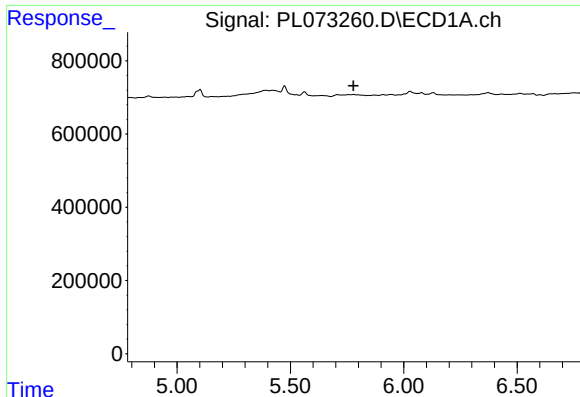

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 5.778 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

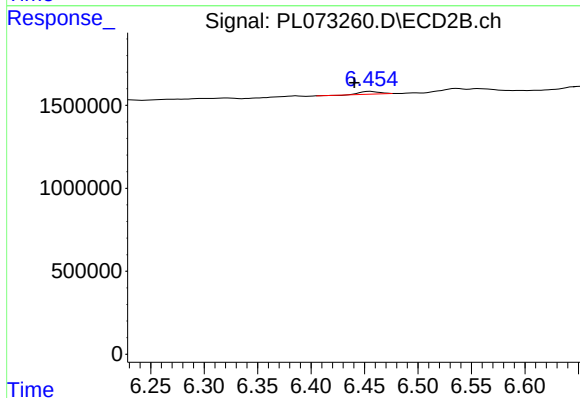


#3 gamma-BHC (Lindane)

R.T.: 6.455 min
Delta R.T.: 0.015 min
Response: 239936
Conc: 0.13 ng/ml

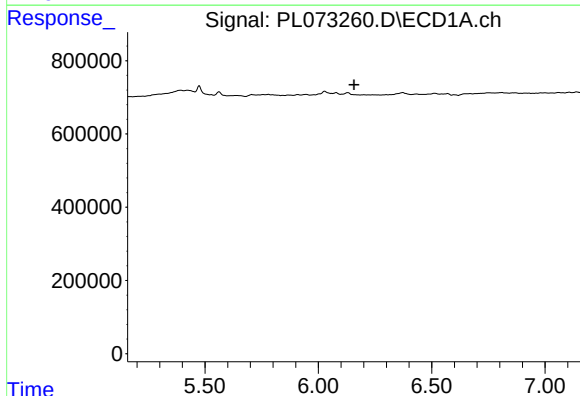


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.158 min
Response: 0
Conc: N.D.

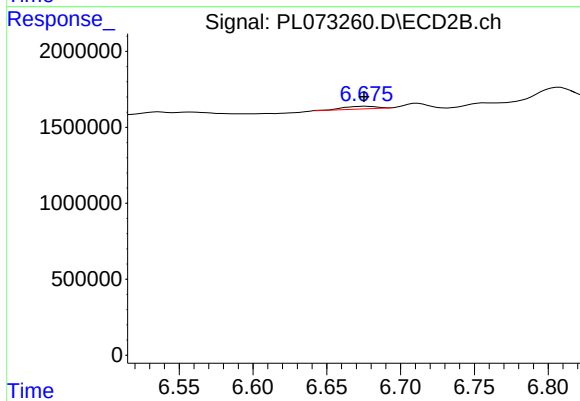

#6 beta-BHC


R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 268837
Conc: 0.27 ng/ml

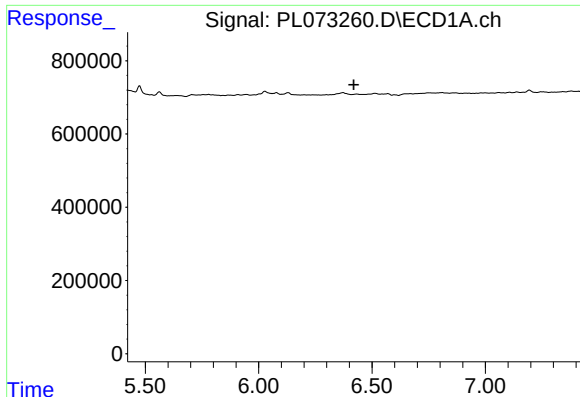

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

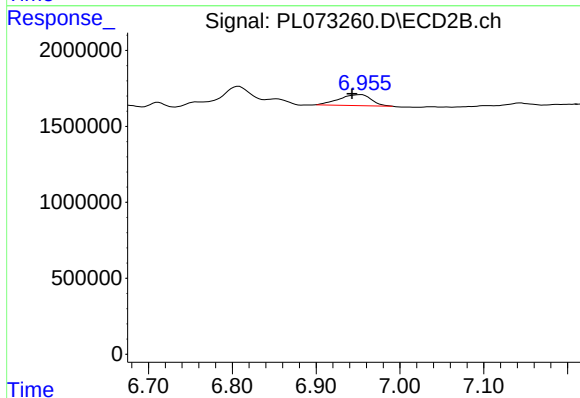


#7 delta-BHC

R.T.: 6.953 min
Delta R.T.: 0.011 min
Response: 1908597
Conc: 0.99 ng/ml

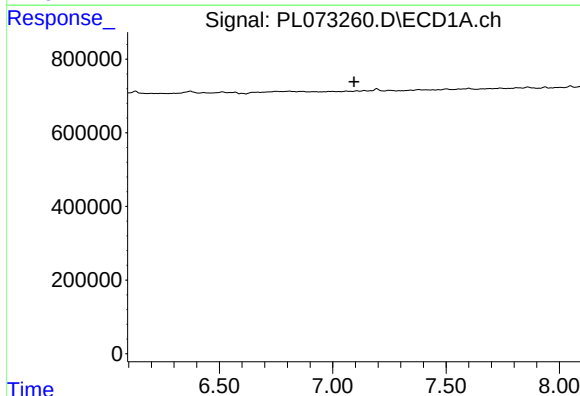


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.094 min
Response: 0
Conc: N.D.

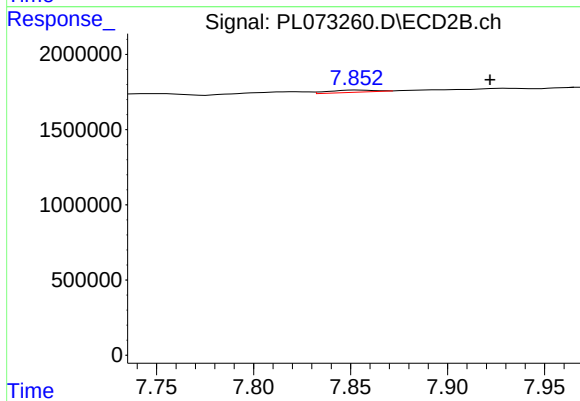

#8 Heptachlor epoxide


R.T.: 7.853 min
Delta R.T.: -0.069 min
Response: 239496
Conc: 0.14 ng/ml

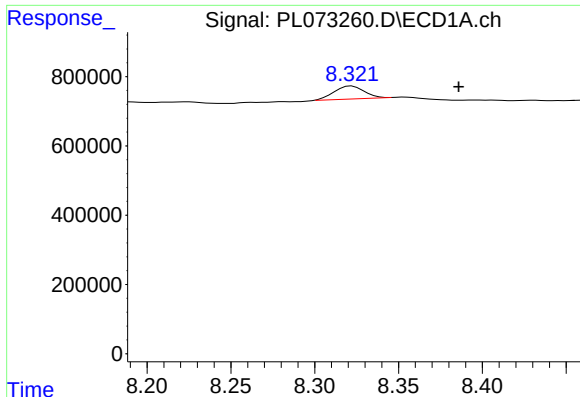

#15 Endosulfan II


R.T.: 8.322 min
Delta R.T.: -0.064 min
Response: 467210
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

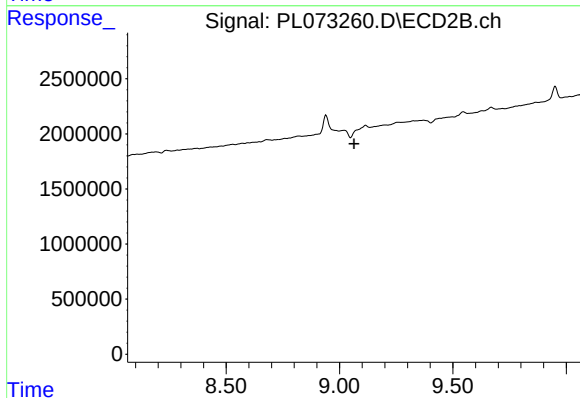


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

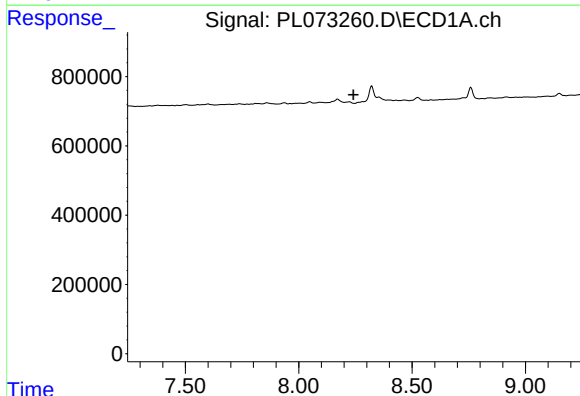


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

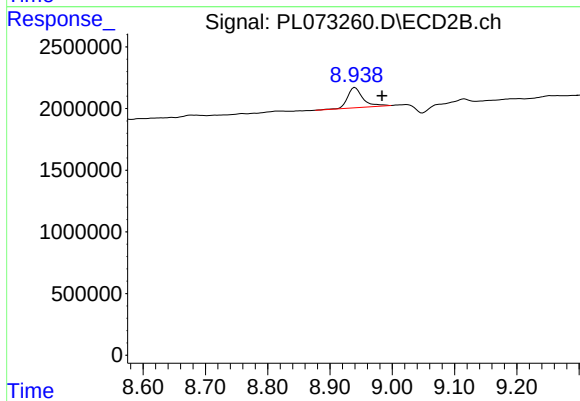

#16 4,4'-DDD


R.T.: 8.940 min
Delta R.T.: -0.044 min
Response: 2797027
Conc: 2.13 ng/ml

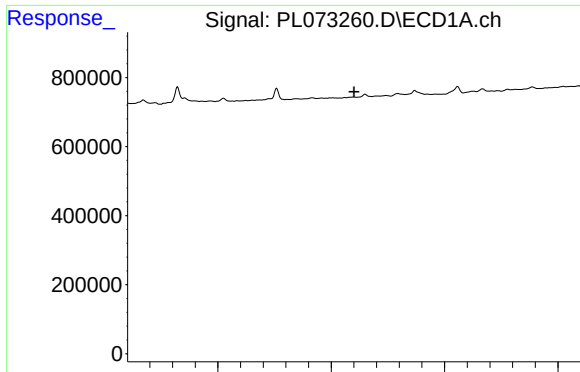

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

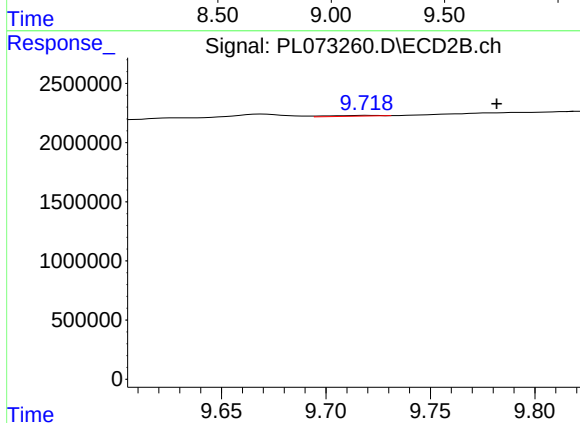


#20 Methoxychlor

R.T.: 9.720 min
Delta R.T.: -0.062 min
Response: 107147
Conc: 0.14 ng/ml

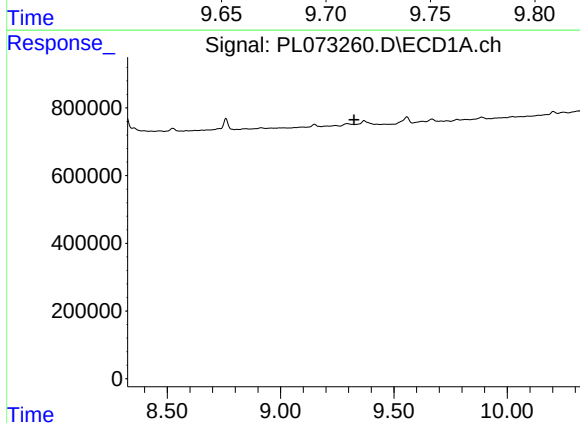


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.324 min
Response: 0
Conc: N.D.

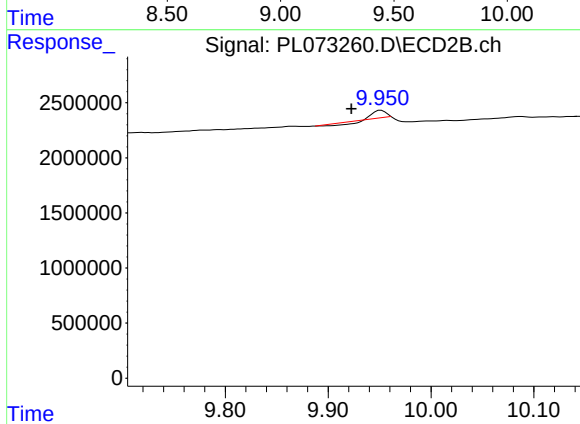

#21 Endrin ketone


R.T.: 9.952 min
Delta R.T.: 0.029 min
Response: 328611
Conc: 0.23 ng/ml

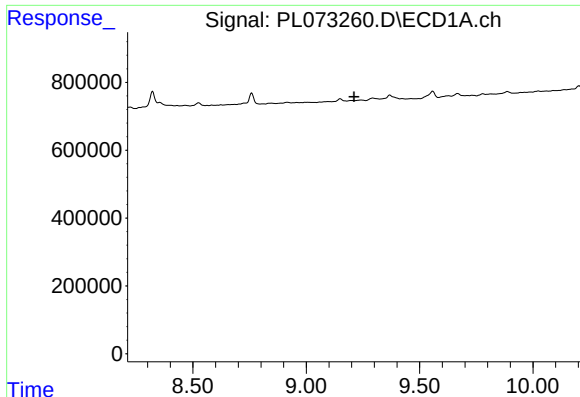

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 9.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

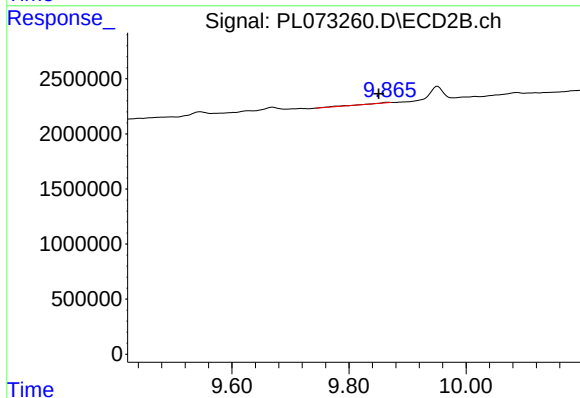


#26 Toxaphene-5

R.T.: 9.867 min
Delta R.T.: 0.016 min
Response: 194299
Conc: 11.45 ng/ml

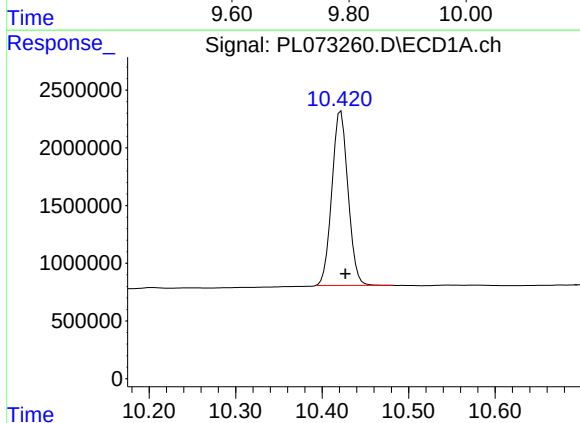

#27 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.005 min
Response: 19548261
Conc: 40.66 ng/ml

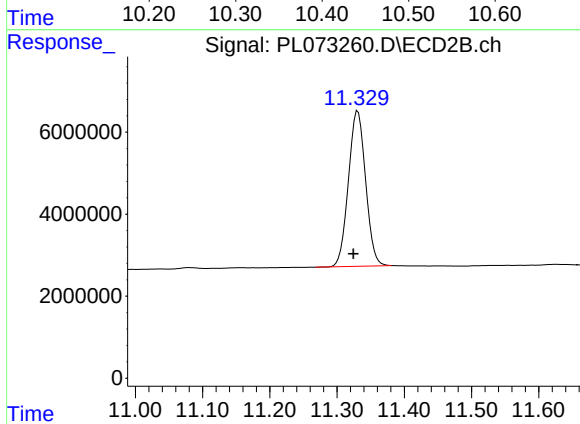

#27 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.007 min
Response: 67295104
Conc: 41.63 ng/ml