

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
 Data File : PL073266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2022 01:10
 Operator : AR\AJ
 Sample : N1816-19
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 05:59:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 01:47:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.492	7664479	37450191	22.287	23.989
27)	SA Decachlor...	10.422	11.331	22331771	76597080	46.446	47.390
Target Compounds							
2)	A alpha-BHC	0.000	6.027f	0	482952	N.D.	0.250
3)	MA gamma-BHC...	0.000	6.455	0	314888	N.D.	0.166
7)	B delta-BHC	0.000	6.956	0	1913058	N.D.	0.989
15)	B Endosulfa...	8.322f	0.000	431114	0	0.920	N.D. #
16)	A 4,4'-DDD	0.000	8.940f	0	2799889	N.D.	2.132
20)	A Methoxychlor	0.000	9.712f	0	103634	N.D.	0.135

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030922\
Data File : PL073266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2022 01:10
Operator : AR\AJ
Sample : N1816-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 05:59:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 01:47:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

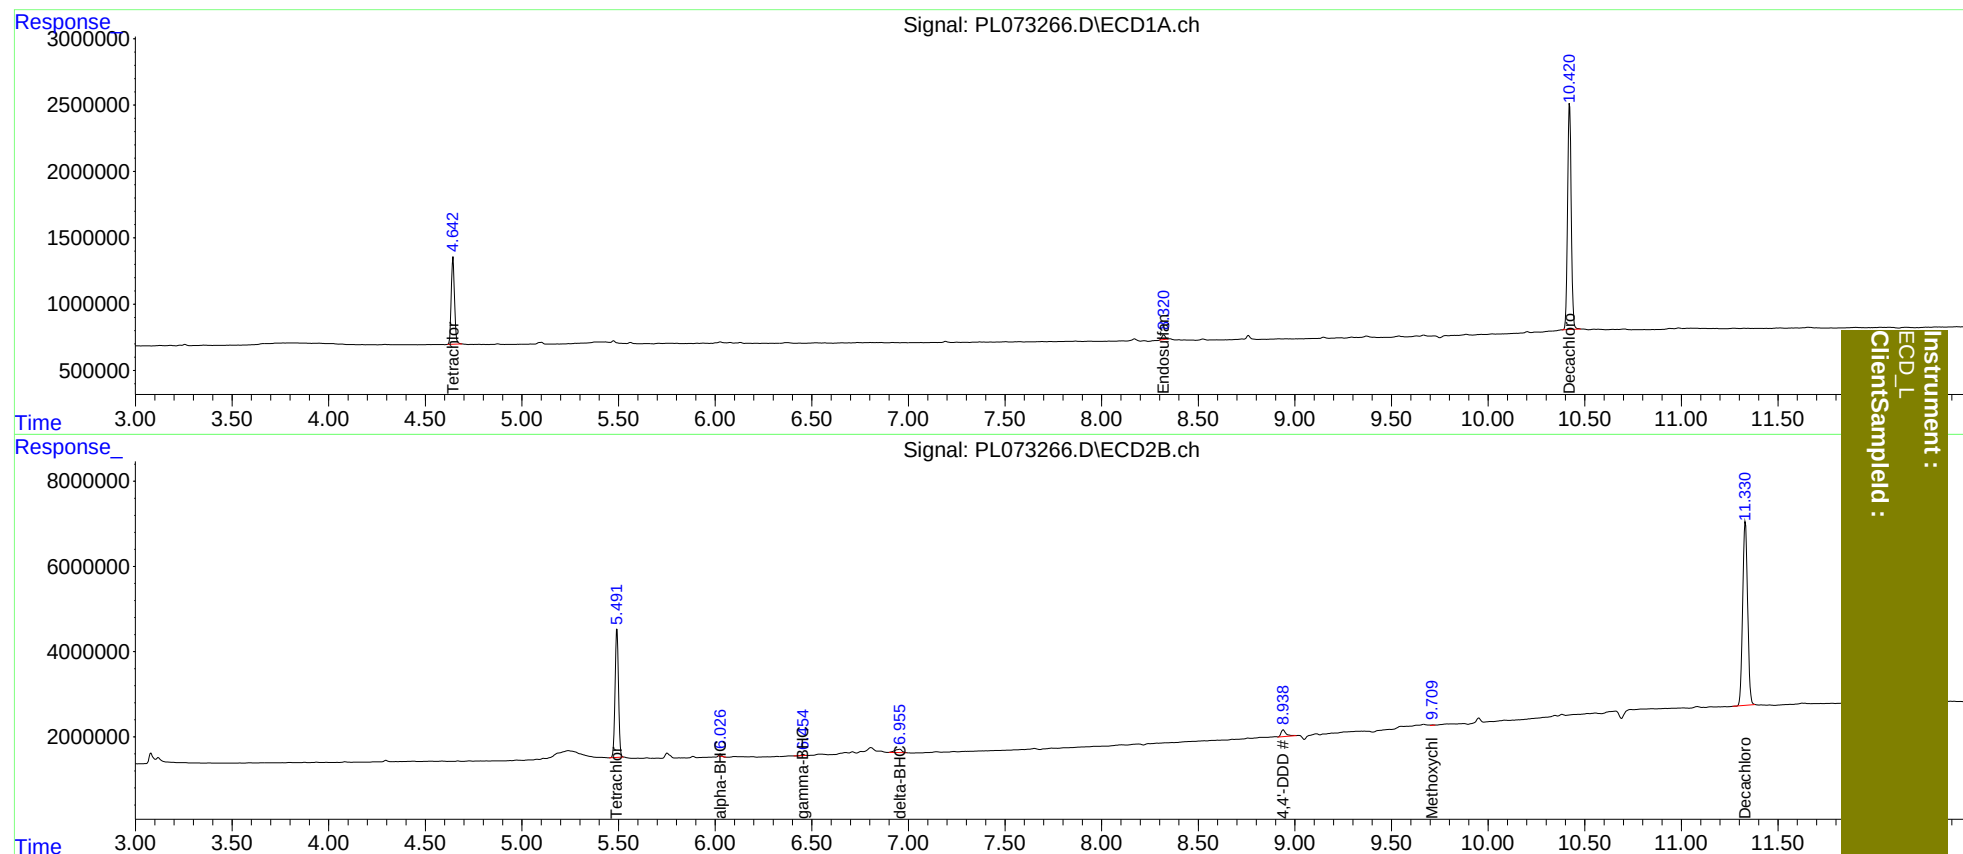


Instrument :
ECD_L
ClientSampled :
N1816-19

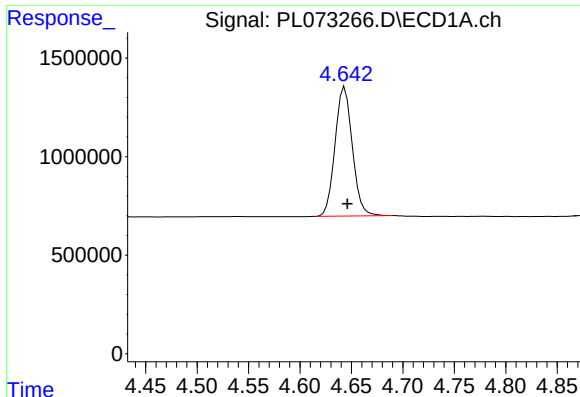

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: -0.002 min
Response: 7664479
Conc: 22.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

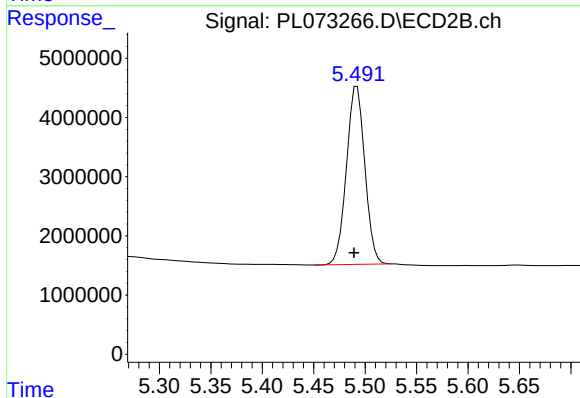


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.003 min
Response: 37450191
Conc: 23.99 ng/ml

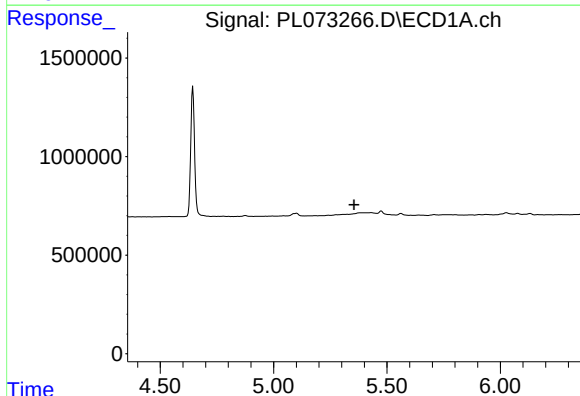


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.355 min
Response: 0
Conc: N.D.

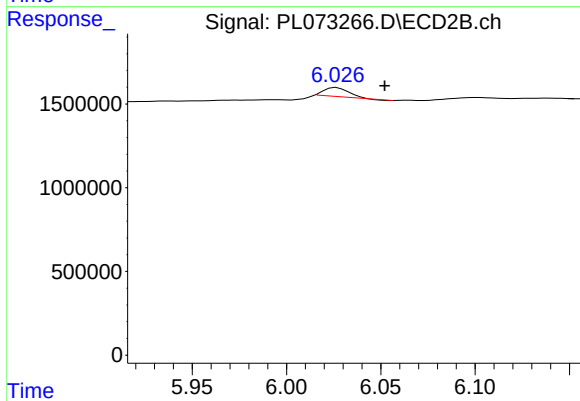

#2 alpha-BHC


R.T.: 6.027 min
Delta R.T.: -0.025 min
Response: 482952
Conc: 0.25 ng/ml

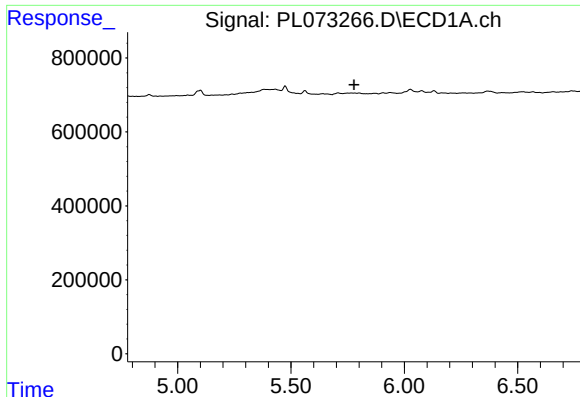

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 5.778 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

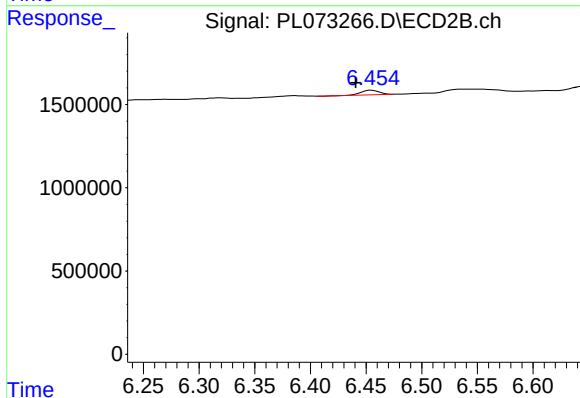


#3 gamma-BHC (Lindane)

R.T.: 6.455 min
Delta R.T.: 0.015 min
Response: 314888
Conc: 0.17 ng/ml

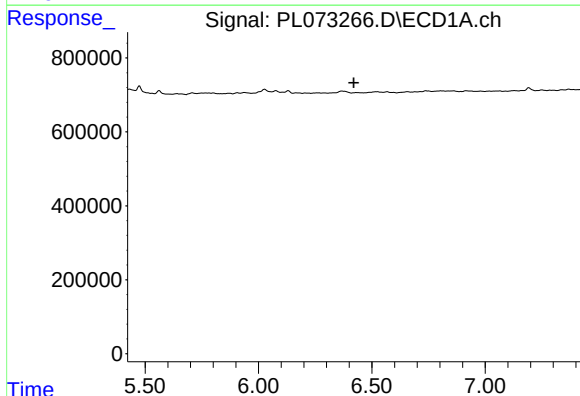


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

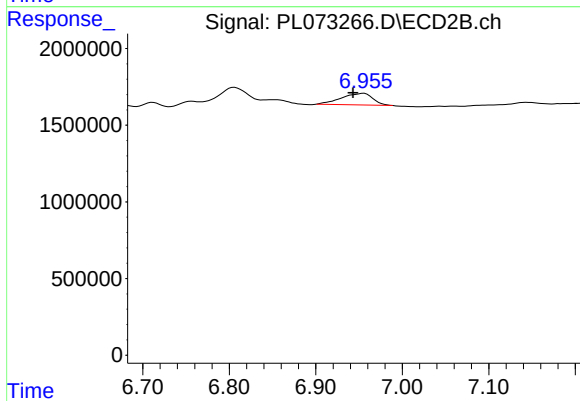

#7 delta-BHC


R.T.: 6.956 min
Delta R.T.: 0.013 min
Response: 1913058
Conc: 0.99 ng/ml

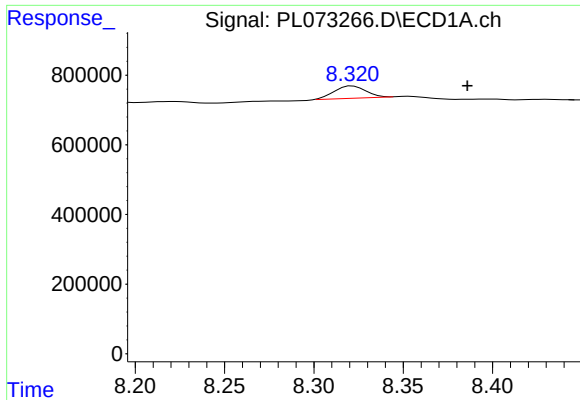

#15 Endosulfan II


R.T.: 8.322 min
Delta R.T.: -0.064 min
Response: 431114
Conc: 0.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

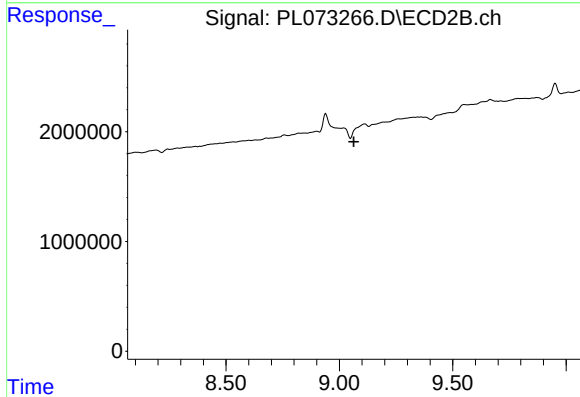


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.064 min
Response: 0
Conc: N.D.

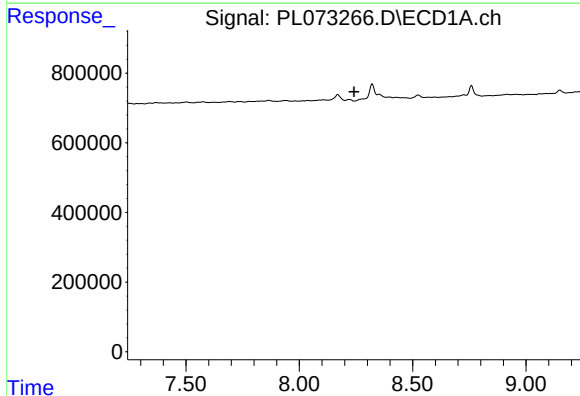


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.242 min
Response: 0
Conc: N.D.

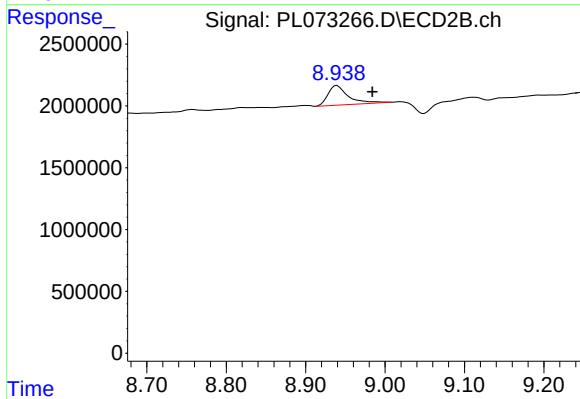

#16 4,4'-DDD


R.T.: 8.940 min
Delta R.T.: -0.044 min
Response: 2799889
Conc: 2.13 ng/ml

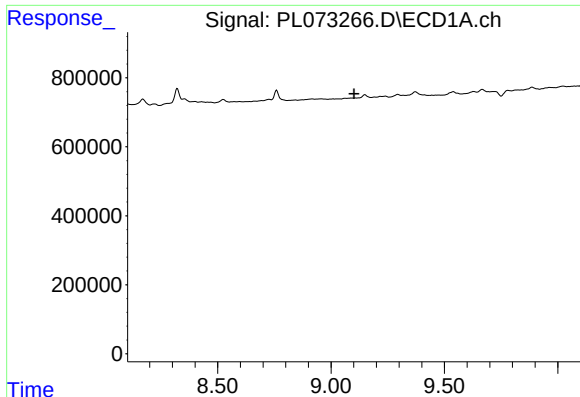

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

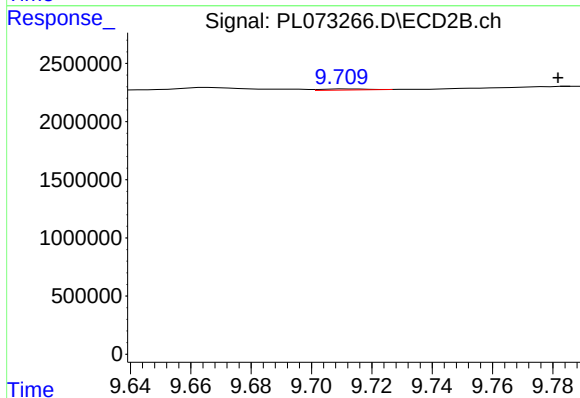


#20 Methoxychlor

R.T.: 9.712 min
Delta R.T.: -0.070 min
Response: 103634
Conc: 0.14 ng/ml

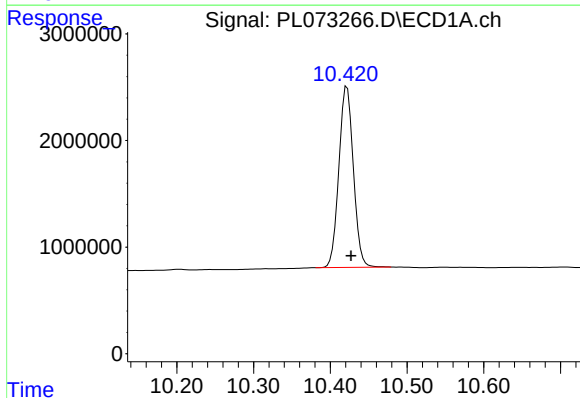

#27 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: -0.005 min
Response: 22331771
Conc: 46.45 ng/ml

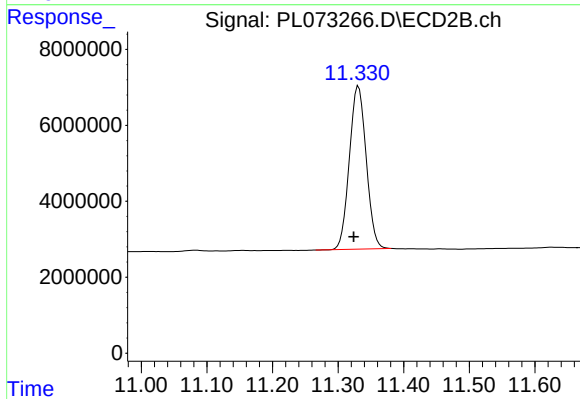

#27 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.007 min
Response: 76597080
Conc: 47.39 ng/ml