

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031021\
 Data File : PL065189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 12:08
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 01:21:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 01:14:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.095	29384585	25096417	10.462	10.200
27)	SA Decachlor...	8.137	9.247	54642773	42123798	22.724	21.664
Target Compounds							
22)	Toxaphene-1	5.653	6.521	23172290	12516298	1052.941	990.461
23)	Toxaphene-2	6.250	6.817	58478529	13151943	1014.651	994.112
24)	Toxaphene-3	6.493	7.303	60236201	39706369	1002.720	988.044
25)	Toxaphene-4	6.845	7.390	43231978	36998621	981.961	996.806
26)	Toxaphene-5	6.976	7.813	64501622	30173191	1014.887	996.440

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031021\
Data File : PL065189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 12:08
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 01:21:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 01:14:49 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

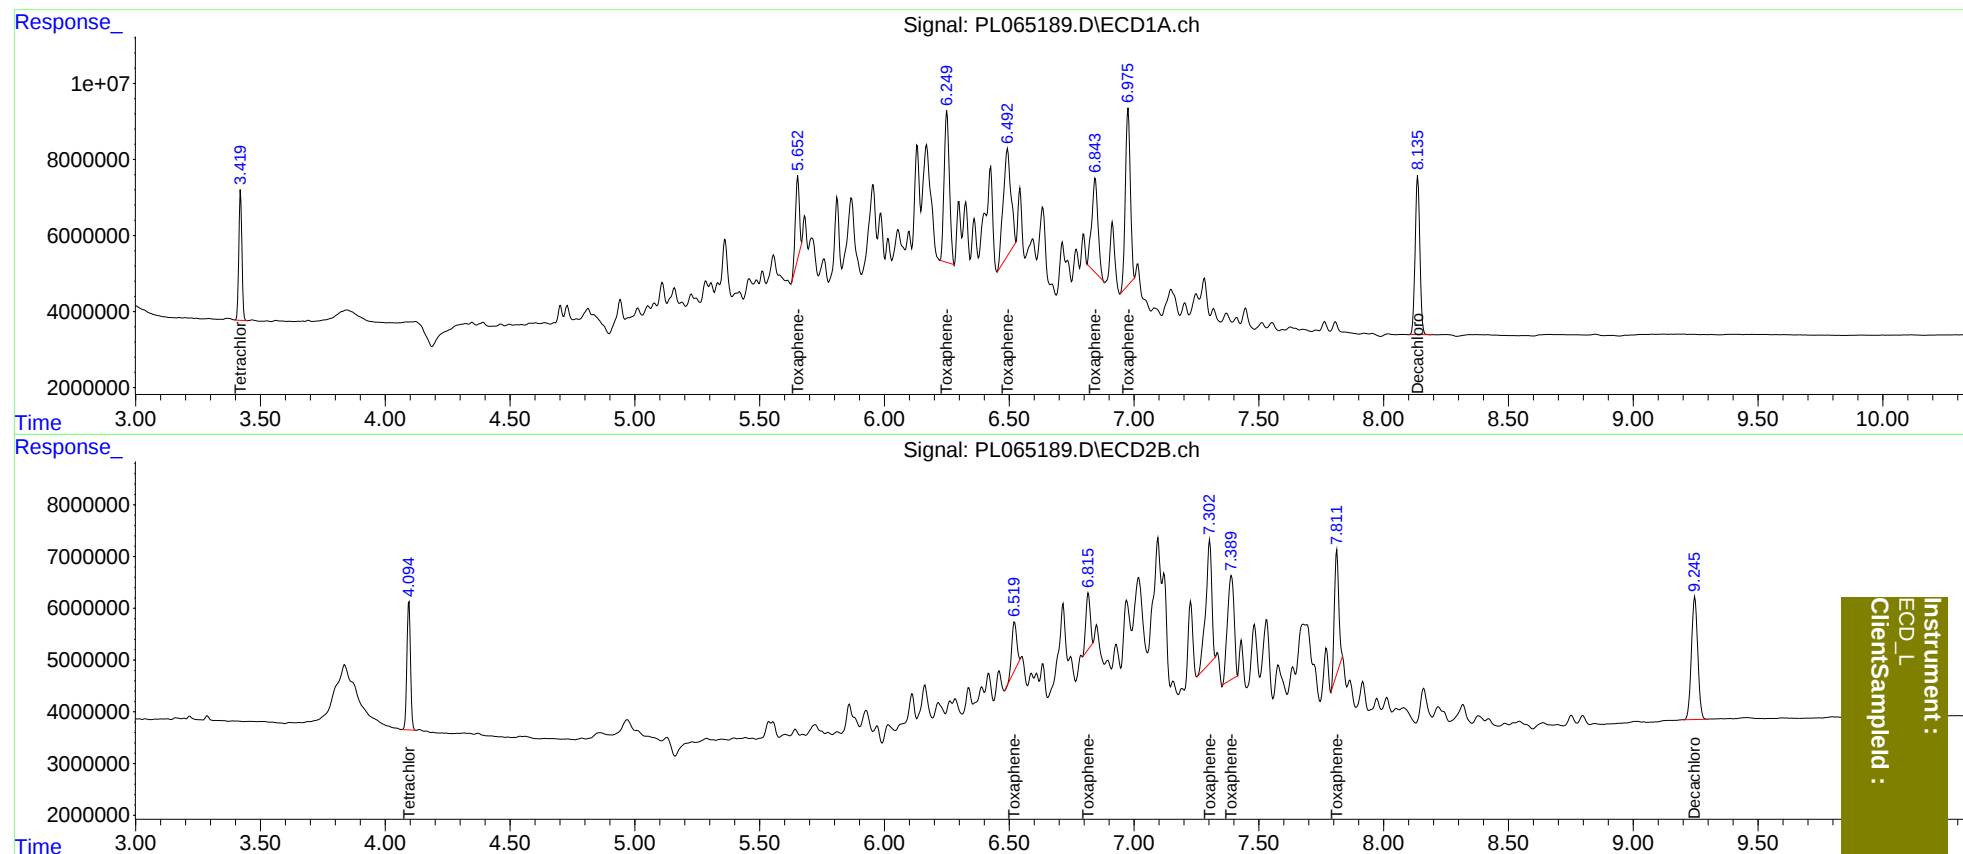

Instrument :
ECD_L
ClientSampled :