

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031021\
 Data File : PL065207.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 16:25
 Operator : AR\AJ
 Sample : M1344-01
 Misc : PEST MDL 1 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 03:13:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 02:46:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	4.095	62137574	54225791	21.215	21.269
2)	SA Decachlor...	8.136	9.246	119.4E6	97282026	42.702	42.687
Target Compounds							
2)	A alpha-BHC	3.851	4.496	3963658	3017978	0.902m	0.912
3)	MA gamma-BHC...	4.131	4.788	3952986	2800682	0.947m	0.894
4)	MA Heptachlor	4.428	5.298	3915708	3700398	0.932	1.125
5)	MB Aldrin	4.673	5.608	3637177	2859860	0.936	0.947
6)	B beta-BHC	4.382	4.969	2158374	5842104	1.046m	2.881 #
7)	B delta-BHC	4.583	5.188	3661069	3068710	0.864	0.998
8)	B Heptachlo...	5.113	6.004	3731359	1814833	1.013	0.760m
9)	A Endosulfan I	5.448	6.364	3345084	2537468	1.012	1.016m
10)	B trans-Chl...	5.338	6.238	3751177	2801953	0.990	0.967m
11)	B cis-Chlor...	5.395	6.309	3680881	2960658	1.001	1.022m
12)	B 4,4'-DDE	5.562	6.467	3307484	2620593	0.949	0.961m
13)	MA Dieldrin	5.687	6.625	3465005	2681067	0.962m	1.012
14)	MA Endrin	5.942	6.848	3647124	1883609	1.145m	0.872
15)	B Endosulfa...	6.215	7.060	3300540	2600989	1.077m	1.174m
16)	A 4,4'-DDD	6.074	6.967	2582708	2095891	0.941	1.062
17)	MA 4,4'-DDT	6.312	7.266	1884296	1570838	0.726	0.795
18)	B Endrin al...	6.385	7.188	2819984	2055370	1.078	1.050
19)	B Endosulfa...	6.595	7.411	3362584	2268507	1.058m	1.030
20)	A Methoxychlor	6.857	7.727	1306845	1096298	0.888m	0.953
21)	B Endrin ke...	7.082	7.890	3131069	2170718	0.973	0.992

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031021\
Data File : PL065207.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 16:25
Operator : AR\AJ
Sample : M1344-01
Misc : PEST MDL 1 PPB
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 03:13:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 02:46:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

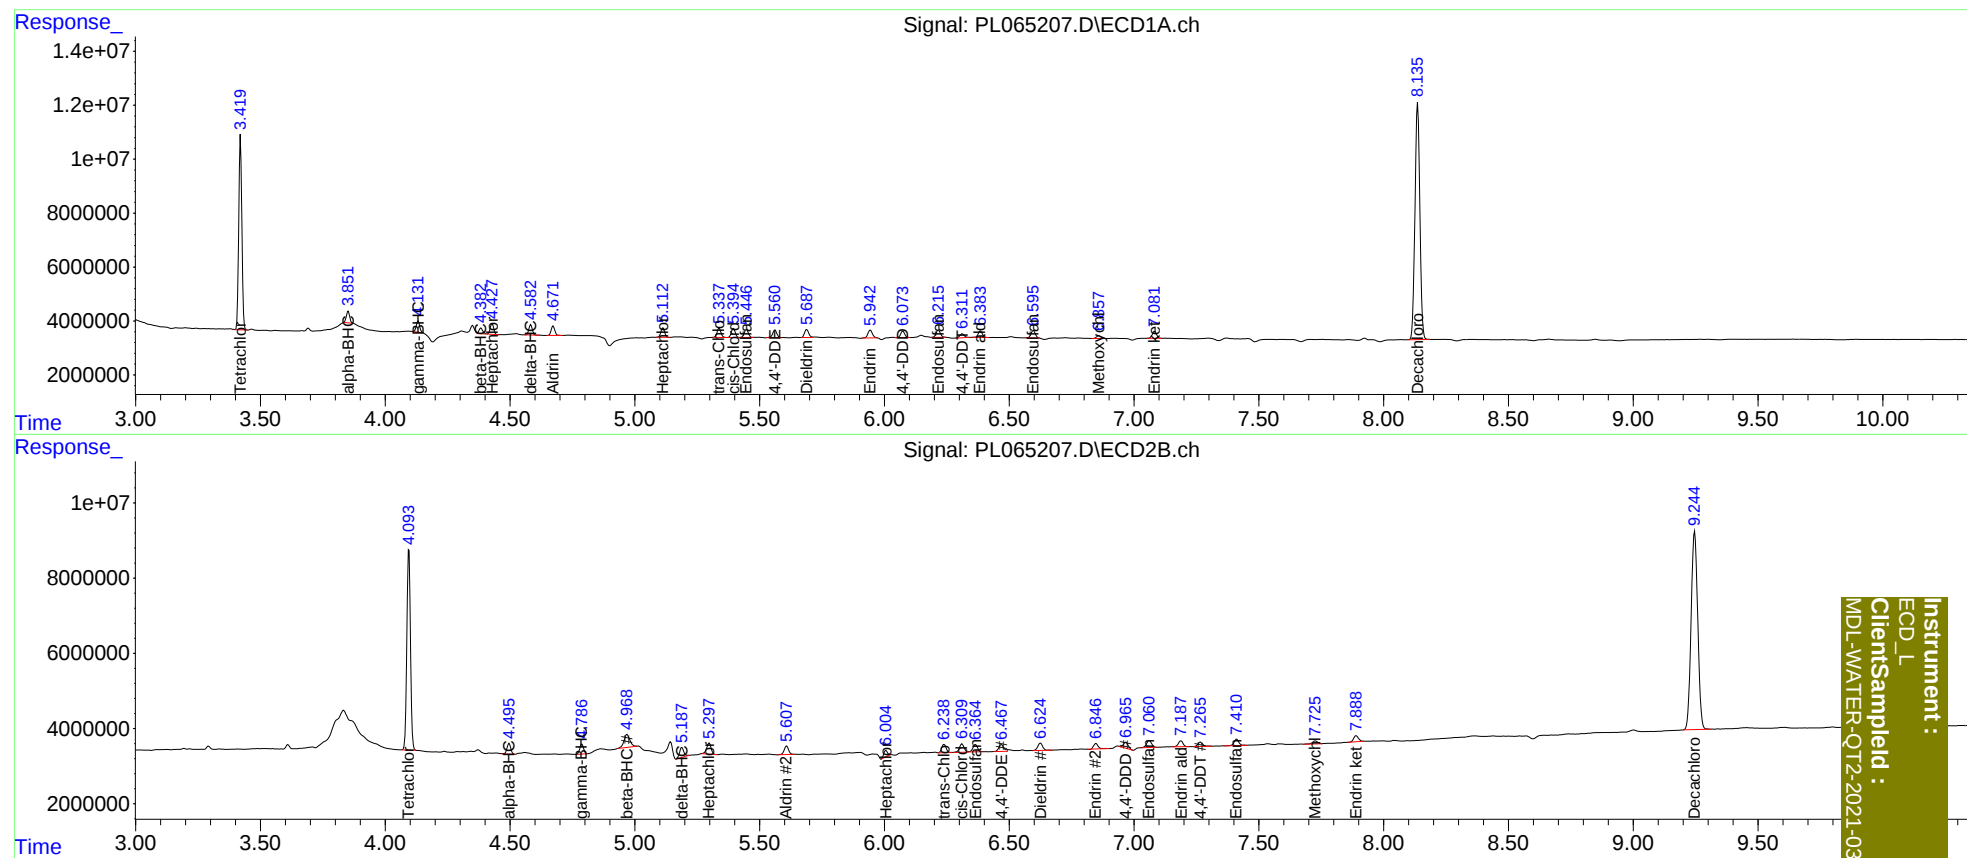

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT2-2021-03