

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031021\
 Data File : PL065208.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2021 16:39
 Operator : AR\AJ
 Sample : M1344-01
 Misc : TOX MDL 100 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 03:29:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 11 02:46:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	4.095	58554076	50294475	19.991	19.727
27)	SA Decachlor...	8.137	9.246	113.3E6	92287724	40.513	40.495
Target Compounds							
22)	Toxaphene-1	5.653	6.520	2154994	1519647	96.254	118.250m
23)	Toxaphene-2	6.248	6.817	6005407	1070987	103.927	81.246
24)	Toxaphene-3	6.492	7.302	4840080	3522820	80.460	87.599
25)	Toxaphene-4	6.846	7.390	2630229	2872540	60.522	77.683 #
26)	Toxaphene-5	6.974	7.813	6079592	2469350	95.462	81.599

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031021\
Data File : PL065208.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2021 16:39
Operator : AR\AJ
Sample : M1344-01
Misc : TOX MDL 100 PPB
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 03:29:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031021CLP.M
Quant Title : GC Extractables
QLast Update : Thu Mar 11 02:46:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

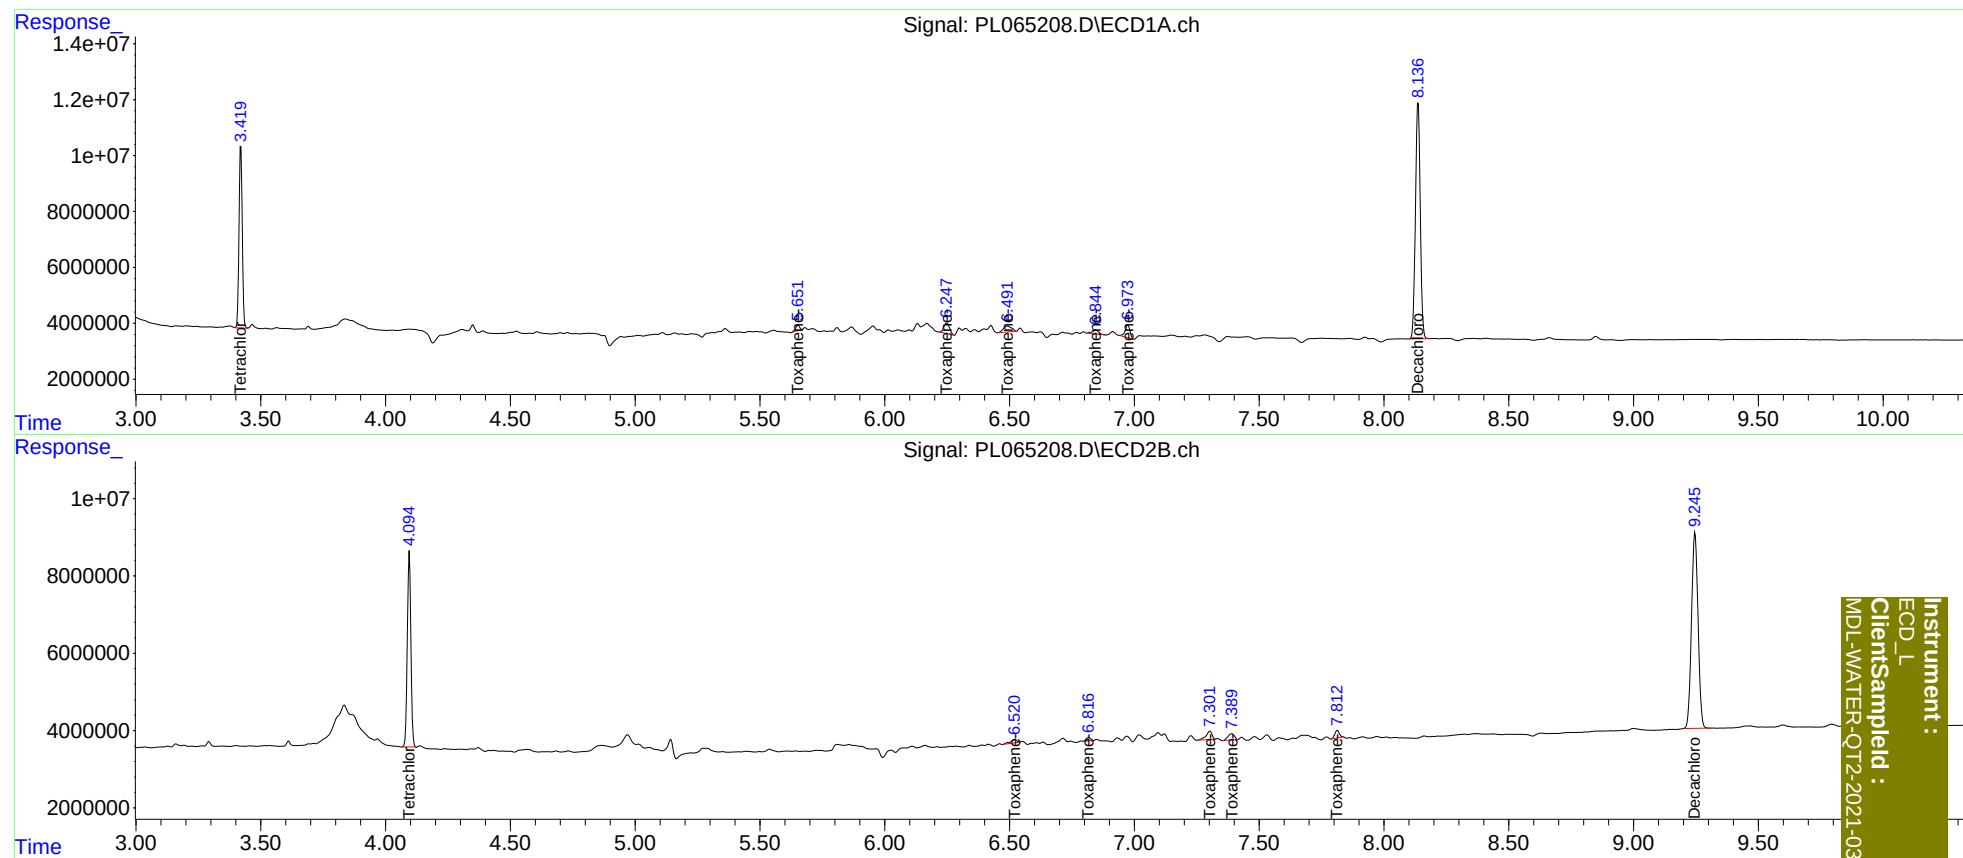

Instrument :
ECD_L
ClientSample :
MDL-WATER-QT2-2021-03